

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052119\
 Data File : PL048762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2019 11:06
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 01:09:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) MB Aldrin	4.585f	0.000	8720811	0	0.636	N.D. #
12) B 4,4'-DDE	5.452	0.000	89617818	0	7.065	N.D. #
13) MA Dieldrin	5.550	0.000	337.9E6	0	25.951	N.D. #
14) MA Endrin	5.789f	0.000	137.2E6	0	11.267	N.D. #
16) A 4,4'-DDD	5.954	0.000	25017478	0	2.570	N.D. #
17) MA 4,4'-DDT	6.185	0.000	209.5E6	0	20.849	N.D. #
18) B Endrin al...	6.282f	0.000	199.1E6	0	20.490	N.D. #
20) A Methoxychlor	6.744f	0.000	251.0E6	0	46.093	N.D. #
21) B Endrin ke...	6.948	0.000	46968244	0	4.030	N.D. #
22) Mirex	7.117	0.000	20666403	0	2.306	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052119\
Data File : PL048762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2019 11:06
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 01:09:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

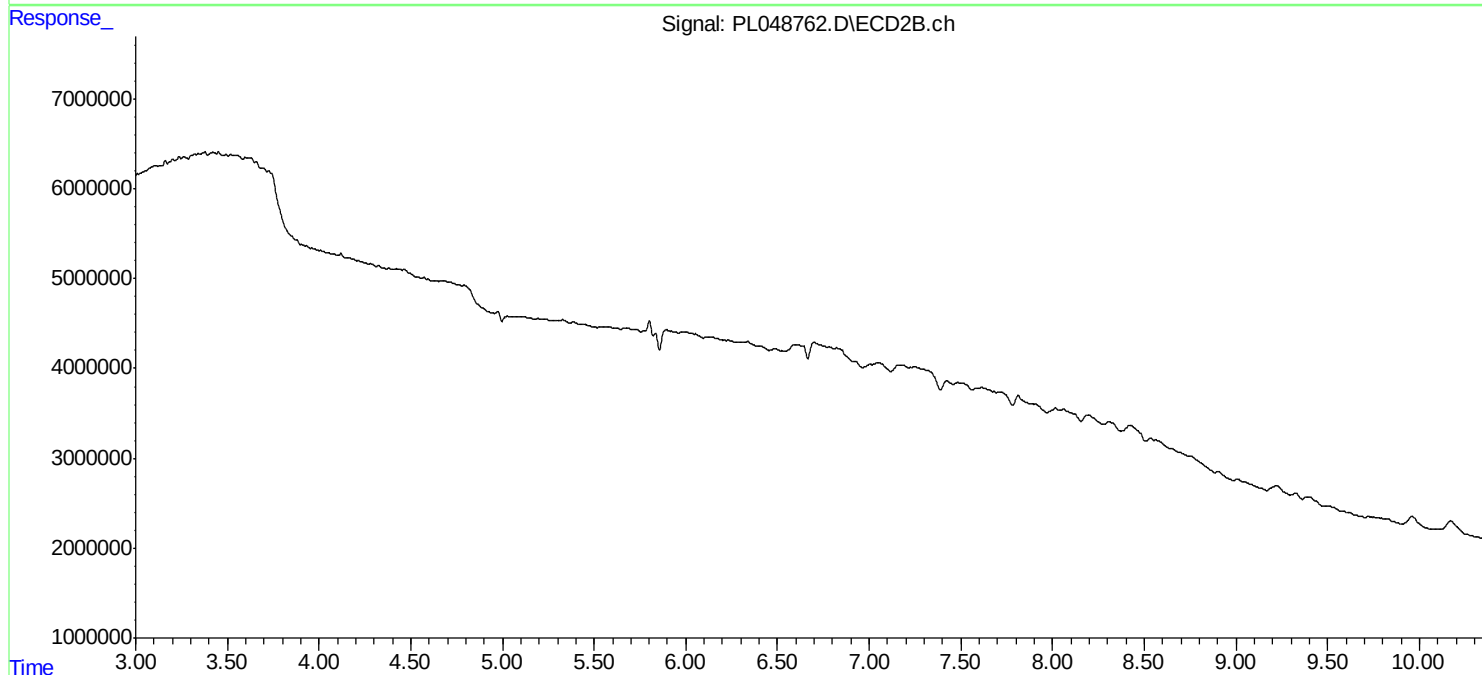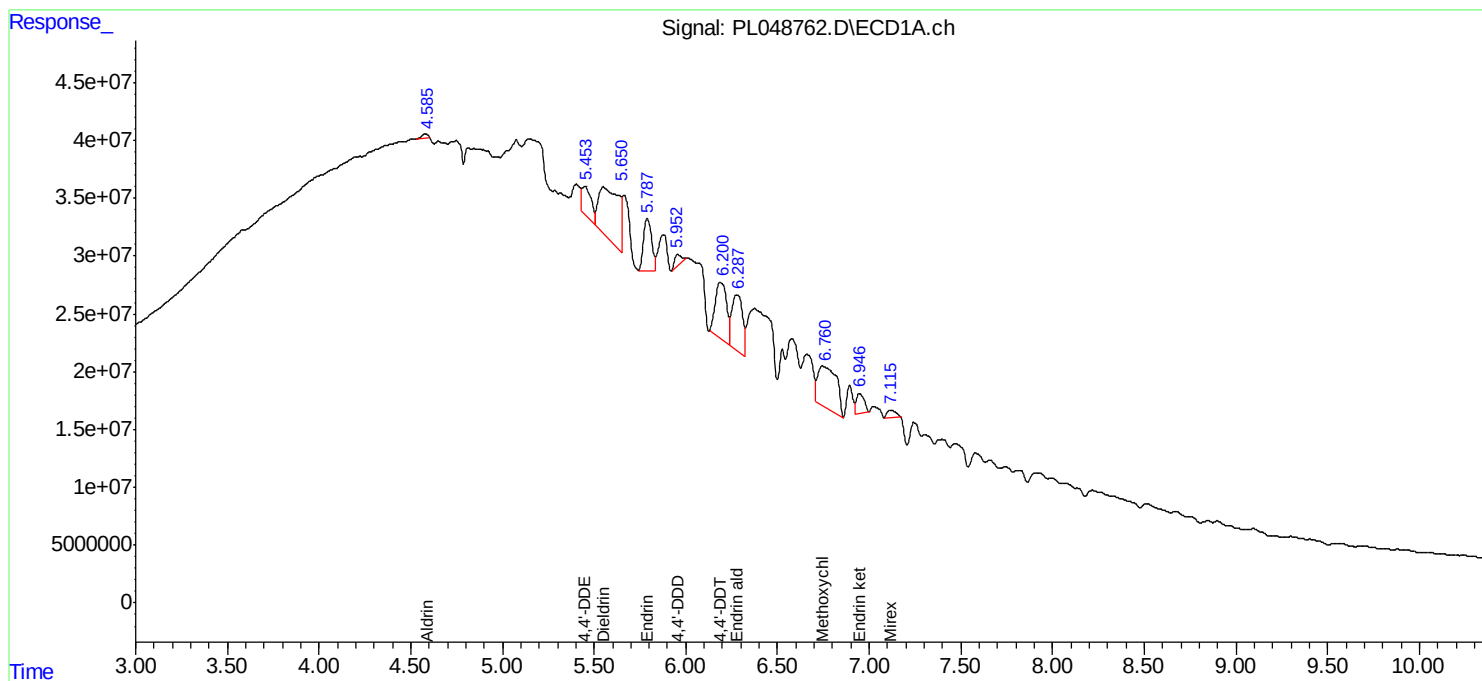


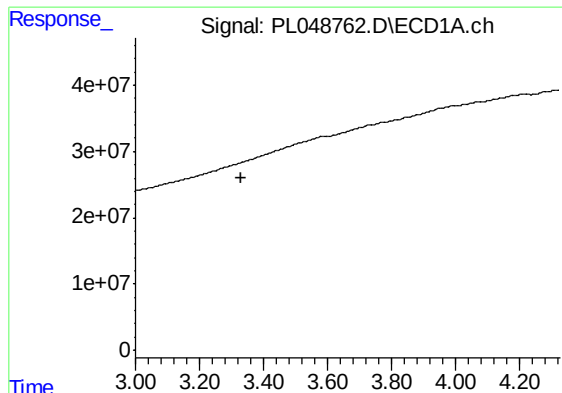

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

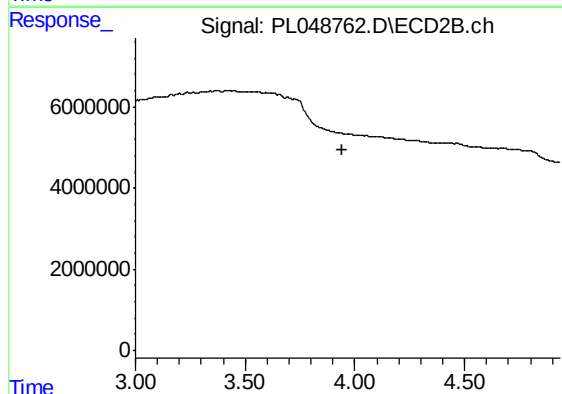


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.940 min
Response: 0
Conc: N.D.

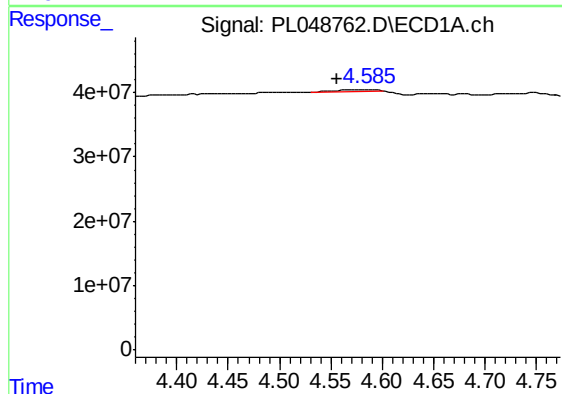


#5 Aldrin

R.T.: 4.585 min
Delta R.T.: 0.030 min
Response: 8720811
Conc: 0.64 ng/ml

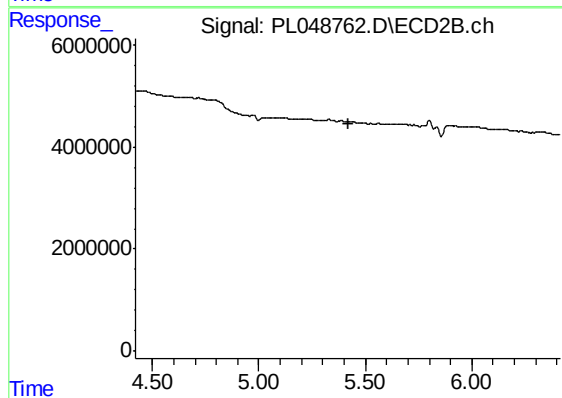

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.418 min
Response: 0
Conc: N.D.

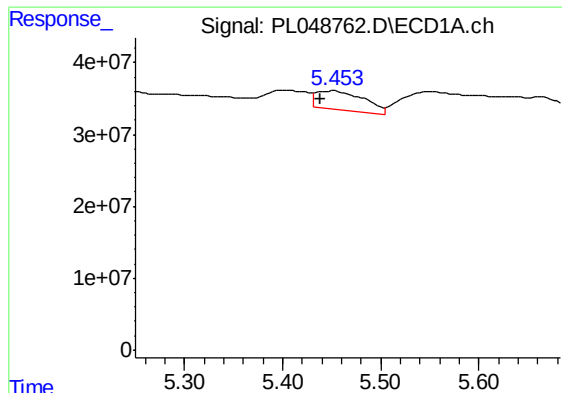

#12 4,4'-DDE


R.T.: 5.452 min
Delta R.T.: 0.014 min
Response: 89617818
Conc: 7.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

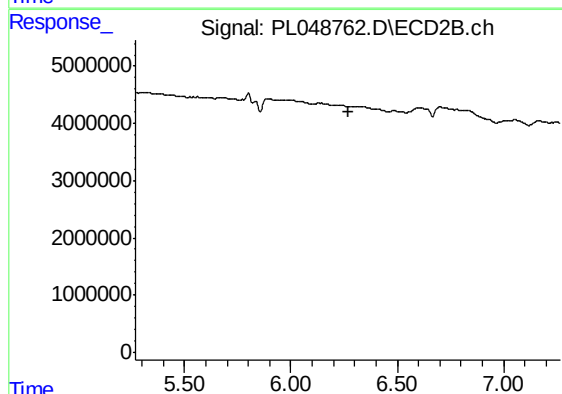


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.269 min
Response: 0
Conc: N.D.

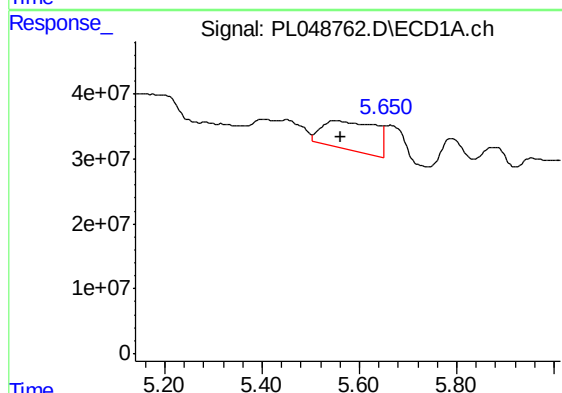


#13 Dieldrin

R.T.: 5.550 min
Delta R.T.: -0.012 min
Response: 337895771
Conc: 25.95 ng/ml

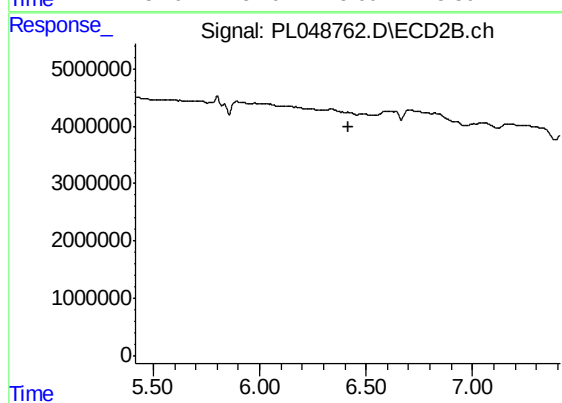

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

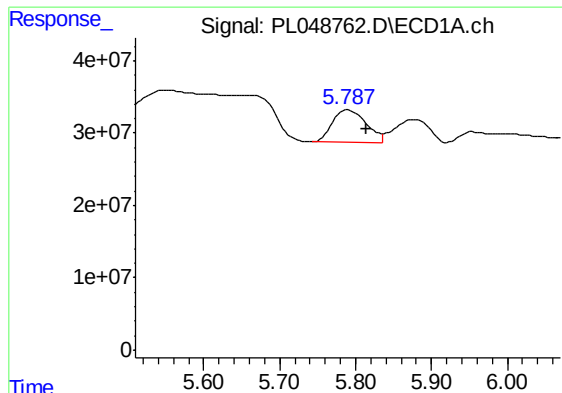

#14 Endrin


R.T.: 5.789 min
Delta R.T.: -0.025 min
Response: 137162385
Conc: 11.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

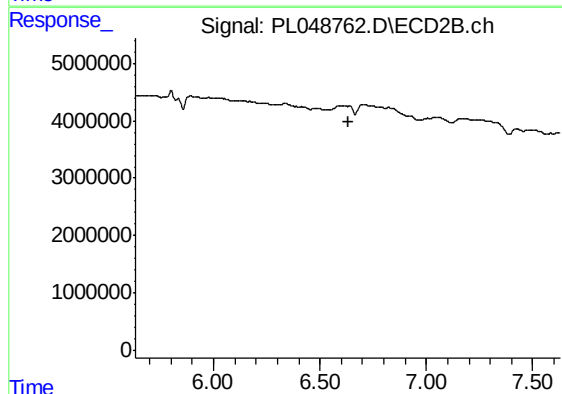


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

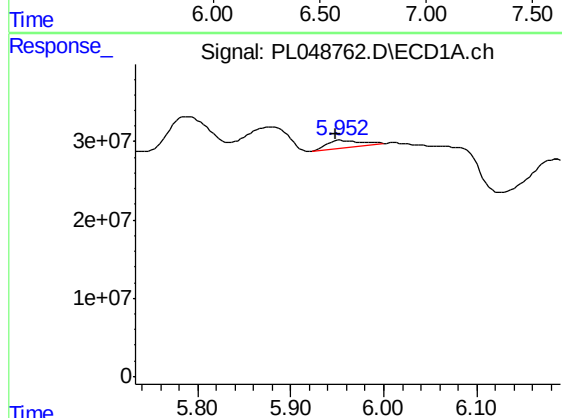


#16 4,4'-DDD

R.T.: 5.954 min
Delta R.T.: 0.005 min
Response: 25017478
Conc: 2.57 ng/ml

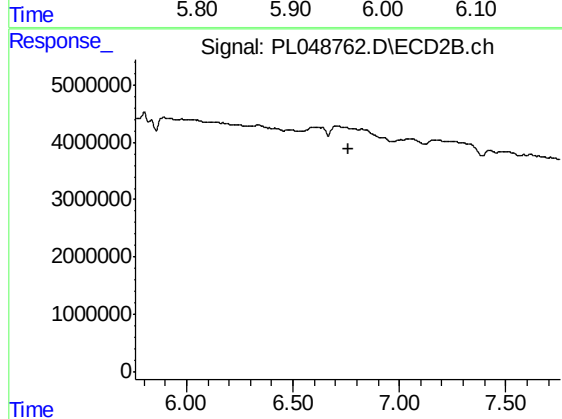

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

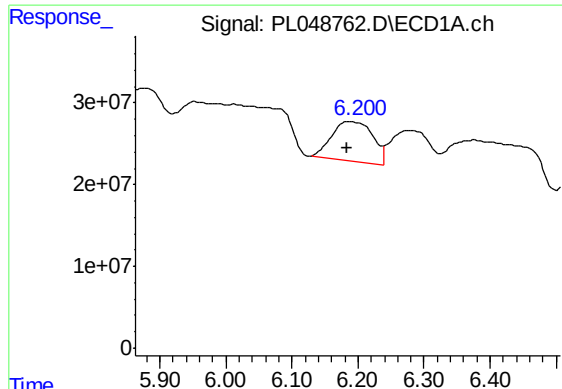

#17 4,4'-DDT


R.T.: 6.185 min
Delta R.T.: 0.001 min
Response: 209458544
Conc: 20.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

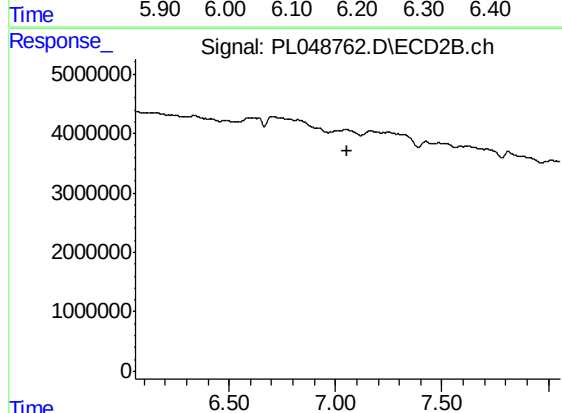


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.057 min
Response: 0
Conc: N.D.

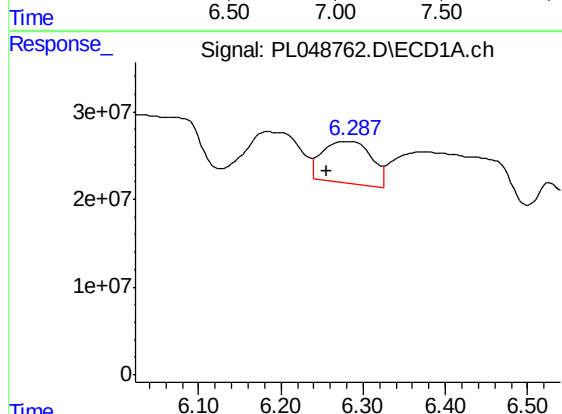


#18 Endrin aldehyde

R.T.: 6.282 min
Delta R.T.: 0.026 min
Response: 199132150
Conc: 20.49 ng/ml

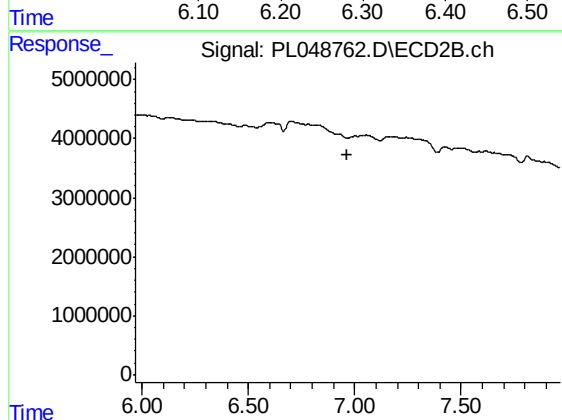

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.967 min
Response: 0
Conc: N.D.

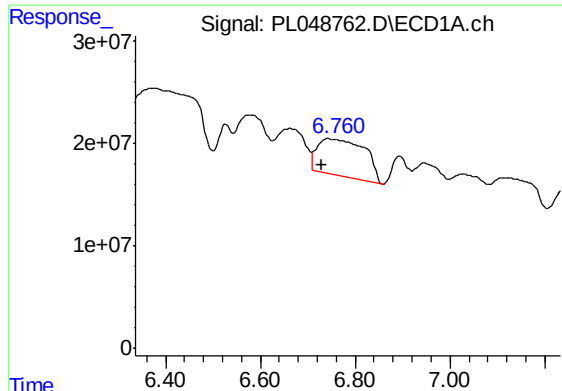

#20 Methoxychlor


R.T.: 6.744 min
Delta R.T.: 0.015 min
Response: 250963102
Conc: 46.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

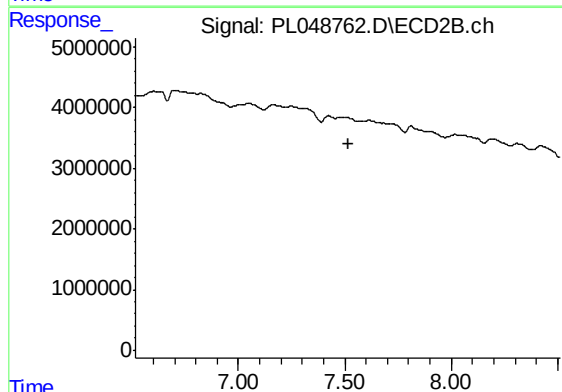


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.516 min
Response: 0
Conc: N.D.

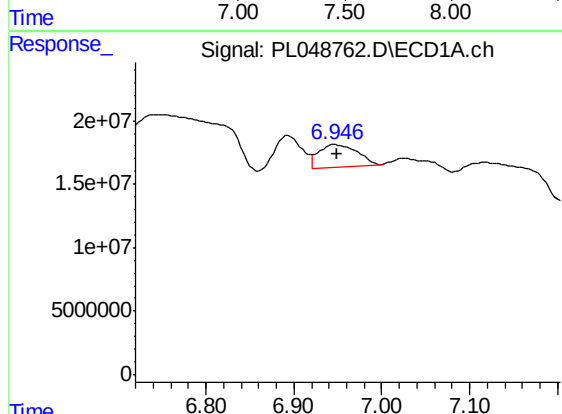


#21 Endrin ketone

R.T.: 6.948 min
Delta R.T.: -0.002 min
Response: 46968244
Conc: 4.03 ng/ml

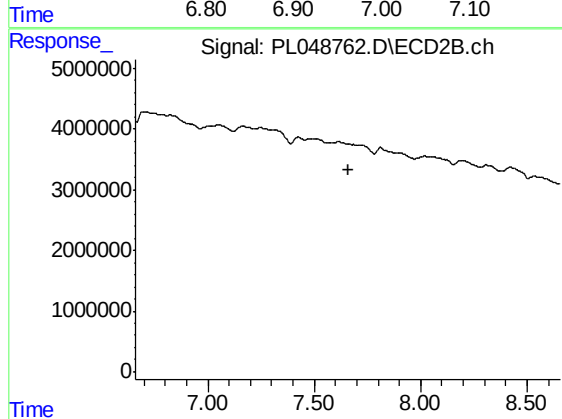

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.658 min
Response: 0
Conc: N.D.

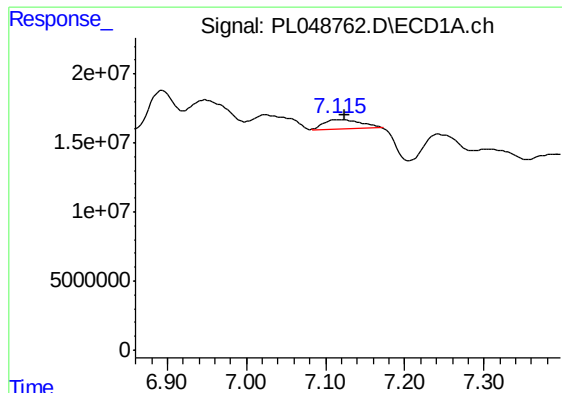

#22 Mirex


R.T.: 7.117 min
Delta R.T.: -0.007 min
Response: 20666403
Conc: 2.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

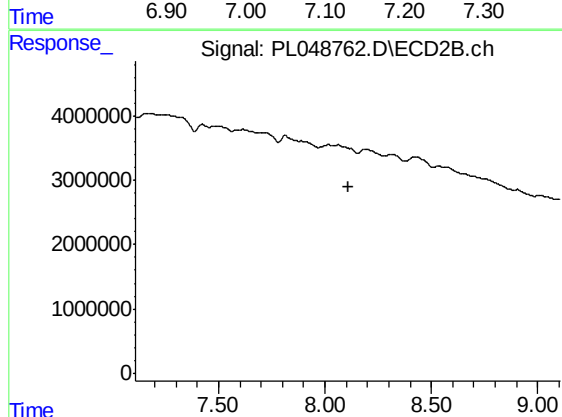


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.109 min
Response: 0
Conc: N.D.

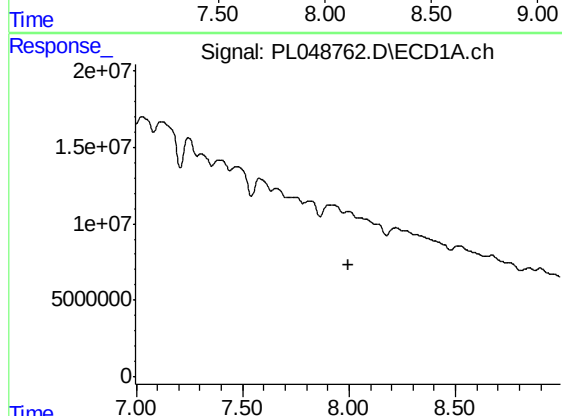

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.996 min
Response: 0
Conc: N.D.

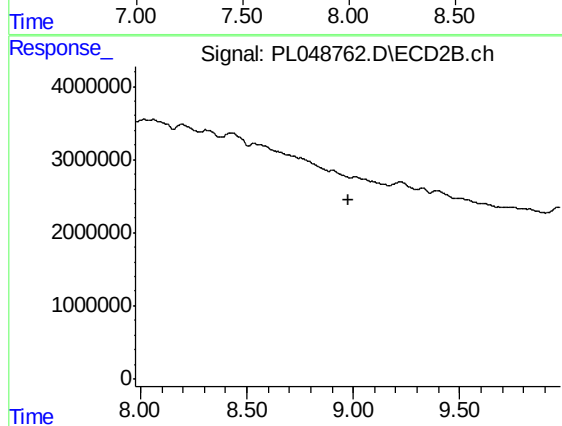

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.975 min
Response: 0
Conc: N.D.