

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052119\
 Data File : PL048780.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2019 18:38
 Operator : SM\AJ
 Sample : K2951-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-14-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 01:13:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.939	0	20907746	N.D.	8.394 #
28)	SA Decachlor...	7.994	8.975	59594682	17371245	5.927	6.545
Target Compounds							
4)	MA Heptachlor	4.301f	0.000	50396694	0	3.426	N.D. #
5)	MB Aldrin	4.542	0.000	1940.0E6	0	141.589	N.D. #
6)	B beta-BHC	4.301f	0.000	50396694	0	8.540	N.D. #
7)	B delta-BHC	0.000	4.976f	0	70104181	N.D.	24.790 #
9)	A Endosulfan I	5.333	6.184f	182.6E6	36336428	15.178	12.851
11)	B alpha-Chl...	5.270	0.000	1992.8E6	0	152.426	N.D. #
23)	Chlordane-1	4.181	0.000	26851051	0	59.814	N.D. #
26)	Chlordane-4	5.270	0.000	1992.8E6	0	1372.591	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052119\
Data File : PL048780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2019 18:38
Operator : SM\AJ
Sample : K2951-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-14-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 01:13:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

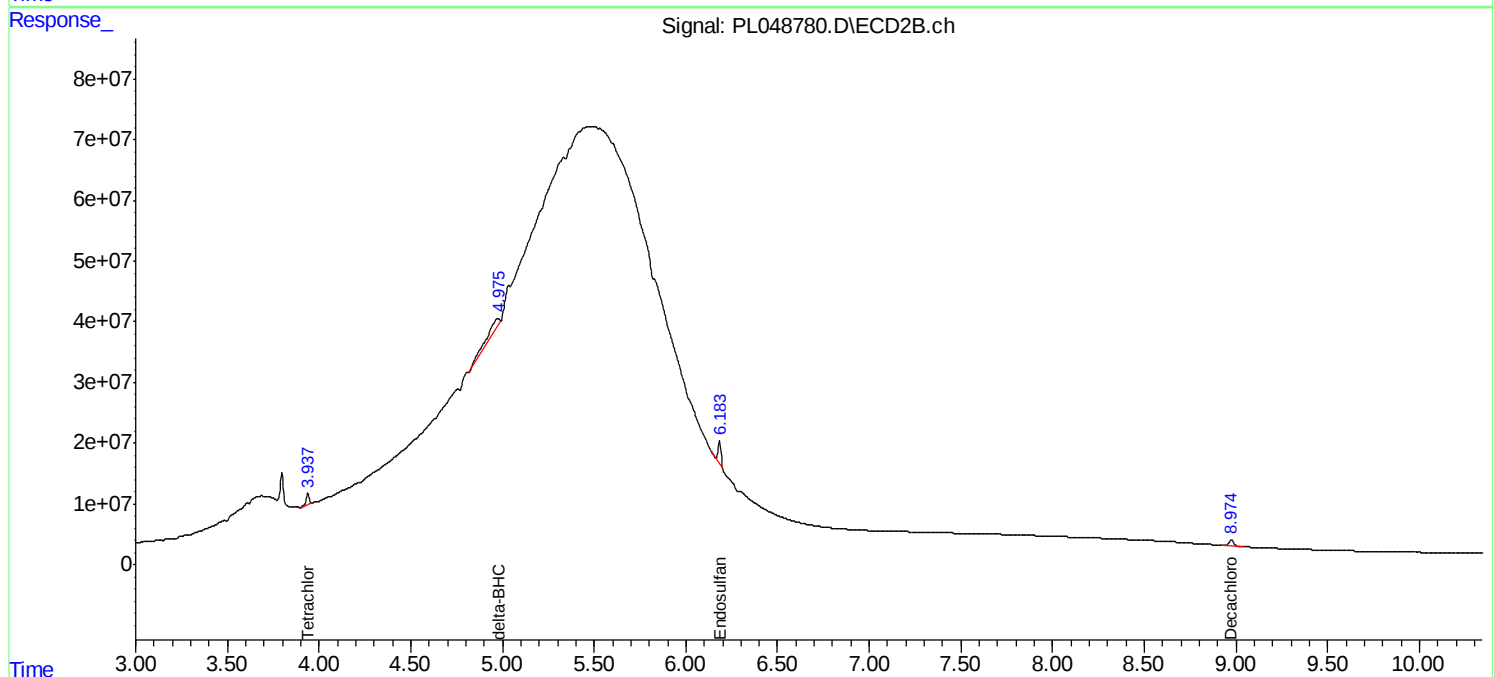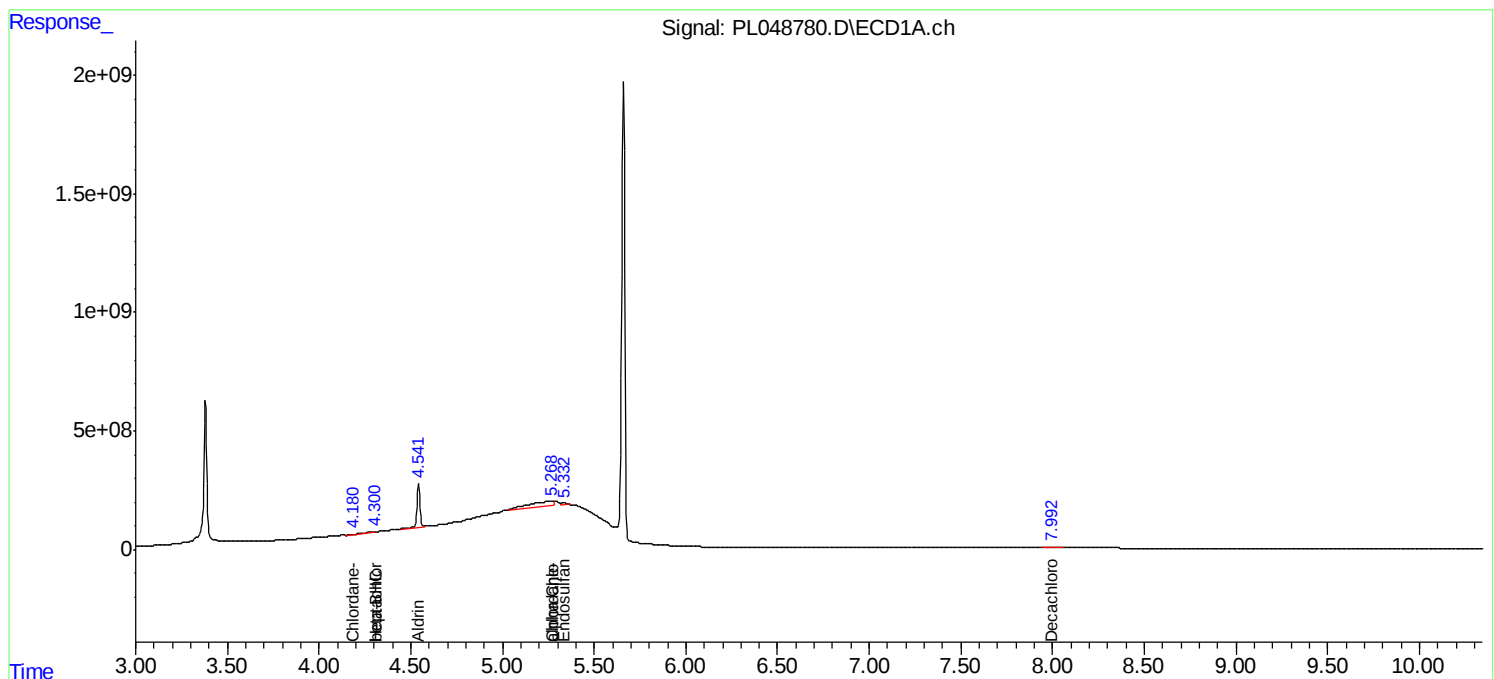


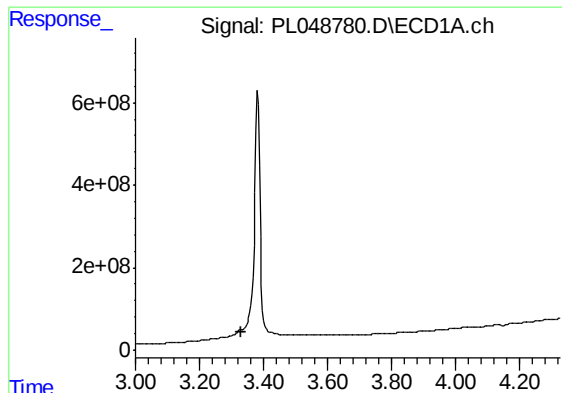

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-14-S

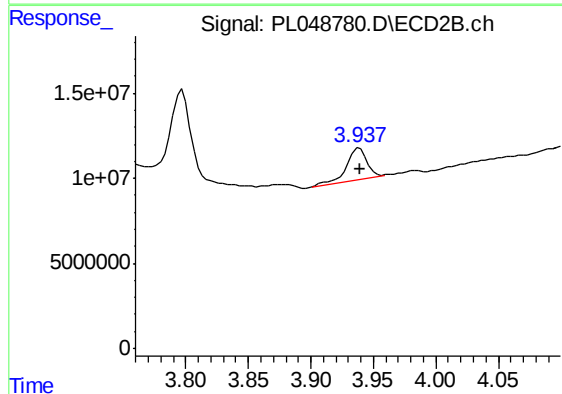


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 20907746
Conc: 8.39 ng/ml

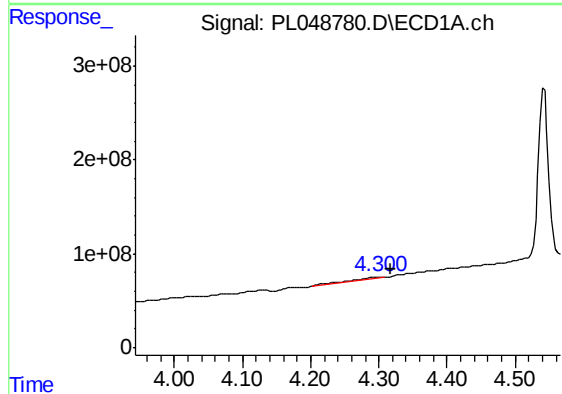


#4 Heptachlor

R.T.: 4.301 min
Delta R.T.: -0.016 min
Response: 50396694
Conc: 3.43 ng/ml

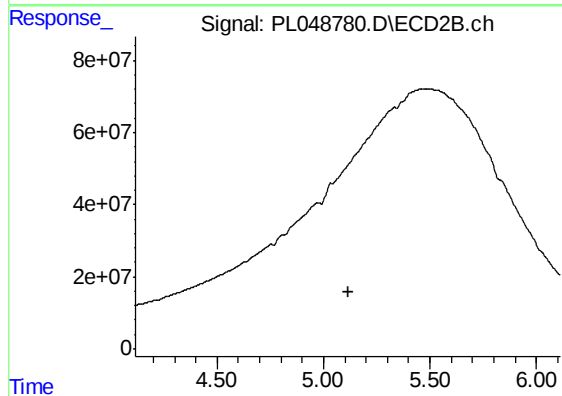

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.116 min
Response: 0
Conc: N.D.

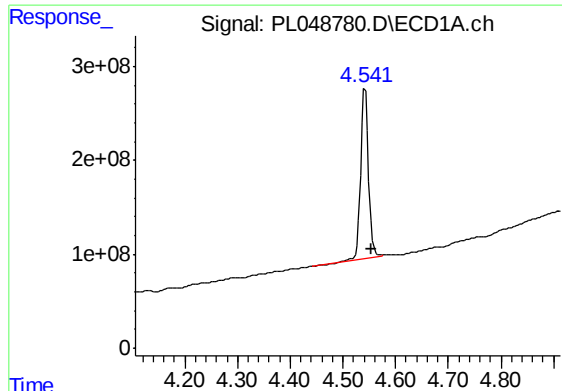

#5 Aldrin


R.T.: 4.542 min
Delta R.T.: -0.013 min
Response: 1939984987
Conc: 141.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

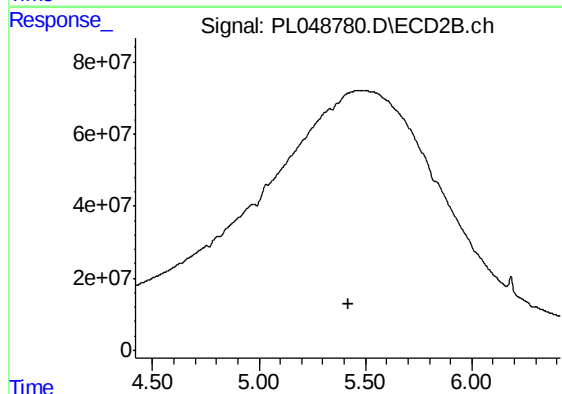


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.418 min
Response: 0
Conc: N.D.

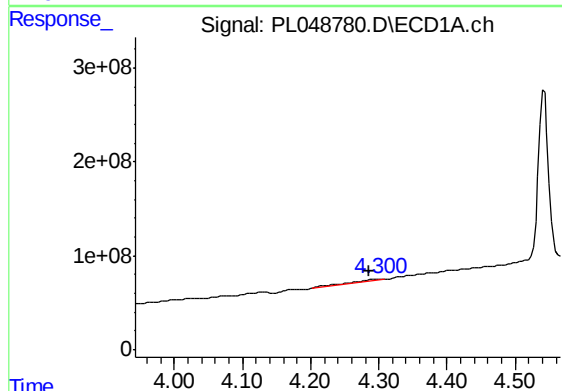


#6 beta-BHC

R.T.: 4.301 min
Delta R.T.: 0.016 min
Response: 50396694
Conc: 8.54 ng/ml

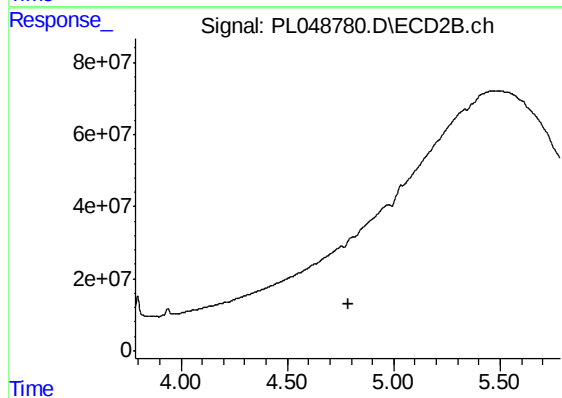

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.786 min
Response: 0
Conc: N.D.

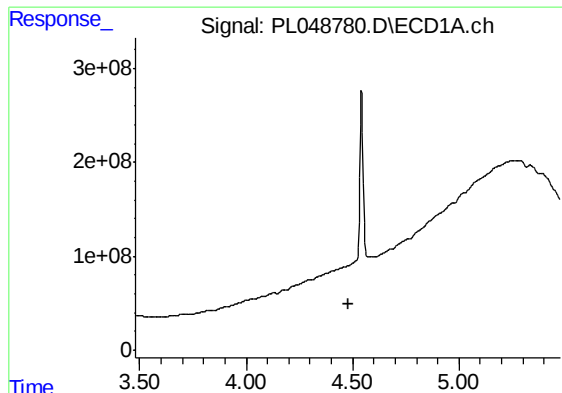

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-14-S

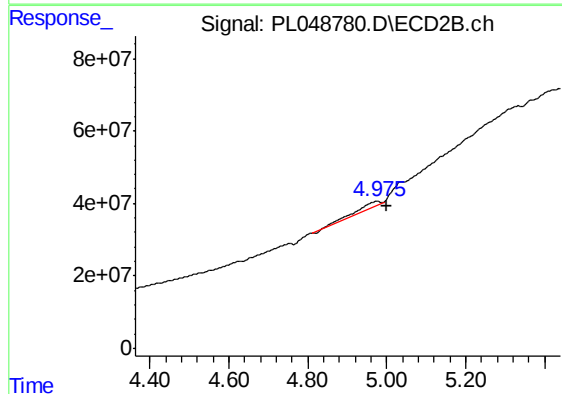


#7 delta-BHC

R.T.: 4.976 min
Delta R.T.: -0.024 min
Response: 70104181
Conc: 24.79 ng/ml

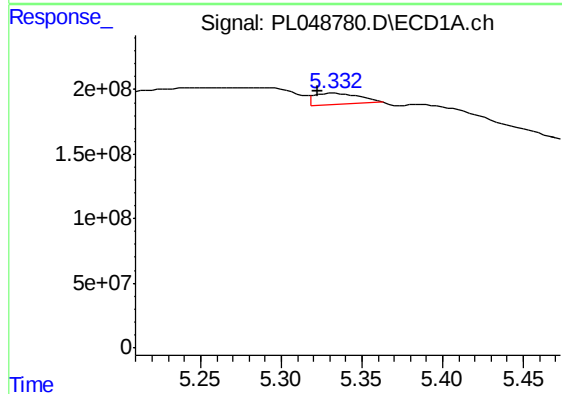


#9 Endosulfan I

R.T.: 5.333 min
Delta R.T.: 0.011 min
Response: 182587504
Conc: 15.18 ng/ml

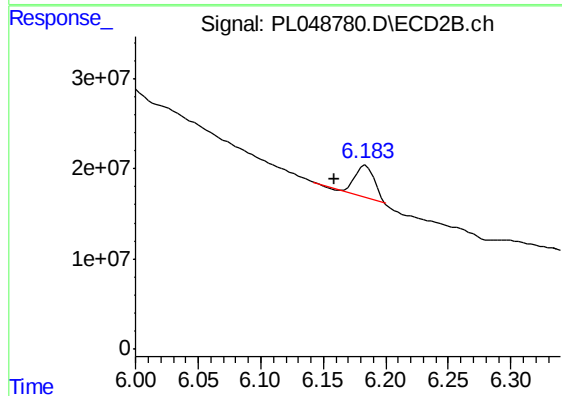

#9 Endosulfan I


R.T.: 6.184 min
Delta R.T.: 0.025 min
Response: 36336428
Conc: 12.85 ng/ml

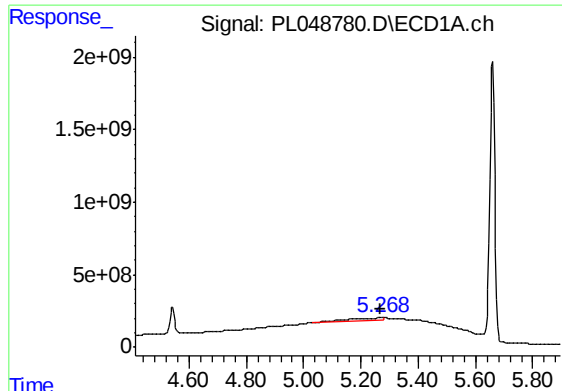

#11 alpha-Chlordane


R.T.: 5.270 min
Delta R.T.: -0.001 min
Response: 1992758397
Conc: 152.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

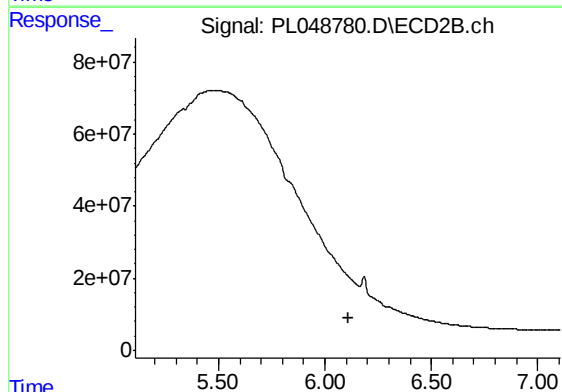


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

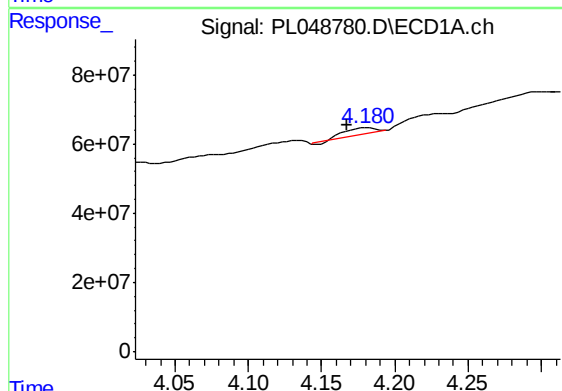


#23 Chlordane-1

R.T.: 4.181 min
Delta R.T.: 0.013 min
Response: 26851051
Conc: 59.81 ng/ml

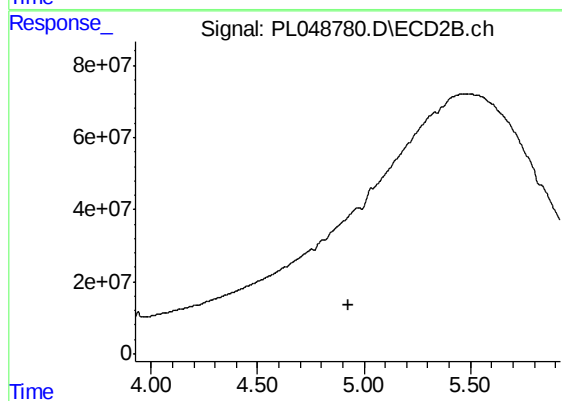

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

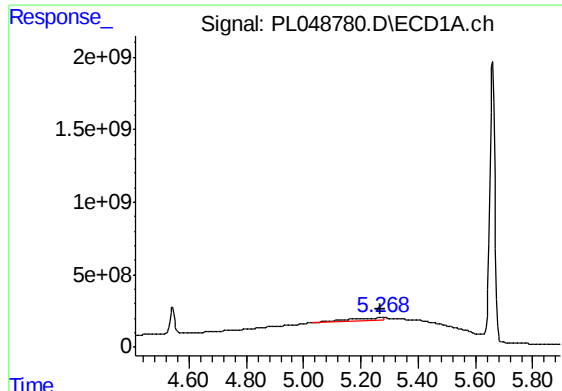

#26 Chlordane-4


R.T.: 5.270 min
Delta R.T.: 0.000 min
Response: 1992758397
Conc: 1372.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

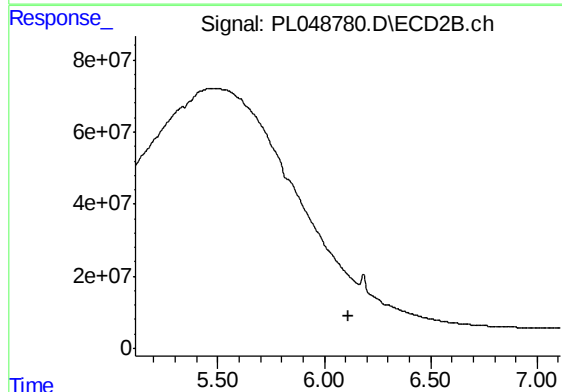


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.111 min
Response: 0
Conc: N.D.

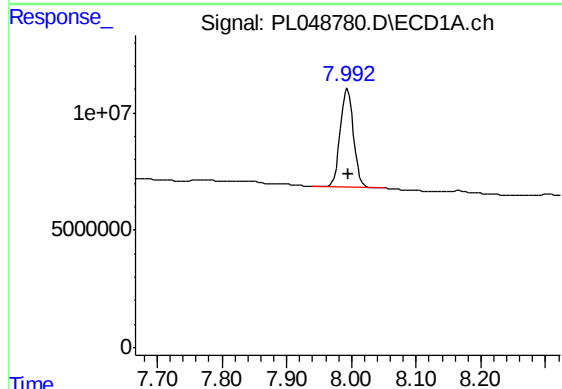

#28 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: -0.002 min
Response: 59594682
Conc: 5.93 ng/ml

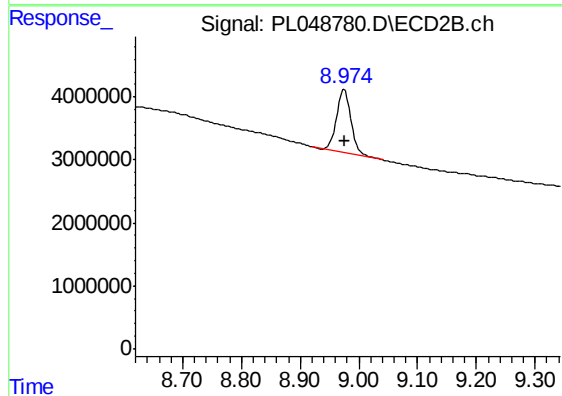

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 17371245
Conc: 6.54 ng/ml