

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052119\
 Data File : PL048803.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2019 00:55
 Operator : SM\AJ
 Sample : K2951-10
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-14-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 01:19:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.326	3.938	181.2E6	50870738	18.710	20.423
28) SA Decachlor...	7.994	8.973	221.0E6	62341319	21.983	23.487
Target Compounds						
7) B delta-BHC	0.000	4.974f	0	12001632	N.D.	4.244 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052119\
Data File : PL048803.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2019 00:55
Operator : SM\AJ
Sample : K2951-10
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-14-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 01:19:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

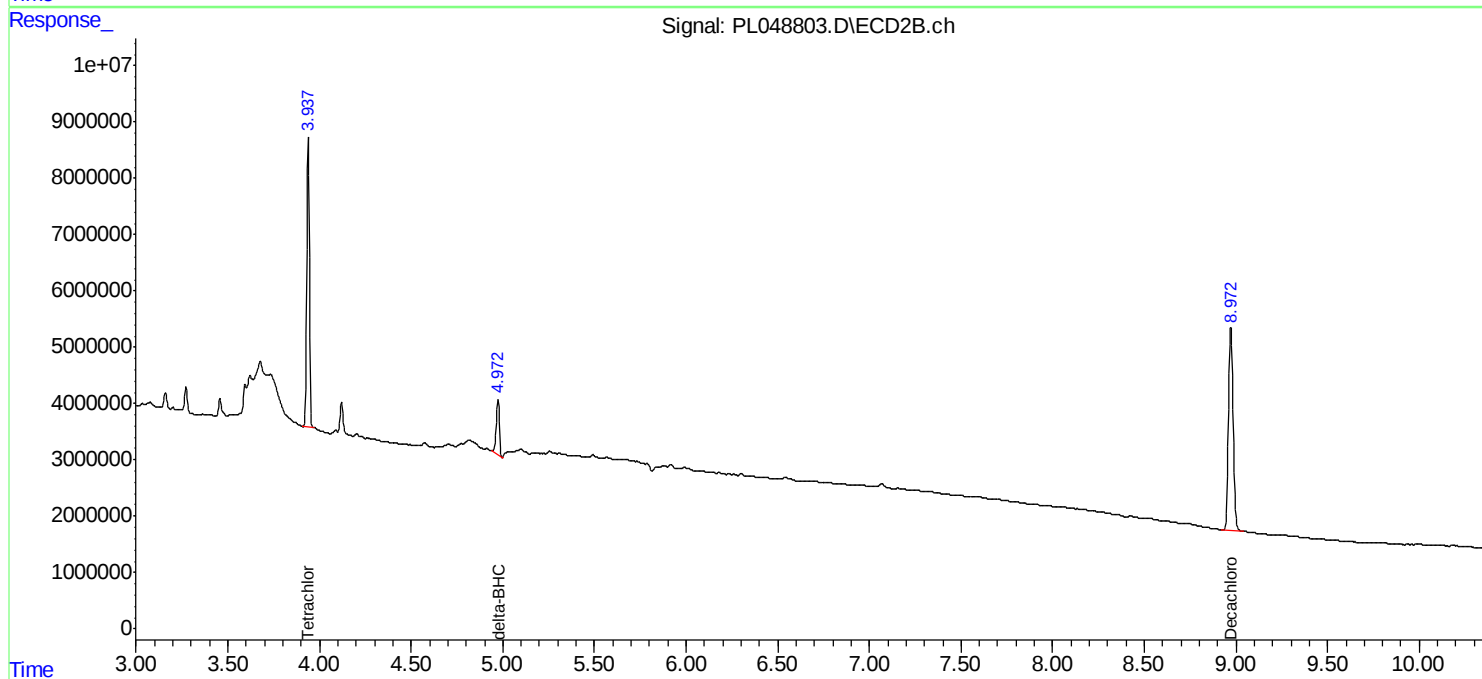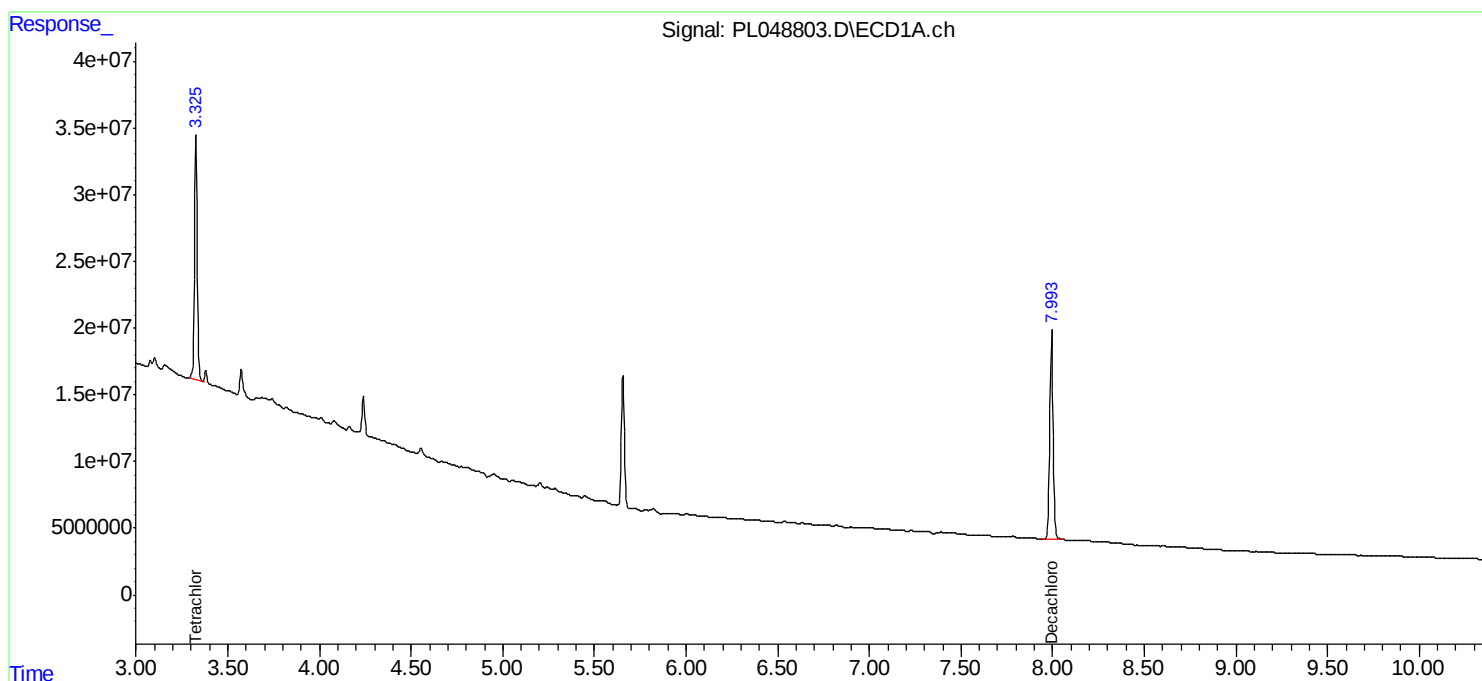


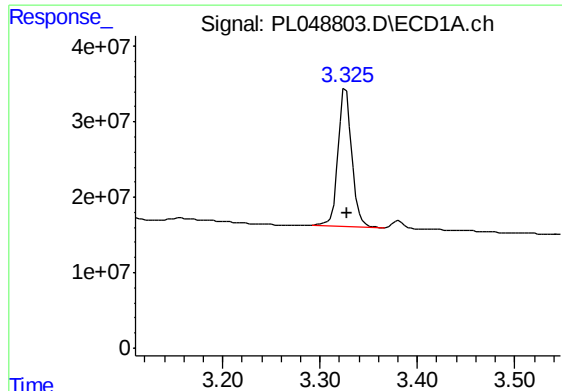

#1 Tetrachloro-m-xylene


R.T.: 3.326 min
Delta R.T.: -0.002 min
Response: 181238052
Conc: 18.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

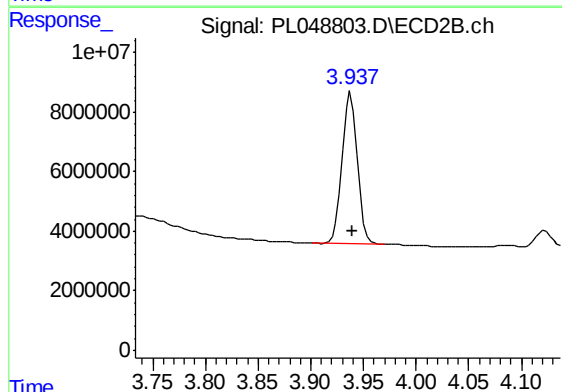


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: -0.002 min
Response: 50870738
Conc: 20.42 ng/ml

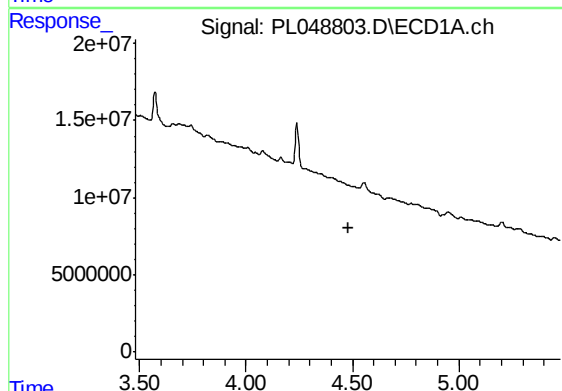


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

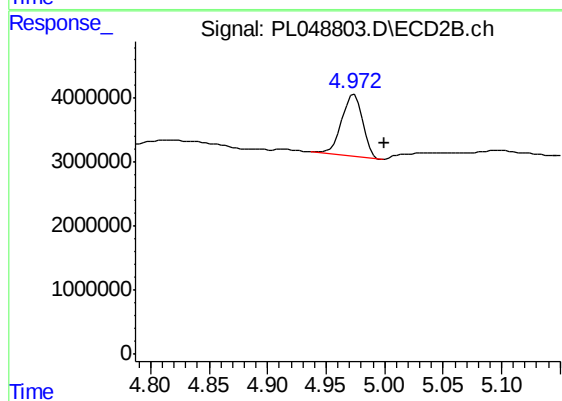

#7 delta-BHC


R.T.: 4.974 min
Delta R.T.: -0.026 min
Response: 12001632
Conc: 4.24 ng/ml

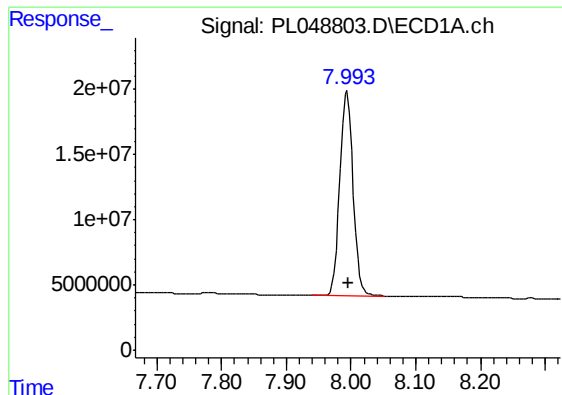

#28 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: -0.002 min
Response: 221016980
Conc: 21.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

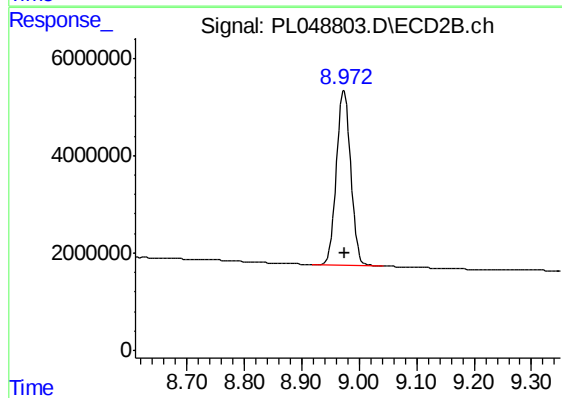

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: -0.002 min
Response: 62341319
Conc: 23.49 ng/ml