

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052119\
 Data File : PL048811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2019 03:26
 Operator : SM\AJ
 Sample : K2909-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20190350-FIELD-BLANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 06:41:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.326	3.938	190.3E6	51410081	19.642	20.639
28)	SA Decachlor...	7.994	8.973	194.7E6	54441414	19.369	20.511
Target Compounds							
7)	B delta-BHC	0.000	4.972f	0	5955176	N.D.	2.106 #
10)	B gamma-Chl...	5.242f	0.000	34994968	0	2.621	N.D. #
11)	B alpha-Chl...	5.242f	6.089f	34994968	2090646	2.677	0.681 #
15)	B Endosulfa...	6.105f	6.859f	9330980	1574113	0.809	0.584 #
25)	Chlordane-3	5.242f	0.000	34994968	0	22.225	N.D. #
26)	Chlordane-4	5.242f	6.089f	34994968	2090646	24.104	3.985 #
27)	Chlordane-5	6.105	0.000	9330980	0	19.872	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052119\
Data File : PL048811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2019 03:26
Operator : SM\AJ
Sample : K2909-01
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20190350-FIELD-BLANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 06:41:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

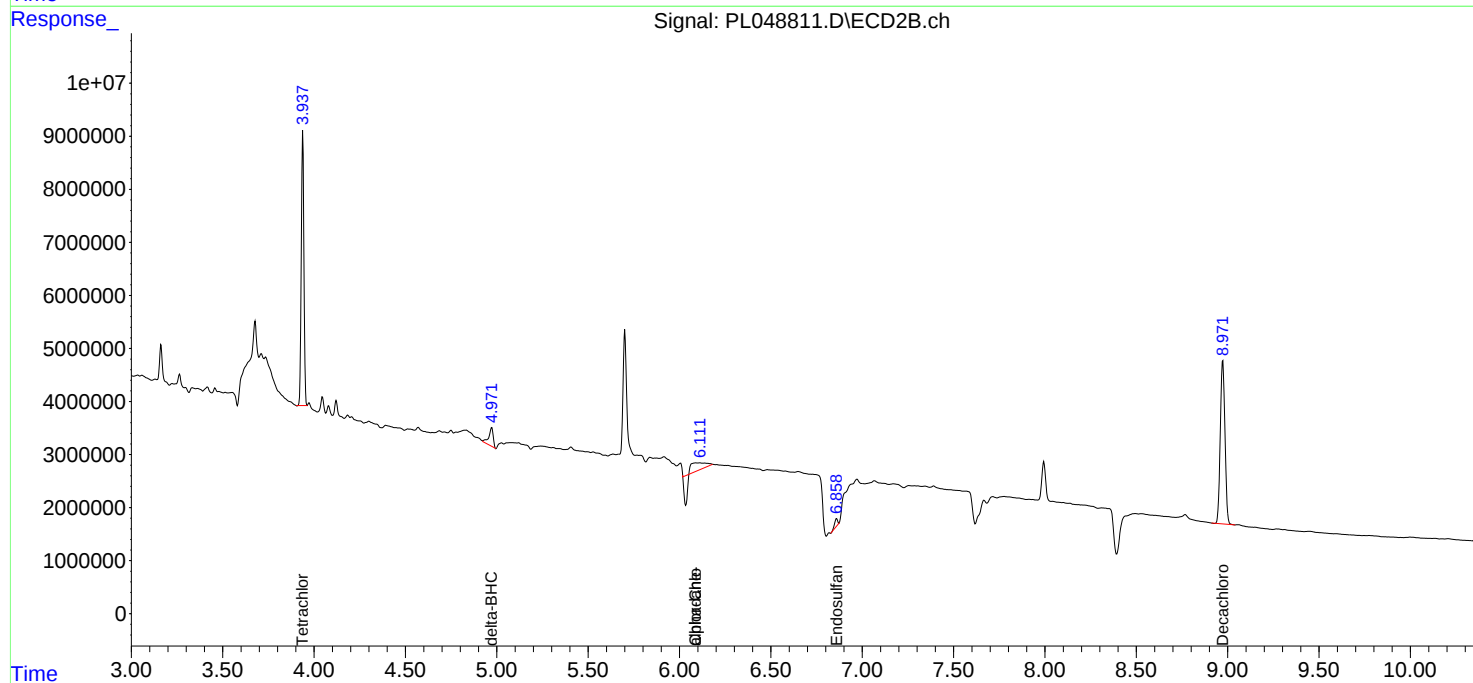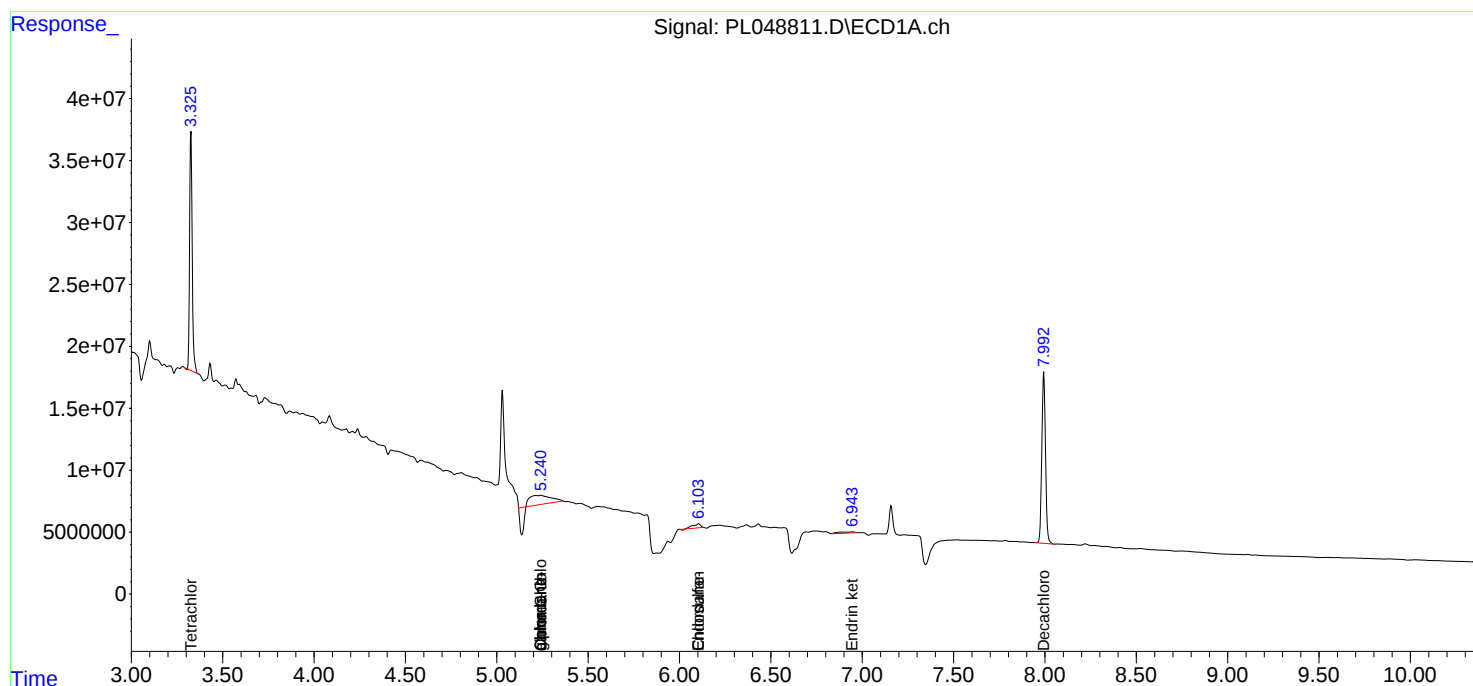


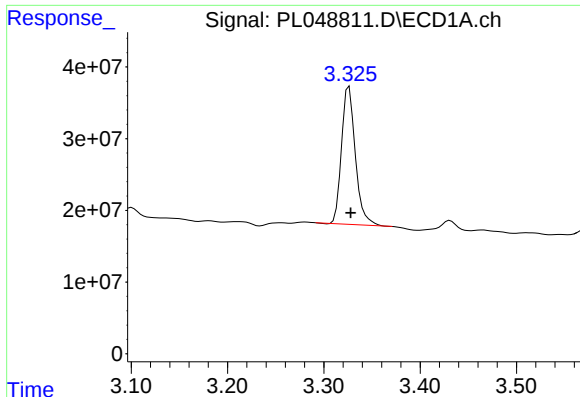

#1 Tetrachloro-m-xylene


R.T.: 3.326 min
Delta R.T.: -0.002 min
Response: 190267762
Conc: 19.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190350-FIELD-BLANK

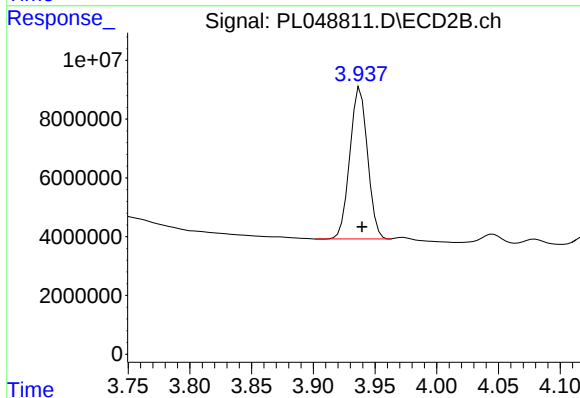


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: -0.002 min
Response: 51410081
Conc: 20.64 ng/ml

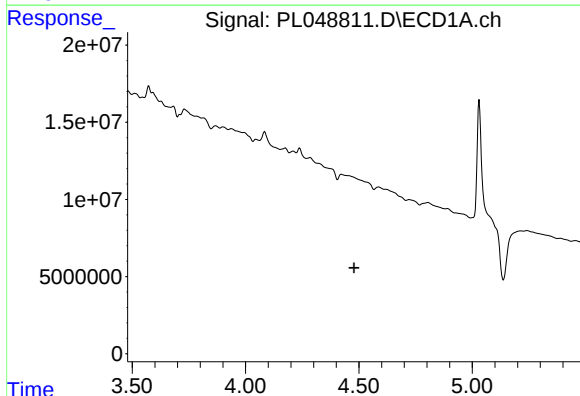


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

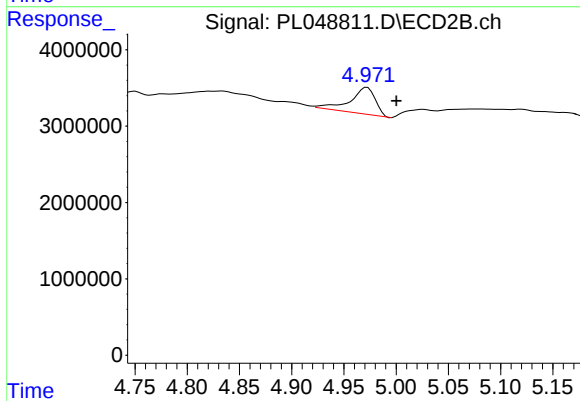

#7 delta-BHC


R.T.: 4.972 min
Delta R.T.: -0.028 min
Response: 5955176
Conc: 2.11 ng/ml

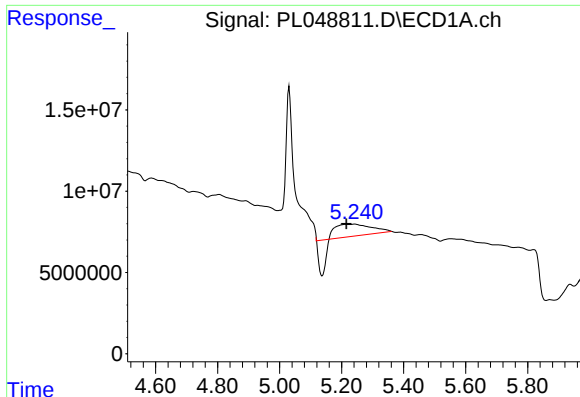

#10 gamma-Chlordane


R.T.: 5.242 min
Delta R.T.: 0.027 min
Response: 34994968
Conc: 2.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190350-FIELD-BLANK

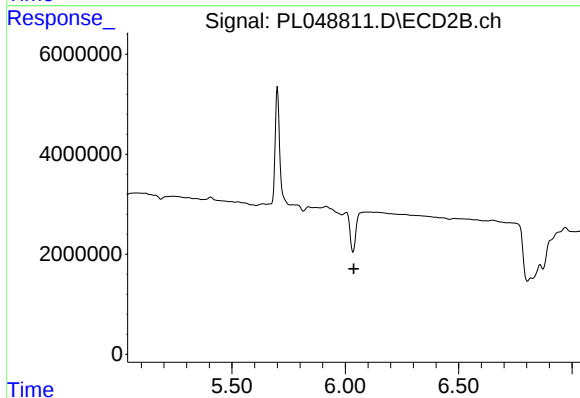


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

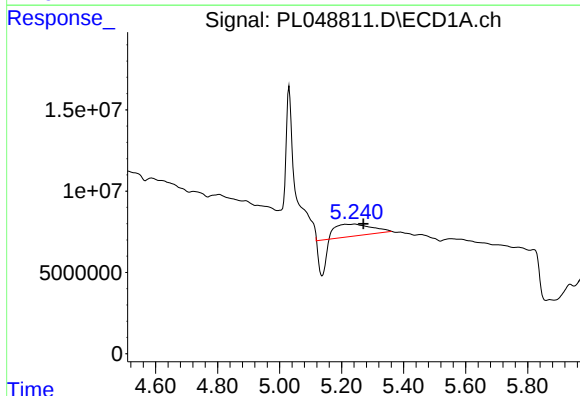


#11 alpha-Chlordane

R.T.: 5.242 min
Delta R.T.: -0.029 min
Response: 34994968
Conc: 2.68 ng/ml

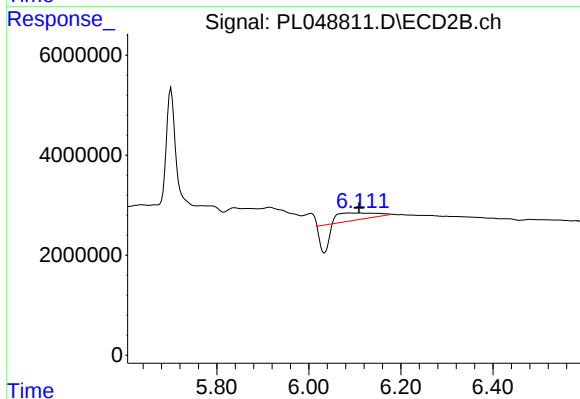

#11 alpha-Chlordane


R.T.: 6.089 min
Delta R.T.: -0.021 min
Response: 2090646
Conc: 0.68 ng/ml

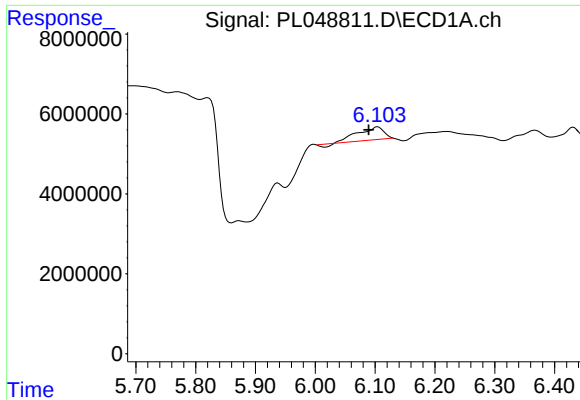

#15 Endosulfan II


R.T.: 6.105 min
Delta R.T.: 0.015 min
Response: 9330980
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190350-FIELD-BLANK

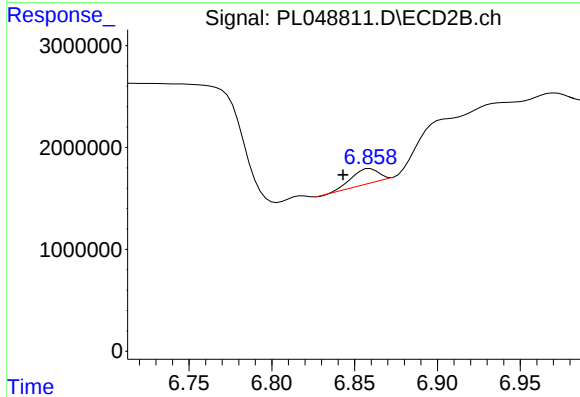


#15 Endosulfan II

R.T.: 6.859 min
Delta R.T.: 0.016 min
Response: 1574113
Conc: 0.58 ng/ml

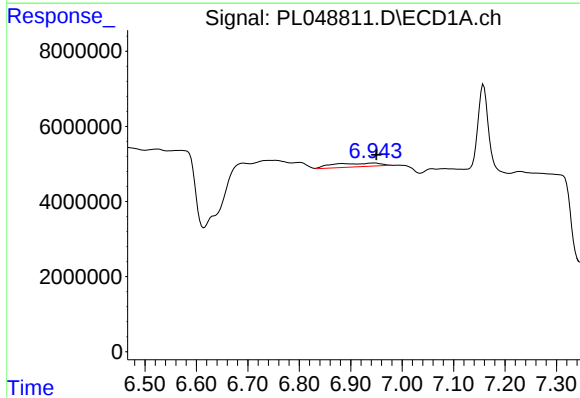


#21 Endrin ketone

R.T.: 6.946 min
Delta R.T.: -0.003 min
Response: 6155370
Conc: 0.53 ng/ml

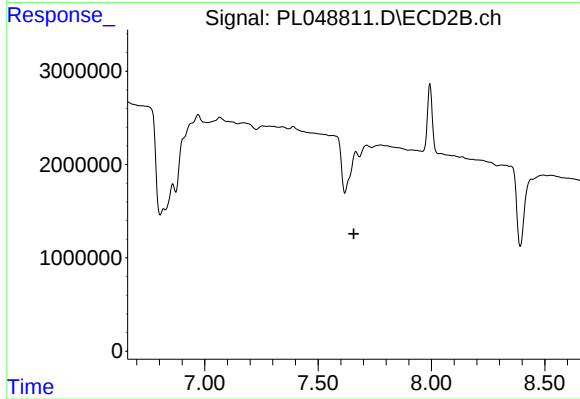

#21 Endrin ketone


R.T.: 7.667 min
Delta R.T.: 0.008 min
Response: -9645028
Conc: N.D.

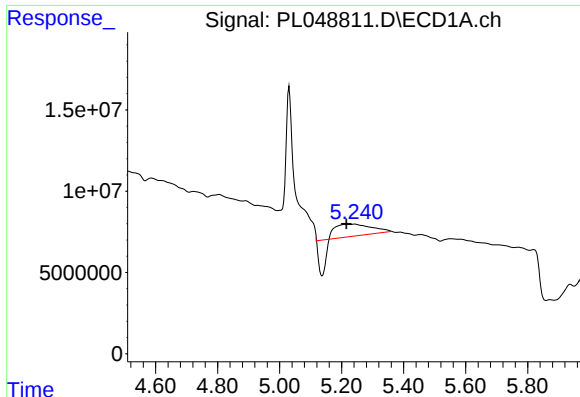

#25 Chlordane-3


R.T.: 5.242 min
Delta R.T.: 0.026 min
Response: 34994968
Conc: 22.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190350-FIELD-BLANK

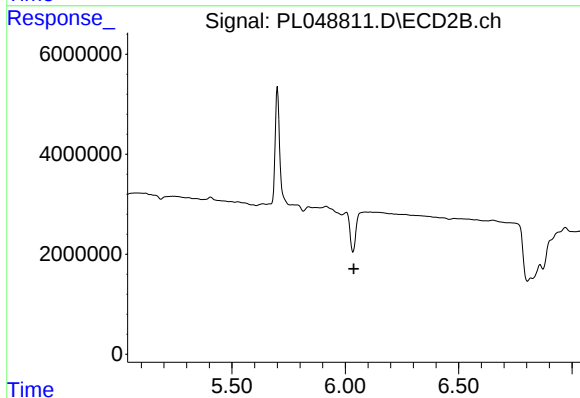


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

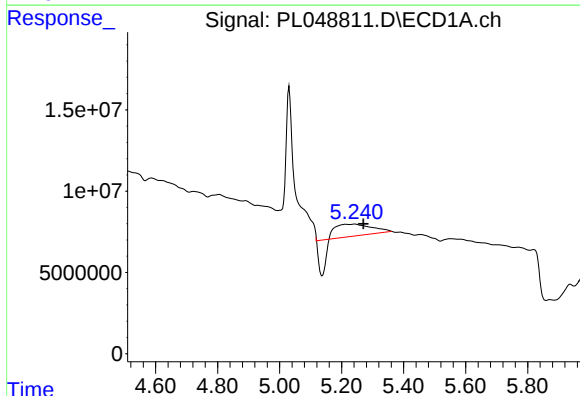


#26 Chlordane-4

R.T.: 5.242 min
Delta R.T.: -0.028 min
Response: 34994968
Conc: 24.10 ng/ml

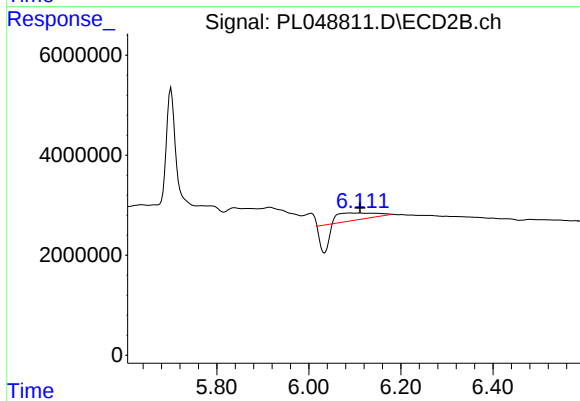

#26 Chlordane-4


R.T.: 6.089 min
Delta R.T.: -0.022 min
Response: 2090646
Conc: 3.99 ng/ml

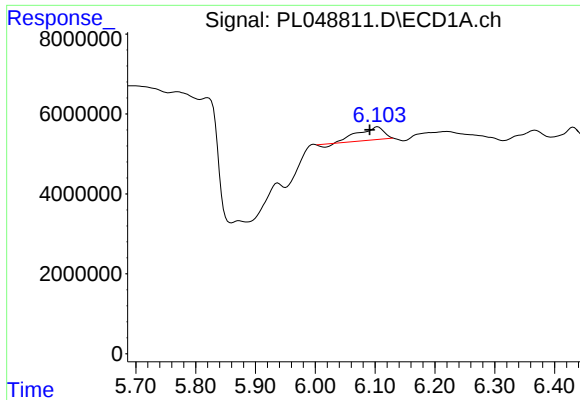

#27 Chlordane-5


R.T.: 6.105 min
Delta R.T.: 0.013 min
Response: 9330980
Conc: 19.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190350-FIELD-BLANK

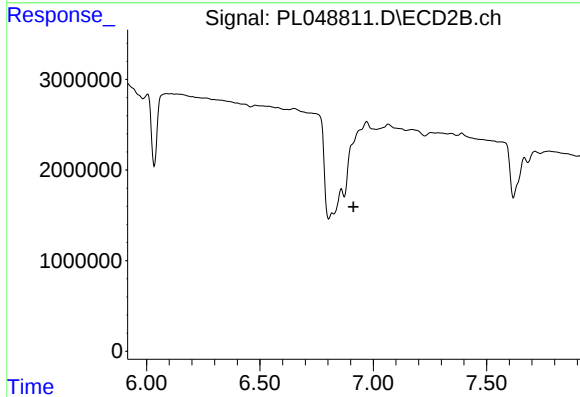


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.913 min
Response: 0
Conc: N.D.

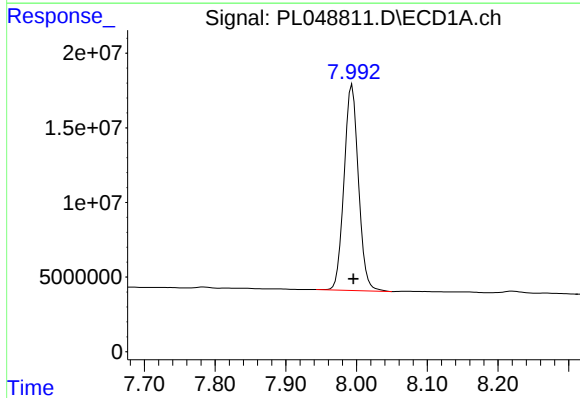

#28 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: -0.002 min
Response: 194734385
Conc: 19.37 ng/ml

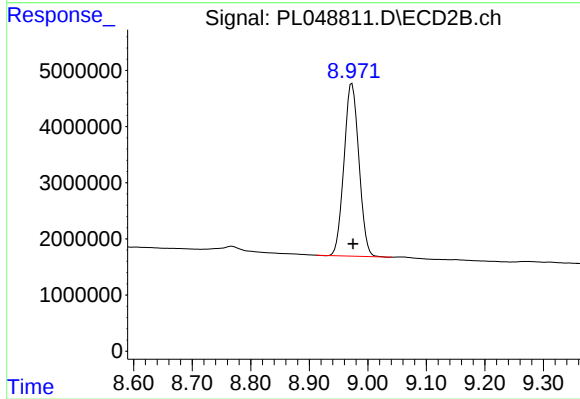

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: -0.002 min
Response: 54441414
Conc: 20.51 ng/ml