

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052120\
 Data File : PL058827.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 12:22
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 13:50:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.529	4.076	40848734	58559270	22.277	21.621
28)	SA Decachlor...	8.311	9.186	36698326	59063139	21.721	22.405
Target Compounds							
2)	A alpha-BHC	3.984	0.000	1342706	0	0.494	N.D. #
7)	B delta-BHC	0.000	5.119f	0	1735541	N.D.	0.476 #
8)	B Heptachlo...	0.000	5.956	0	232655	N.D.	0.071 #
13)	MA Dieldrin	0.000	6.557f	0	99103	N.D.	0.033 #
14)	MA Endrin	0.000	6.824f	0	220160	N.D.	0.088 #
15)	B Endosulfa...	0.000	7.011	0	1630573	N.D.	0.582 #
21)	B Endrin ke...	0.000	7.829	0	386721	N.D.	0.140 #
22)	Mirex	0.000	8.311f	0	538293	N.D.	0.246 #
23)	Chlordane-1	0.000	5.058f	0	1312802	N.D.	13.687 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052120\
Data File : PL058827.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 12:22
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 13:50:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

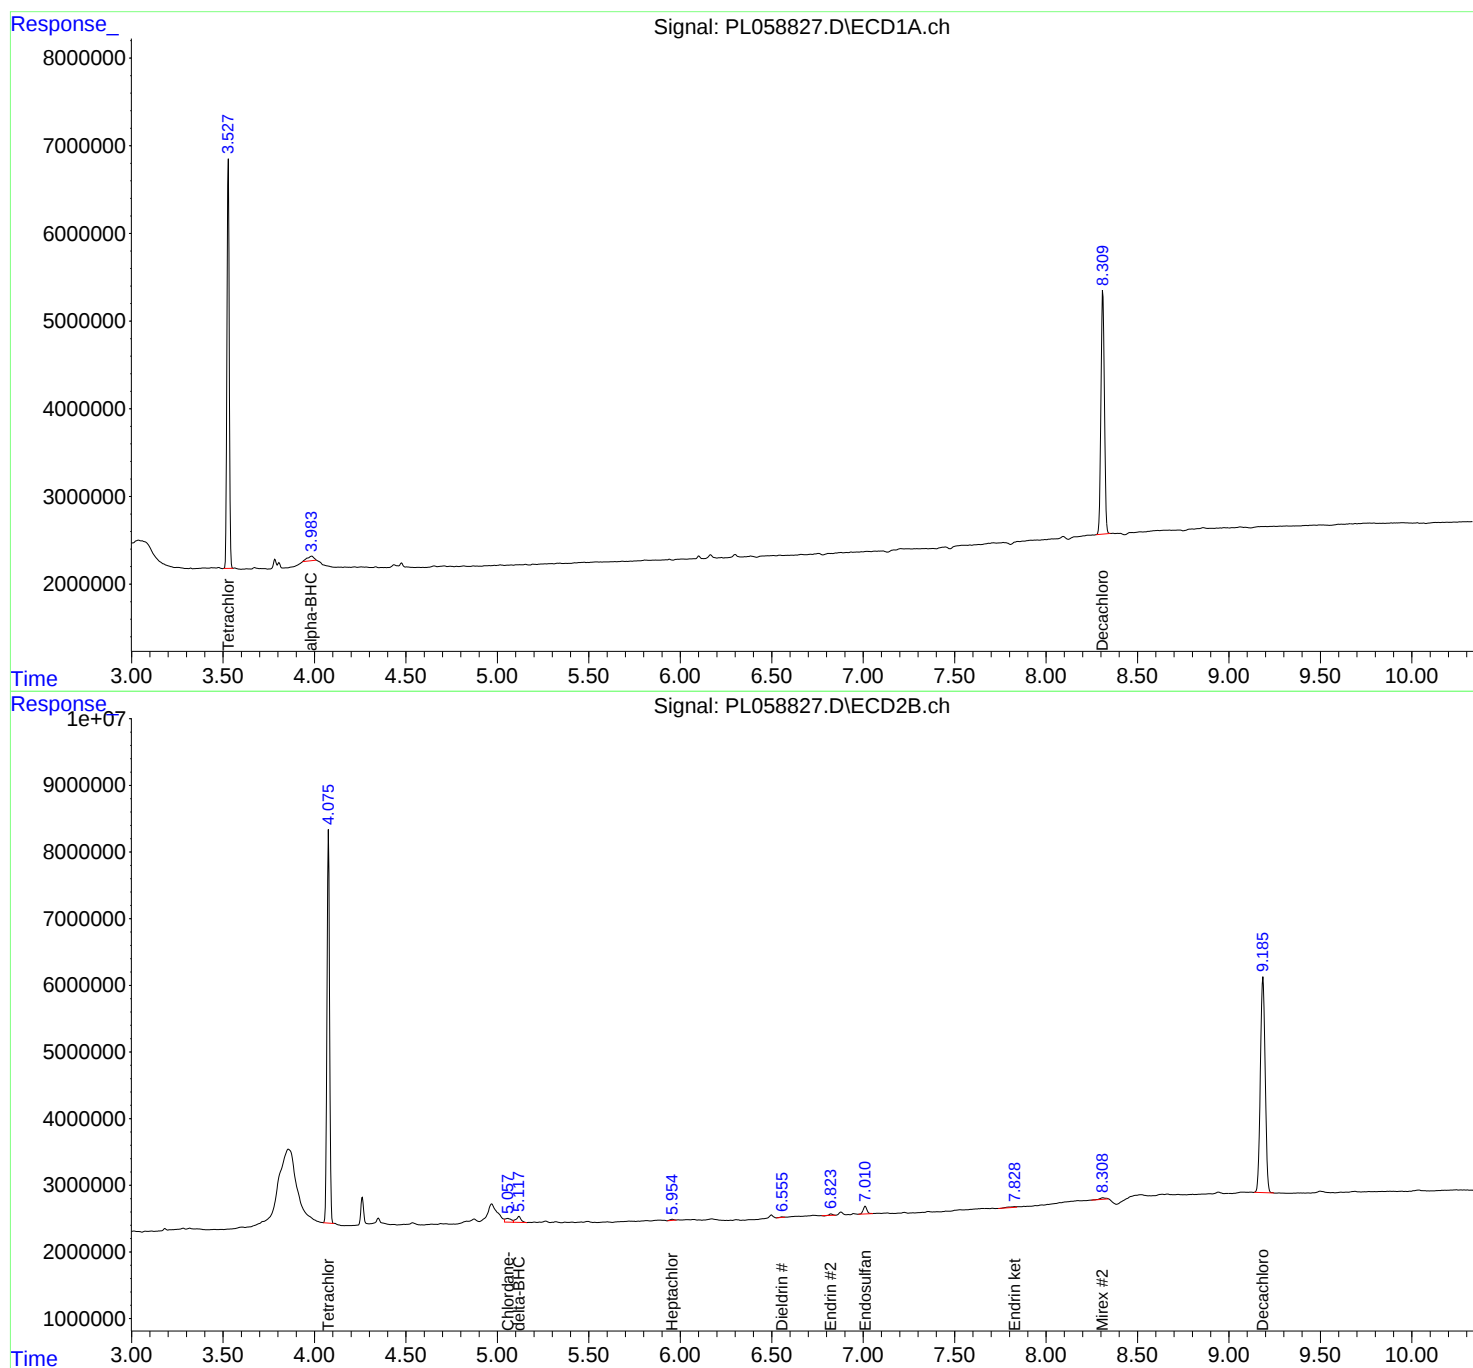


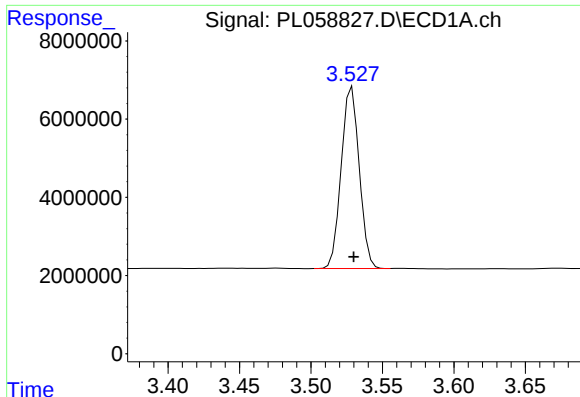

#1 Tetrachloro-m-xylene


R.T.: 3.529 min
Delta R.T.: -0.001 min
Response: 40848734
Conc: 22.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

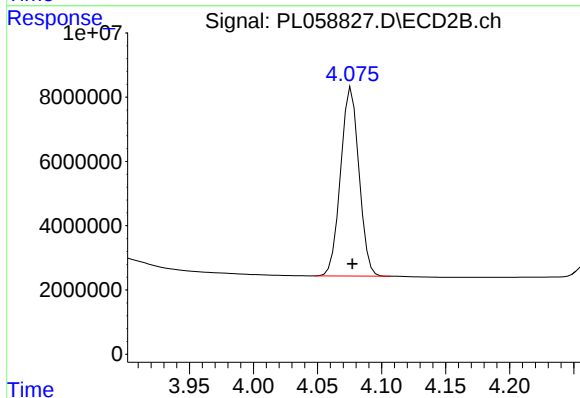


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: 0.000 min
Response: 58559270
Conc: 21.62 ng/ml

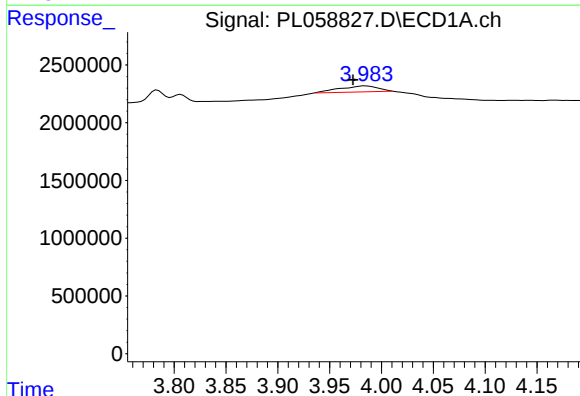


#2 alpha-BHC

R.T.: 3.984 min
Delta R.T.: 0.012 min
Response: 1342706
Conc: 0.49 ng/ml

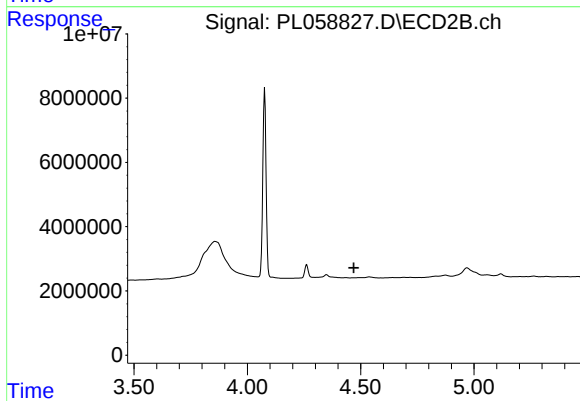

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.469 min
Response: 0
Conc: N.D.

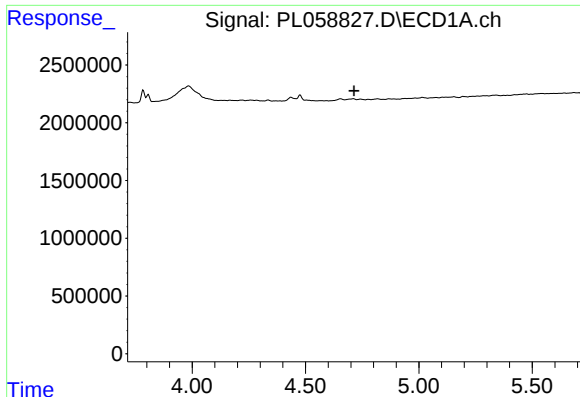

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

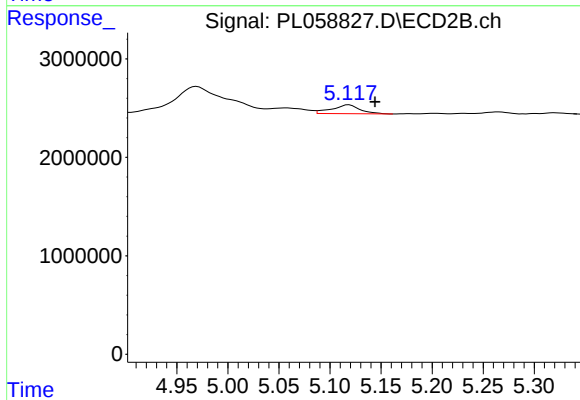


#7 delta-BHC

R.T.: 5.119 min
Delta R.T.: -0.025 min
Response: 1735541
Conc: 0.48 ng/ml

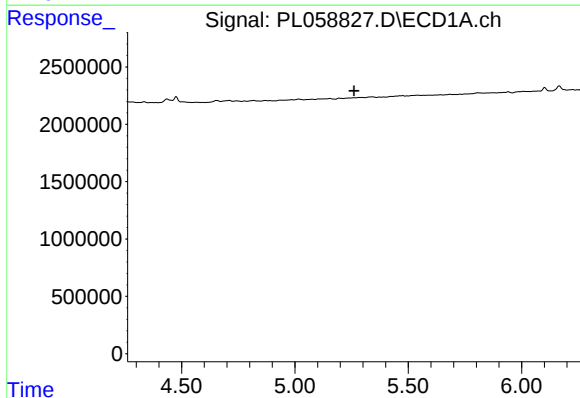


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

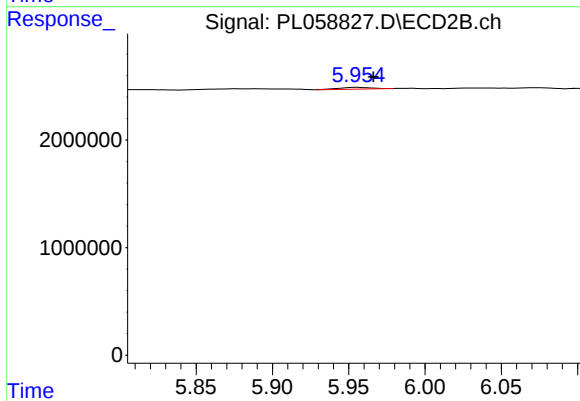

#8 Heptachlor epoxide


R.T.: 5.956 min
Delta R.T.: -0.010 min
Response: 232655
Conc: 0.07 ng/ml

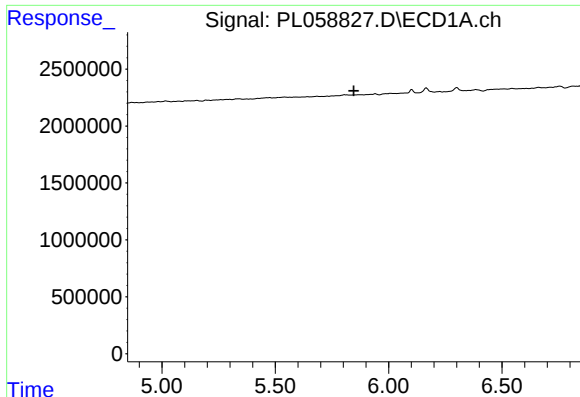

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.847 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

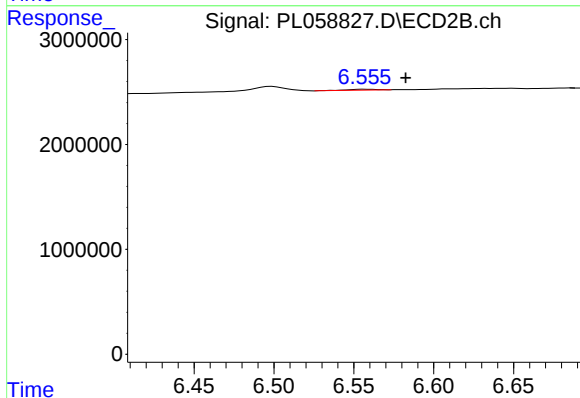


#13 Dieldrin

R.T.: 6.557 min
Delta R.T.: -0.026 min
Response: 99103
Conc: 0.03 ng/ml

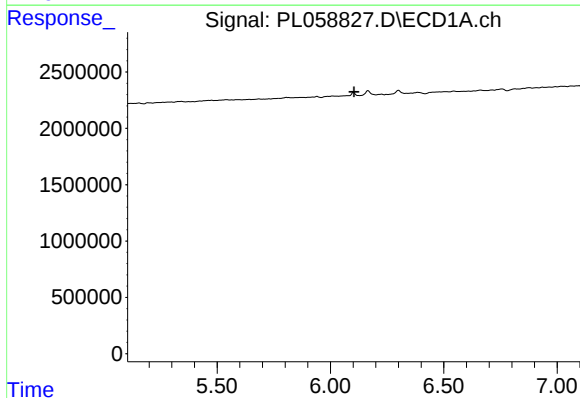


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.105 min
Response: 0
Conc: N.D.

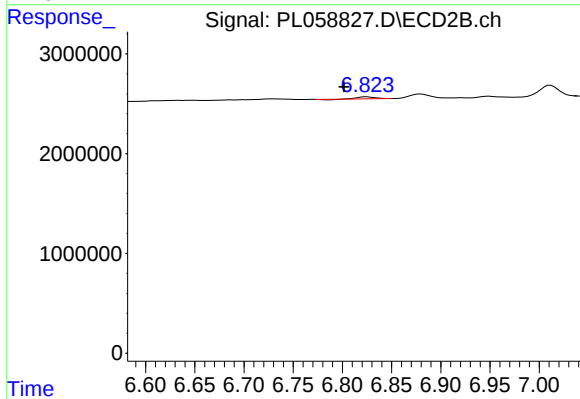

#14 Endrin


R.T.: 6.824 min
Delta R.T.: 0.023 min
Response: 220160
Conc: 0.09 ng/ml

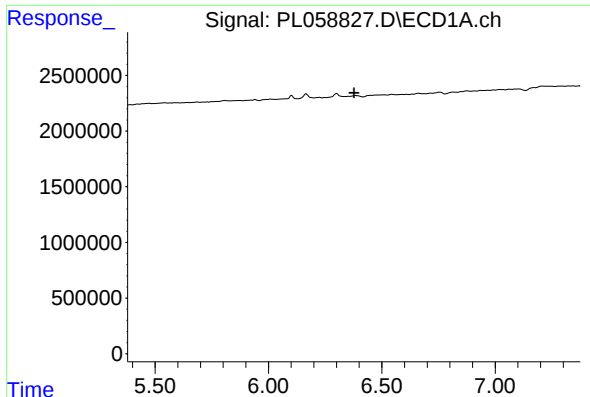

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

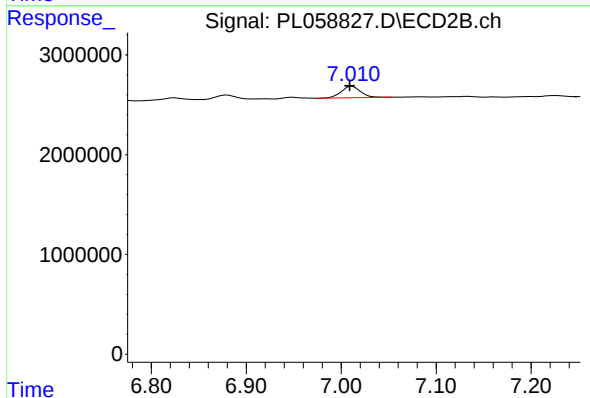


#15 Endosulfan II

R.T.: 7.011 min
Delta R.T.: 0.002 min
Response: 1630573
Conc: 0.58 ng/ml

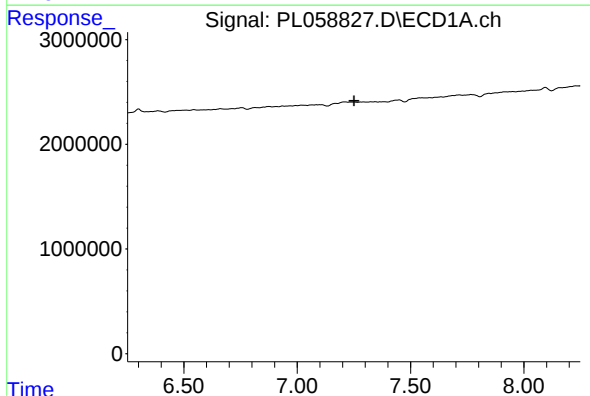


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

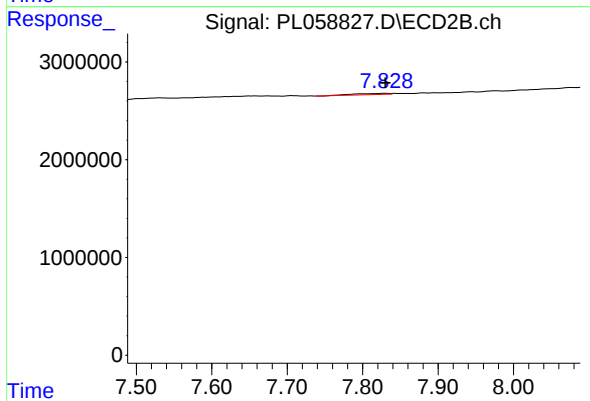

#21 Endrin ketone


R.T.: 7.829 min
Delta R.T.: -0.001 min
Response: 386721
Conc: 0.14 ng/ml

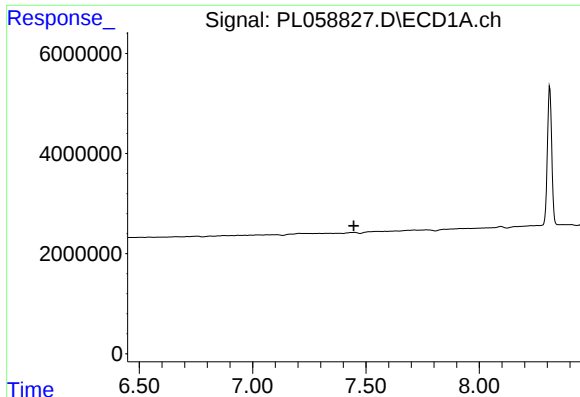

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.446 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

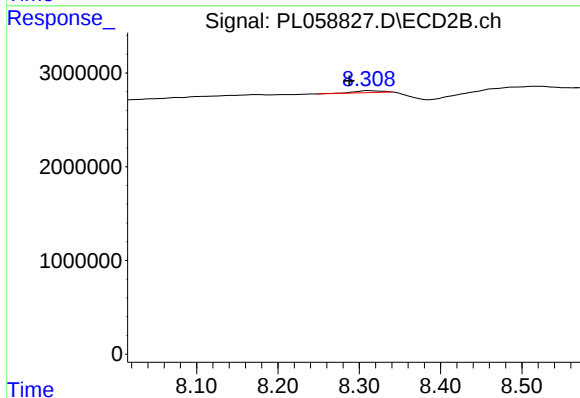


#22 Mirex

R.T.: 8.311 min
Delta R.T.: 0.024 min
Response: 538293
Conc: 0.25 ng/ml

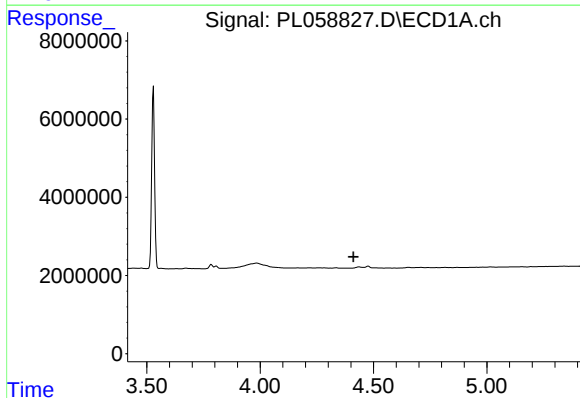


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.412 min
Response: 0
Conc: N.D.

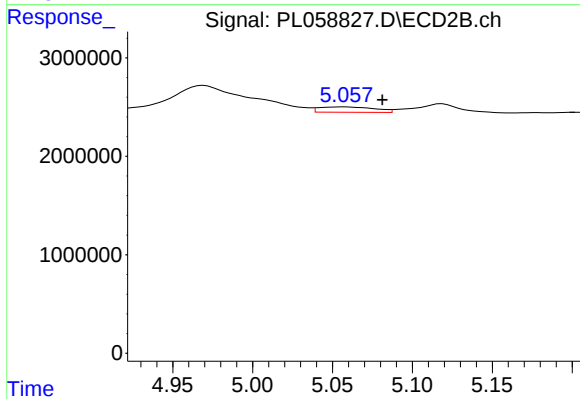

#23 Chlordane-1


R.T.: 5.058 min
Delta R.T.: -0.023 min
Response: 1312802
Conc: 13.69 ng/ml

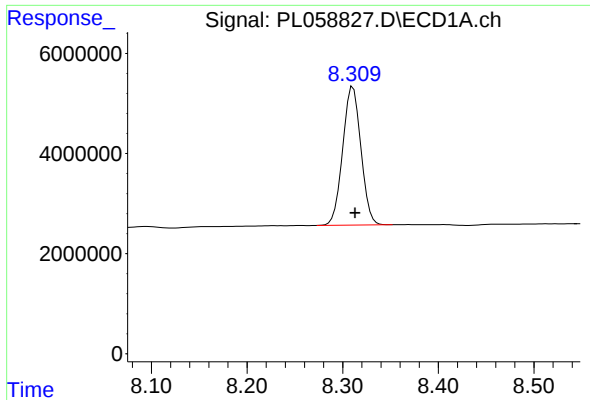

#28 Decachlorobiphenyl

R.T.: 8.311 min
Delta R.T.: -0.002 min
Response: 36698326
Conc: 21.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

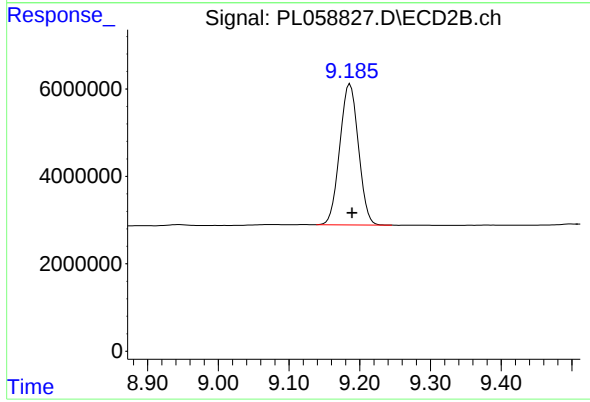

#28 Decachlorobiphenyl

R.T.: 9.186 min
Delta R.T.: -0.003 min
Response: 59063139
Conc: 22.40 ng/ml