

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052120\
 Data File : PL058845.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 16:36
 Operator : AJ\MA
 Sample : PB129041BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 17:12:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	4.077	33660339	44294404	18.357	16.354
28)	SA Decachlor...	8.311	9.190	30804059	42783522	18.232	16.229
Target Compounds							
2)	A alpha-BHC	3.984	0.000	1801258	0	0.663	N.D. #
4)	MA Heptachlor	0.000	5.263	0	600216	N.D.	0.157 #
7)	B delta-BHC	0.000	5.119f	0	1366150	N.D.	0.375 #
8)	B Heptachlo...	0.000	5.954	0	300960	N.D.	0.091 #
9)	A Endosulfan I	0.000	6.316	0	978642	N.D.	0.333 #
13)	MA Dieldrin	0.000	6.561f	0	298770	N.D.	0.099 #
15)	B Endosulfa...	0.000	7.012	0	2435747	N.D.	0.869 #
17)	MA 4,4'-DDT	0.000	7.218	0	619440	N.D.	0.260 #
18)	B Endrin al...	0.000	7.158f	0	2062192	N.D.	0.874 #
22)	Mirex	0.000	8.309f	0	339202	N.D.	0.155 #
23)	Chlordane-1	0.000	5.056f	0	1324942	N.D.	13.814 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052120\
Data File : PL058845.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 16:36
Operator : AJ\MA
Sample : PB129041BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 17:12:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

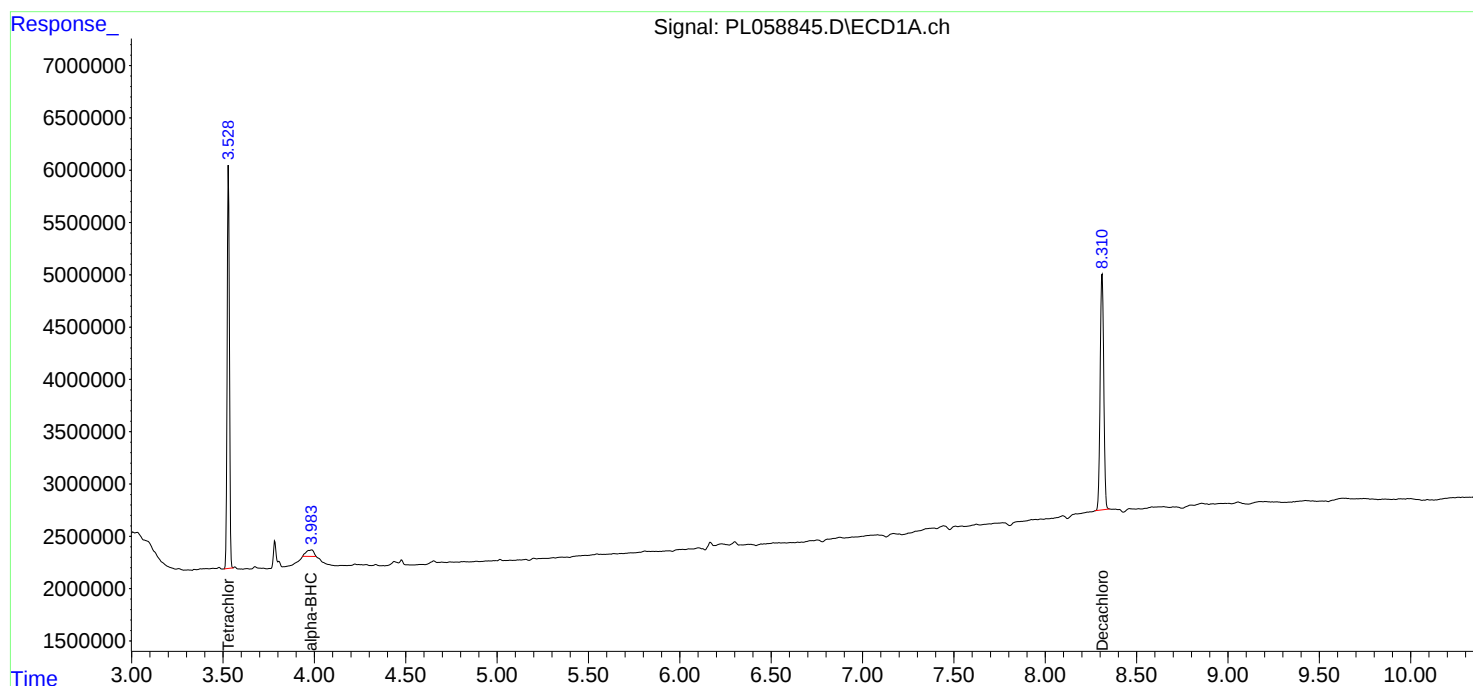


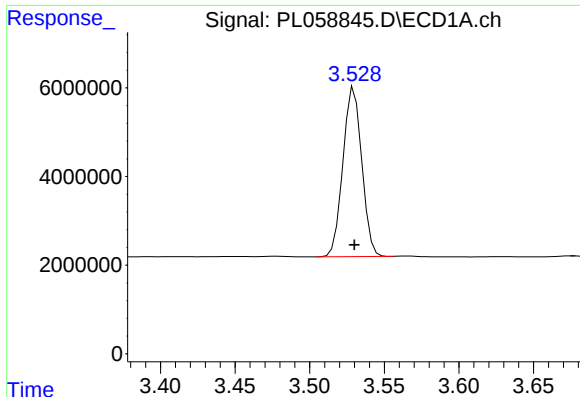

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: 0.000 min
Response: 33660339
Conc: 18.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

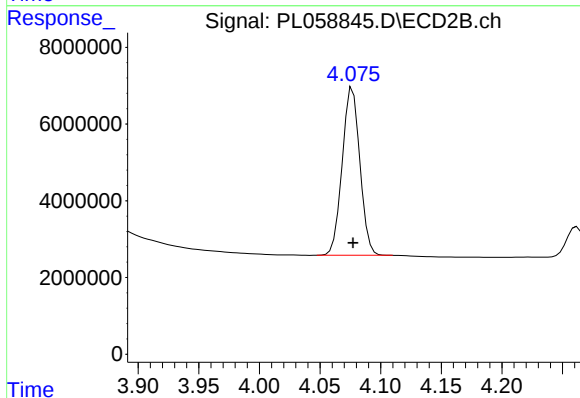


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: 0.000 min
Response: 44294404
Conc: 16.35 ng/ml

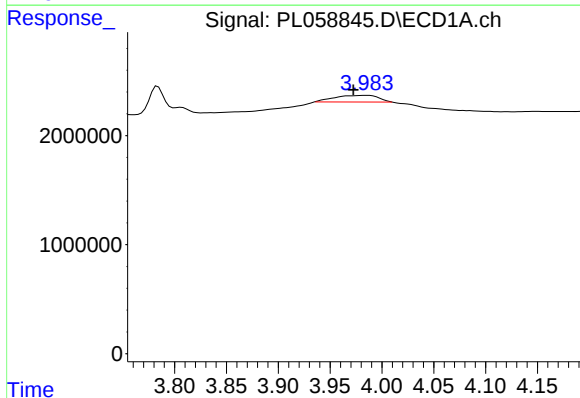


#2 alpha-BHC

R.T.: 3.984 min
Delta R.T.: 0.012 min
Response: 1801258
Conc: 0.66 ng/ml

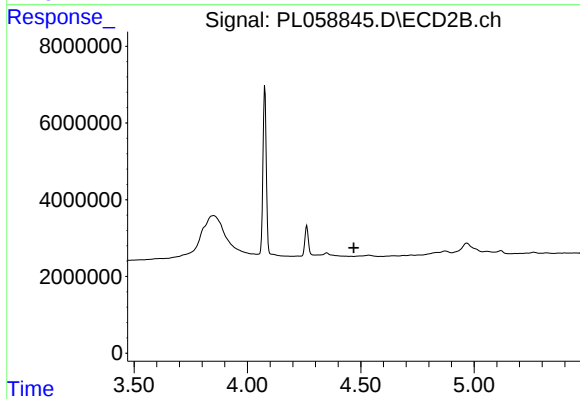

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.469 min
Response: 0
Conc: N.D.

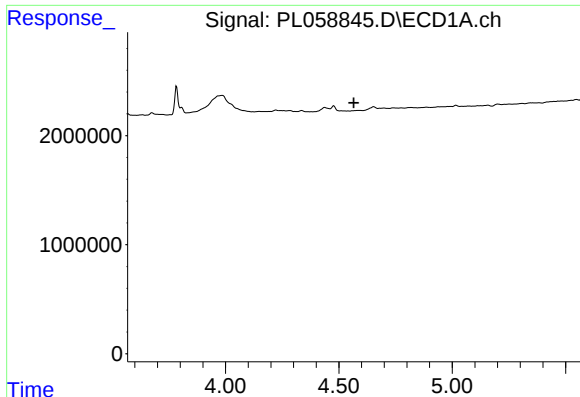

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

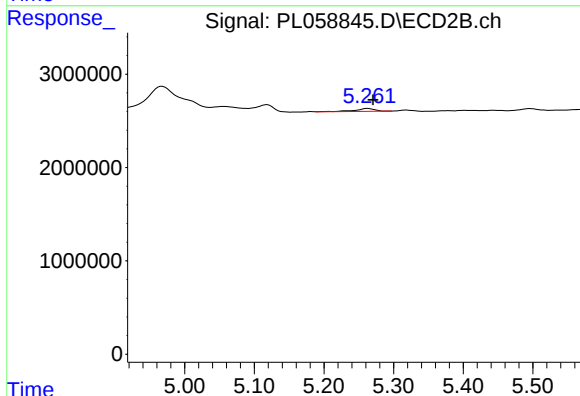


#4 Heptachlor

R.T.: 5.263 min
Delta R.T.: -0.008 min
Response: 600216
Conc: 0.16 ng/ml

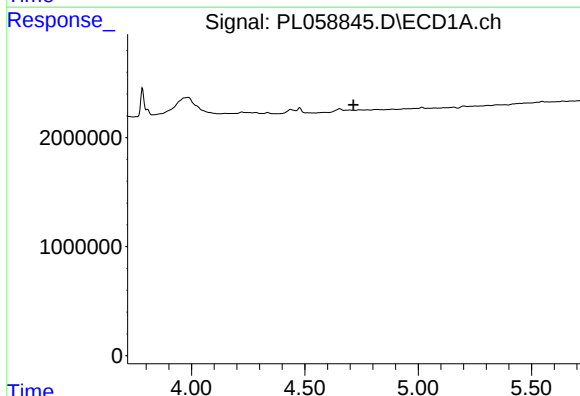


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.715 min
Response: 0
Conc: N.D.

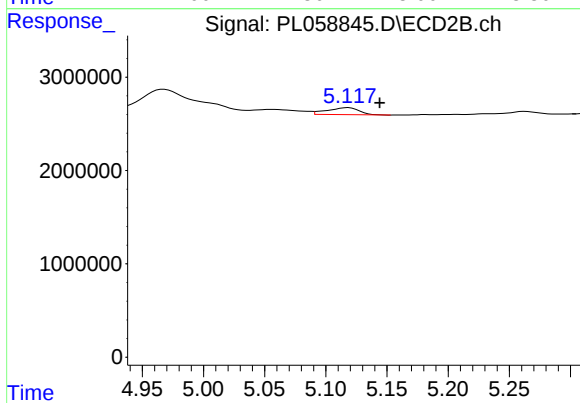

#7 delta-BHC


R.T.: 5.119 min
Delta R.T.: -0.025 min
Response: 1366150
Conc: 0.37 ng/ml

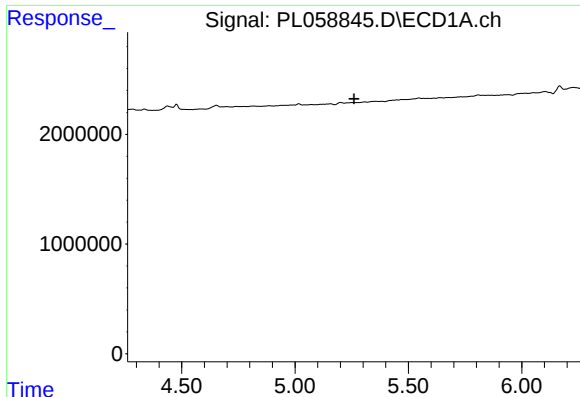

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

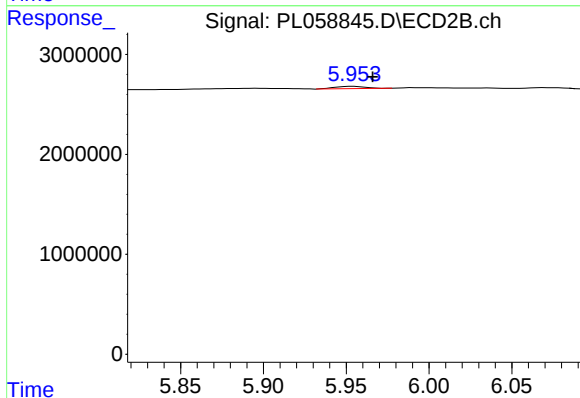


#8 Heptachlor epoxide

R.T.: 5.954 min
Delta R.T.: -0.012 min
Response: 300960
Conc: 0.09 ng/ml

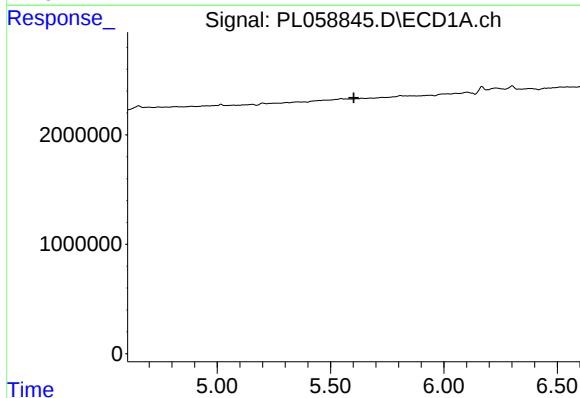


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.603 min
Response: 0
Conc: N.D.

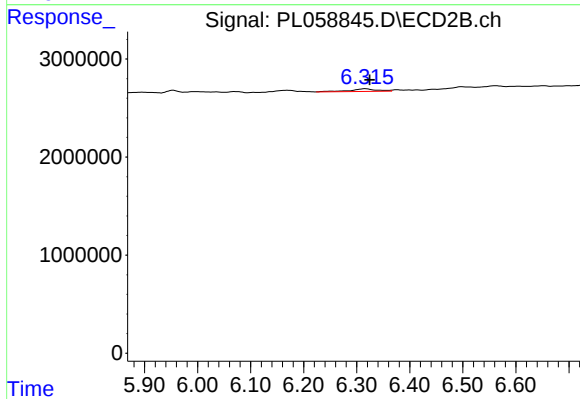

#9 Endosulfan I


R.T.: 6.316 min
Delta R.T.: -0.009 min
Response: 978642
Conc: 0.33 ng/ml

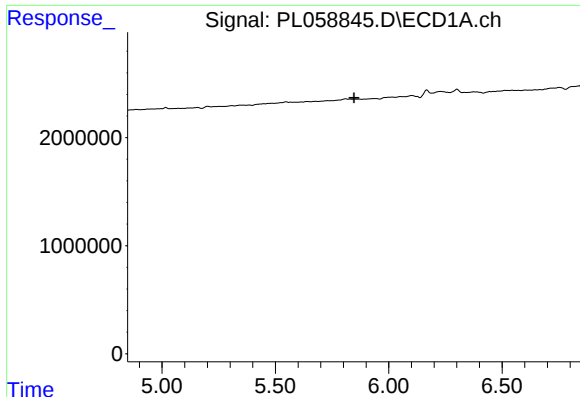

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.847 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

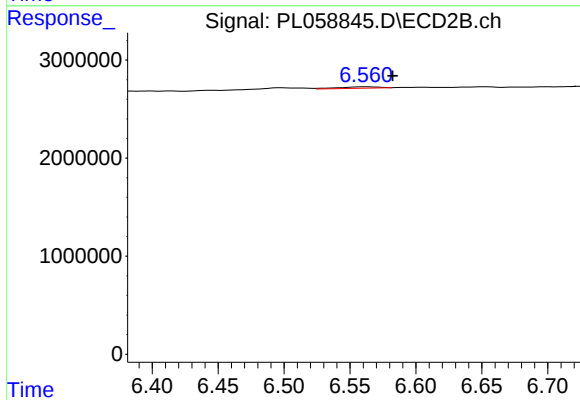


#13 Dieldrin

R.T.: 6.561 min
Delta R.T.: -0.021 min
Response: 298770
Conc: 0.10 ng/ml

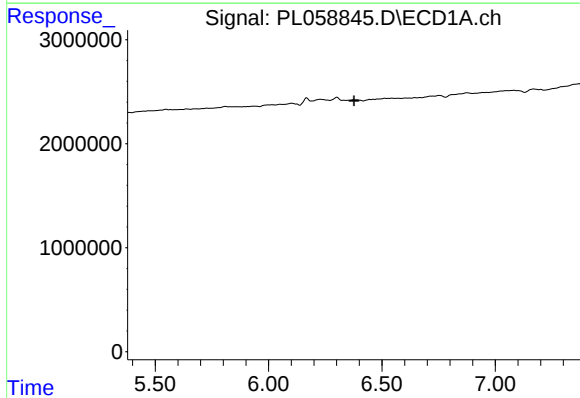


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

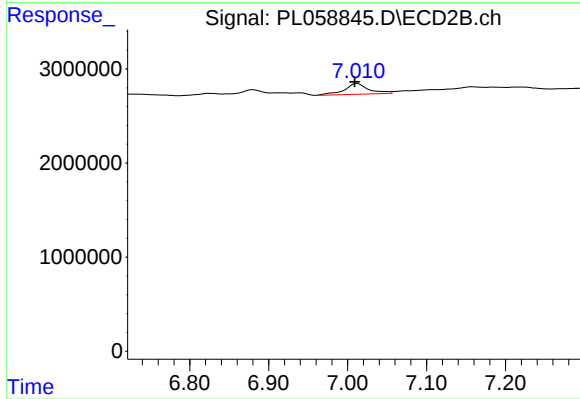

#15 Endosulfan II


R.T.: 7.012 min
Delta R.T.: 0.003 min
Response: 2435747
Conc: 0.87 ng/ml

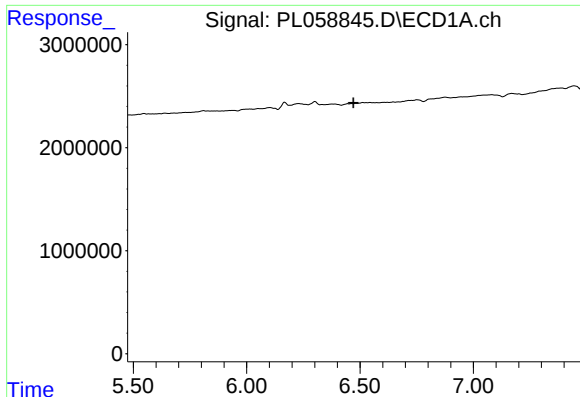

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.471 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

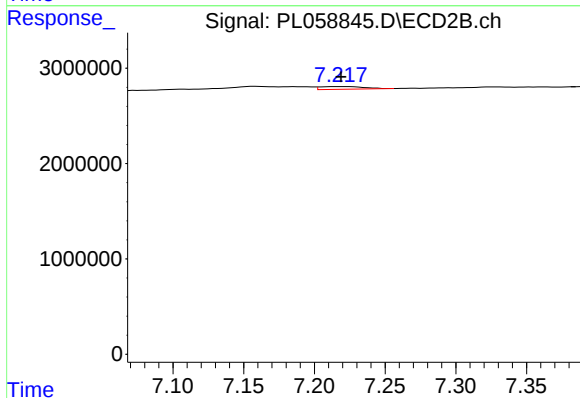


#17 4,4'-DDT

R.T.: 7.218 min
Delta R.T.: 0.000 min
Response: 619440
Conc: 0.26 ng/ml

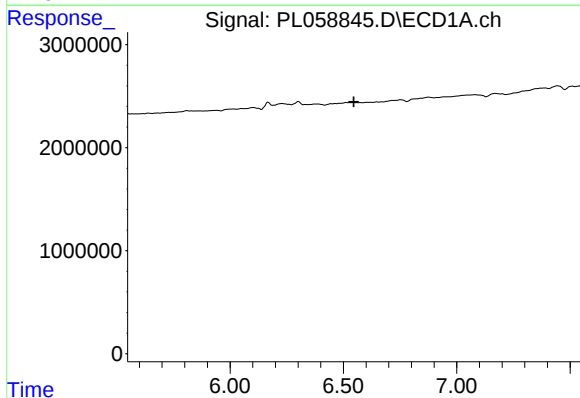


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.545 min
Response: 0
Conc: N.D.

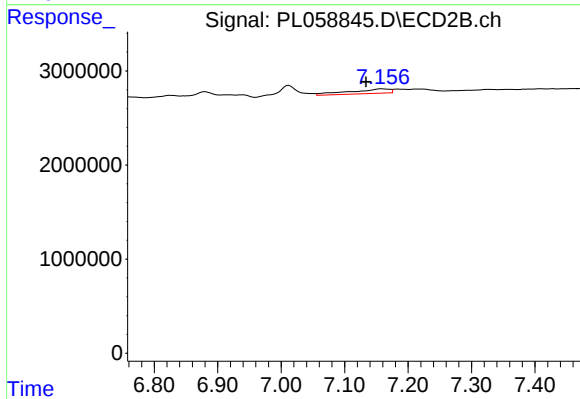

#18 Endrin aldehyde


R.T.: 7.158 min
Delta R.T.: 0.024 min
Response: 2062192
Conc: 0.87 ng/ml

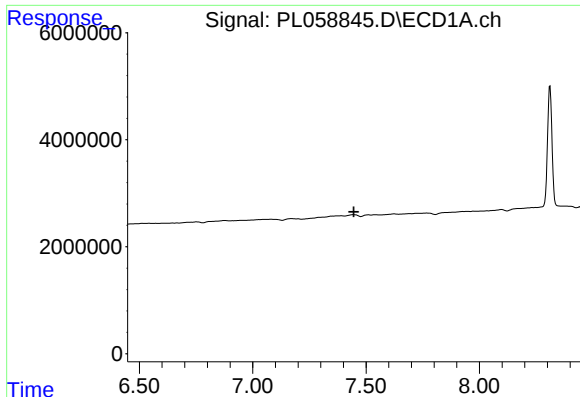

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.446 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

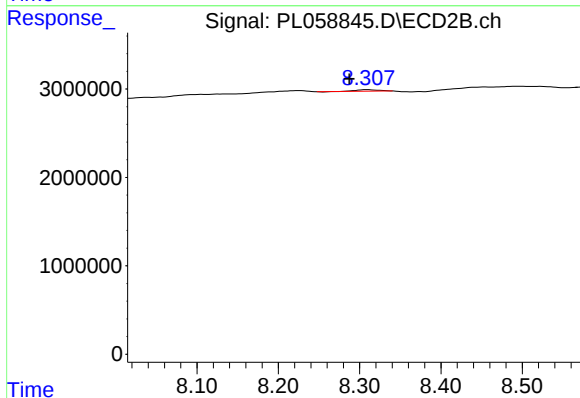


#22 Mirex

R.T.: 8.309 min
Delta R.T.: 0.021 min
Response: 339202
Conc: 0.15 ng/ml

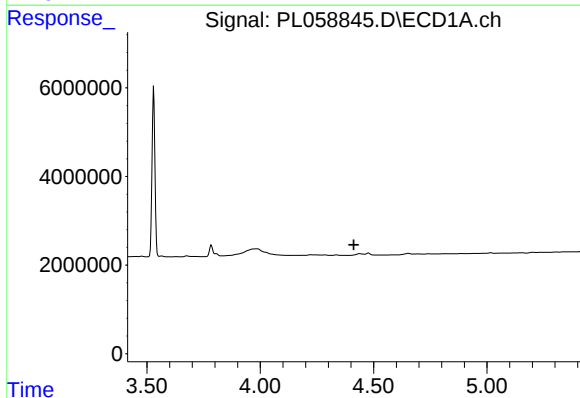


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.412 min
Response: 0
Conc: N.D.

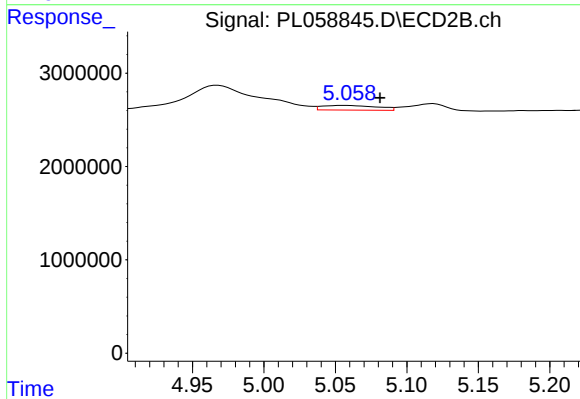

#23 Chlordane-1


R.T.: 5.056 min
Delta R.T.: -0.025 min
Response: 1324942
Conc: 13.81 ng/ml

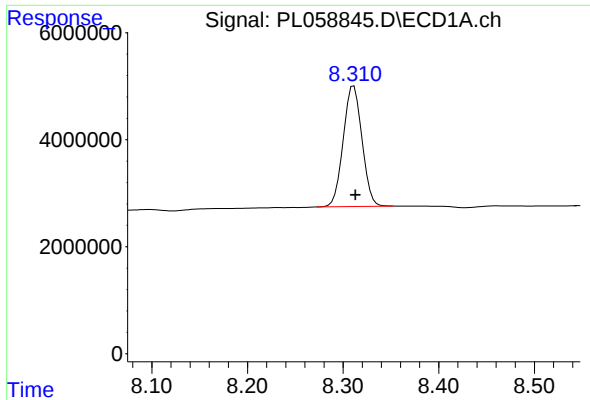

#28 Decachlorobiphenyl

R.T.: 8.311 min
Delta R.T.: -0.002 min
Response: 30804059
Conc: 18.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

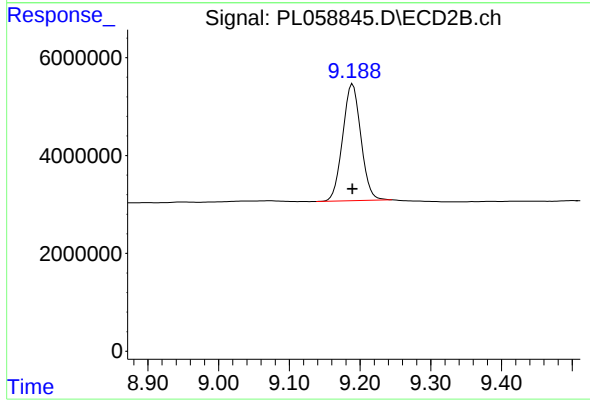

#28 Decachlorobiphenyl

R.T.: 9.190 min
Delta R.T.: 0.000 min
Response: 42783522
Conc: 16.23 ng/ml