

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052120\
 Data File : PL058852.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 20:45
 Operator : AJ\MA
 Sample : L2506-17
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 00:44:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	4.078	36310645	49780129	19.803	18.380
28)	SA Decachlor...	8.311	9.188	27940106	38048247	16.537	14.433
Target Compounds							
4)	MA Heptachlor	4.569	5.265	765097	550933	0.340	0.144 #
6)	B beta-BHC	0.000	4.925	0	671404	N.D.	0.386 #
7)	B delta-BHC	0.000	5.120f	0	1930959	N.D.	0.529 #
10)	B gamma-Chl...	0.000	6.183f	0	1239798	N.D.	0.374 #
14)	MA Endrin	0.000	6.828f	0	300189	N.D.	0.120 #
15)	B Endosulfa...	0.000	7.013	0	3237414	N.D.	1.155 #
25)	Chlordane-3	0.000	6.183f	0	1239798	N.D.	3.257 #
27)	Chlordane-5	0.000	7.104f	0	147627	N.D.	1.863 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052120\
Data File : PL058852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 20:45
Operator : AJ\MA
Sample : L2506-17
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 00:44:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

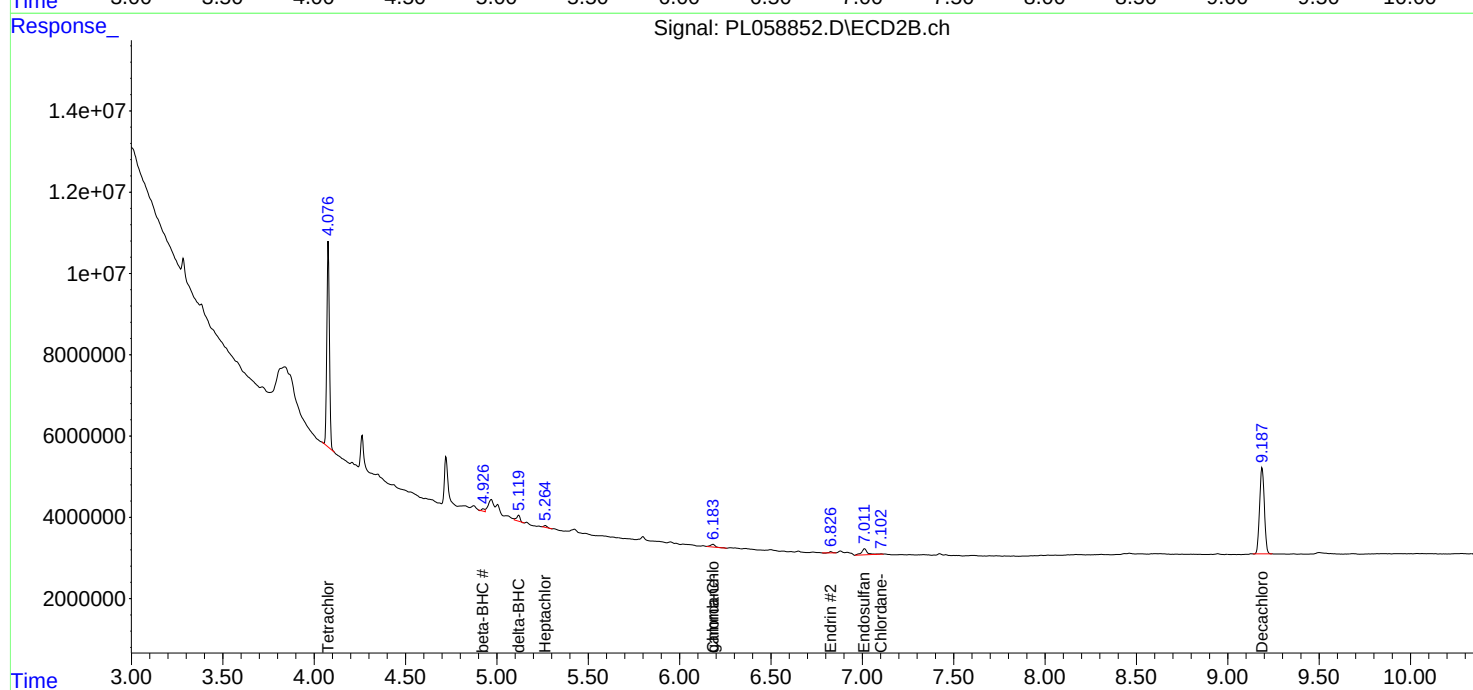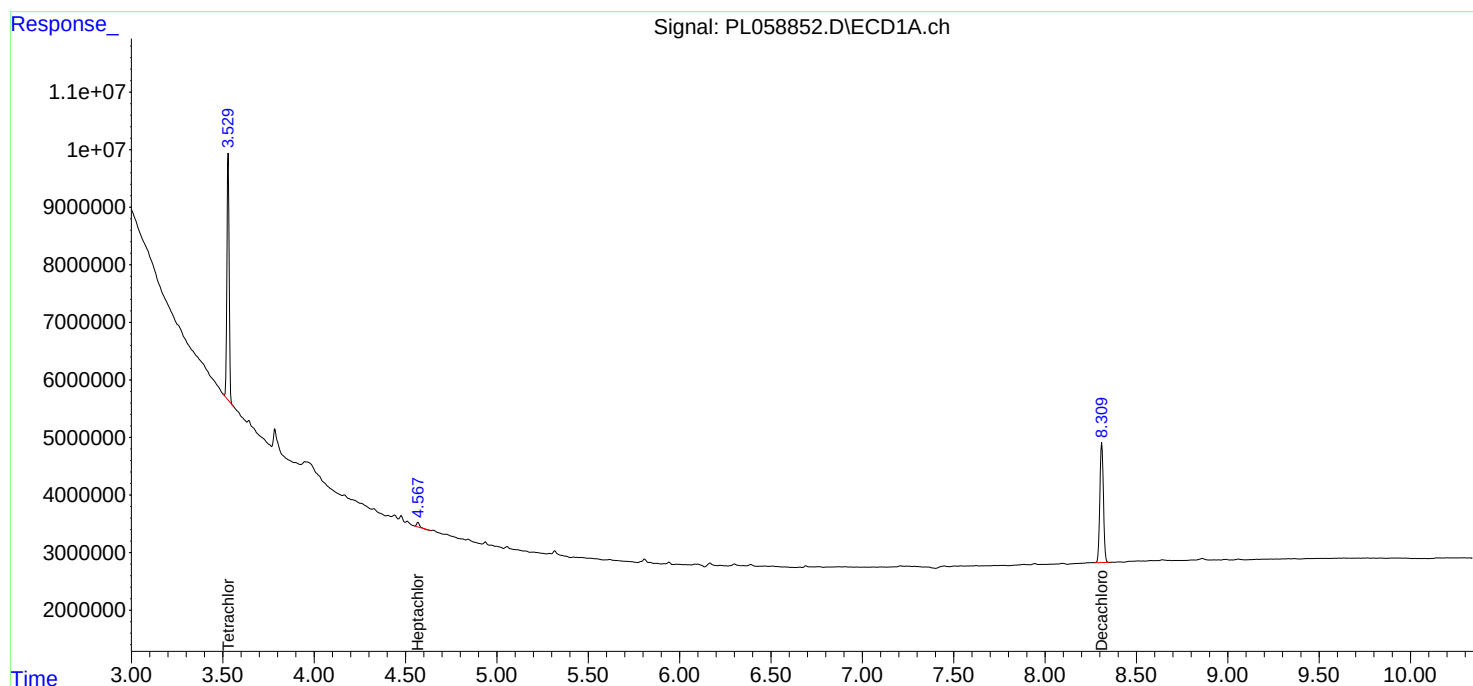


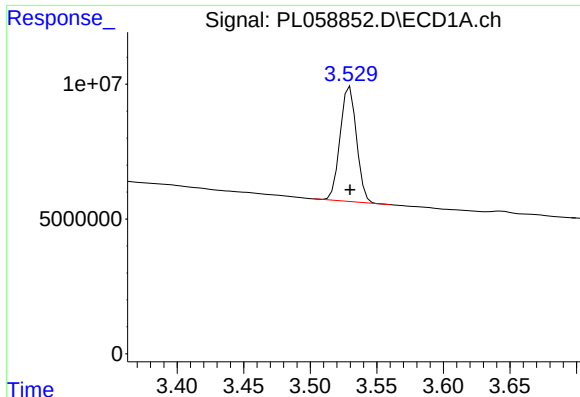

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: 0.000 min
Response: 36310645
Conc: 19.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

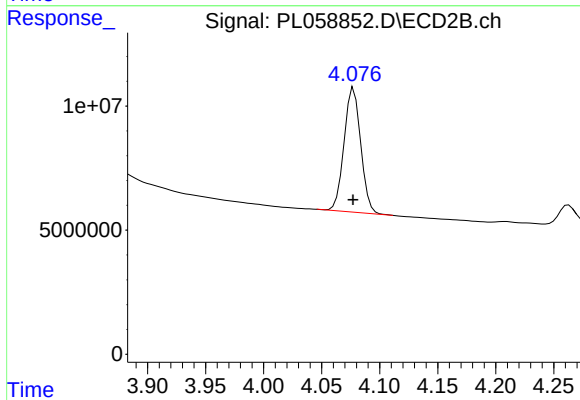


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 49780129
Conc: 18.38 ng/ml

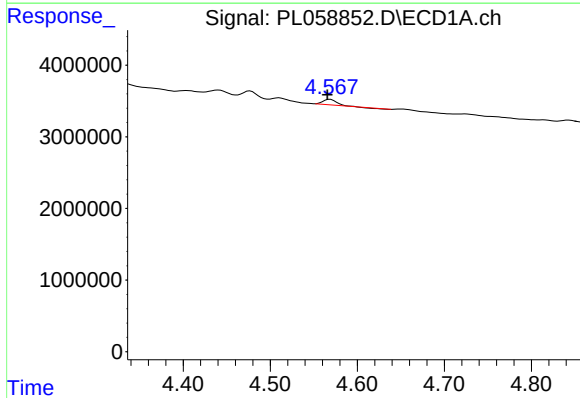


#4 Heptachlor

R.T.: 4.569 min
Delta R.T.: 0.003 min
Response: 765097
Conc: 0.34 ng/ml

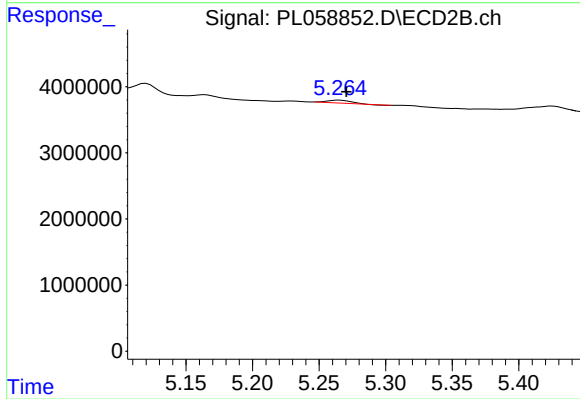

#4 Heptachlor


R.T.: 5.265 min
Delta R.T.: -0.005 min
Response: 550933
Conc: 0.14 ng/ml

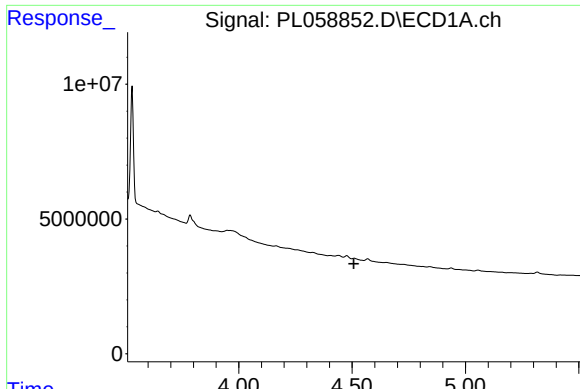

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

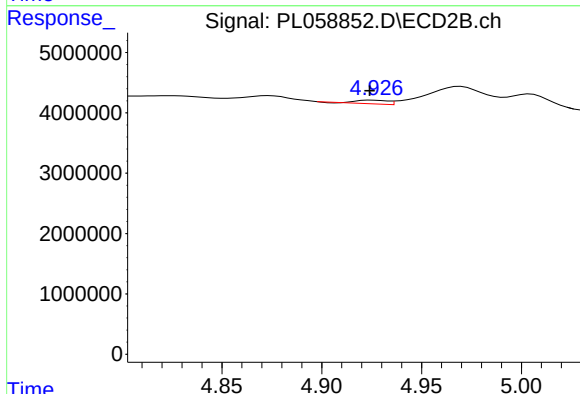


#6 beta-BHC

R.T.: 4.925 min
Delta R.T.: 0.001 min
Response: 671404
Conc: 0.39 ng/ml

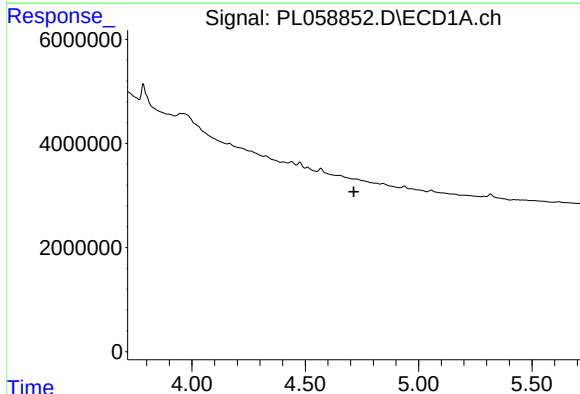


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.715 min
Response: 0
Conc: N.D.

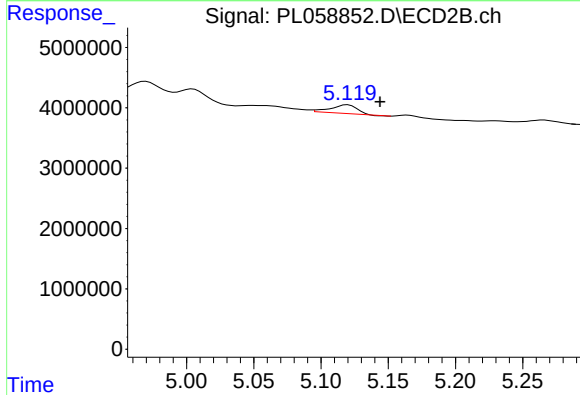

#7 delta-BHC


R.T.: 5.120 min
Delta R.T.: -0.024 min
Response: 1930959
Conc: 0.53 ng/ml

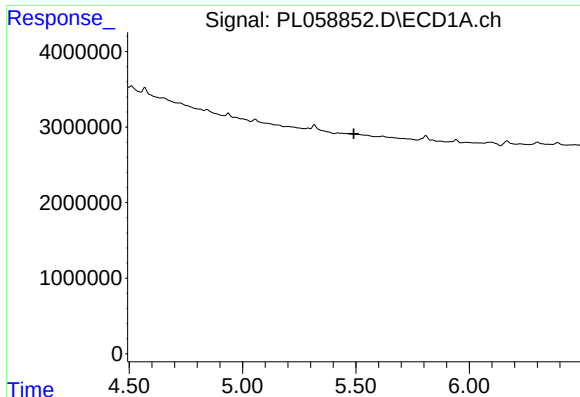

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

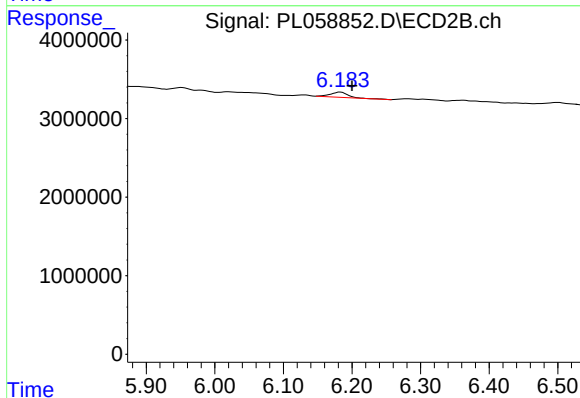


#10 gamma-Chlordane

R.T.: 6.183 min
Delta R.T.: -0.017 min
Response: 1239798
Conc: 0.37 ng/ml

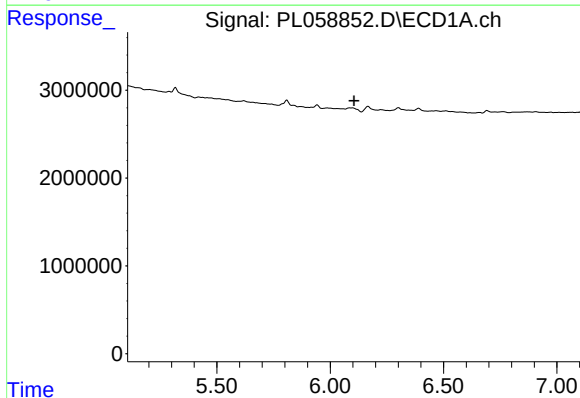


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.105 min
Response: 0
Conc: N.D.

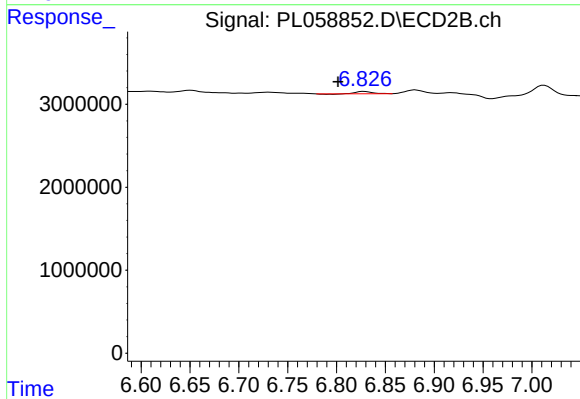

#14 Endrin


R.T.: 6.828 min
Delta R.T.: 0.026 min
Response: 300189
Conc: 0.12 ng/ml

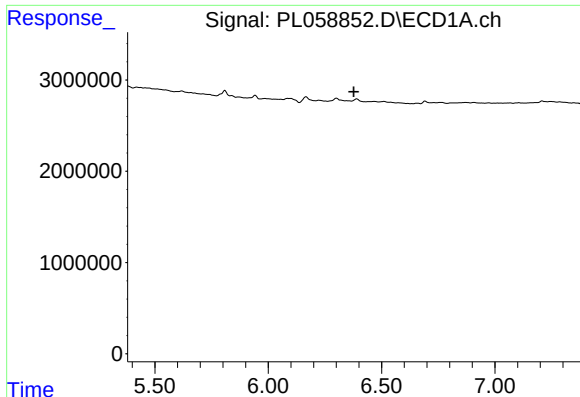

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

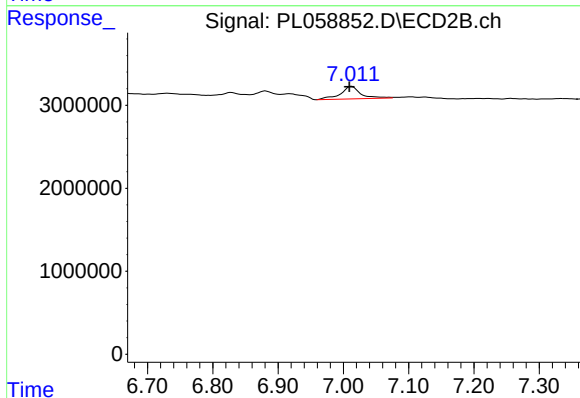


#15 Endosulfan II

R.T.: 7.013 min
Delta R.T.: 0.003 min
Response: 3237414
Conc: 1.15 ng/ml

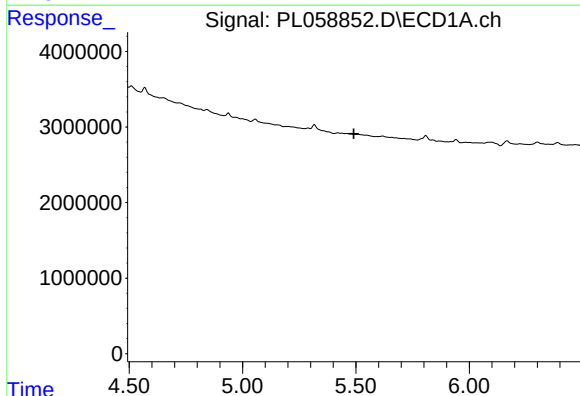


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.491 min
Response: 0
Conc: N.D.

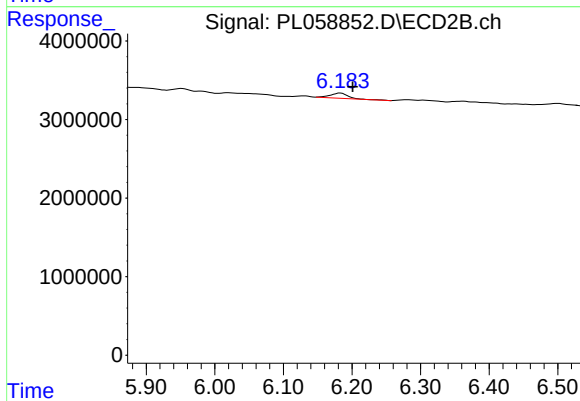

#25 Chlordane-3

R.T.: 6.183 min
Delta R.T.: -0.018 min
Response: 1239798
Conc: 3.26 ng/ml

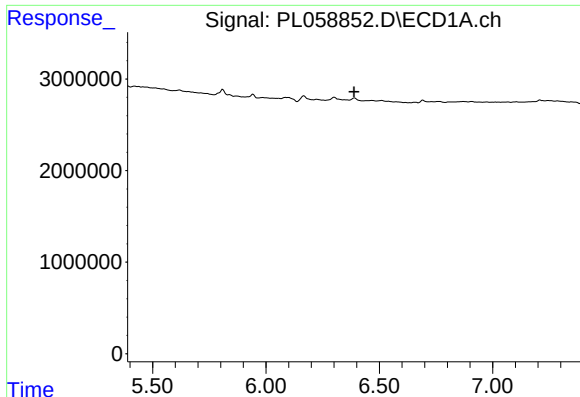


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :


#27 Chlordane-5

R.T.: 7.104 min
Delta R.T.: 0.019 min
Response: 147627
Conc: 1.86 ng/ml

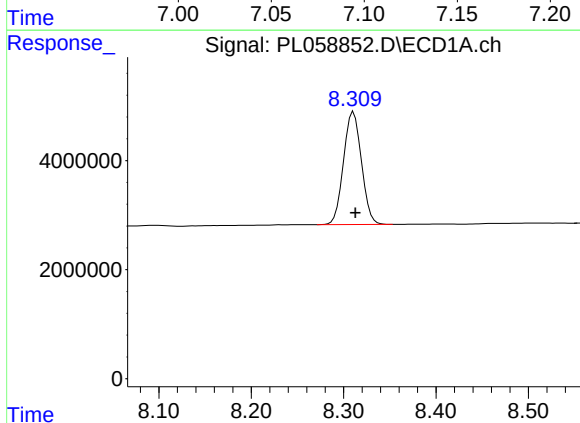

#28 Decachlorobiphenyl

R.T.: 8.311 min
Delta R.T.: -0.002 min
Response: 27940106
Conc: 16.54 ng/ml

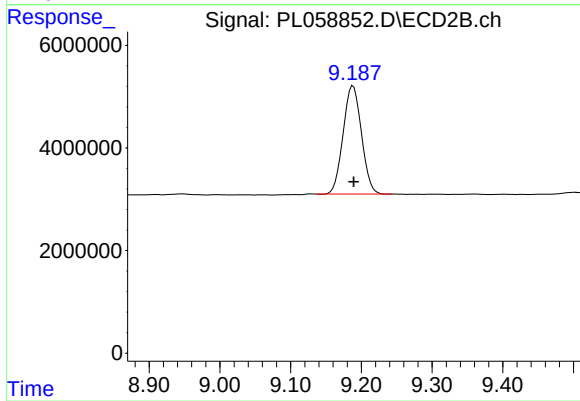

#28 Decachlorobiphenyl

R.T.: 9.188 min
Delta R.T.: 0.000 min
Response: 38048247
Conc: 14.43 ng/ml