

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052120\
 Data File : PL058860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 22:39
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 00:46:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	4.077	39733866	52861898	21.669	19.518
28)	SA Decachlor...	8.310	9.189	34986012	46826147	20.707	17.763
Target Compounds							
2)	A alpha-BHC	3.980	0.000	3122795	0	1.149	N.D. #
4)	MA Heptachlor	0.000	5.264	0	630715	N.D.	0.165 #
7)	B delta-BHC	0.000	5.118f	0	1407770	N.D.	0.386 #
8)	B Heptachlo...	0.000	5.956	0	457000	N.D.	0.139 #
10)	B gamma-Chl...	0.000	6.174f	0	778253	N.D.	0.235 #
15)	B Endosulfa...	0.000	7.012	0	1429616	N.D.	0.510 #
23)	Chlordane-1	0.000	5.060f	0	1588857	N.D.	16.566 #
25)	Chlordane-3	0.000	6.174f	0	778253	N.D.	2.044 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052120\
Data File : PL058860.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 22:39
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 00:46:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

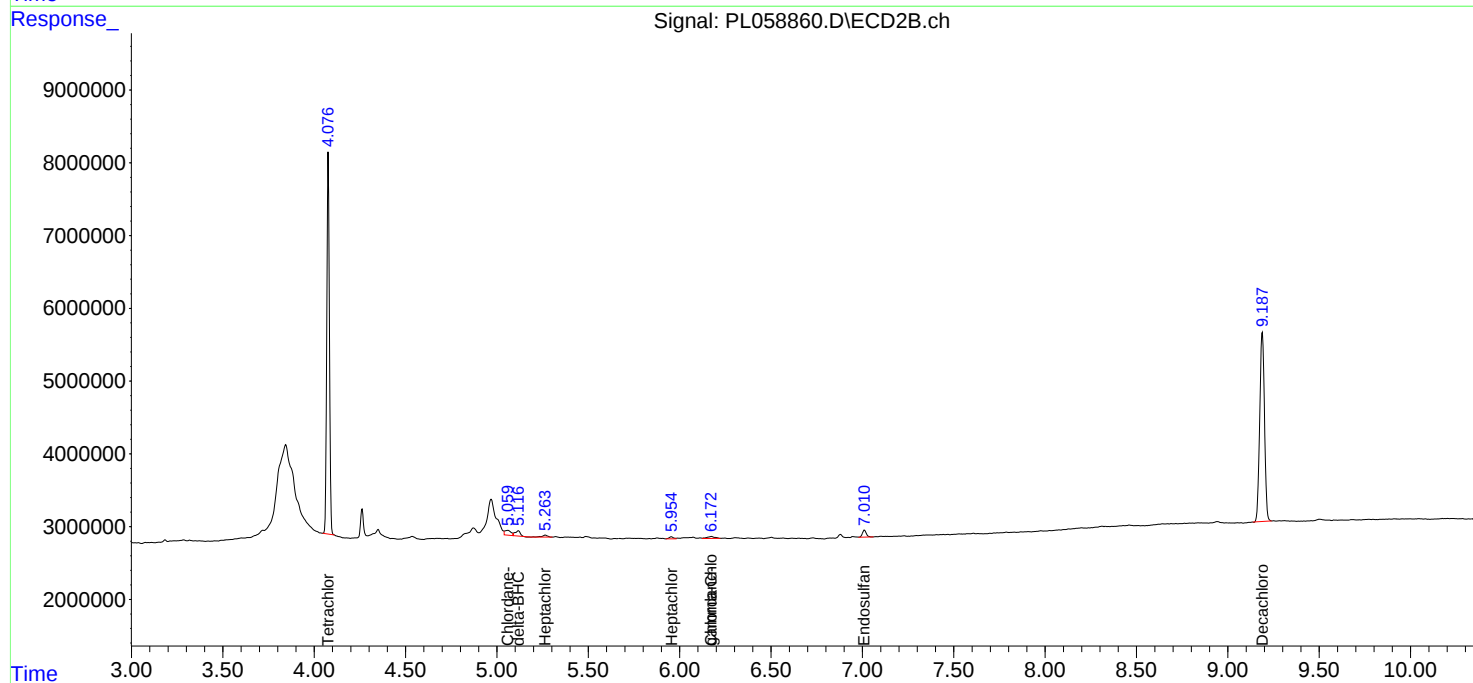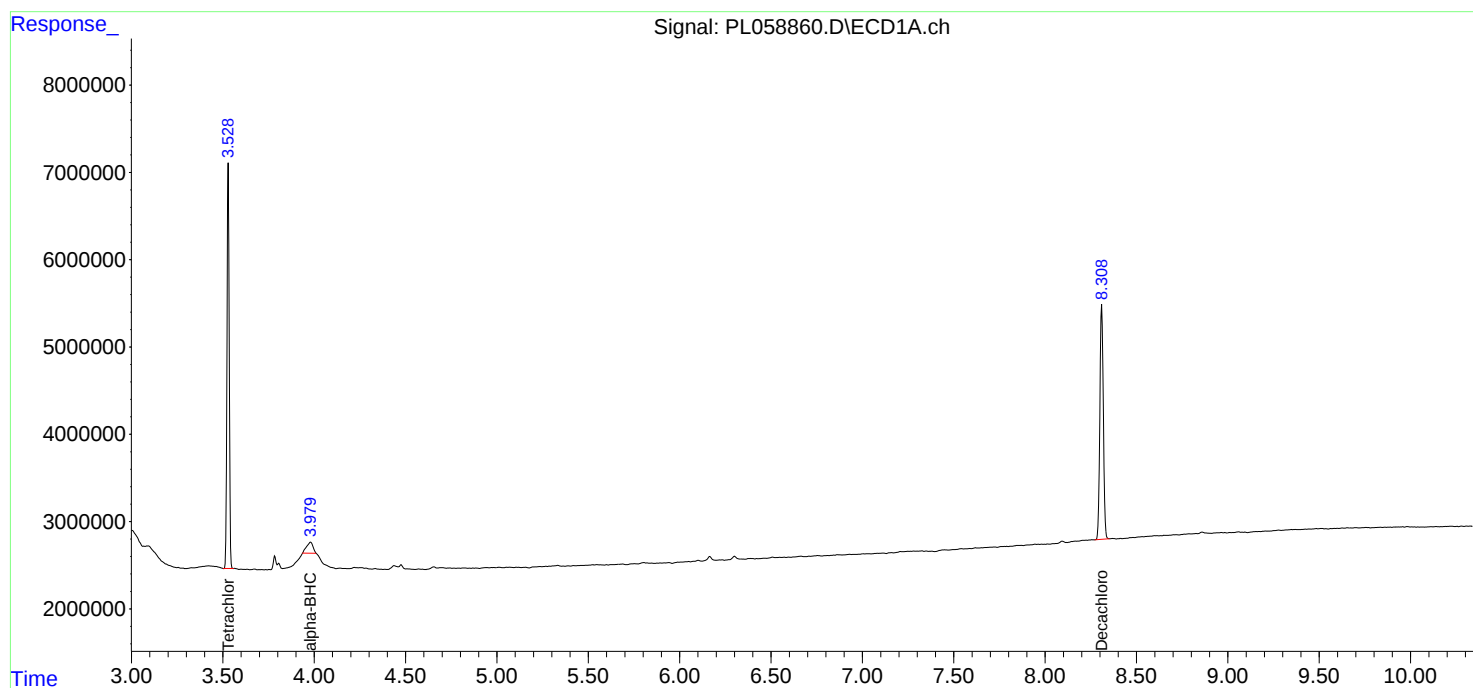


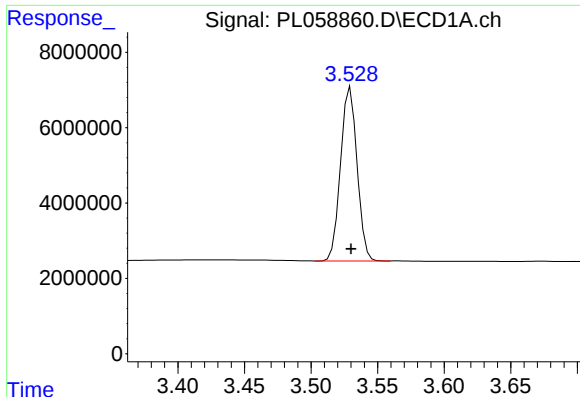

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: 0.000 min
Response: 39733866
Conc: 21.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

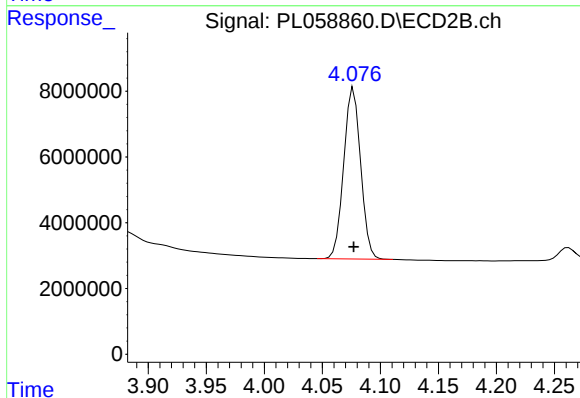


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: 0.000 min
Response: 52861898
Conc: 19.52 ng/ml

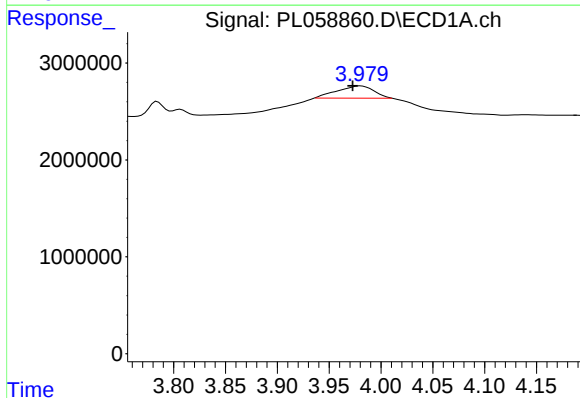


#2 alpha-BHC

R.T.: 3.980 min
Delta R.T.: 0.008 min
Response: 3122795
Conc: 1.15 ng/ml

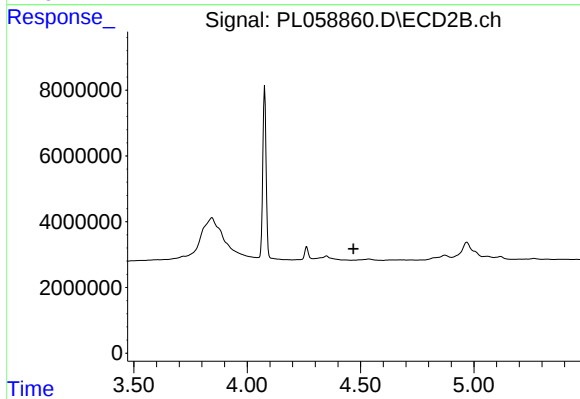

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.469 min
Response: 0
Conc: N.D.

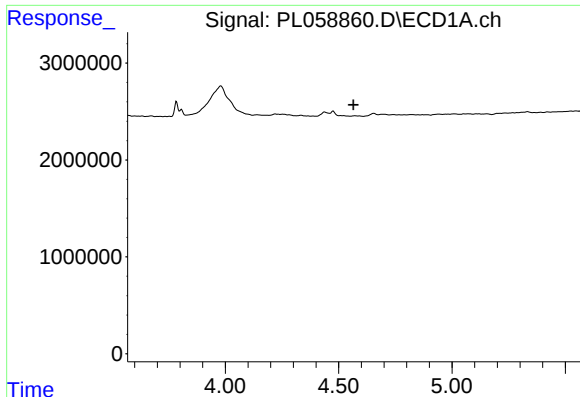

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

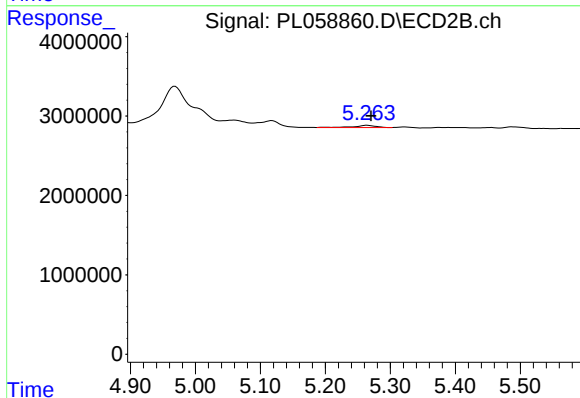


#4 Heptachlor

R.T.: 5.264 min
Delta R.T.: -0.006 min
Response: 630715
Conc: 0.16 ng/ml

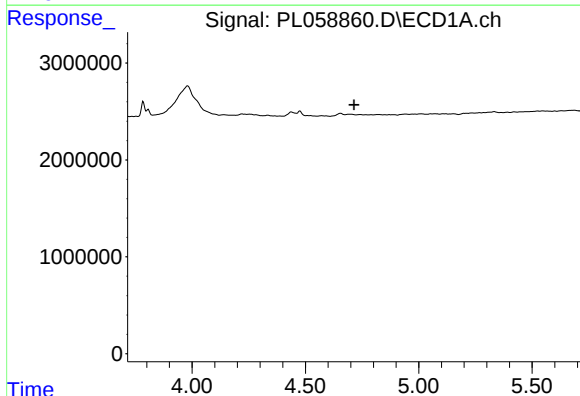


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.715 min
Response: 0
Conc: N.D.

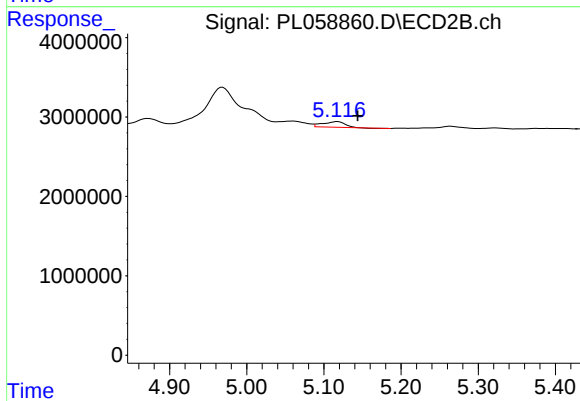

#7 delta-BHC


R.T.: 5.118 min
Delta R.T.: -0.026 min
Response: 1407770
Conc: 0.39 ng/ml

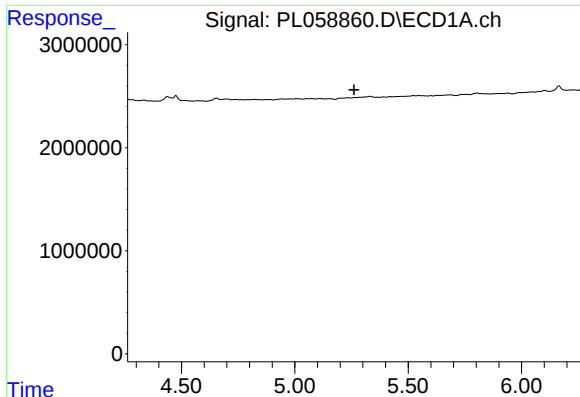

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

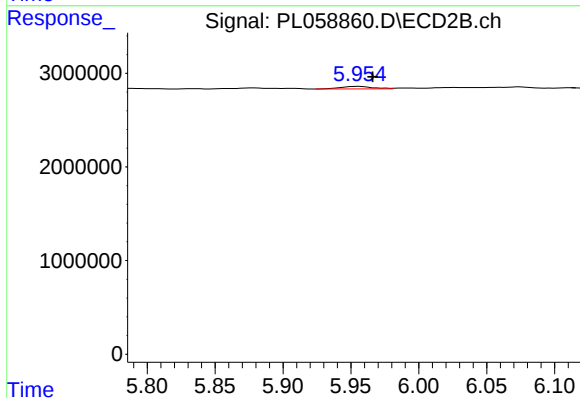


#8 Heptachlor epoxide

R.T.: 5.956 min
Delta R.T.: -0.010 min
Response: 457000
Conc: 0.14 ng/ml

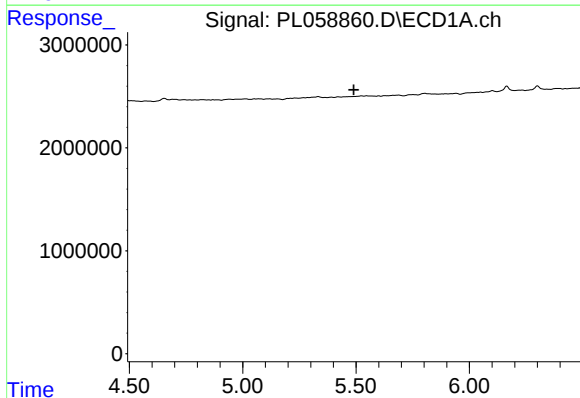


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.490 min
Response: 0
Conc: N.D.

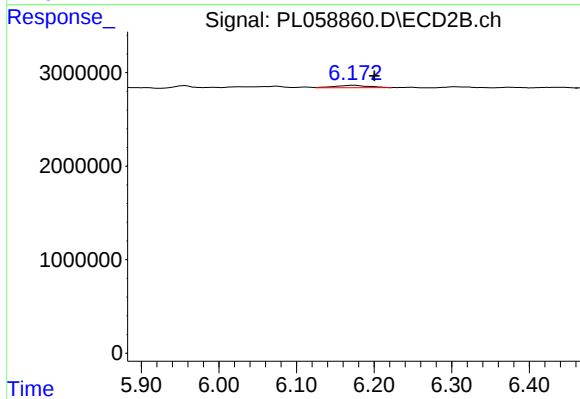

#10 gamma-Chlordane


R.T.: 6.174 min
Delta R.T.: -0.026 min
Response: 778253
Conc: 0.23 ng/ml

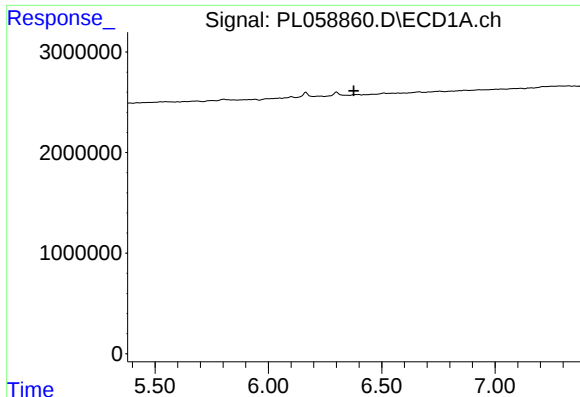

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

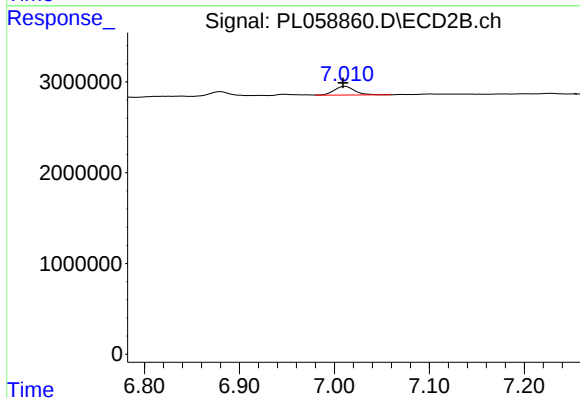


#15 Endosulfan II

R.T.: 7.012 min
Delta R.T.: 0.002 min
Response: 1429616
Conc: 0.51 ng/ml

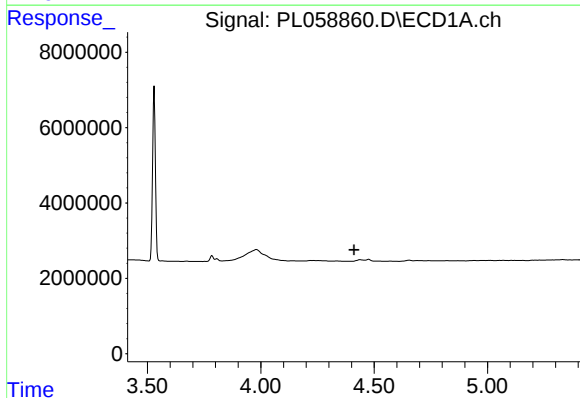


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.412 min
Response: 0
Conc: N.D.

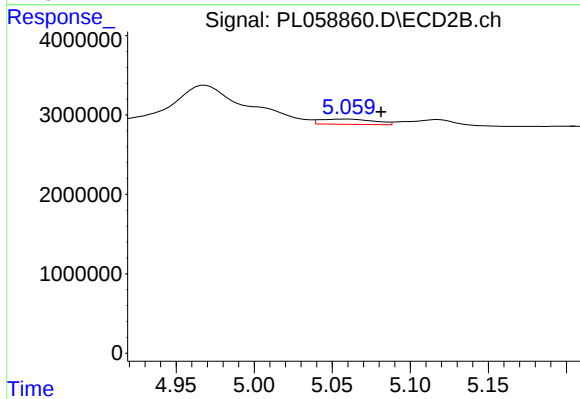

#23 Chlordane-1


R.T.: 5.060 min
Delta R.T.: -0.022 min
Response: 1588857
Conc: 16.57 ng/ml

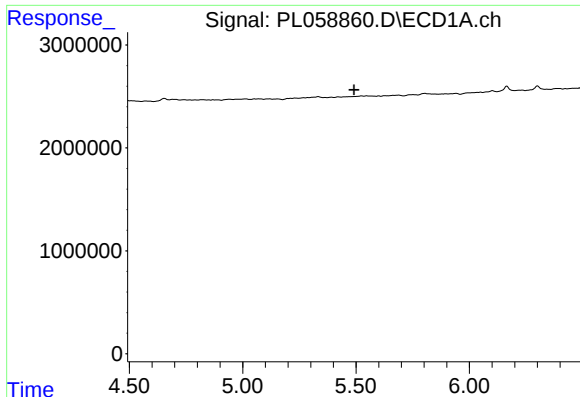

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

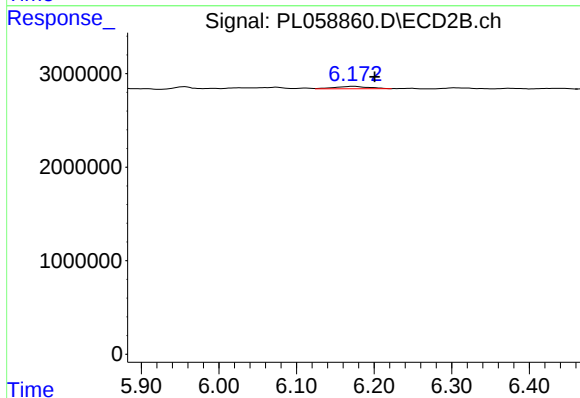


#25 Chlordane-3

R.T.: 6.174 min
Delta R.T.: -0.027 min
Response: 778253
Conc: 2.04 ng/ml

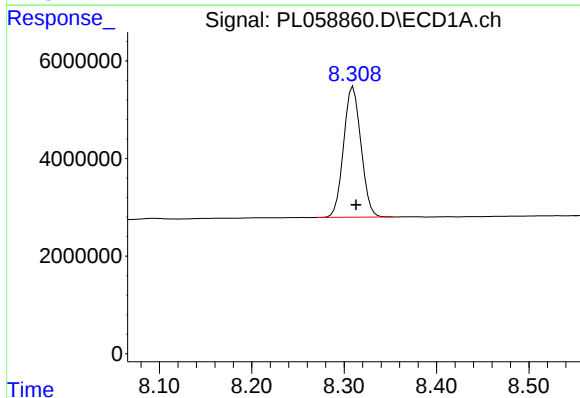

#28 Decachlorobiphenyl

R.T.: 8.310 min
Delta R.T.: -0.003 min
Response: 34986012
Conc: 20.71 ng/ml

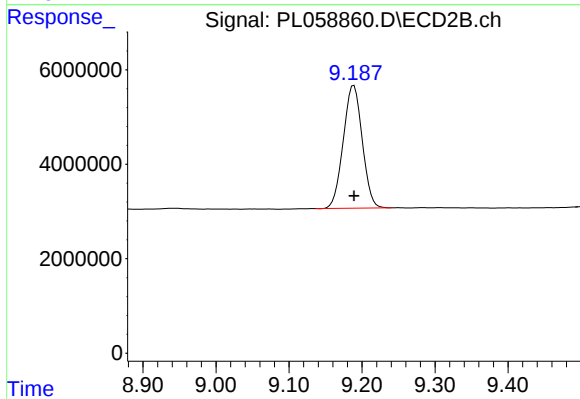

#28 Decachlorobiphenyl

R.T.: 9.189 min
Delta R.T.: 0.000 min
Response: 46826147
Conc: 17.76 ng/ml