

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052120\
 Data File : PL058833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 13:48
 Operator : AJ\MA
 Sample : L2506-14
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-04-052020

Manual Integrations
 APPROVED

mohammad
 5/22/2020 12:13:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 15:08:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	4.076	20556725	28211886	11.211	10.416
28)	SA Decachlor...	8.311	9.187	17514359	29240294	10.366	11.092
Target Compounds							
12)	B 4,4'-DDE	5.710	6.428	684156	1810284	0.417m	0.634 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052120\
Data File : PL058833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 13:48
Operator : AJ\MA
Sample : L2506-14
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TR-04-052020


Manual Integrations
APPROVED

mohammad
5/22/2020 12:13:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 15:08:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

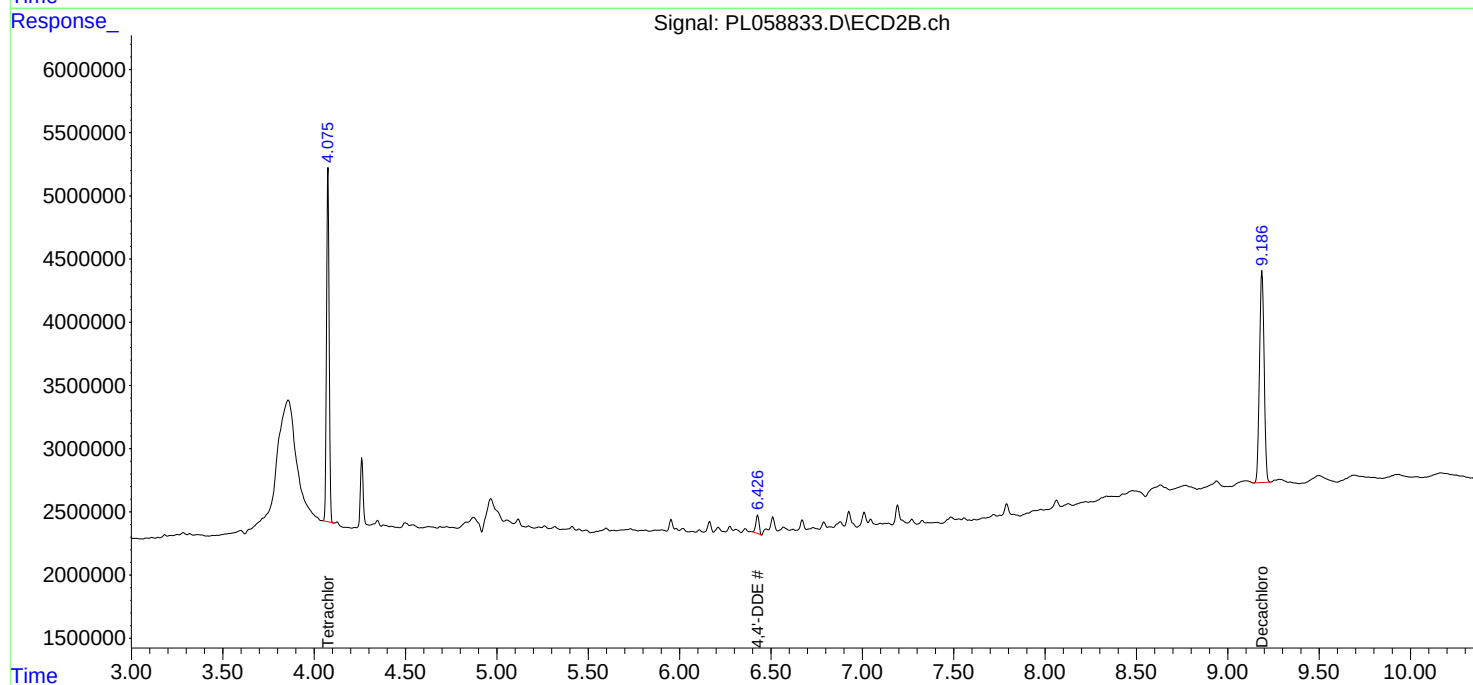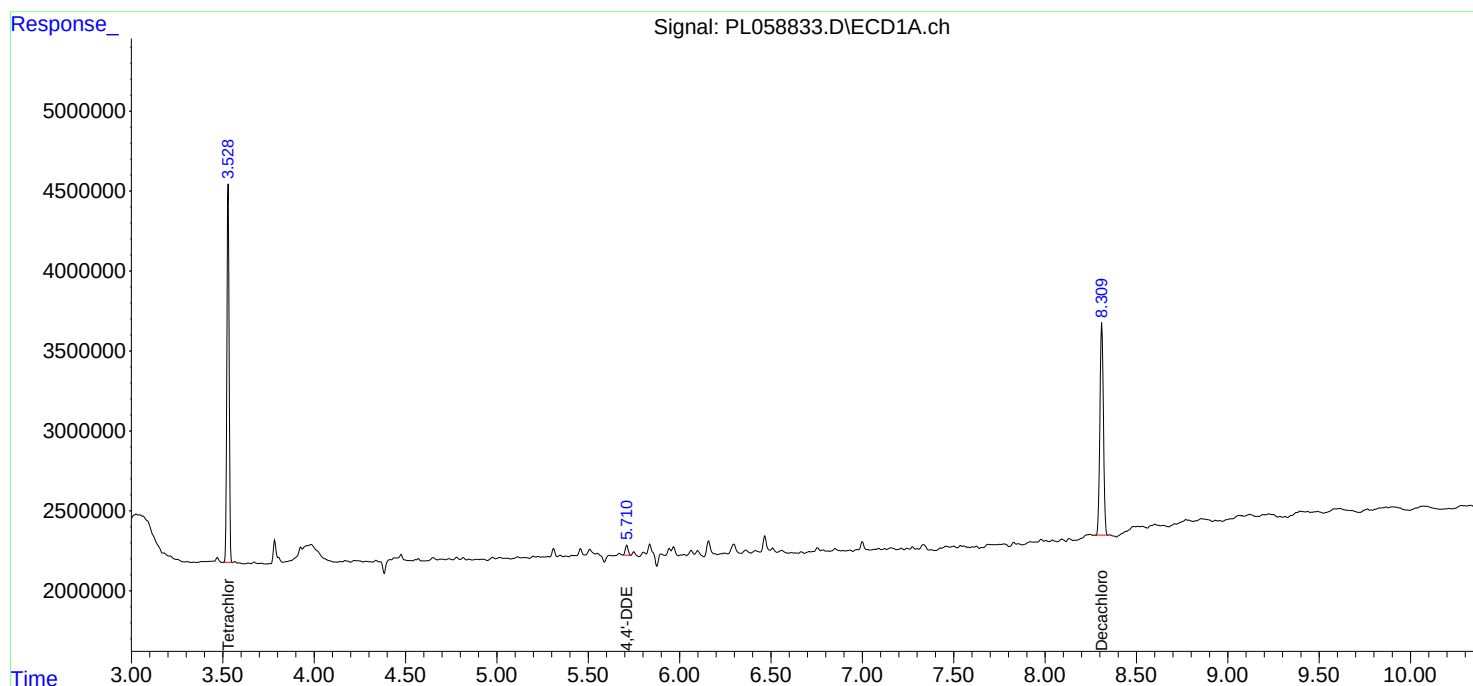

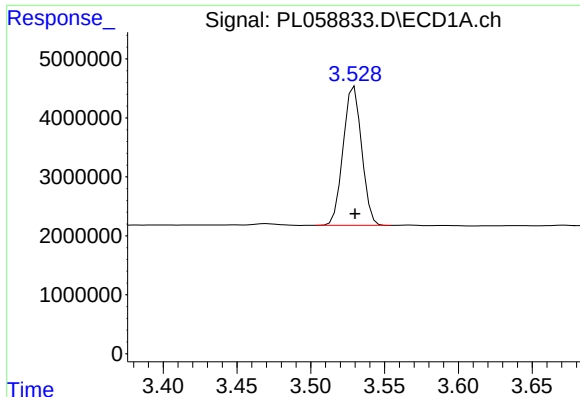


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: 0.000 min
Response: 20556725
Conc: 11.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-052020


Manual Integrations
APPROVED

mohammad
5/22/2020 12:13:19 PM

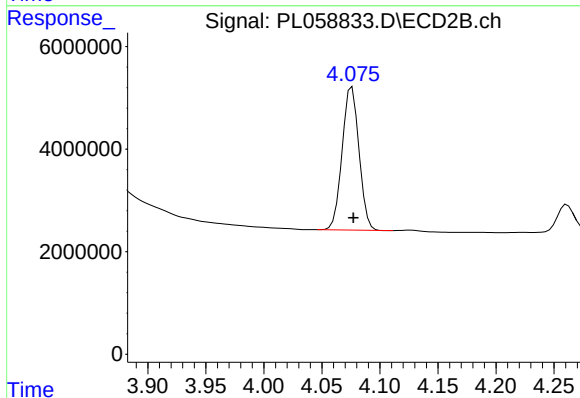


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.001 min
Response: 28211886
Conc: 10.42 ng/ml

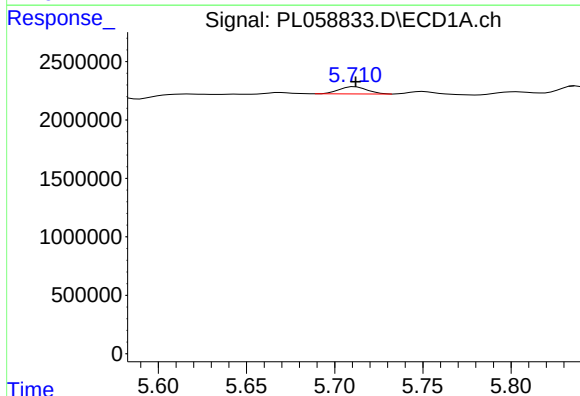


#12 4,4'-DDE

R.T.: 5.710 min
Delta R.T.: -0.002 min
Response: 684156
Conc: 0.42 ng/ml m

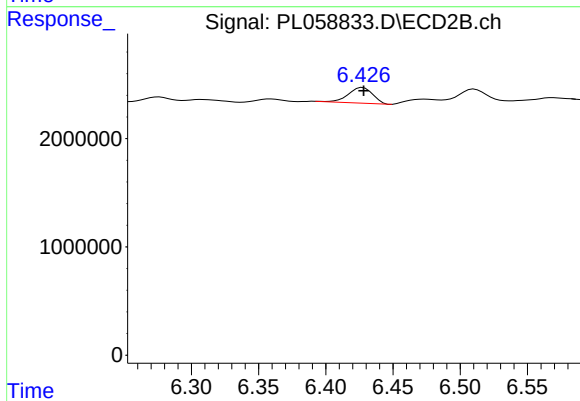

#12 4,4'-DDE

R.T.: 6.428 min
Delta R.T.: 0.000 min
Response: 1810284
Conc: 0.63 ng/ml

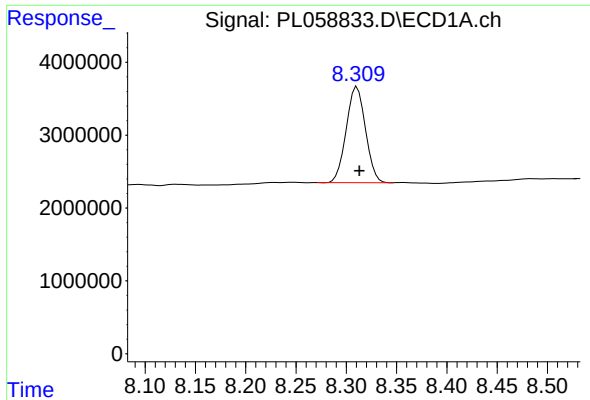


#28 Decachlorobiphenyl

R.T.: 8.311 min
Delta R.T.: -0.002 min
Response: 17514359
Conc: 10.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-052020

Manual Integrations
APPROVED

mohammad

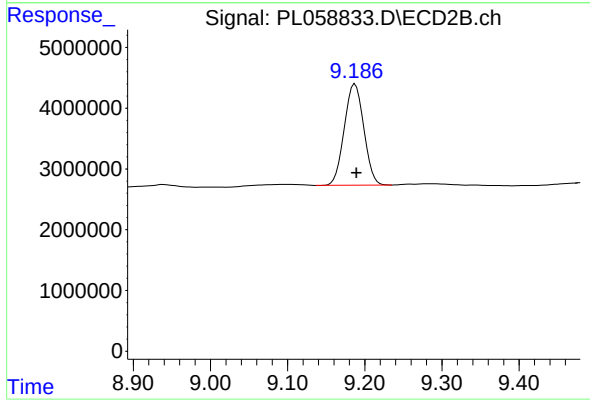

#28 Decachlorobiphenyl

R.T.: 9.187 min
Delta R.T.: -0.002 min
Response: 29240294
Conc: 11.09 ng/ml

5/22/2020 12:13:19 PM