

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL052122\  
 Data File : PL074905.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 21 May 2022 09:05  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 22 13:49:37 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL051122.M  
 Quant Title : GC Extractables  
 QLast Update : Sat May 14 02:37:15 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-----------------|--------|--------|----------|----------|--------|---------|
| -----                       |                 |        |        |          |          |        |         |
| System Monitoring Compounds |                 |        |        |          |          |        |         |
| 1)                          | SA Tetrachlo... | 5.646  | 4.650  | 10751998 | 28236702 | 21.176 | 20.573  |
| 28)                         | SA Decachlor... | 11.643 | 10.400 | 10670914 | 25049990 | 23.895 | 24.405  |
| Target Compounds            |                 |        |        |          |          |        |         |
| 8)                          | B Heptachlo...  | 8.128  | 0.000  | 3810508  | 0        | 6.700  | N.D. #  |
| 9)                          | A Endosulfan I  | 8.519f | 0.000  | 5398624  | 0        | 9.365  | N.D. #  |
| 13)                         | MA Dieldrin     | 0.000  | 7.776  | 0        | 3902298  | N.D.   | 3.063 # |
| 14)                         | MA Endrin       | 0.000  | 8.080f | 0        | 2091211  | N.D.   | 1.980 # |
| 15)                         | B Endosulfa...  | 0.000  | 8.371  | 0        | 102623   | N.D.   | 0.091 # |
| -----                       |                 |        |        |          |          |        |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL052122\  
Data File : PL074905.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 21 May 2022 09:05  
Operator : AR\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 22 13:49:37 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL051122.M  
Quant Title : GC Extractables  
QLast Update : Sat May 14 02:37:15 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

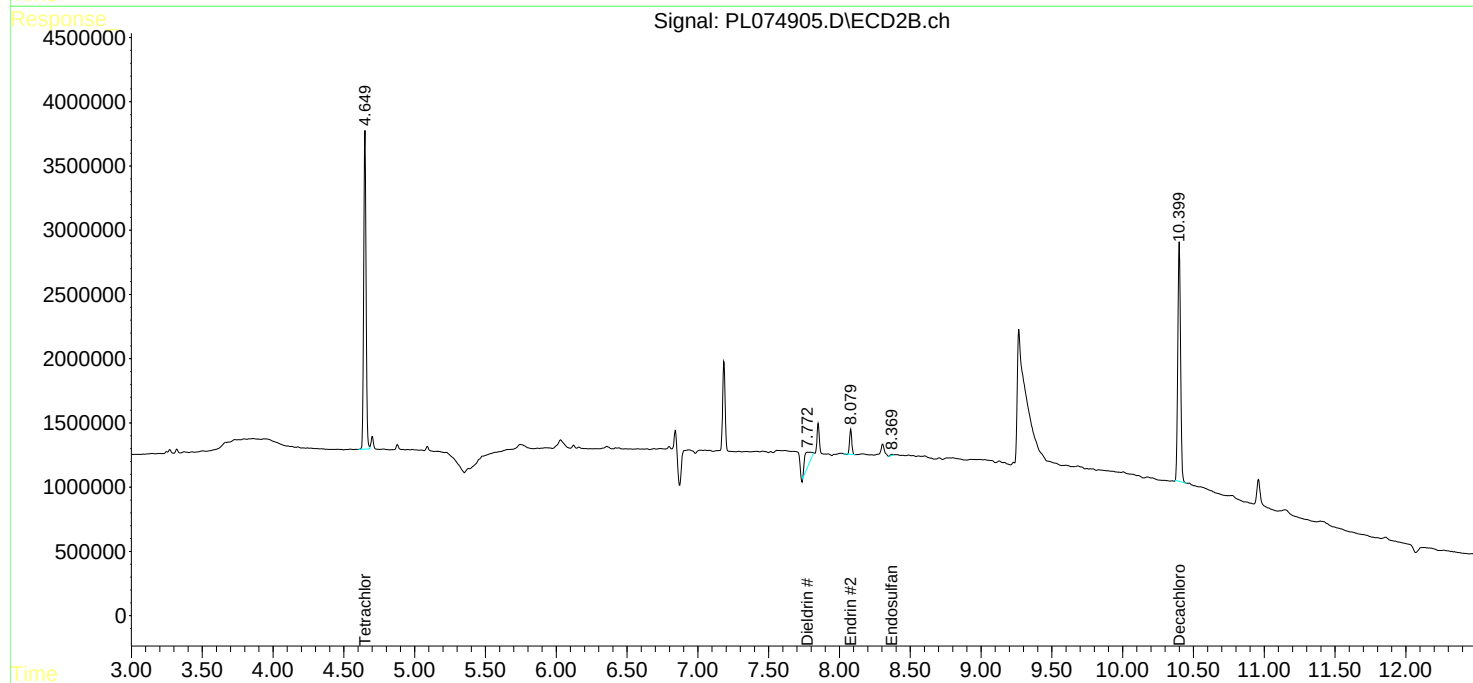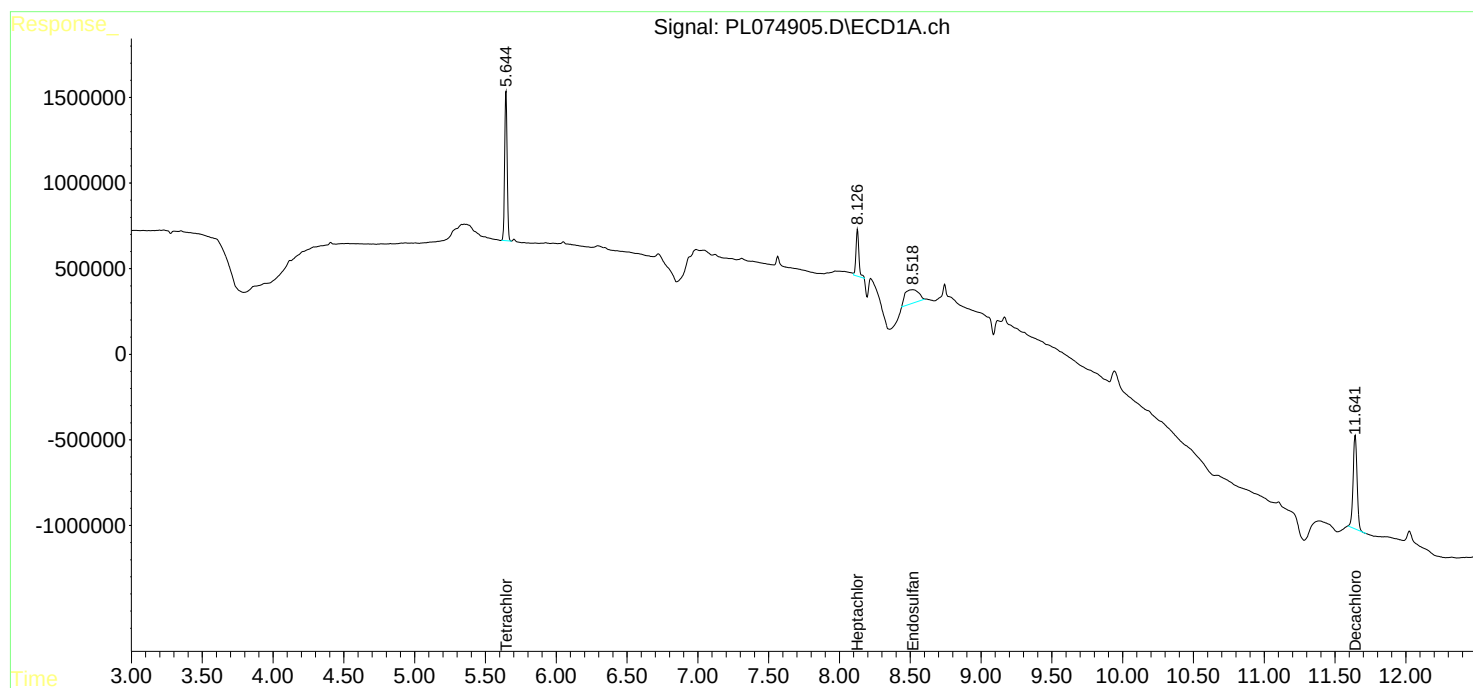


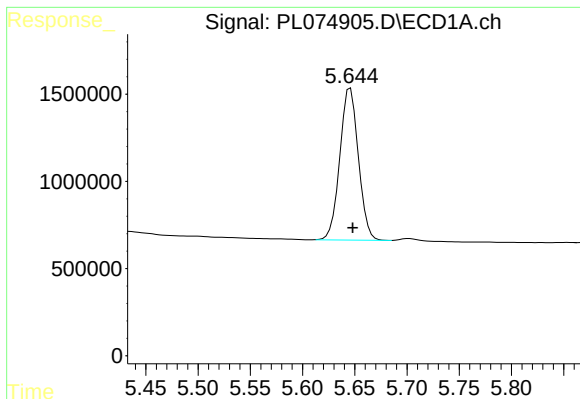

#1 Tetrachloro-m-xylene


R.T.: 5.646 min  
Delta R.T.: -0.002 min  
Response: 10751998  
Conc: 21.18 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

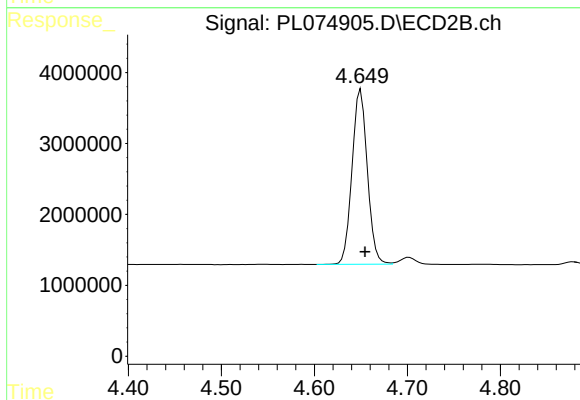


#1 Tetrachloro-m-xylene

R.T.: 4.650 min  
Delta R.T.: -0.005 min  
Response: 28236702  
Conc: 20.57 ng/ml

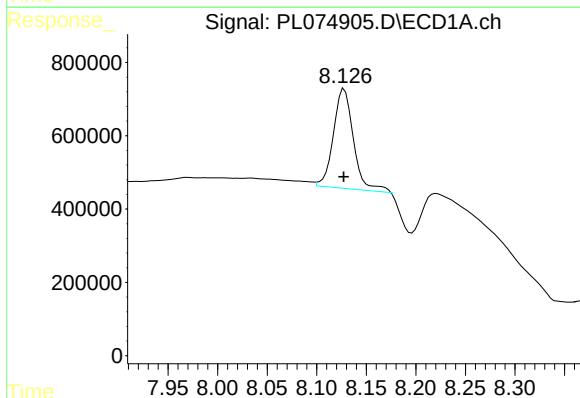


#8 Heptachlor epoxide

R.T.: 8.128 min  
Delta R.T.: 0.000 min  
Response: 3810508  
Conc: 6.70 ng/ml

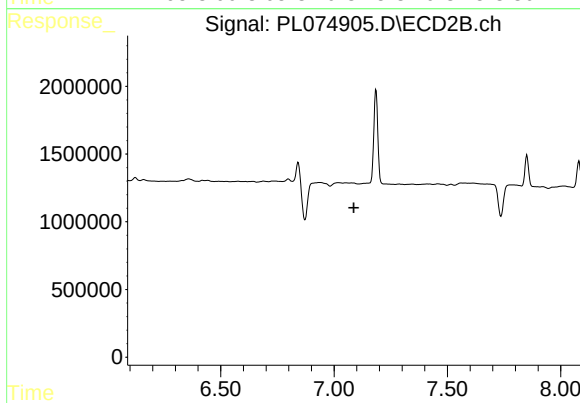

#8 Heptachlor epoxide


R.T.: 0.000 min  
Exp R.T. : 7.087 min  
Response: 0  
Conc: N.D.

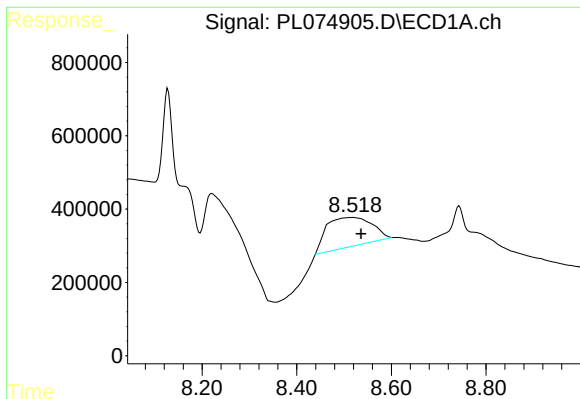

#9 Endosulfan I


R.T.: 8.519 min  
Delta R.T.: -0.017 min  
Response: 5398624  
Conc: 9.36 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

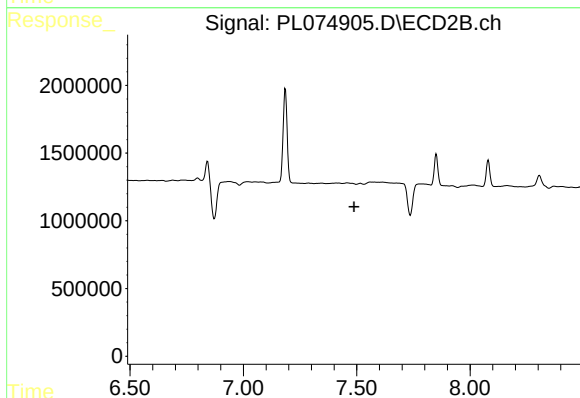


#9 Endosulfan I

R.T.: 0.000 min  
Exp R.T. : 7.489 min  
Response: 0  
Conc: N.D.

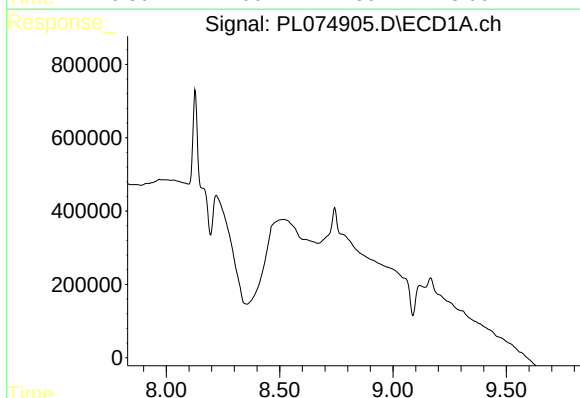


#13 Dieldrin

R.T.: 0.000 min  
Exp R.T. : 8.827 min  
Response: 0  
Conc: N.D.

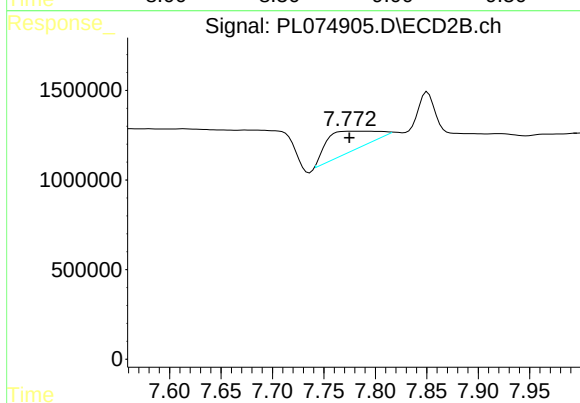

#13 Dieldrin


R.T.: 7.776 min  
Delta R.T.: 0.000 min  
Response: 3902298  
Conc: 3.06 ng/ml

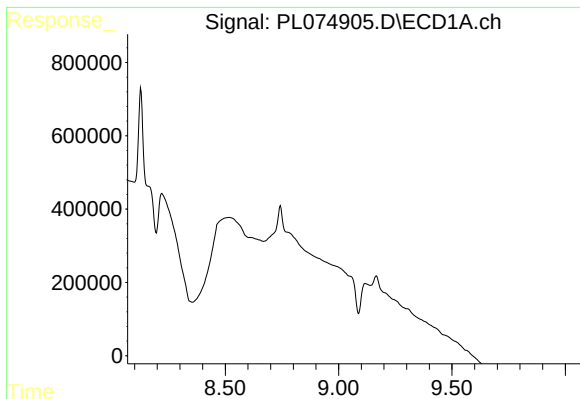

#14 Endrin


R.T.: 0.000 min  
Exp R.T.: 9.068 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

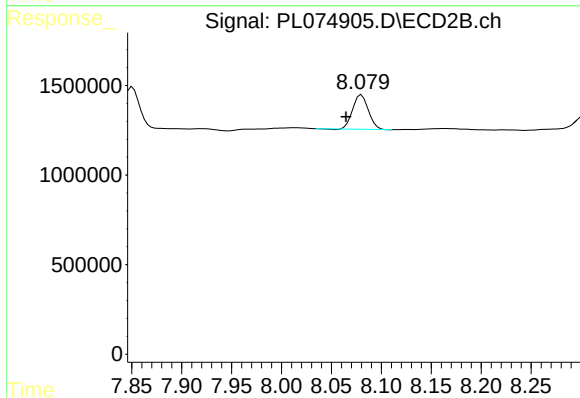


#14 Endrin

R.T.: 8.080 min  
Delta R.T.: 0.016 min  
Response: 2091211  
Conc: 1.98 ng/ml

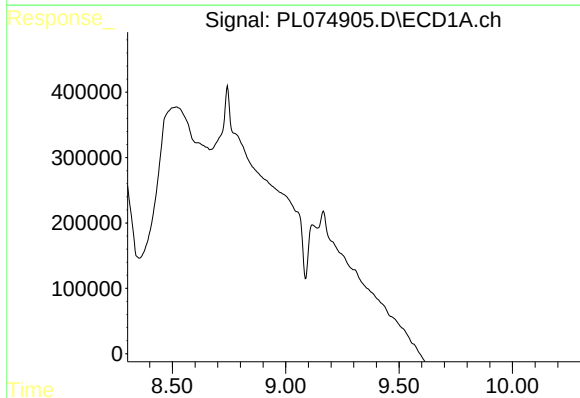


#15 Endosulfan II

R.T.: 0.000 min  
Exp R.T.: 9.302 min  
Response: 0  
Conc: N.D.

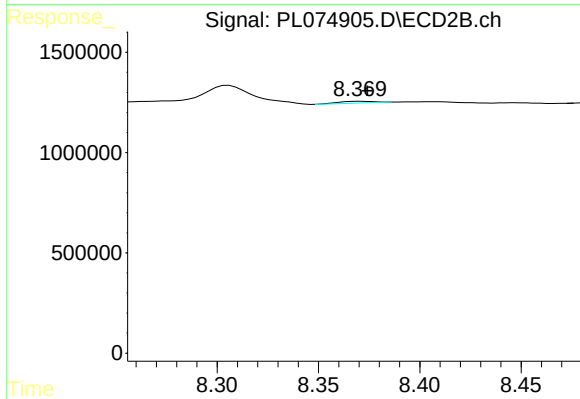

#15 Endosulfan II


R.T.: 8.371 min  
Delta R.T.: -0.003 min  
Response: 102623  
Conc: 0.09 ng/ml

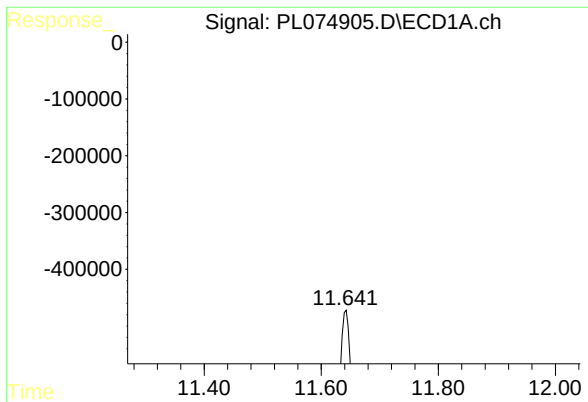

#28 Decachlorobiphenyl

R.T.: 11.643 min  
Delta R.T.: -0.008 min  
Response: 10670914  
Conc: 23.89 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

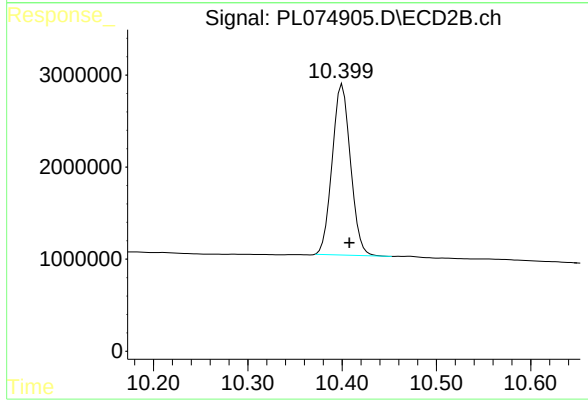

#28 Decachlorobiphenyl

R.T.: 10.400 min  
Delta R.T.: -0.008 min  
Response: 25049990  
Conc: 24.41 ng/ml