

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052122\
 Data File : PL074926.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2022 02:39
 Operator : AR\AJ
 Sample : N2874-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 13:54:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.667	3228027	9100007	6.358	6.630
28)	SA Decachlor...	11.642	10.416	4481361	13134311	10.035	12.796 #
Target Compounds							
3)	MA gamma-BHC...	0.000	5.786	0	634249	N.D.	0.384 #
6)	B beta-BHC	0.000	6.139	0	614032	N.D.	0.773 #
9)	A Endosulfan I	8.515f	0.000	5202404	0	9.024	N.D. #
14)	MA Endrin	0.000	8.092f	0	516691	N.D.	0.489 #
15)	B Endosulfa...	0.000	8.355f	0	681461	N.D.	0.603 #
16)	A 4,4'-DDD	9.205	0.000	466084	0	1.031	N.D. #
17)	MA 4,4'-DDT	0.000	8.492	0	981390	N.D.	0.981 #
18)	B Endrin al...	0.000	8.542f	0	465668	N.D.	0.583 #
19)	B Endosulfa...	0.000	8.803	0	727458	N.D.	0.668 #
20)	A Methoxychlor	0.000	9.065f	0	2101564	N.D.	3.596 #
22)	Mirex	0.000	9.527f	0	1109869	N.D.	1.146 #
27)	Chlordane-5	0.000	8.155	0	1144053	N.D.	30.942 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052122\
Data File : PL074926.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2022 02:39
Operator : AR\AJ
Sample : N2874-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 13:54:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

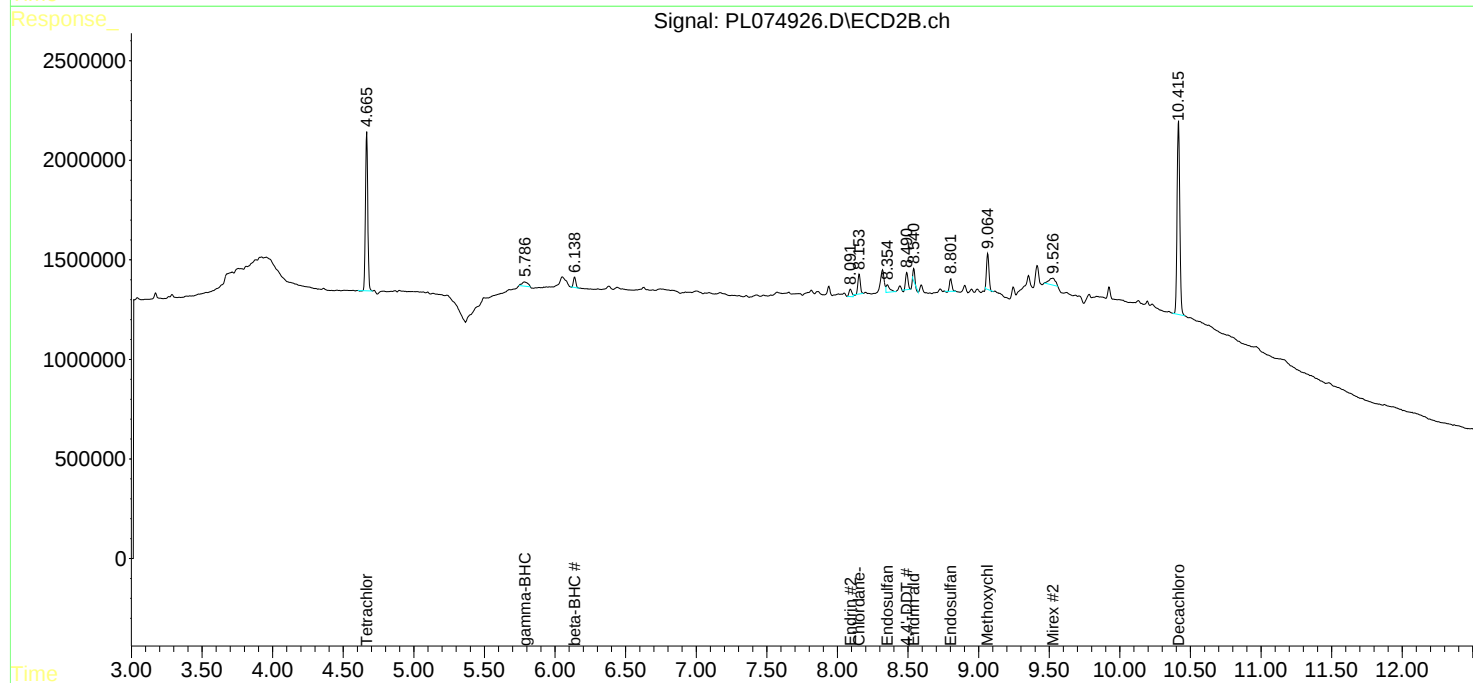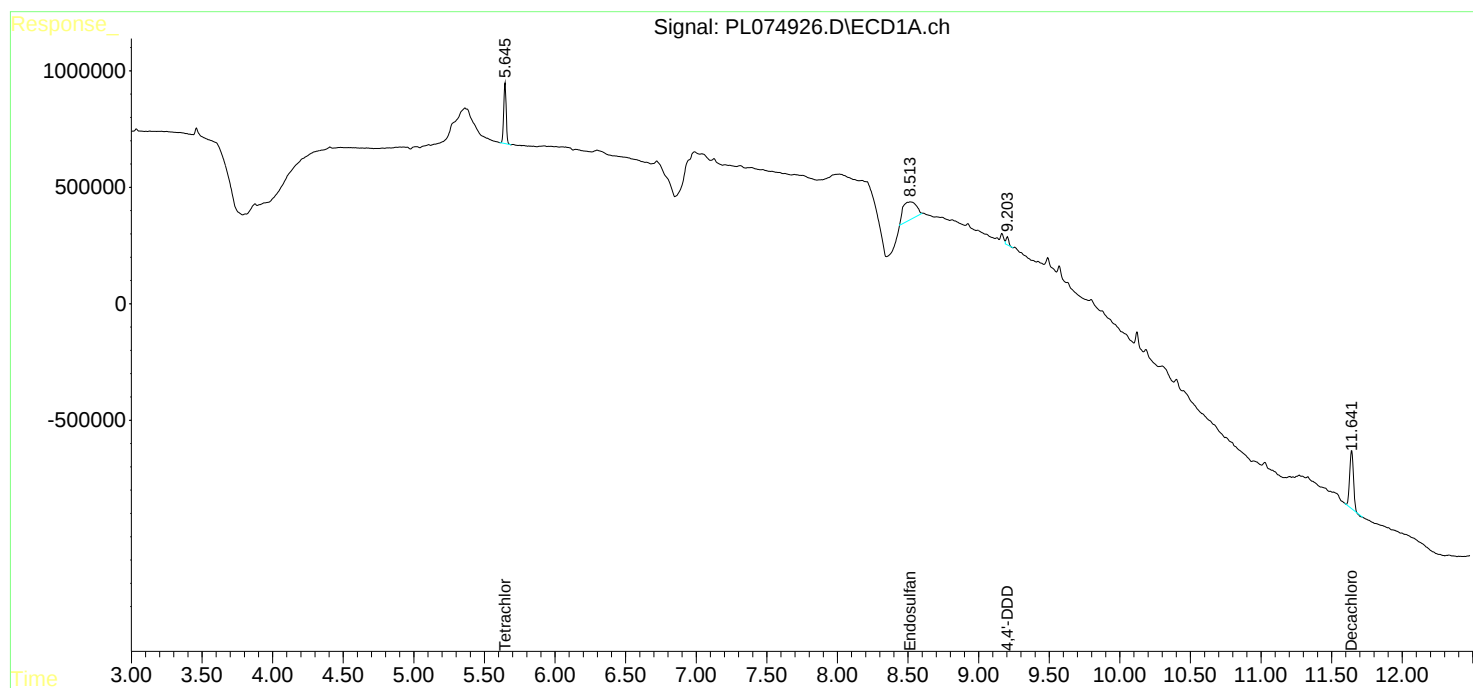


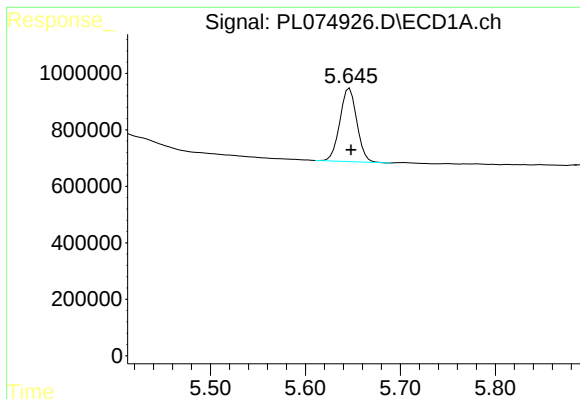

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 3228027
Conc: 6.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

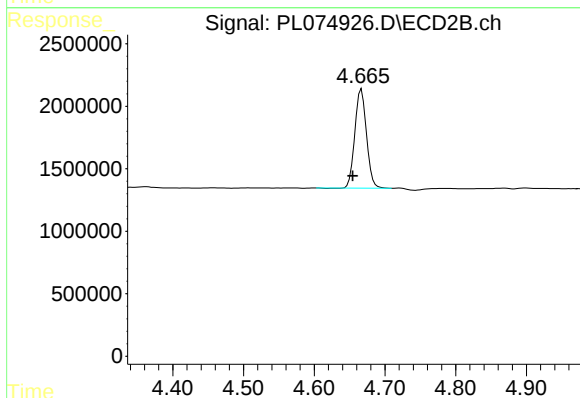


#1 Tetrachloro-m-xylene

R.T.: 4.667 min
Delta R.T.: 0.012 min
Response: 9100007
Conc: 6.63 ng/ml

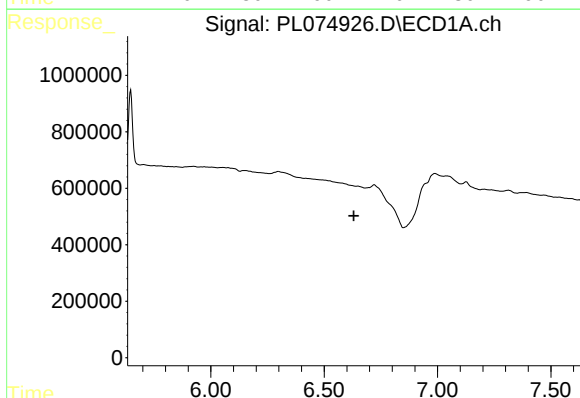


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 6.630 min
Response: 0
Conc: N.D.

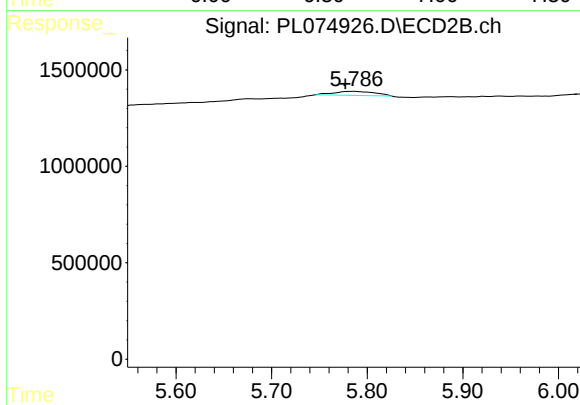

#3 gamma-BHC (Lindane)


R.T.: 5.786 min
Delta R.T.: 0.009 min
Response: 634249
Conc: 0.38 ng/ml

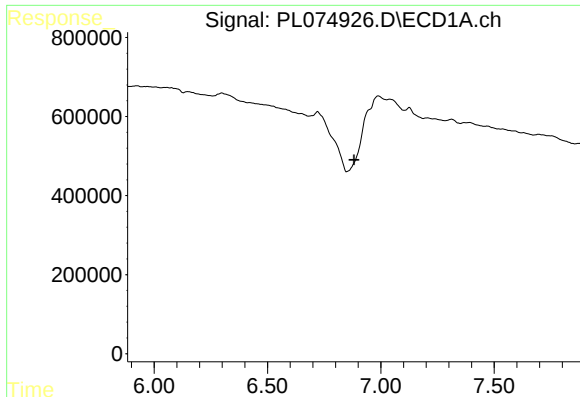

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

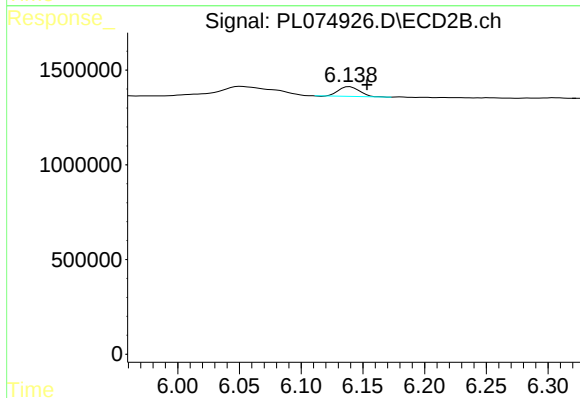


#6 beta-BHC

R.T.: 6.139 min
Delta R.T.: -0.014 min
Response: 614032
Conc: 0.77 ng/ml

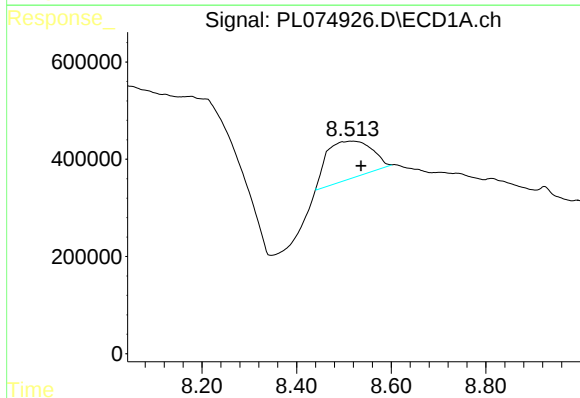


#9 Endosulfan I

R.T.: 8.515 min
Delta R.T.: -0.021 min
Response: 5202404
Conc: 9.02 ng/ml

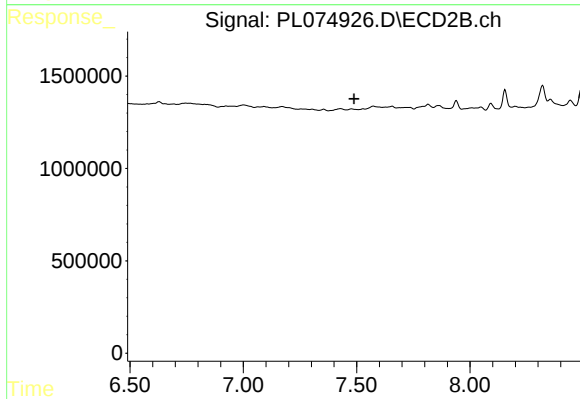

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.489 min
Response: 0
Conc: N.D.

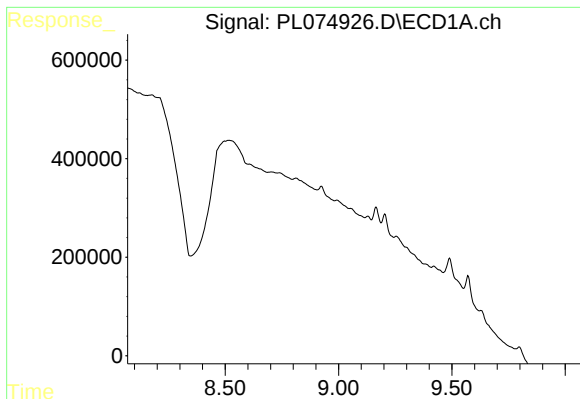

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

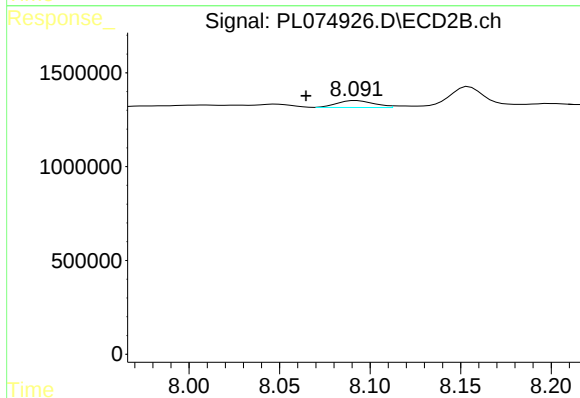


#14 Endrin

R.T.: 8.092 min
Delta R.T.: 0.028 min
Response: 516691
Conc: 0.49 ng/ml

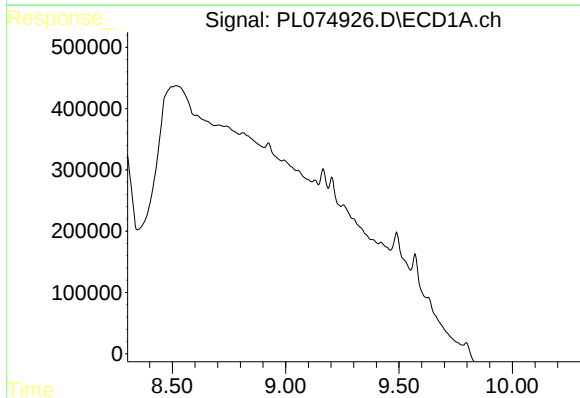


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 9.302 min
Response: 0
Conc: N.D.

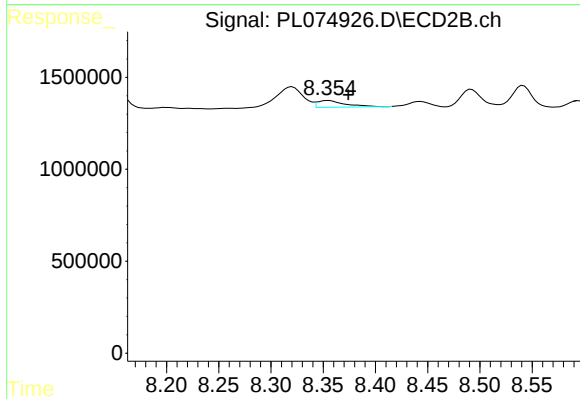

#15 Endosulfan II


R.T.: 8.355 min
Delta R.T.: -0.019 min
Response: 681461
Conc: 0.60 ng/ml

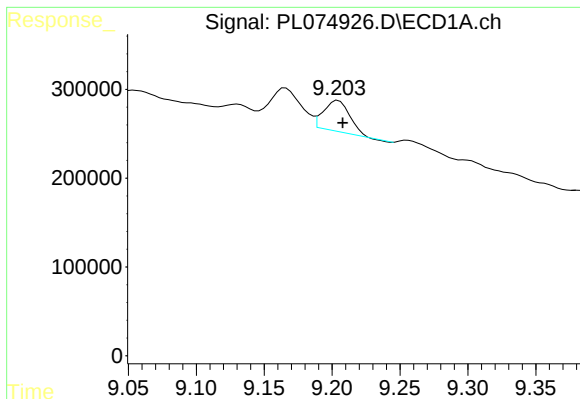

#16 4,4'-DDD


R.T.: 9.205 min
Delta R.T.: -0.003 min
Response: 466084
Conc: 1.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

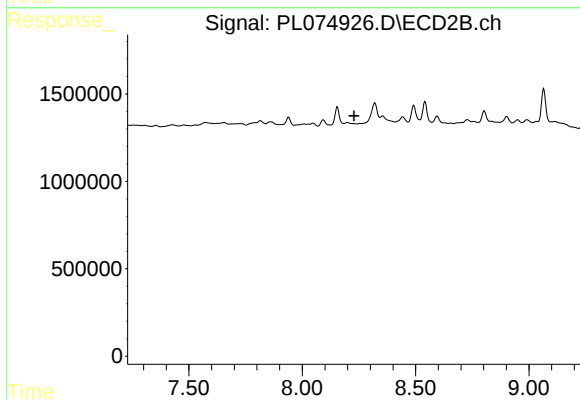


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.229 min
Response: 0
Conc: N.D.

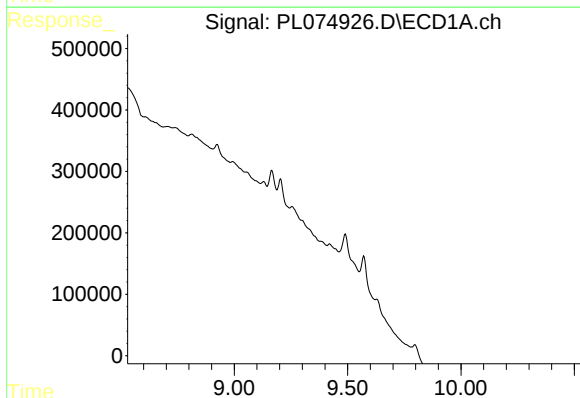


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.527 min
Response: 0
Conc: N.D.

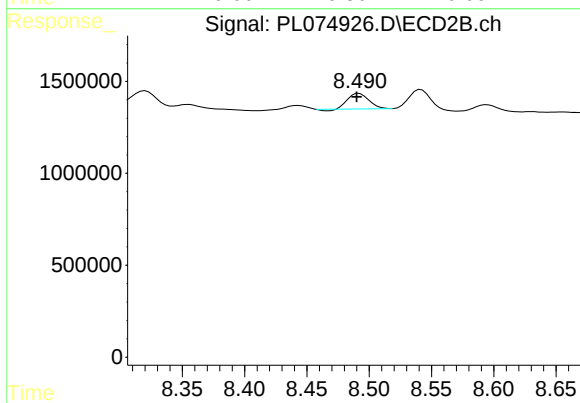

#17 4,4'-DDT


R.T.: 8.492 min
Delta R.T.: 0.002 min
Response: 981390
Conc: 0.98 ng/ml

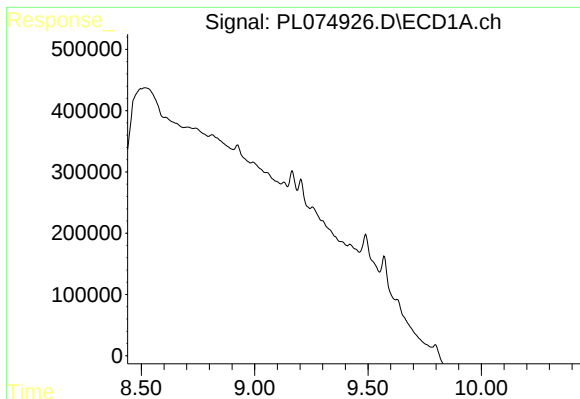

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 9.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

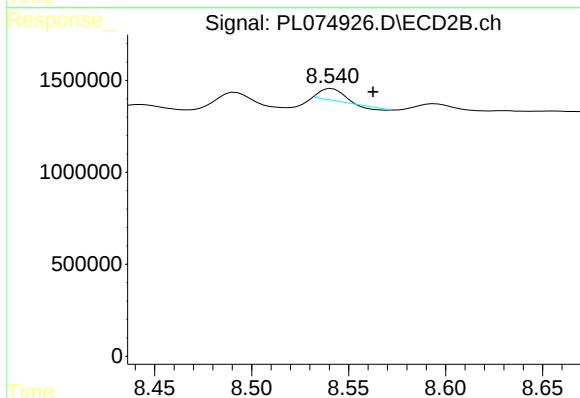


#18 Endrin aldehyde

R.T.: 8.542 min
Delta R.T.: -0.021 min
Response: 465668
Conc: 0.58 ng/ml

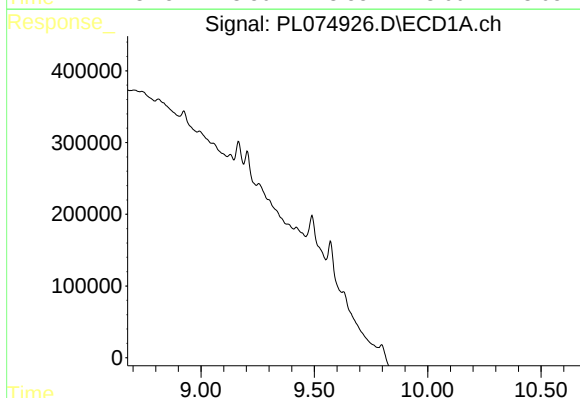


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

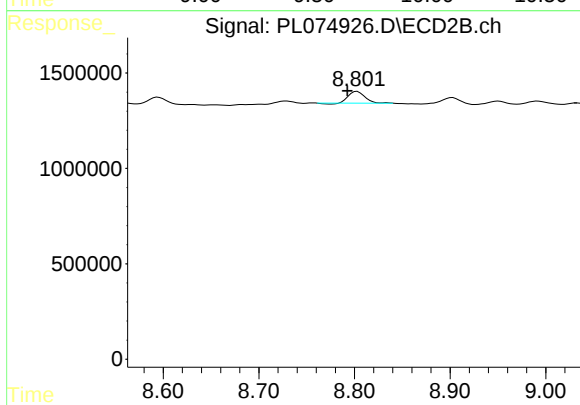

#19 Endosulfan Sulfate


R.T.: 8.803 min
Delta R.T.: 0.010 min
Response: 727458
Conc: 0.67 ng/ml

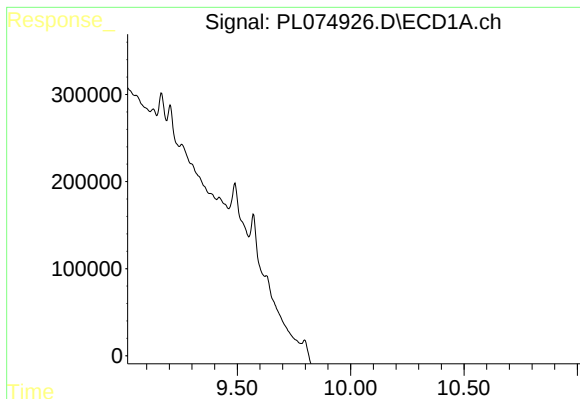

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 10.013 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

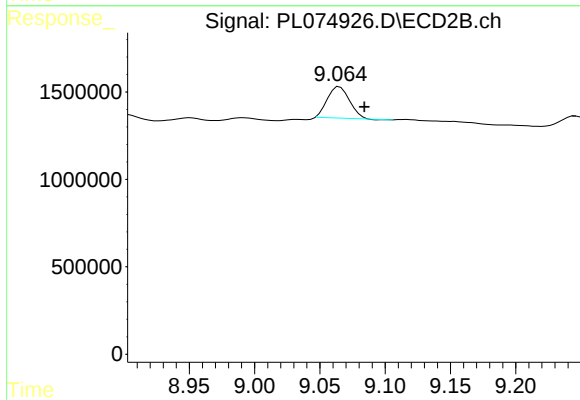


#20 Methoxychlor

R.T.: 9.065 min
Delta R.T.: -0.019 min
Response: 2101564
Conc: 3.60 ng/ml

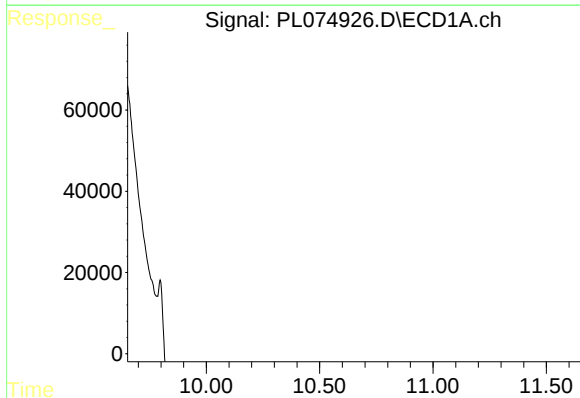


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 10.652 min
Response: 0
Conc: N.D.

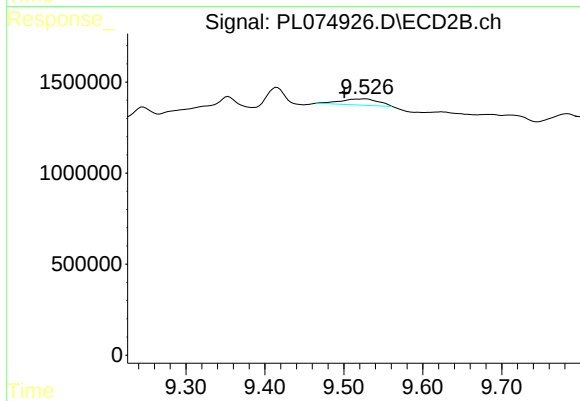

#22 Mirex


R.T.: 9.527 min
Delta R.T.: 0.026 min
Response: 1109869
Conc: 1.15 ng/ml

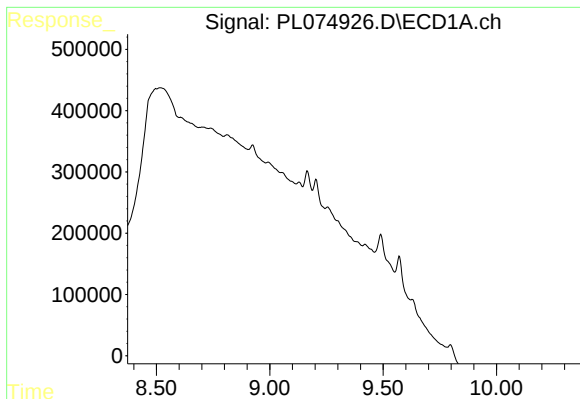

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

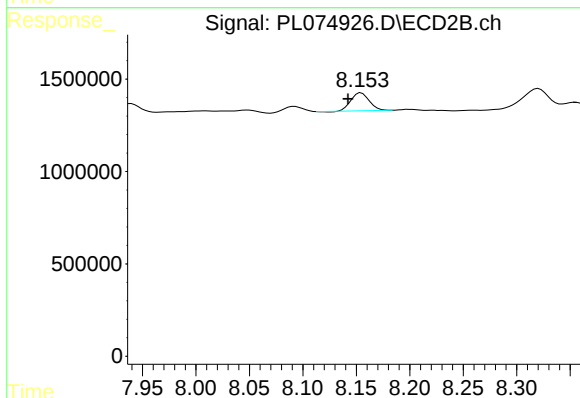


#27 Chlordane-5

R.T.: 8.155 min
Delta R.T.: 0.012 min
Response: 1144053
Conc: 30.94 ng/ml

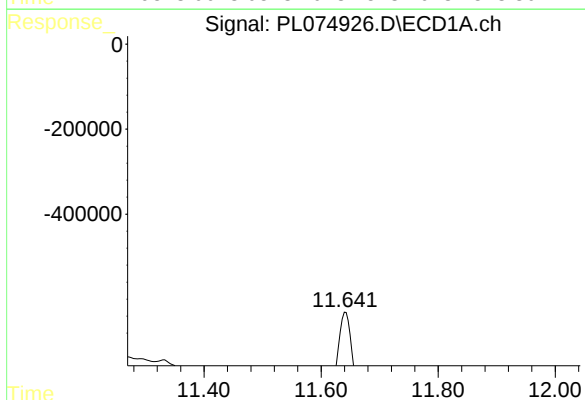

#28 Decachlorobiphenyl

R.T.: 11.642 min
Delta R.T.: -0.009 min
Response: 4481361
Conc: 10.03 ng/ml

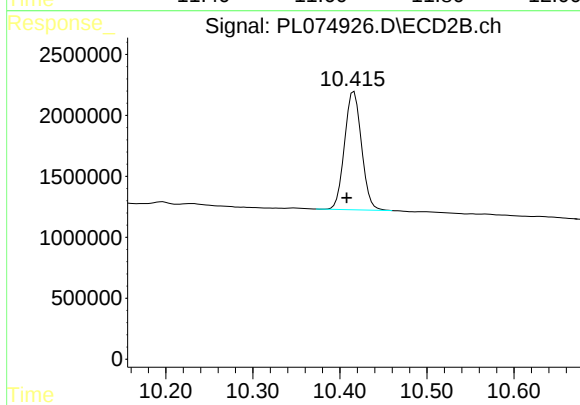

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: 0.008 min
Response: 13134311
Conc: 12.80 ng/ml