

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052122\
 Data File : PL074927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2022 02:56
 Operator : AR\AJ
 Sample : N2874-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 13:54:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.649	3856629	10873264	7.596	7.922
28)	SA Decachlor...	11.642	10.399	6380272	16967926	14.287	16.531
Target Compounds							
9)	A Endosulfan I	8.513f	0.000	5349589	0	9.279	N.D. #
10)	B gamma-Chl...	0.000	7.339f	0	236270	N.D.	0.170 #
12)	B 4,4'-DDE	8.662	7.638	765770	2300700	1.654	1.955
13)	MA Dieldrin	0.000	7.775	0	216779	N.D.	0.170 #
14)	MA Endrin	0.000	8.076	0	643528	N.D.	0.609 #
16)	A 4,4'-DDD	9.205	0.000	596411	0	1.319	N.D. #
17)	MA 4,4'-DDT	0.000	8.475	0	1861965	N.D.	1.861 #
19)	B Endosulfa...	0.000	8.786	0	1294795	N.D.	1.189 #
21)	B Endrin ke...	0.000	9.338f	0	1574034	N.D.	1.412 #
25)	Chlordane-3	0.000	7.339f	0	236270	N.D.	1.820 #
27)	Chlordane-5	0.000	8.138	0	1656006	N.D.	44.789 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052122\
Data File : PL074927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2022 02:56
Operator : AR\AJ
Sample : N2874-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 13:54:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

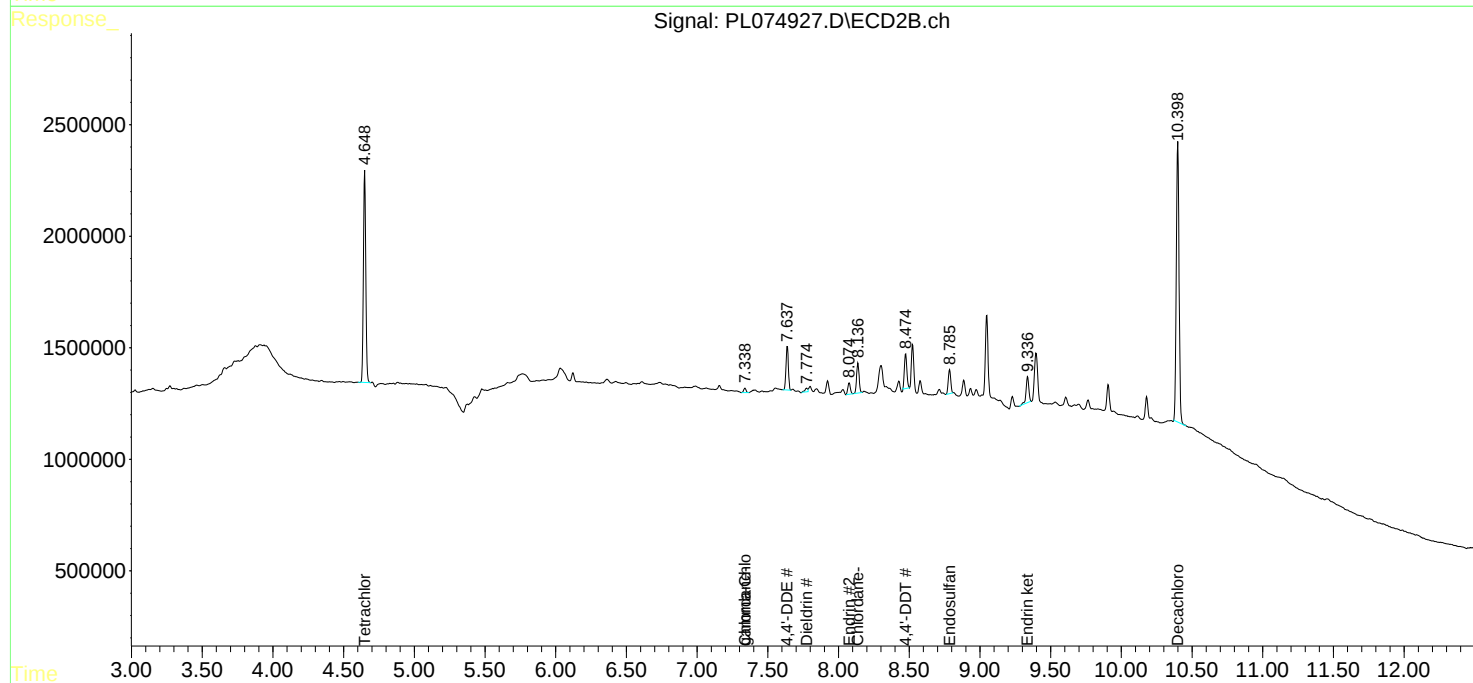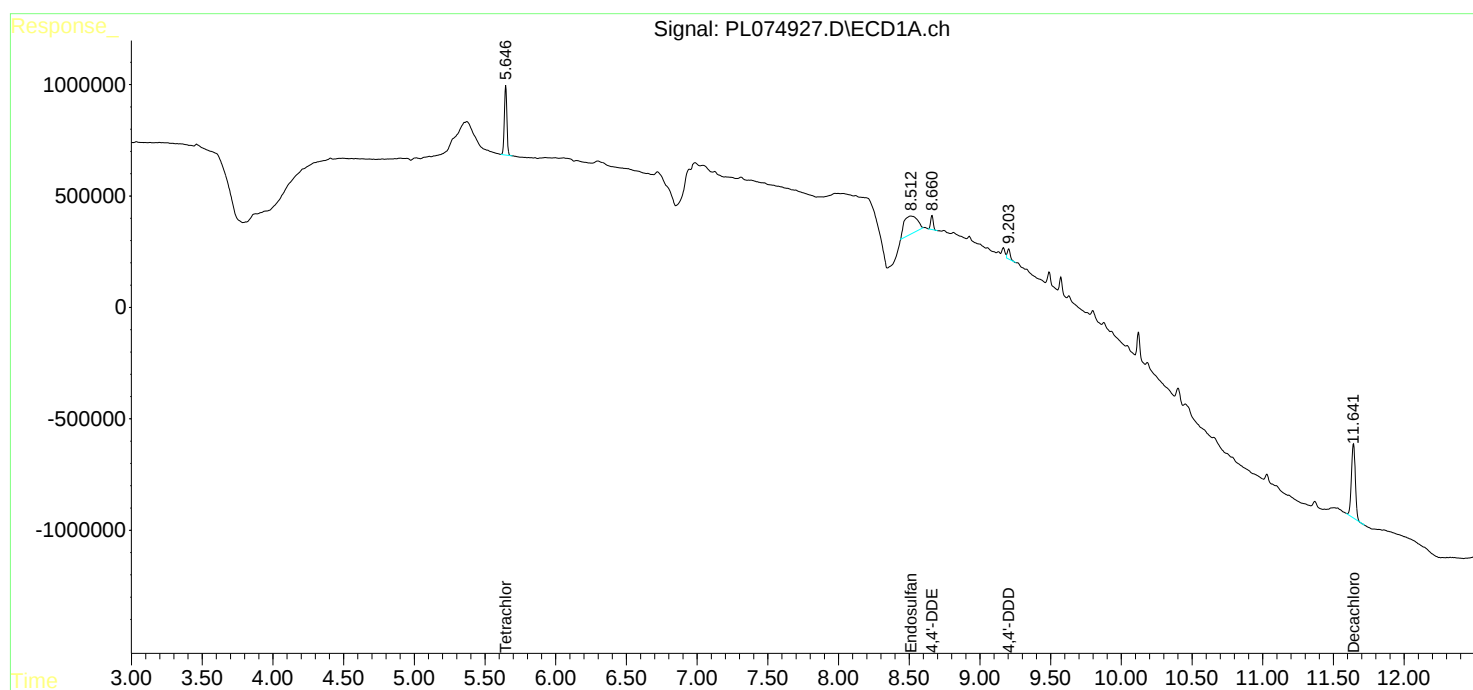


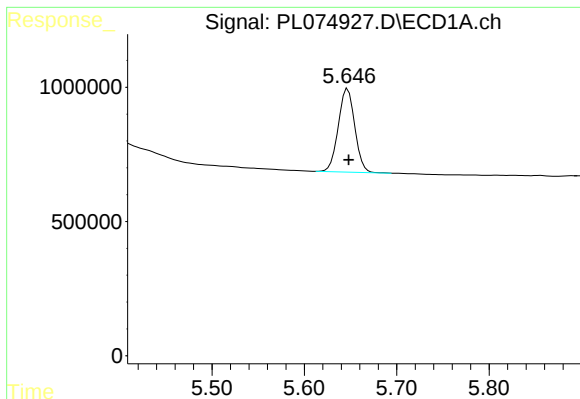

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: -0.001 min
Response: 3856629
Conc: 7.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

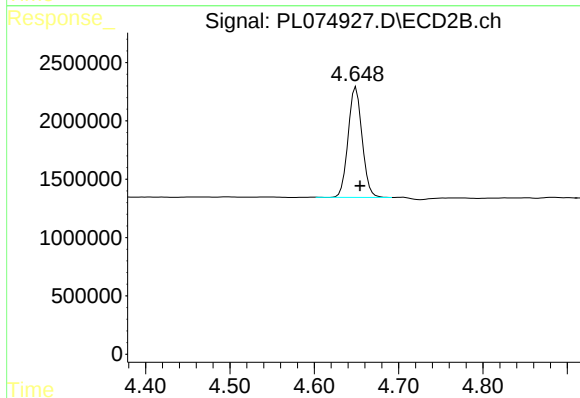


#1 Tetrachloro-m-xylene

R.T.: 4.649 min
Delta R.T.: -0.005 min
Response: 10873264
Conc: 7.92 ng/ml

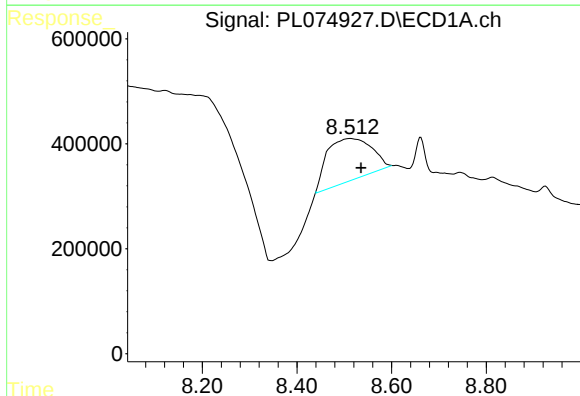


#9 Endosulfan I

R.T.: 8.513 min
Delta R.T.: -0.023 min
Response: 5349589
Conc: 9.28 ng/ml

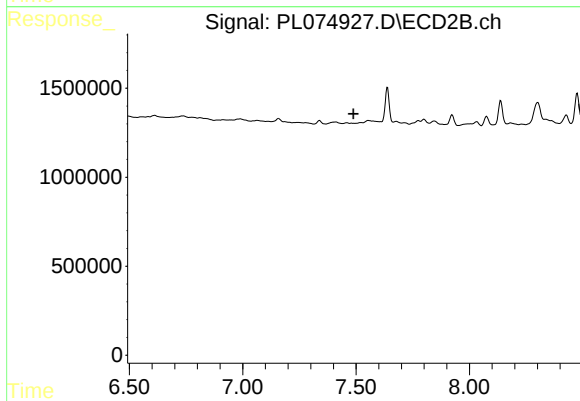

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.489 min
Response: 0
Conc: N.D.

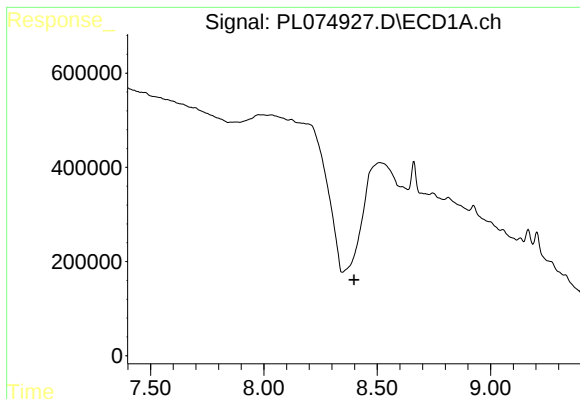

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

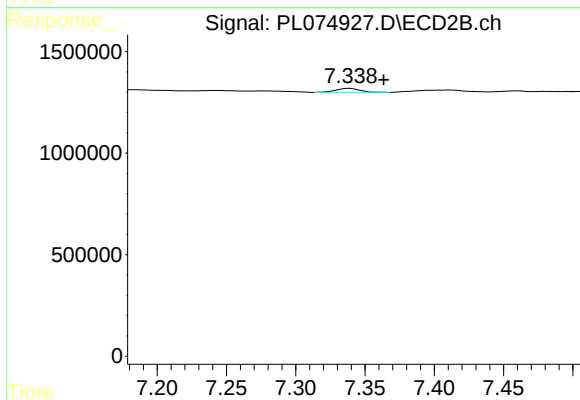


#10 gamma-Chlordane

R.T.: 7.339 min
Delta R.T.: -0.024 min
Response: 236270
Conc: 0.17 ng/ml

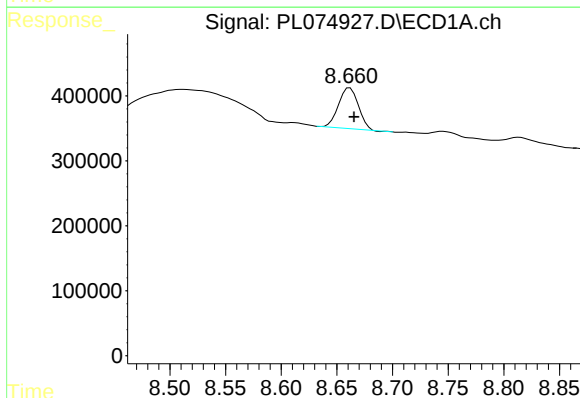


#12 4,4'-DDE

R.T.: 8.662 min
Delta R.T.: -0.004 min
Response: 765770
Conc: 1.65 ng/ml

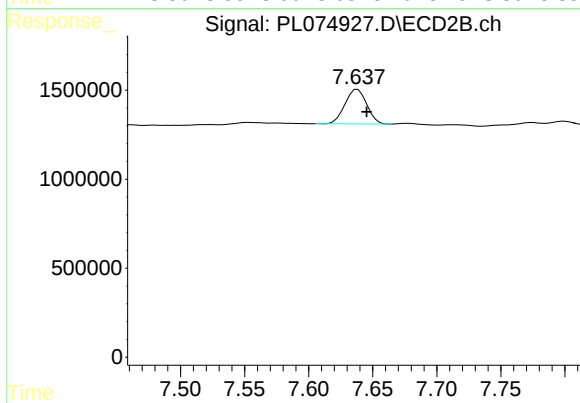

#12 4,4'-DDE


R.T.: 7.638 min
Delta R.T.: -0.007 min
Response: 2300700
Conc: 1.96 ng/ml

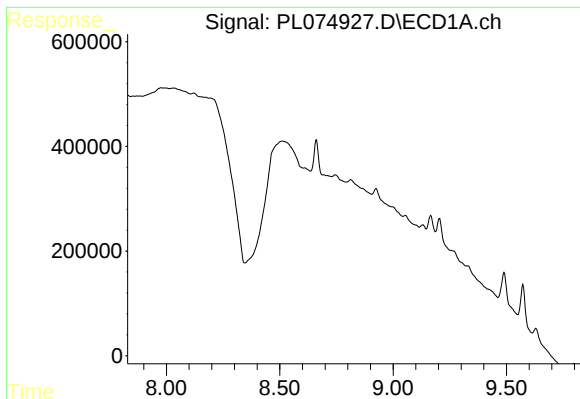

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

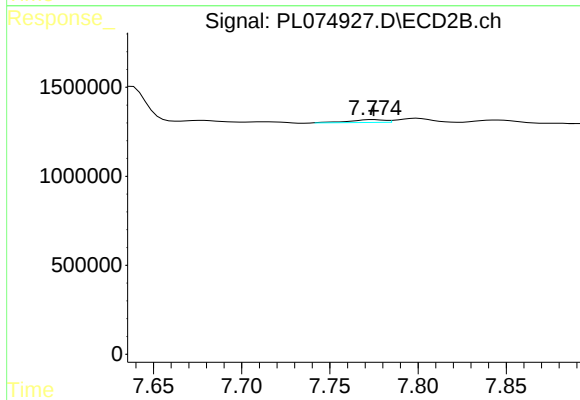


#13 Dieldrin

R.T.: 7.775 min
Delta R.T.: 0.000 min
Response: 216779
Conc: 0.17 ng/ml

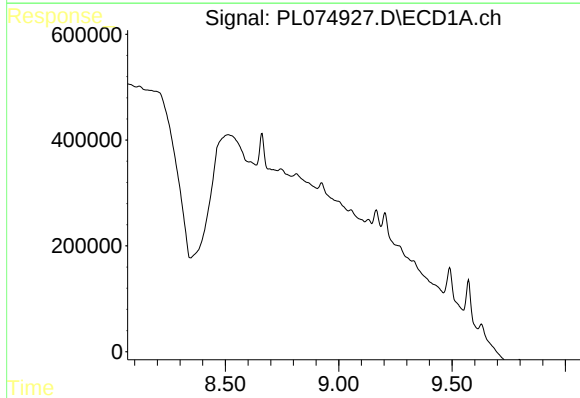


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

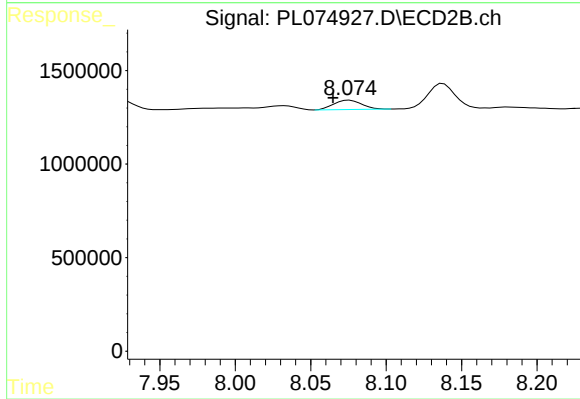

#14 Endrin


R.T.: 8.076 min
Delta R.T.: 0.011 min
Response: 643528
Conc: 0.61 ng/ml

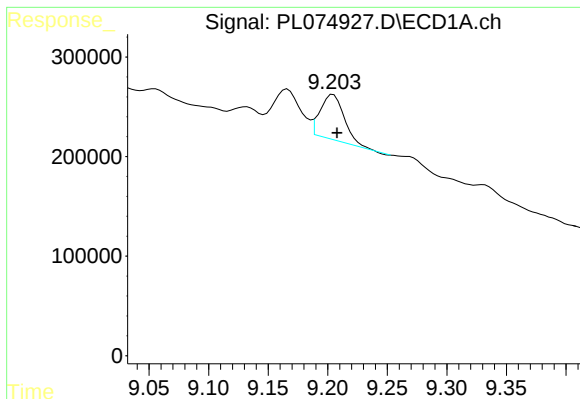

#16 4,4'-DDD


R.T.: 9.205 min
Delta R.T.: -0.003 min
Response: 596411
Conc: 1.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

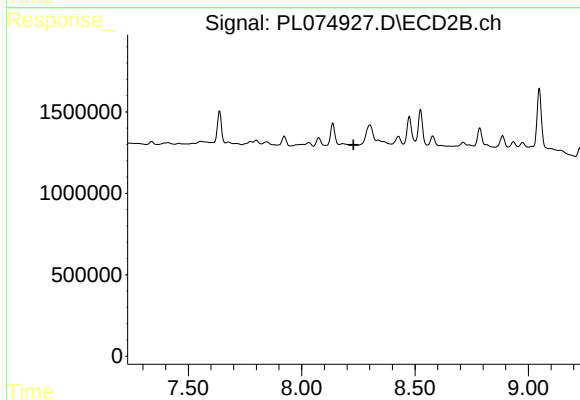


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.229 min
Response: 0
Conc: N.D.

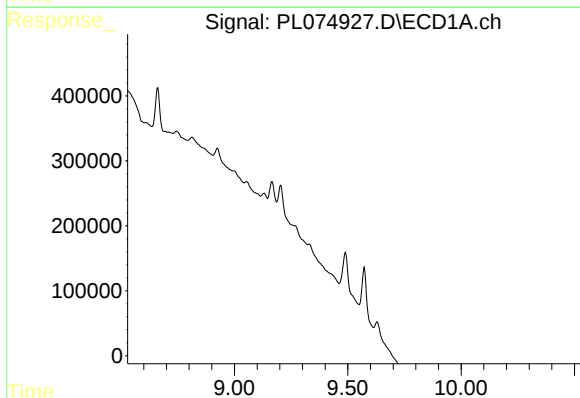


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.527 min
Response: 0
Conc: N.D.

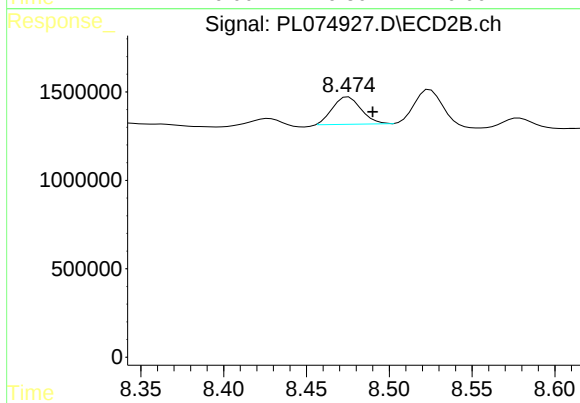

#17 4,4'-DDT


R.T.: 8.475 min
Delta R.T.: -0.015 min
Response: 1861965
Conc: 1.86 ng/ml

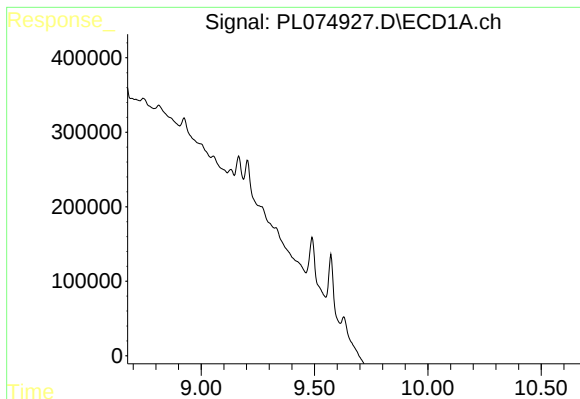

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

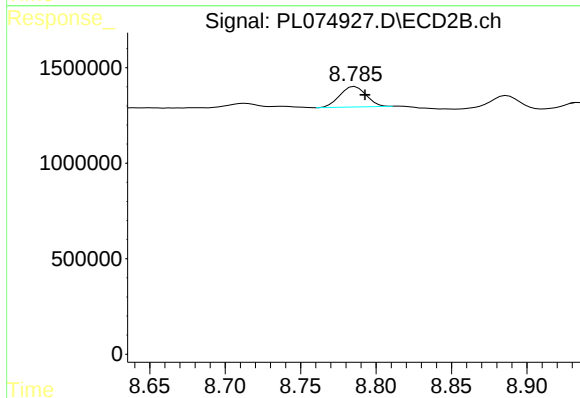


#19 Endosulfan Sulfate

R.T.: 8.786 min
Delta R.T.: -0.007 min
Response: 1294795
Conc: 1.19 ng/ml

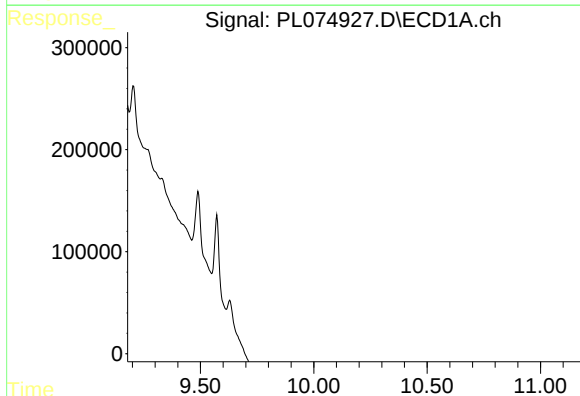


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 10.177 min
Response: 0
Conc: N.D.

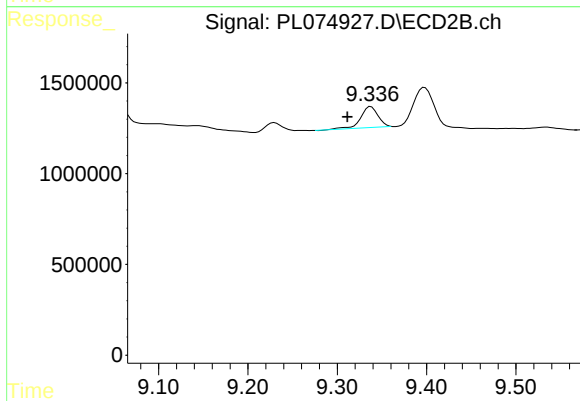

#21 Endrin ketone


R.T.: 9.338 min
Delta R.T.: 0.026 min
Response: 1574034
Conc: 1.41 ng/ml

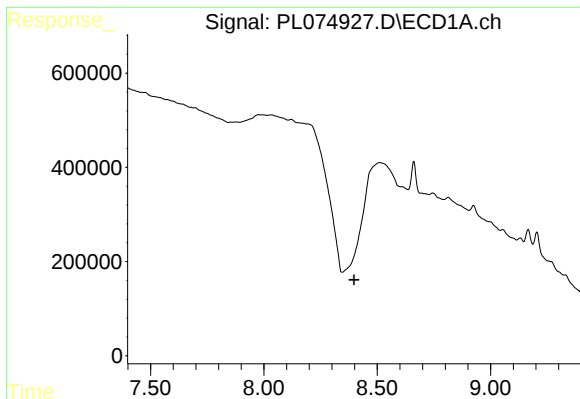

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

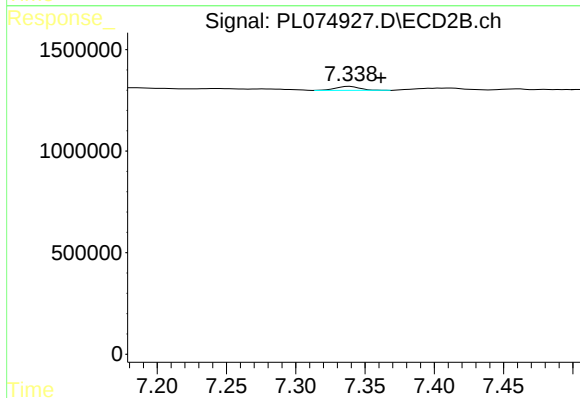


#25 Chlordane-3

R.T.: 7.339 min
Delta R.T.: -0.023 min
Response: 236270
Conc: 1.82 ng/ml

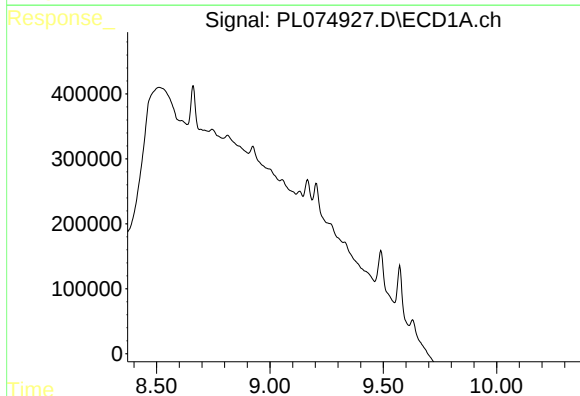


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

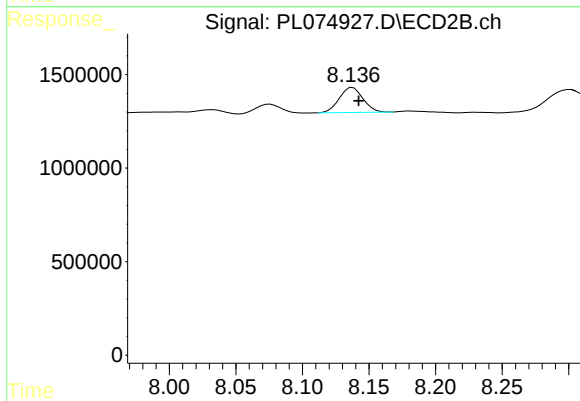

#27 Chlordane-5


R.T.: 8.138 min
Delta R.T.: -0.004 min
Response: 1656006
Conc: 44.79 ng/ml

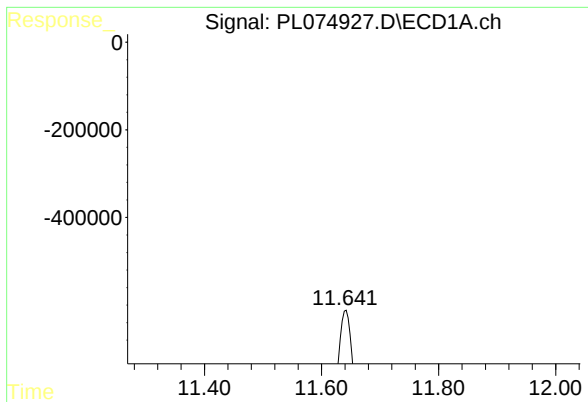

#28 Decachlorobiphenyl

R.T.: 11.642 min
Delta R.T.: -0.009 min
Response: 6380272
Conc: 14.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

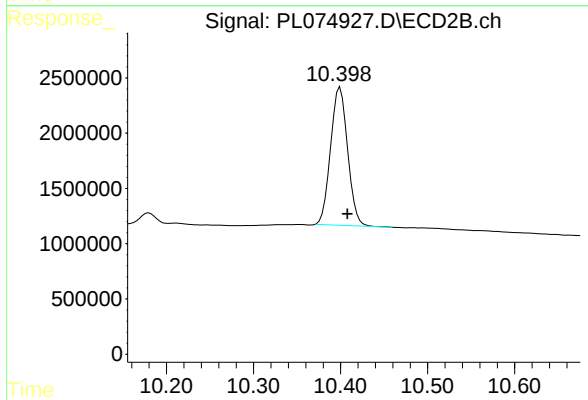

#28 Decachlorobiphenyl

R.T.: 10.399 min
Delta R.T.: -0.008 min
Response: 16967926
Conc: 16.53 ng/ml