

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052122\
 Data File : PL074929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2022 03:29
 Operator : AR\AJ
 Sample : N2874-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 13:54:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.650	2773817	7825313	5.463	5.701
28)	SA Decachlor...	11.643	10.399	4878656	12722630	10.924	12.395
Target Compounds							
9)	A Endosulfan I	8.510f	0.000	5423580	0	9.408	N.D. #
11)	B alpha-Chl...	8.510f	0.000	5423580	0	8.884	N.D. #
12)	B 4,4'-DDE	0.000	7.637	0	537832	N.D.	0.457 #
13)	MA Dieldrin	0.000	7.800f	0	206530	N.D.	0.162 #
14)	MA Endrin	0.000	8.076	0	510334	N.D.	0.483 #
17)	MA 4,4'-DDT	0.000	8.475	0	972120	N.D.	0.972 #
19)	B Endosulfa...	0.000	8.786	0	865375	N.D.	0.795 #
21)	B Endrin ke...	0.000	9.337f	0	659087	N.D.	0.591 #
27)	Chlordane-5	0.000	8.137	0	820317	N.D.	22.186 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052122\
Data File : PL074929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2022 03:29
Operator : AR\AJ
Sample : N2874-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 13:54:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

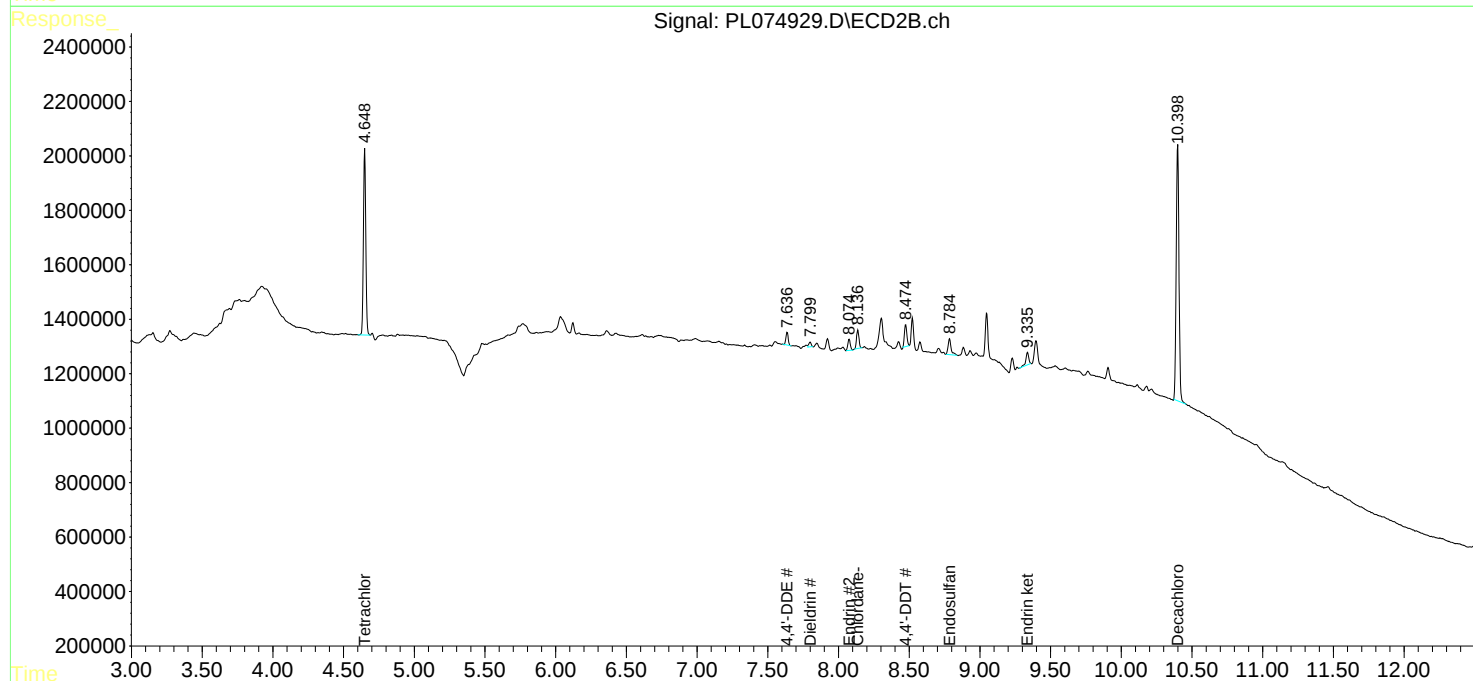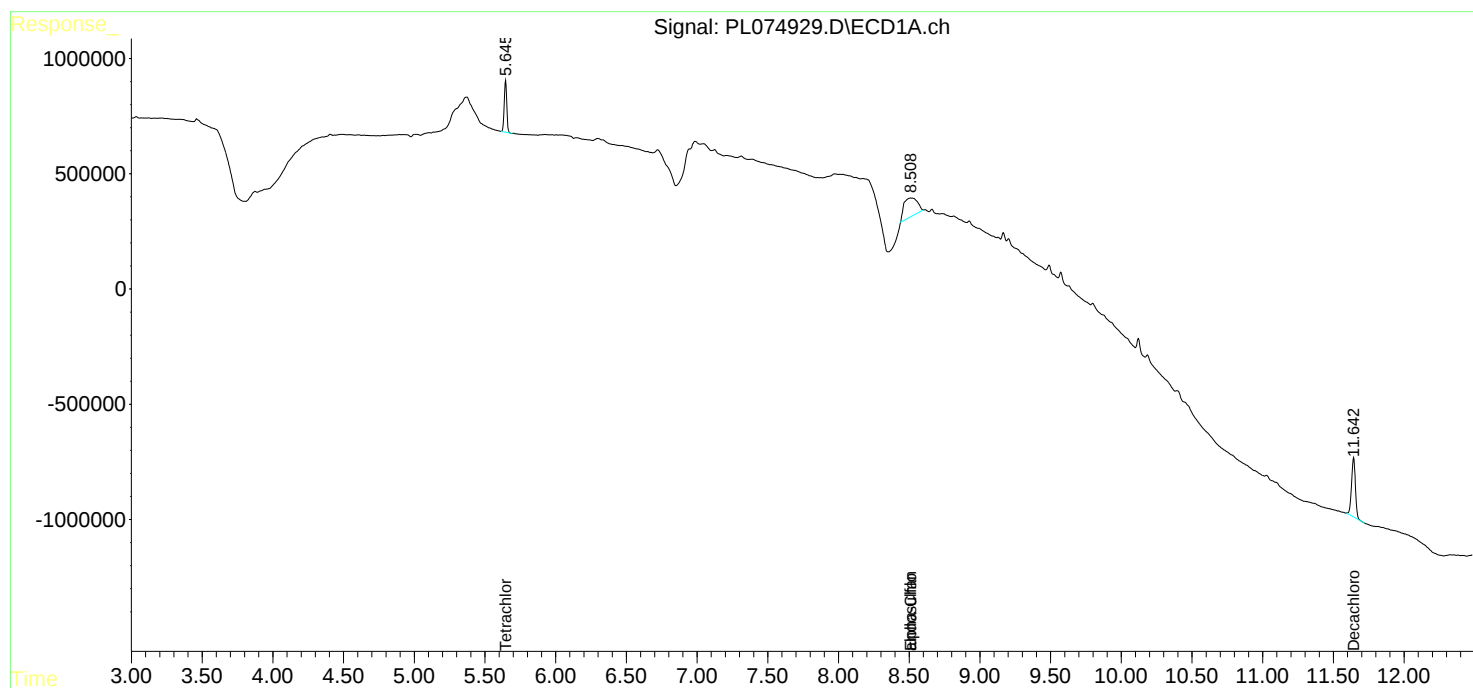


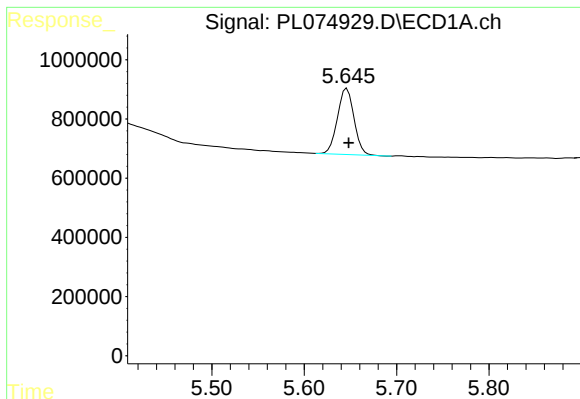

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 2773817
Conc: 5.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

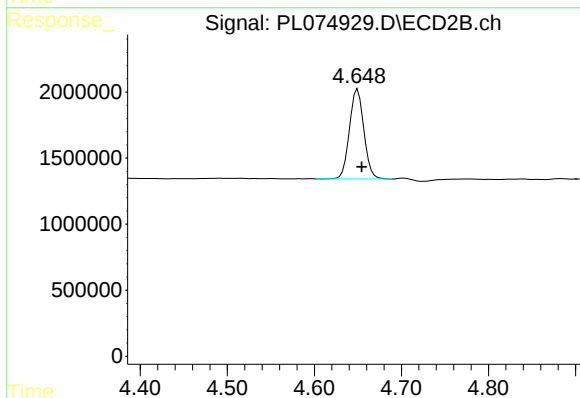


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.005 min
Response: 7825313
Conc: 5.70 ng/ml

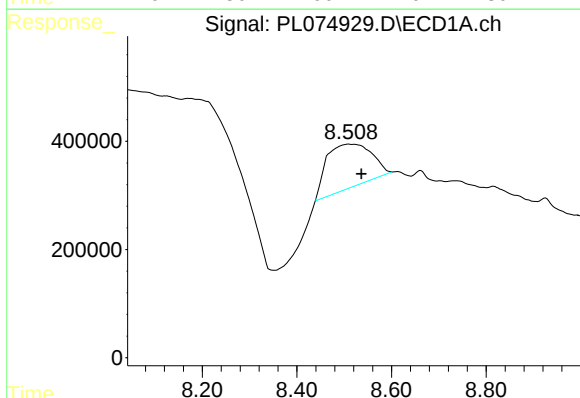


#9 Endosulfan I

R.T.: 8.510 min
Delta R.T.: -0.026 min
Response: 5423580
Conc: 9.41 ng/ml

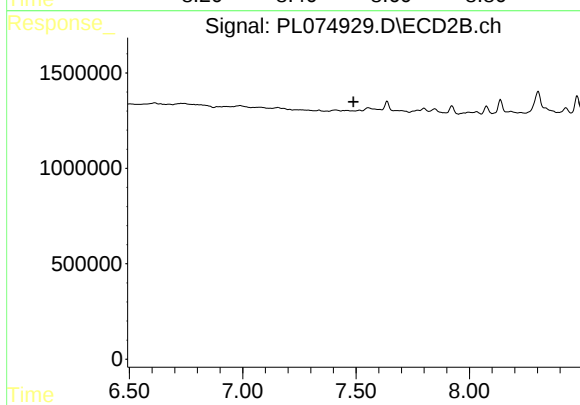

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.489 min
Response: 0
Conc: N.D.

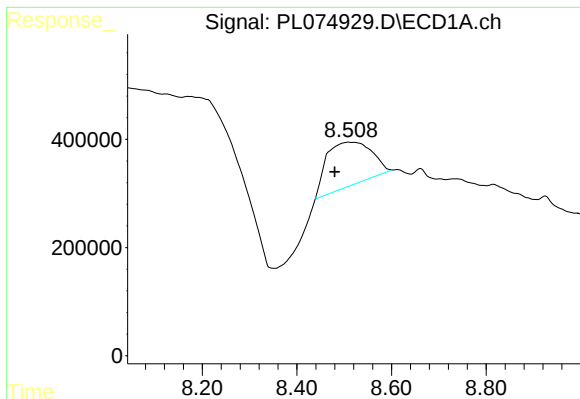

#11 alpha-Chlordane


R.T.: 8.510 min
Delta R.T.: 0.030 min
Response: 5423580
Conc: 8.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

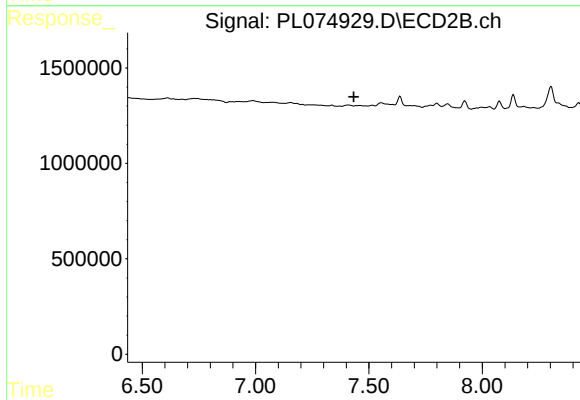


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.433 min
Response: 0
Conc: N.D.

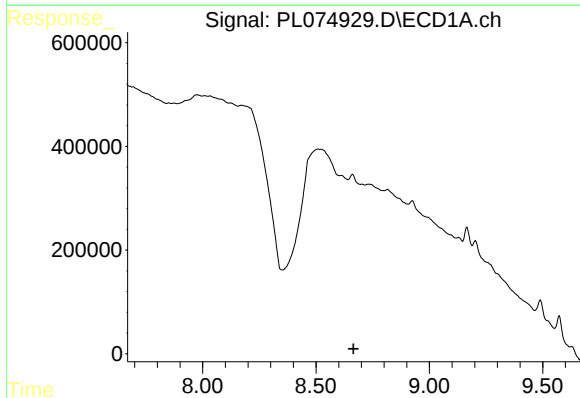


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 8.665 min
Response: 0
Conc: N.D.

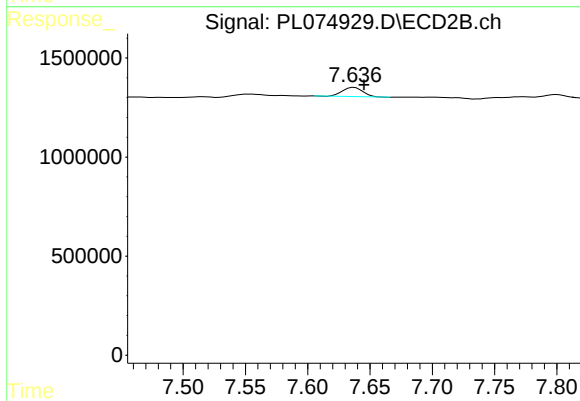

#12 4,4'-DDE


R.T.: 7.637 min
Delta R.T.: -0.008 min
Response: 537832
Conc: 0.46 ng/ml

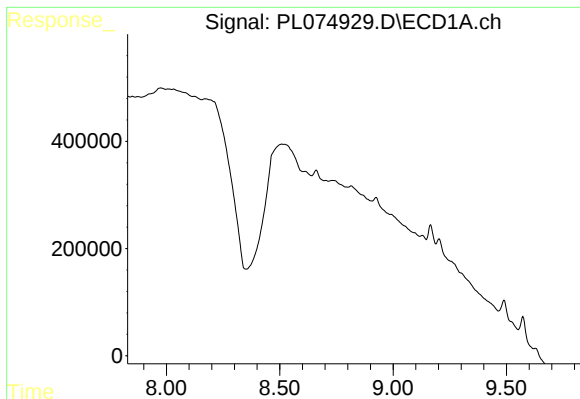

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

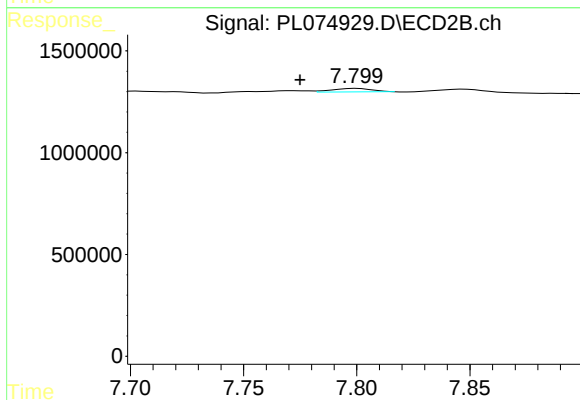


#13 Dieldrin

R.T.: 7.800 min
Delta R.T.: 0.025 min
Response: 206530
Conc: 0.16 ng/ml

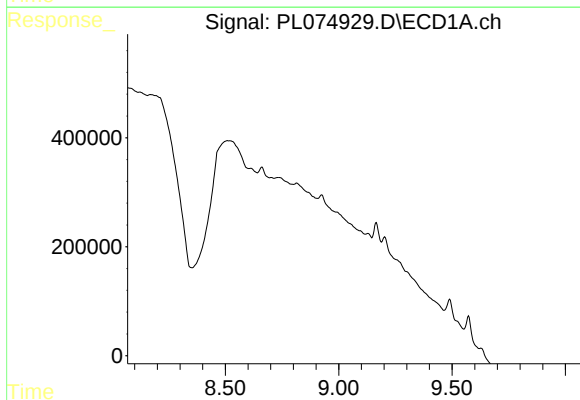


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.068 min
Response: 0
Conc: N.D.

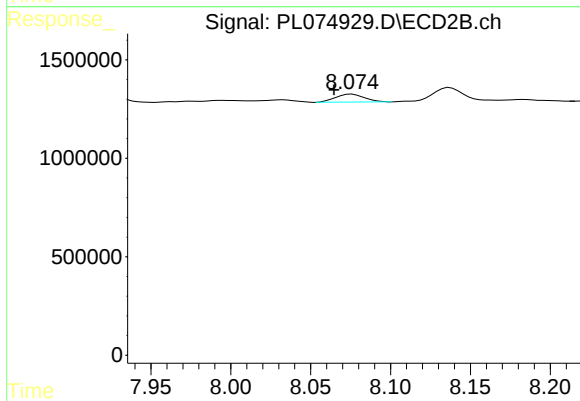

#14 Endrin


R.T.: 8.076 min
Delta R.T.: 0.011 min
Response: 510334
Conc: 0.48 ng/ml

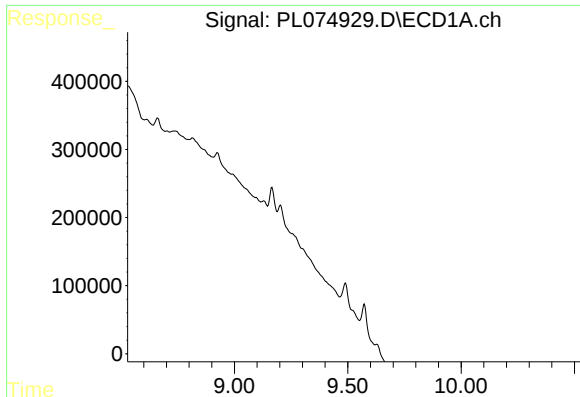

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

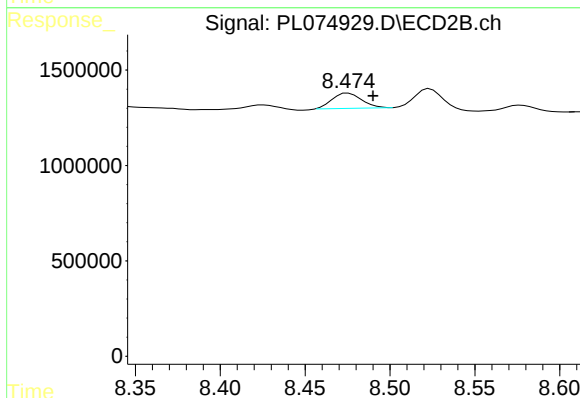


#17 4,4'-DDT

R.T.: 8.475 min
Delta R.T.: -0.015 min
Response: 972120
Conc: 0.97 ng/ml

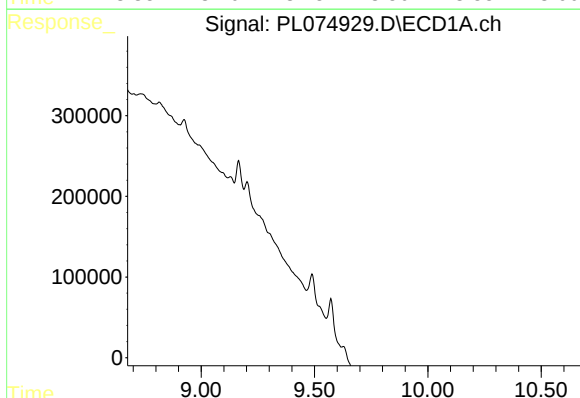


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 9.675 min
Response: 0
Conc: N.D.

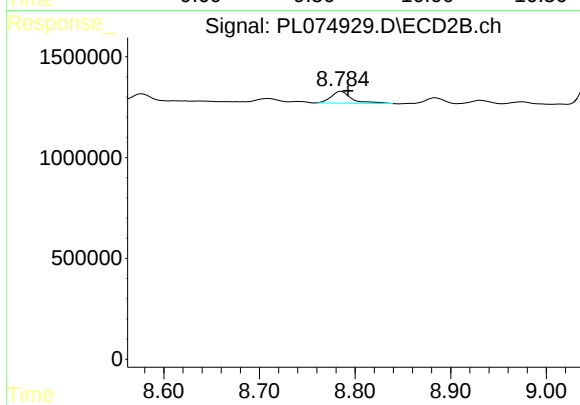

#19 Endosulfan Sulfate


R.T.: 8.786 min
Delta R.T.: -0.007 min
Response: 865375
Conc: 0.79 ng/ml

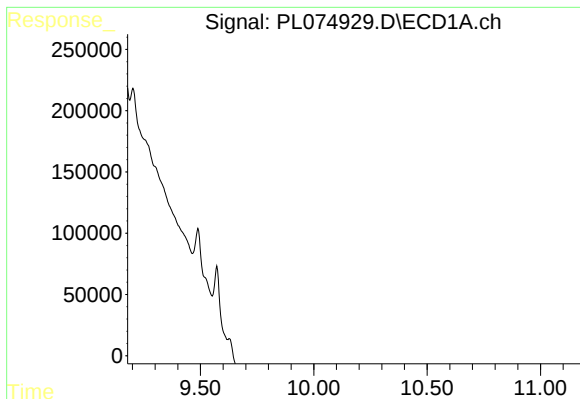

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 10.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

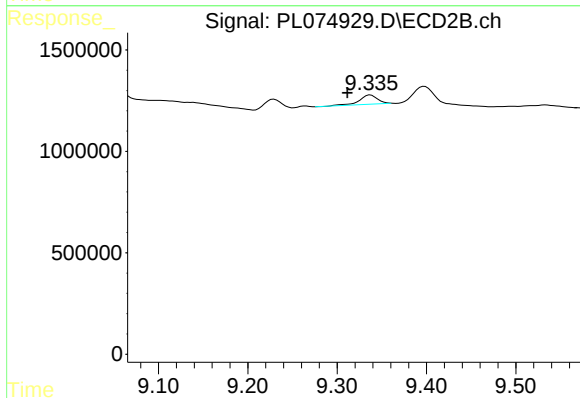


#21 Endrin ketone

R.T.: 9.337 min
Delta R.T.: 0.026 min
Response: 659087
Conc: 0.59 ng/ml

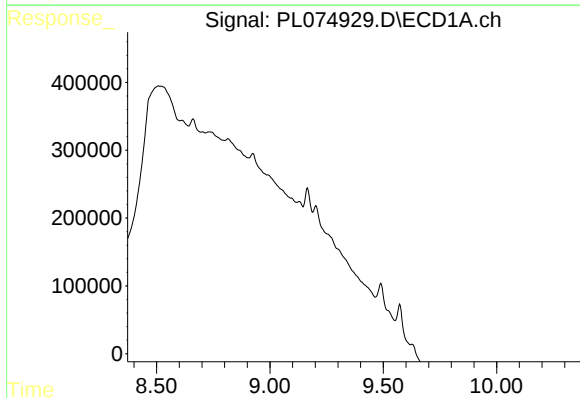


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

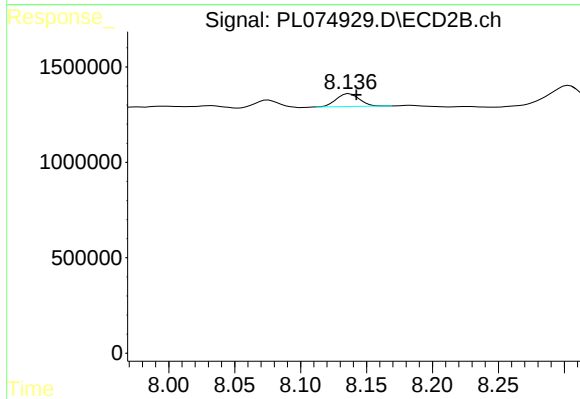

#27 Chlordane-5


R.T.: 8.137 min
Delta R.T.: -0.005 min
Response: 820317
Conc: 22.19 ng/ml

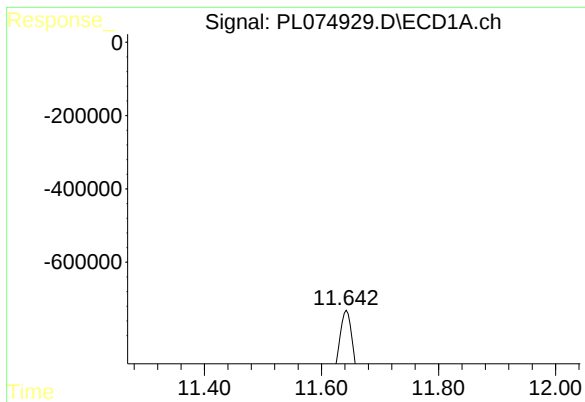

#28 Decachlorobiphenyl

R.T.: 11.643 min
Delta R.T.: -0.008 min
Response: 4878656
Conc: 10.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

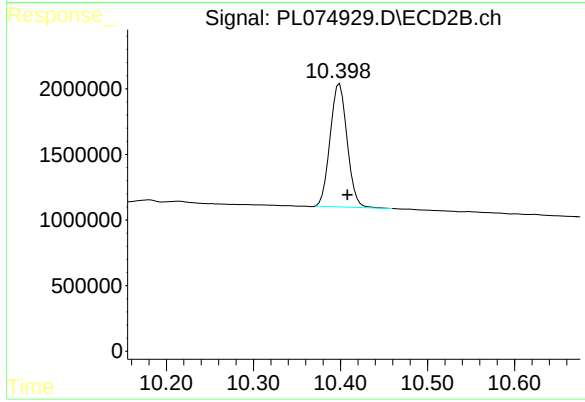

#28 Decachlorobiphenyl

R.T.: 10.399 min
Delta R.T.: -0.009 min
Response: 12722630
Conc: 12.40 ng/ml