

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052122\
 Data File : PL074935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2022 05:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 13:56:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.650	10999201	29732046	21.663	21.662
28)	SA Decachlor...	11.644	10.400	10850867	27782563	24.297	27.068
Target Compounds							
7)	B delta-BHC	0.000	6.426	0	90005	N.D.	0.058 #
8)	B Heptachlo...	8.128	0.000	5917109	0	10.404	N.D. #
9)	A Endosulfan I	8.508f	7.514f	5278097	159346	9.155	0.127 #
11)	B alpha-Chl...	8.508f	7.412f	5278097	592696	8.646	0.438 #
13)	MA Dieldrin	0.000	7.771	0	4306293	N.D.	3.380 #
14)	MA Endrin	0.000	8.081f	0	2558508	N.D.	2.422 #
15)	B Endosulfa...	0.000	8.373	0	168608	N.D.	0.149 #
26)	Chlordane-4	8.508f	7.412f	5278097	592696	54.786	4.323 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052122\
Data File : PL074935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2022 05:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 13:56:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

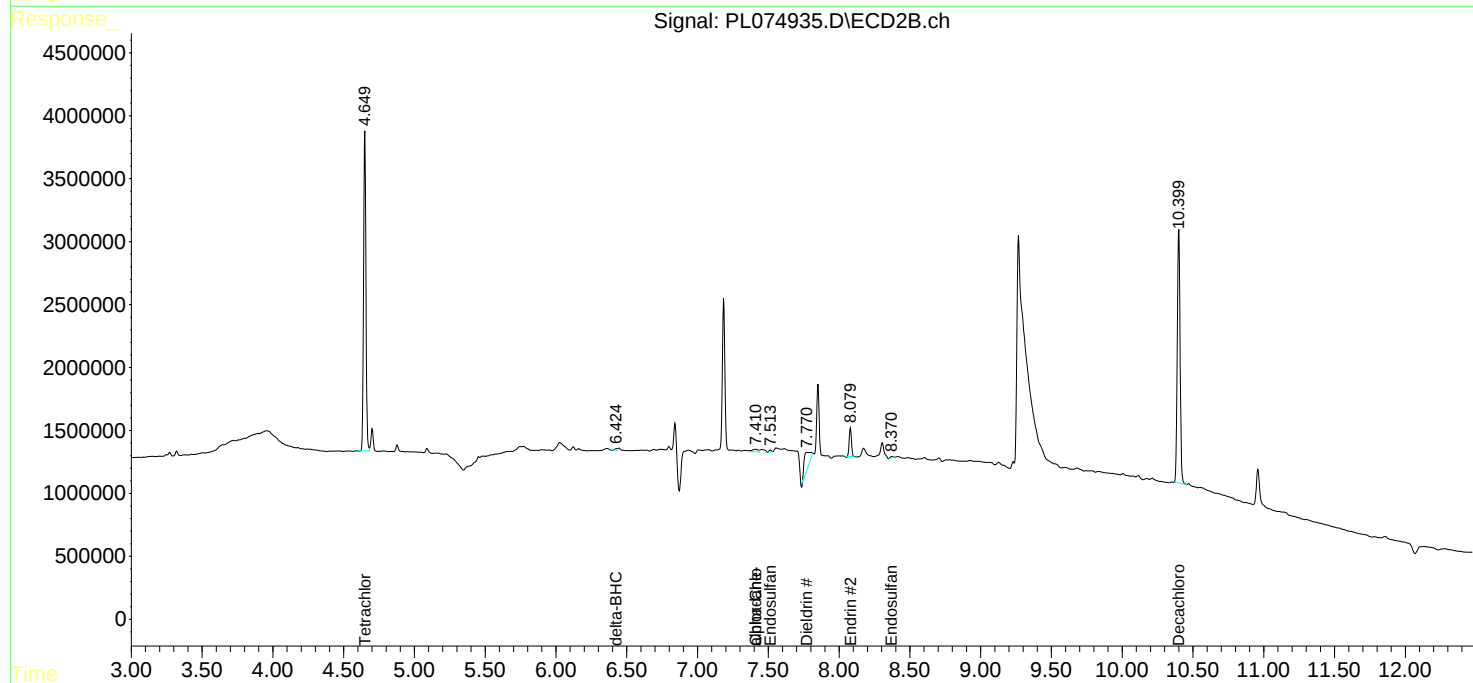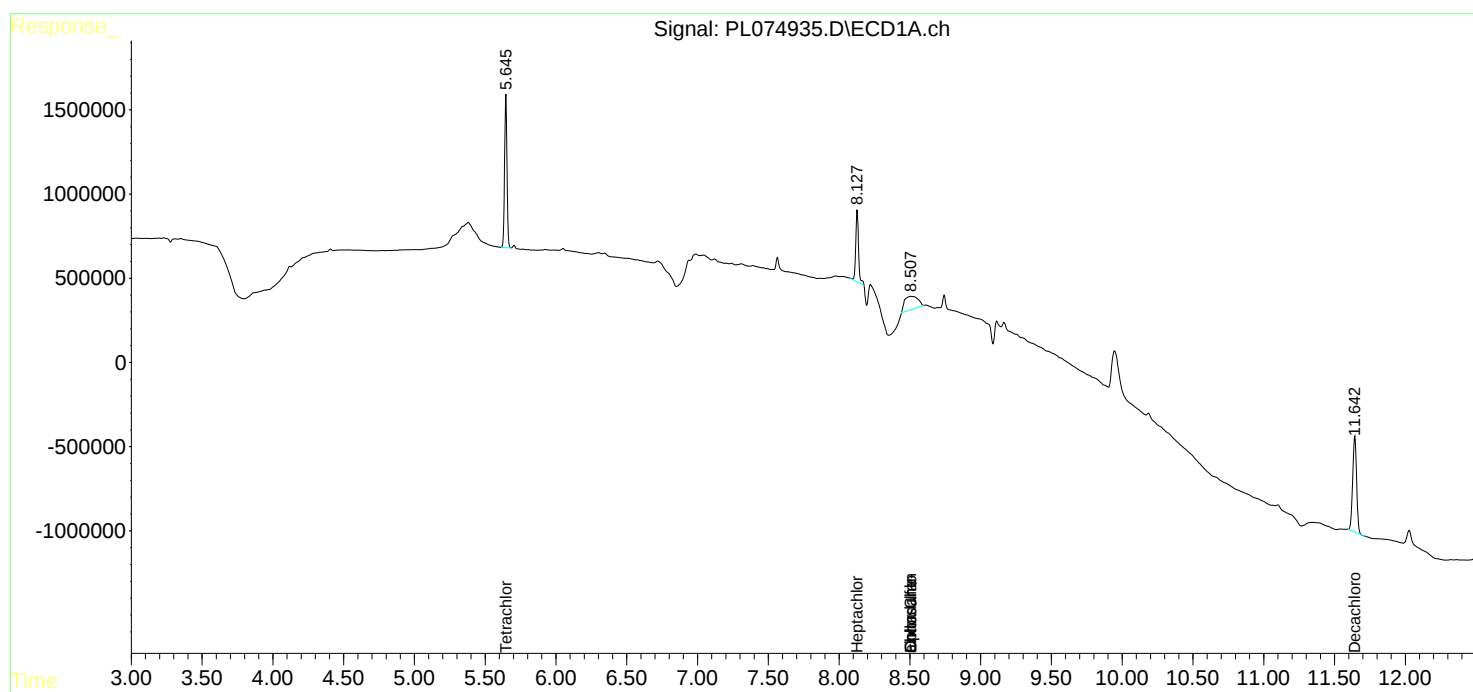


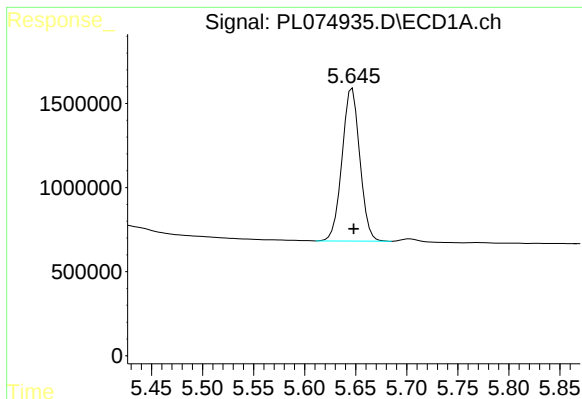

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: -0.001 min
Response: 10999201
Conc: 21.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

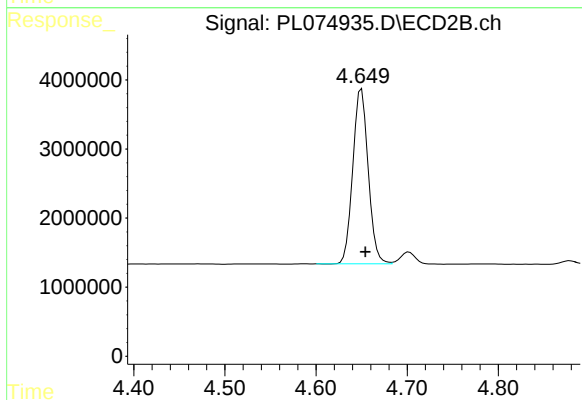


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 29732046
Conc: 21.66 ng/ml

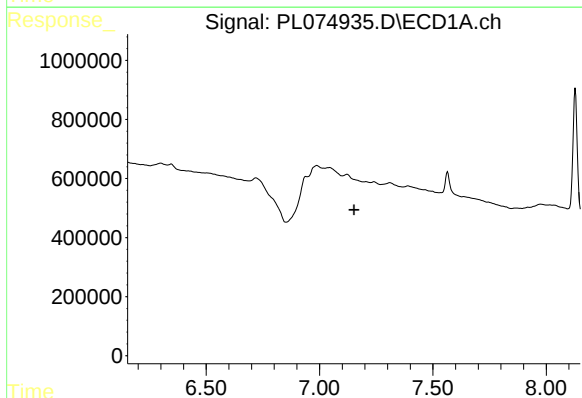


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.152 min
Response: 0
Conc: N.D.

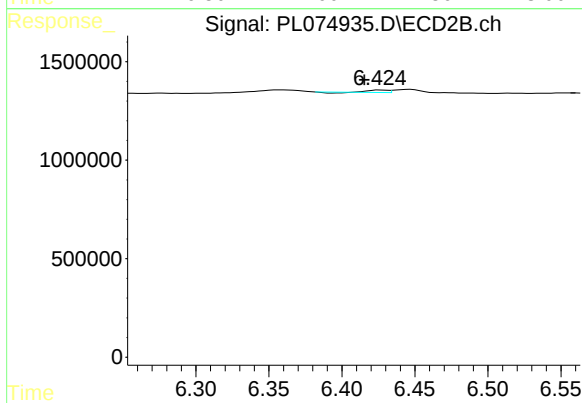

#7 delta-BHC


R.T.: 6.426 min
Delta R.T.: 0.011 min
Response: 90005
Conc: 0.06 ng/ml

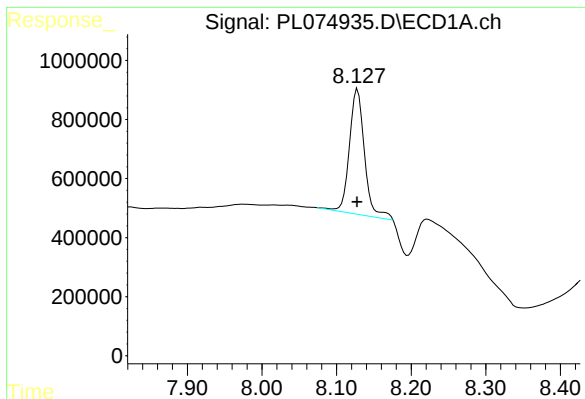

#8 Heptachlor epoxide


R.T.: 8.128 min
Delta R.T.: 0.000 min
Response: 5917109
Conc: 10.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

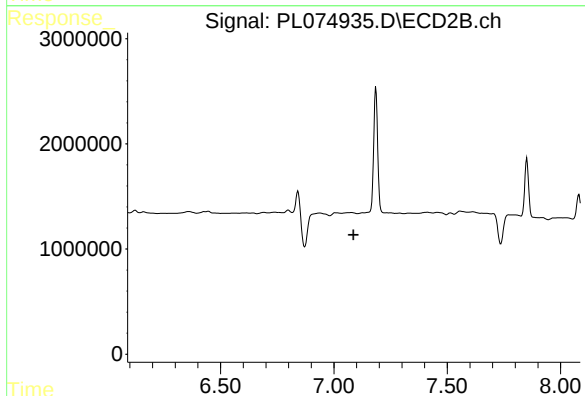


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.087 min
Response: 0
Conc: N.D.

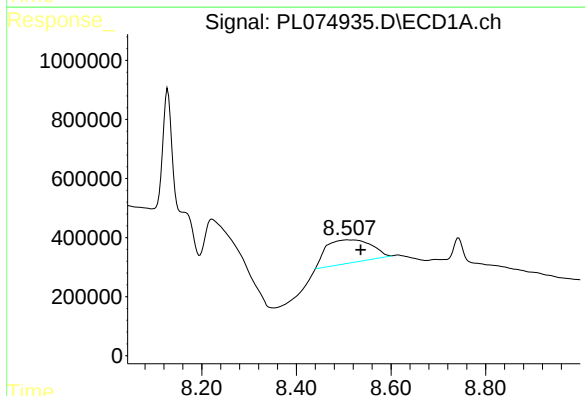


#9 Endosulfan I

R.T.: 8.508 min
Delta R.T.: -0.028 min
Response: 5278097
Conc: 9.16 ng/ml

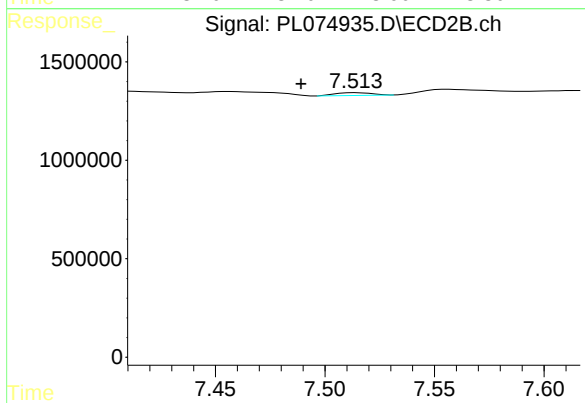

#9 Endosulfan I


R.T.: 7.514 min
Delta R.T.: 0.025 min
Response: 159346
Conc: 0.13 ng/ml

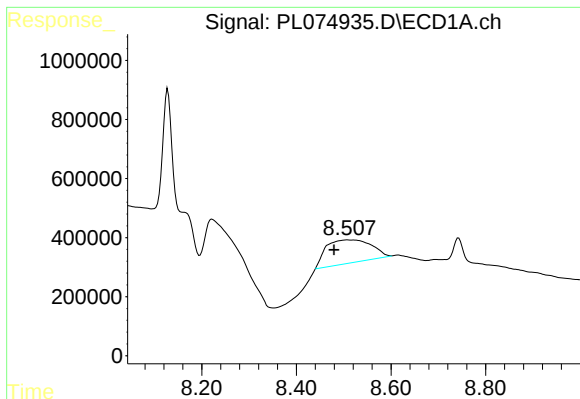

#11 alpha-Chlordane


R.T.: 8.508 min
Delta R.T.: 0.028 min
Response: 5278097
Conc: 8.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

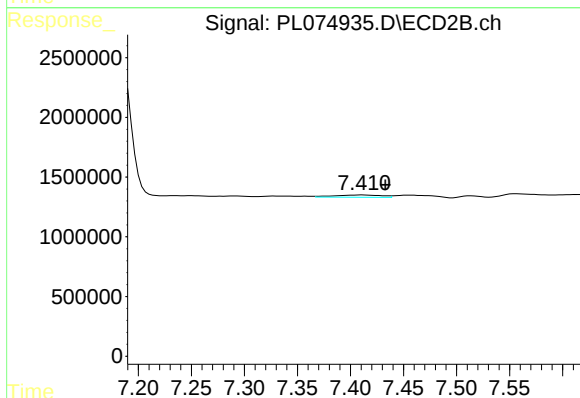


#11 alpha-Chlordane

R.T.: 7.412 min
Delta R.T.: -0.021 min
Response: 592696
Conc: 0.44 ng/ml

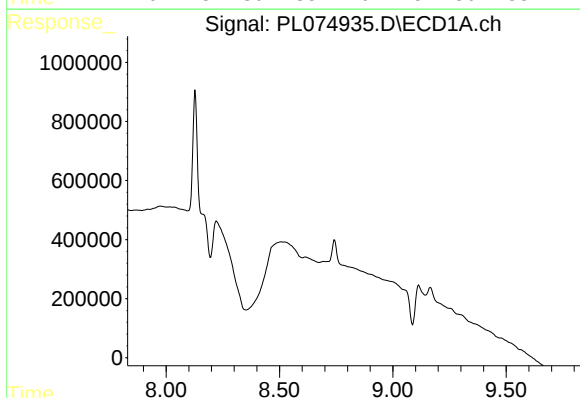


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.827 min
Response: 0
Conc: N.D.

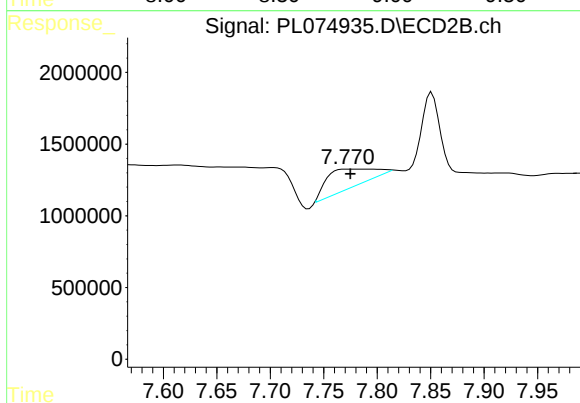

#13 Dieldrin


R.T.: 7.771 min
Delta R.T.: -0.003 min
Response: 4306293
Conc: 3.38 ng/ml

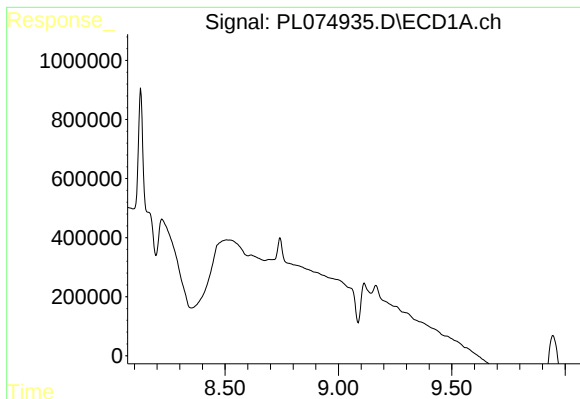

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

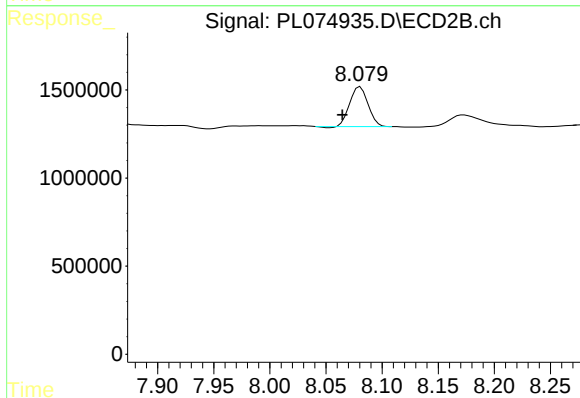


#14 Endrin

R.T.: 8.081 min
Delta R.T.: 0.016 min
Response: 2558508
Conc: 2.42 ng/ml

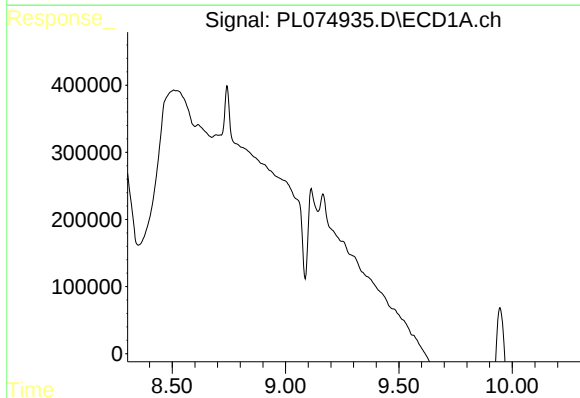


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 9.302 min
Response: 0
Conc: N.D.

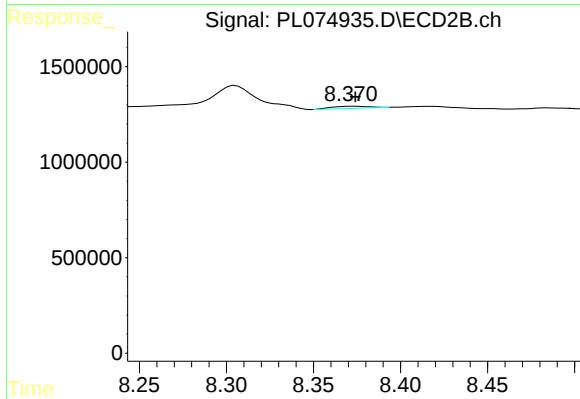

#15 Endosulfan II


R.T.: 8.373 min
Delta R.T.: -0.001 min
Response: 168608
Conc: 0.15 ng/ml

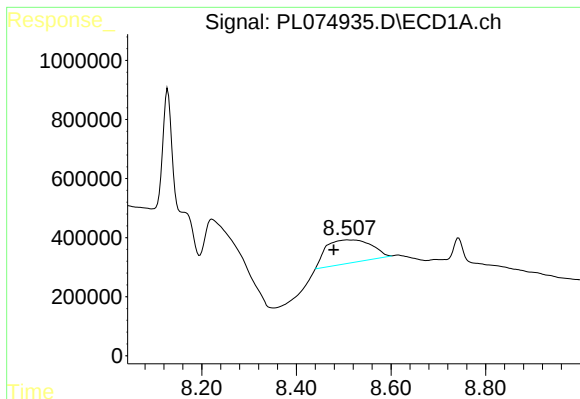

#26 Chlordane-4


R.T.: 8.508 min
Delta R.T.: 0.029 min
Response: 5278097
Conc: 54.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

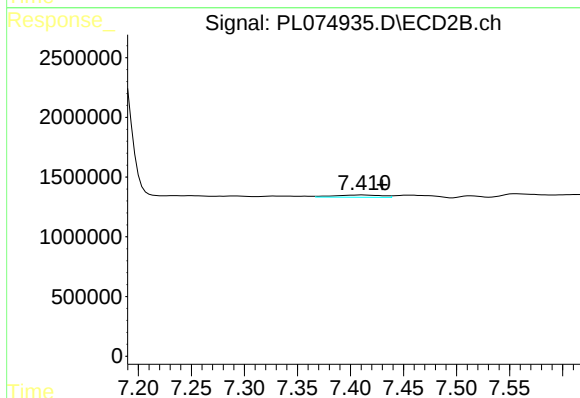


#26 Chlordane-4

R.T.: 7.412 min
Delta R.T.: -0.018 min
Response: 592696
Conc: 4.32 ng/ml

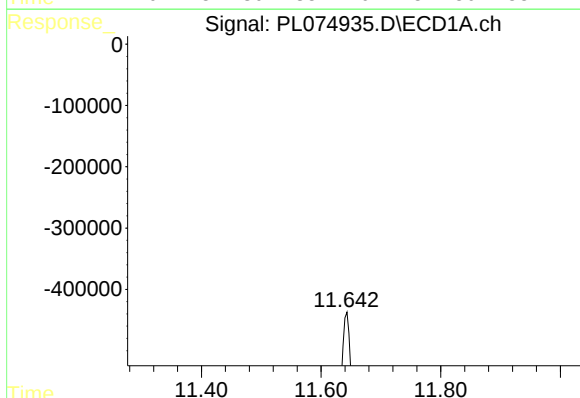

#28 Decachlorobiphenyl

R.T.: 11.644 min
Delta R.T.: -0.007 min
Response: 10850867
Conc: 24.30 ng/ml

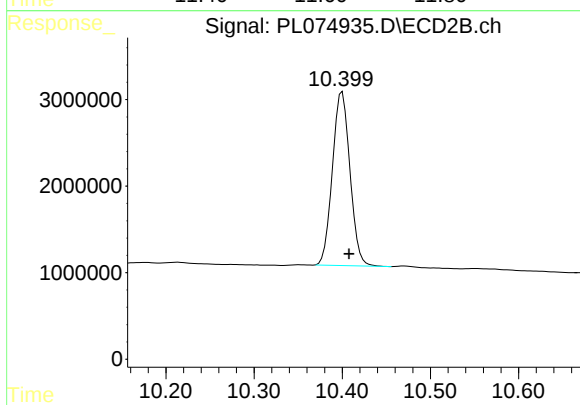

#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.008 min
Response: 27782563
Conc: 27.07 ng/ml