

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052122\
 Data File : PL074932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2022 04:19
 Operator : AR\AJ
 Sample : N2874-21
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P007-SS005-0006-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 13:55:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.646	4.650	3179484	9297913	6.262	6.774
28) SA Decachlor...	11.643	10.399	6500027	16956656	14.555	16.520

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052122\
Data File : PL074932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2022 04:19
Operator : AR\AJ
Sample : N2874-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
P007-SS005-0006-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 13:55:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

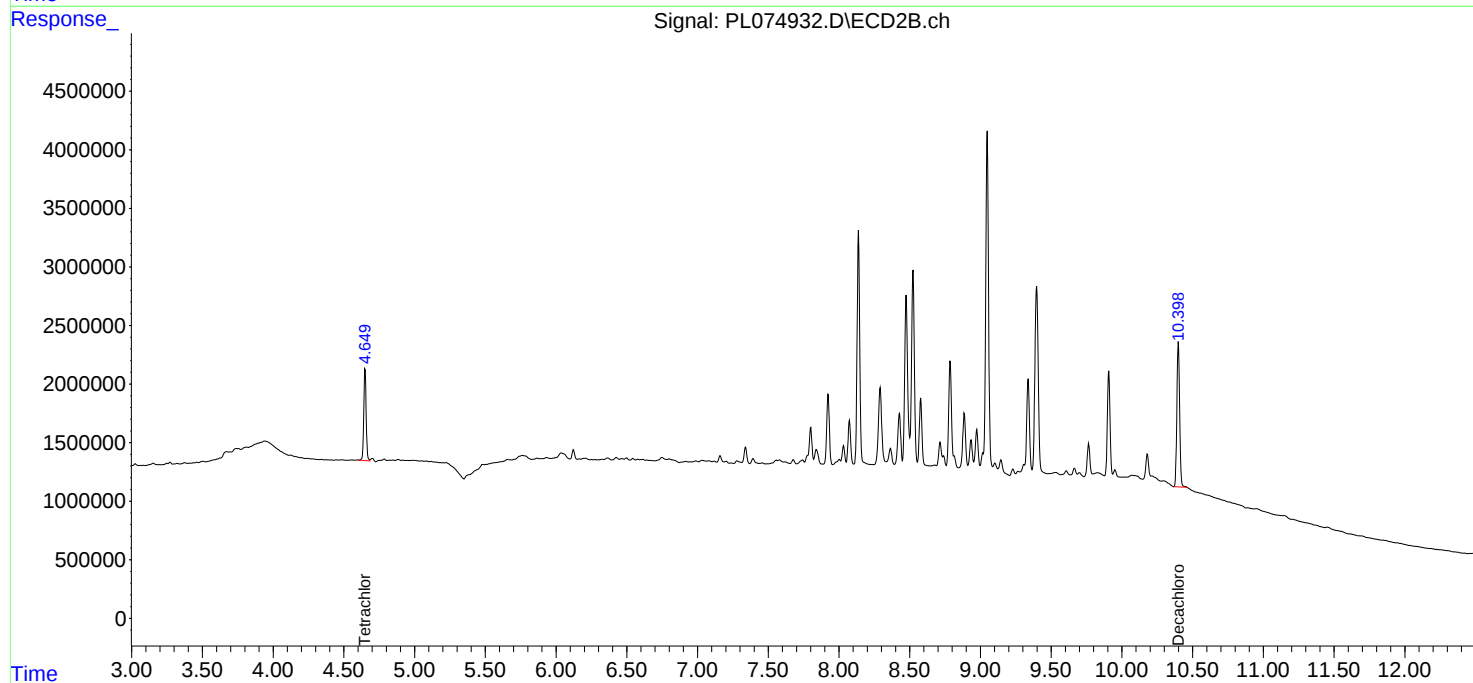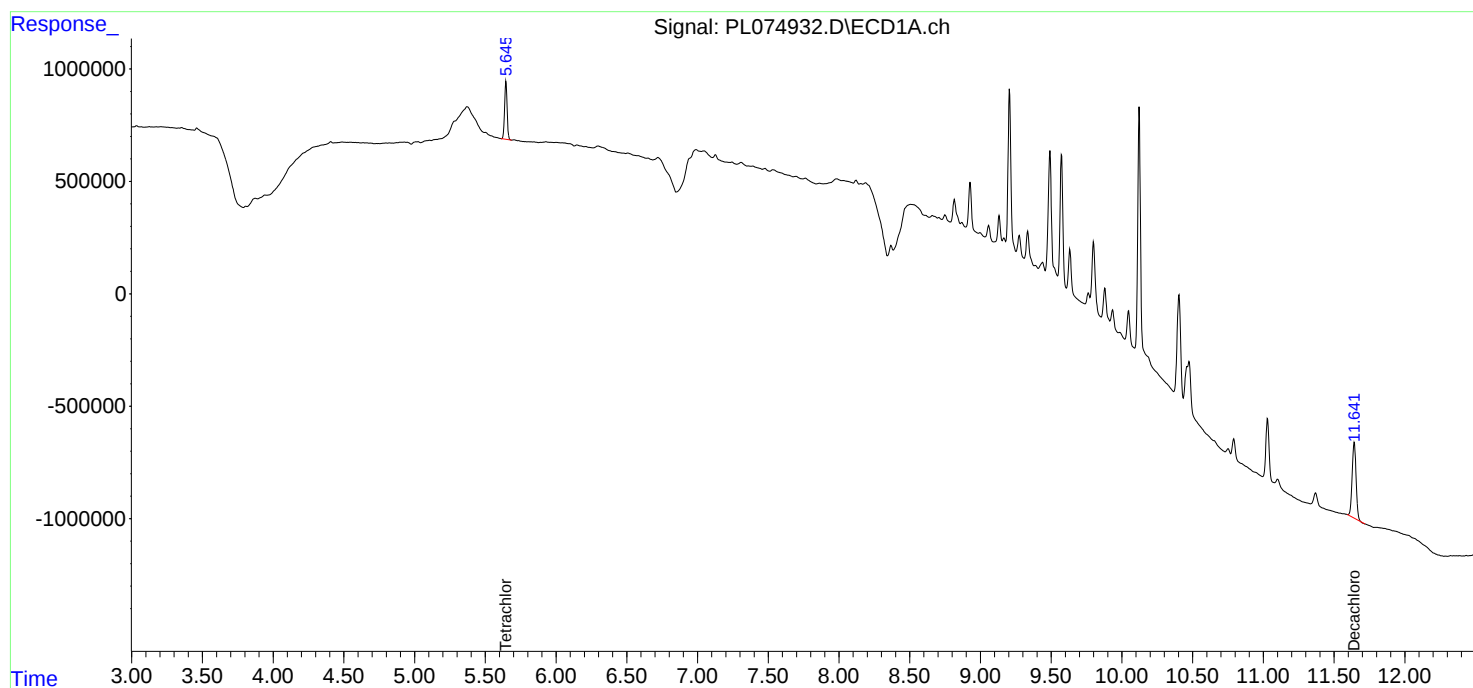


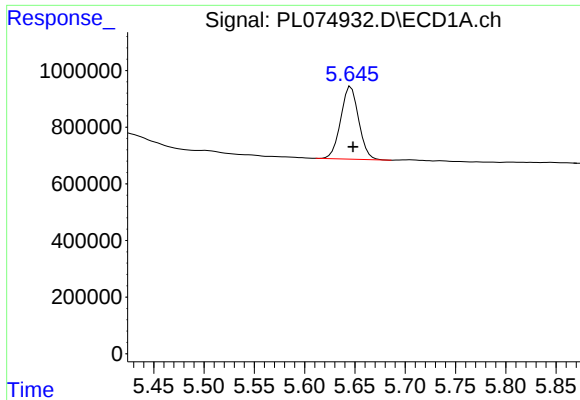

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 3179484
Conc: 6.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
P007-SS005-0006-01

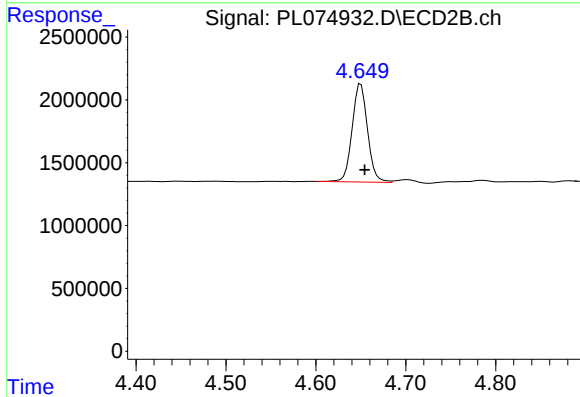


#1 Tetrachloro-m-xylene

R.T.: 4.650 min
Delta R.T.: -0.004 min
Response: 9297913
Conc: 6.77 ng/ml

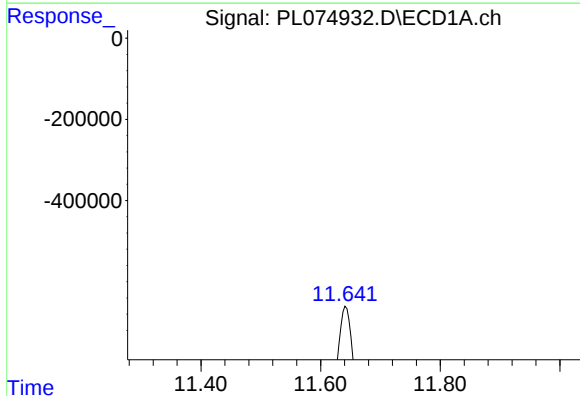

#28 Decachlorobiphenyl

R.T.: 11.643 min
Delta R.T.: -0.008 min
Response: 6500027
Conc: 14.55 ng/ml

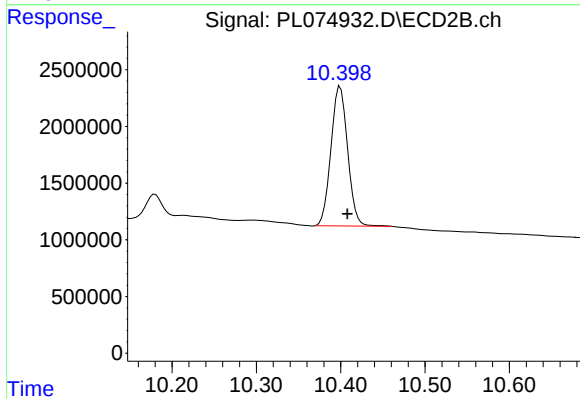

#28 Decachlorobiphenyl

R.T.: 10.399 min
Delta R.T.: -0.008 min
Response: 16956656
Conc: 16.52 ng/ml