

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052125\
 Data File : PL095742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2025 13:10
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 05:53:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 05:52:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.573	2.885	151.3E6	249.3E6	50.000	50.000
28)	SA Decachlor...	9.104	8.063	112.9E6	221.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.739	3.906	87581330	95105811	500.000	500.000
24)	Chlordane-2	5.267	4.487	93352484	108.4E6	500.000	500.000
25)	Chlordane-3	5.973	5.123	364.7E6	326.3E6	500.000	500.000
26)	Chlordane-4	6.058	5.187	443.9E6	282.5E6	500.000	500.000
27)	Chlordane-5	6.899	6.082	66738900	124.7E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052125\
Data File : PL095742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2025 13:10
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 05:53:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 05:52:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

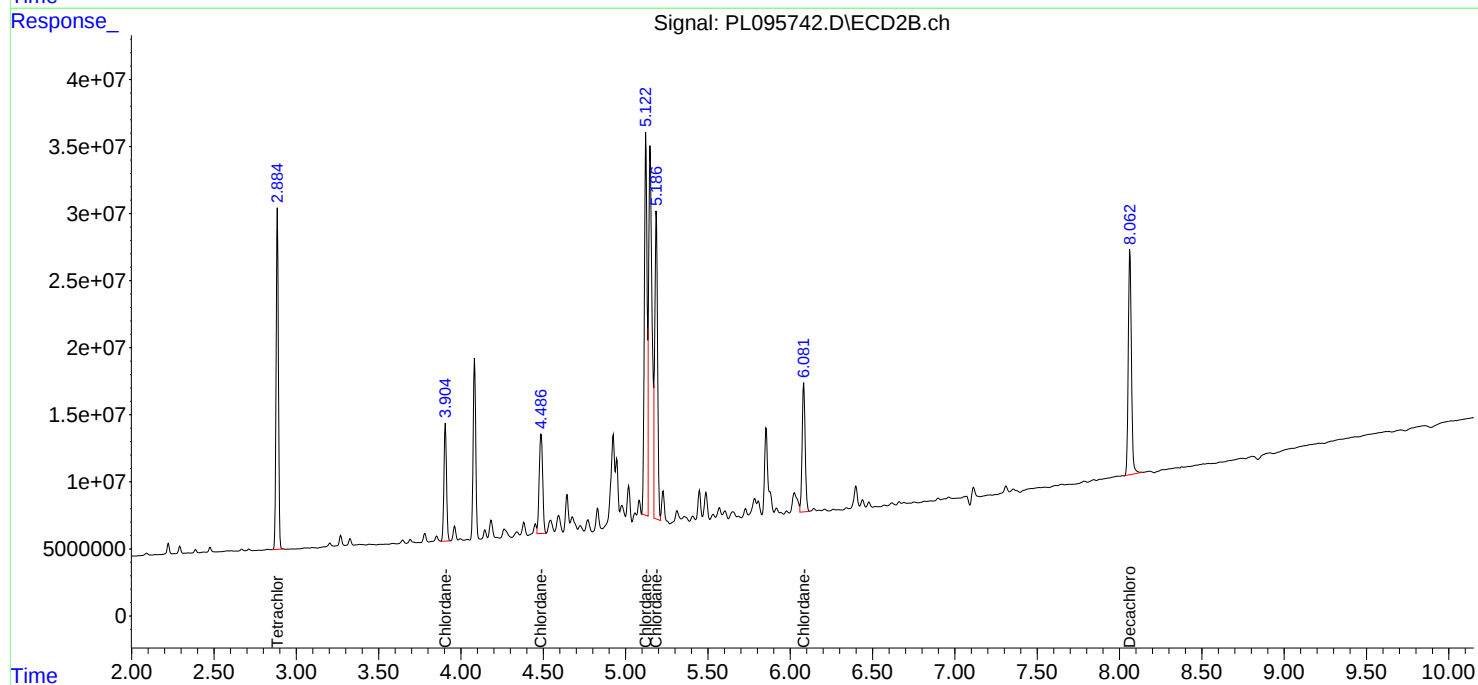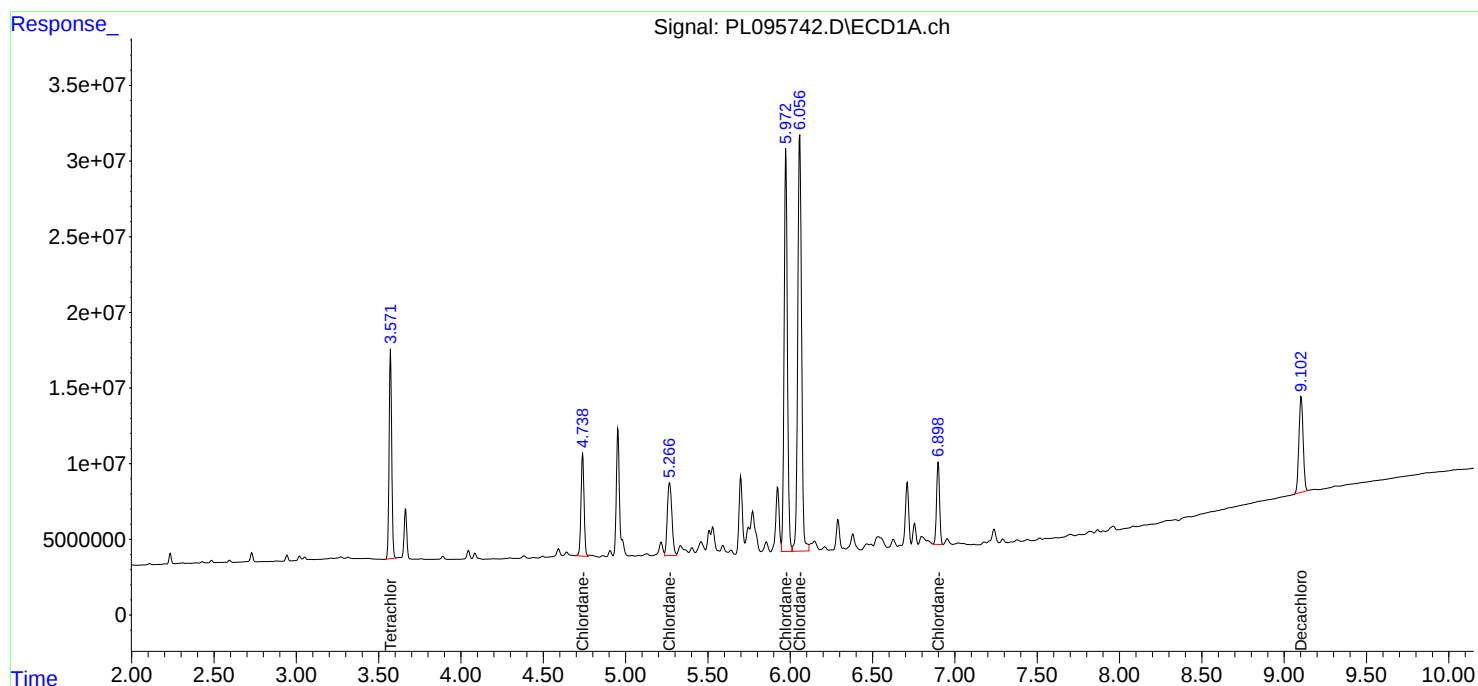


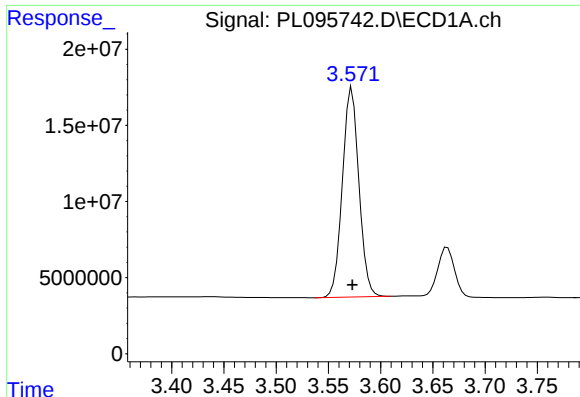

#1 Tetrachloro-m-xylene


R.T.: 3.573 min
Delta R.T.: 0.000 min
Response: 151287484
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

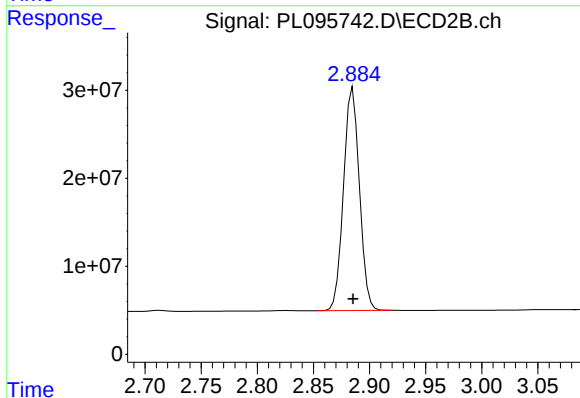


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.000 min
Response: 249308265
Conc: 50.00 ng/ml

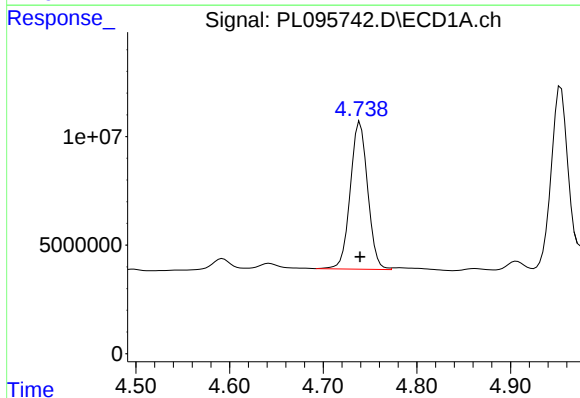


#23 Chlordane-1

R.T.: 4.739 min
Delta R.T.: 0.000 min
Response: 87581330
Conc: 500.00 ng/ml

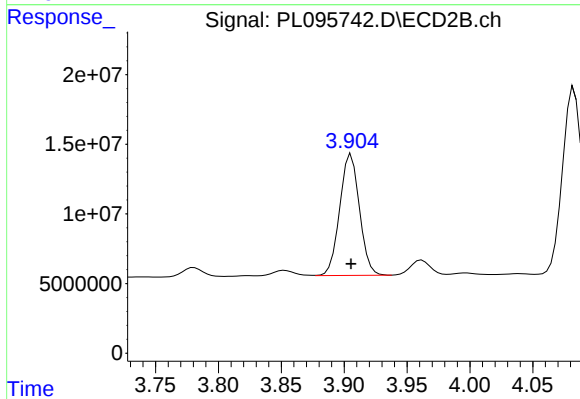

#23 Chlordane-1


R.T.: 3.906 min
Delta R.T.: 0.000 min
Response: 95105811
Conc: 500.00 ng/ml

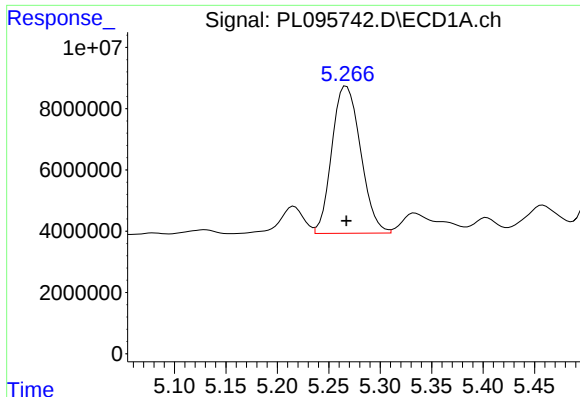

#24 Chlordane-2


R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 93352484
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

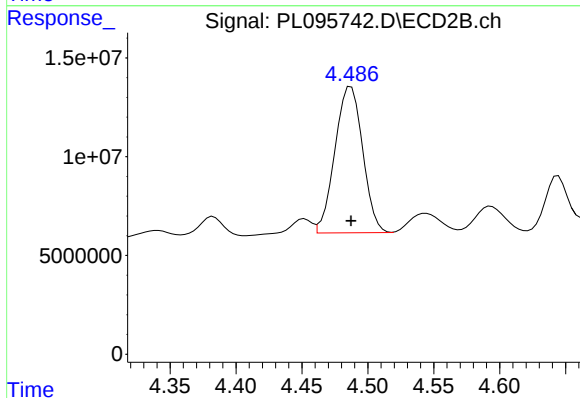


#24 Chlordane-2

R.T.: 4.487 min
Delta R.T.: 0.000 min
Response: 108383676
Conc: 500.00 ng/ml

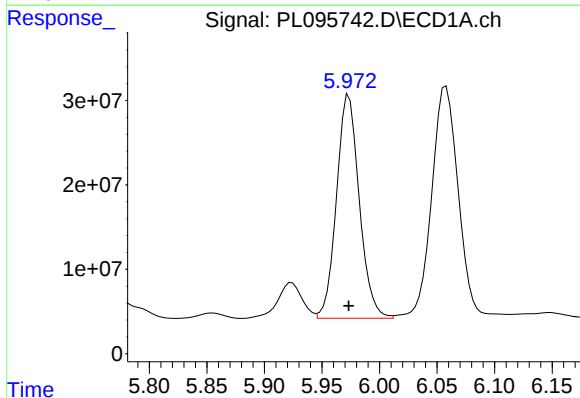


#25 Chlordane-3

R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 364691357
Conc: 500.00 ng/ml

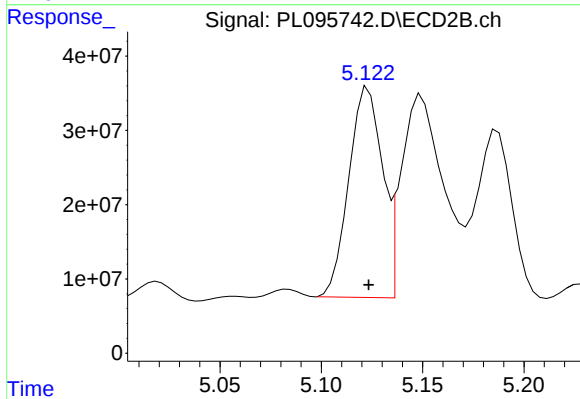

#25 Chlordane-3


R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 326252241
Conc: 500.00 ng/ml

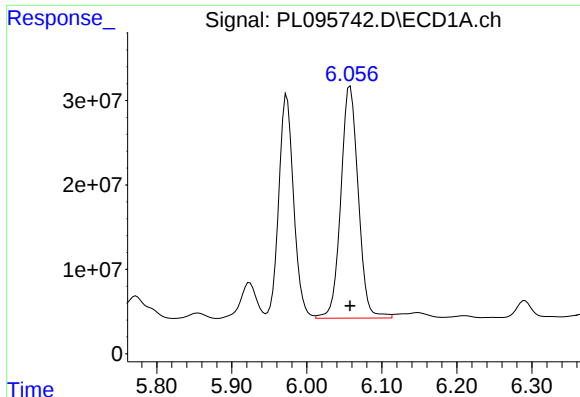

#26 Chlordane-4


R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 443912706
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

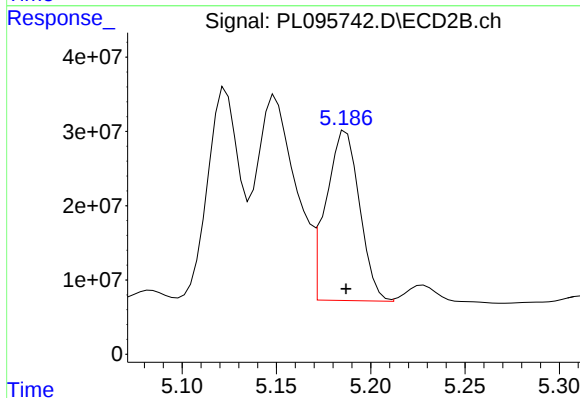


#26 Chlordane-4

R.T.: 5.187 min
Delta R.T.: 0.000 min
Response: 282469516
Conc: 500.00 ng/ml

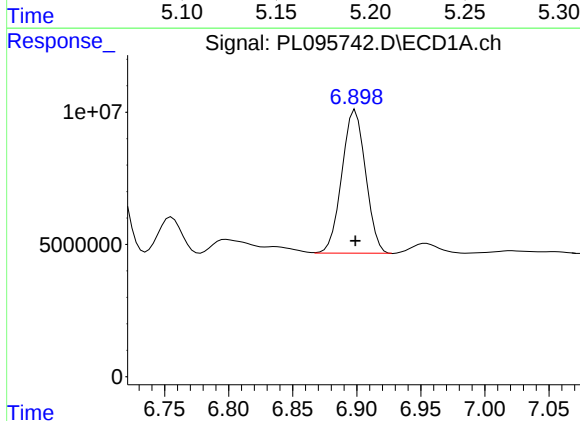


#27 Chlordane-5

R.T.: 6.899 min
Delta R.T.: 0.000 min
Response: 66738900
Conc: 500.00 ng/ml

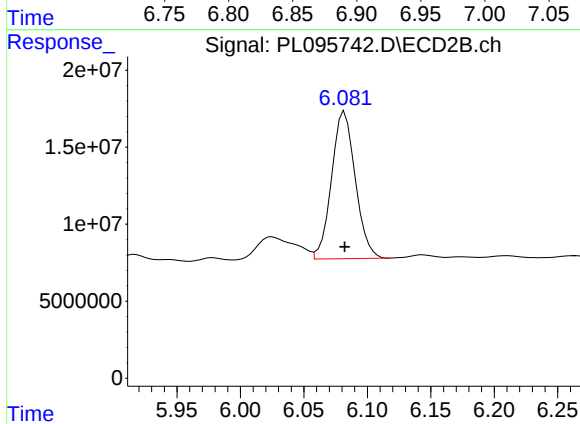

#27 Chlordane-5

R.T.: 6.082 min
Delta R.T.: 0.000 min
Response: 124727963
Conc: 500.00 ng/ml

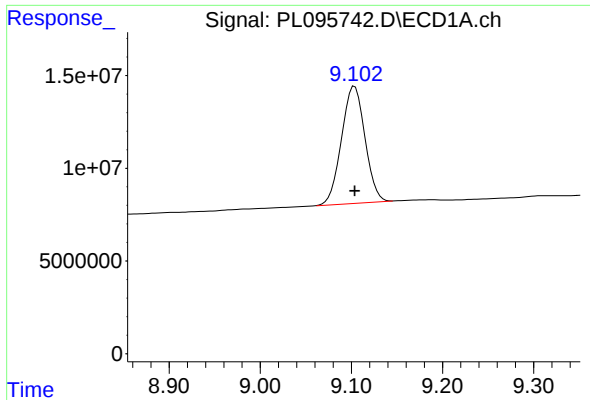

#28 Decachlorobiphenyl


R.T.: 9.104 min

Delta R.T.: 0.000 min

Response: 112917337

Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

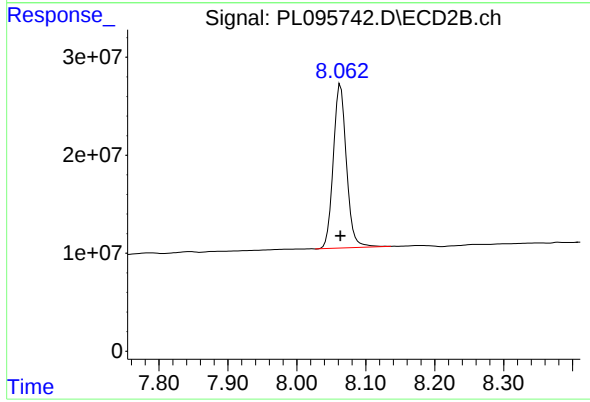

#28 Decachlorobiphenyl

R.T.: 8.063 min

Delta R.T.: 0.000 min

Response: 221461141

Conc: 50.00 ng/ml