

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052125\
 Data File : PL095751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2025 15:12
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL052125CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 05:59:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 05:59:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.573	2.885	156.9E6	252.7E6	50.100	49.840
28)	SA Decachlor...	9.104	8.064	115.9E6	229.0E6	50.010	51.351
Target Compounds							
23)	Chlordane-1	4.740	3.906	88597152	96171041	497.300	493.232
24)	Chlordane-2	5.268	4.488	96121246	109.3E6	500.182	490.592
25)	Chlordane-3	5.974	5.124	377.3E6	331.4E6	510.592	502.970
26)	Chlordane-4	6.059	5.187	457.2E6	287.0E6	508.677	502.673
27)	Chlordane-5	6.900	6.082	69143587	126.8E6	504.904	497.202



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052125\
Data File : PL095751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2025 15:12
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL052125CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 05:59:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 05:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

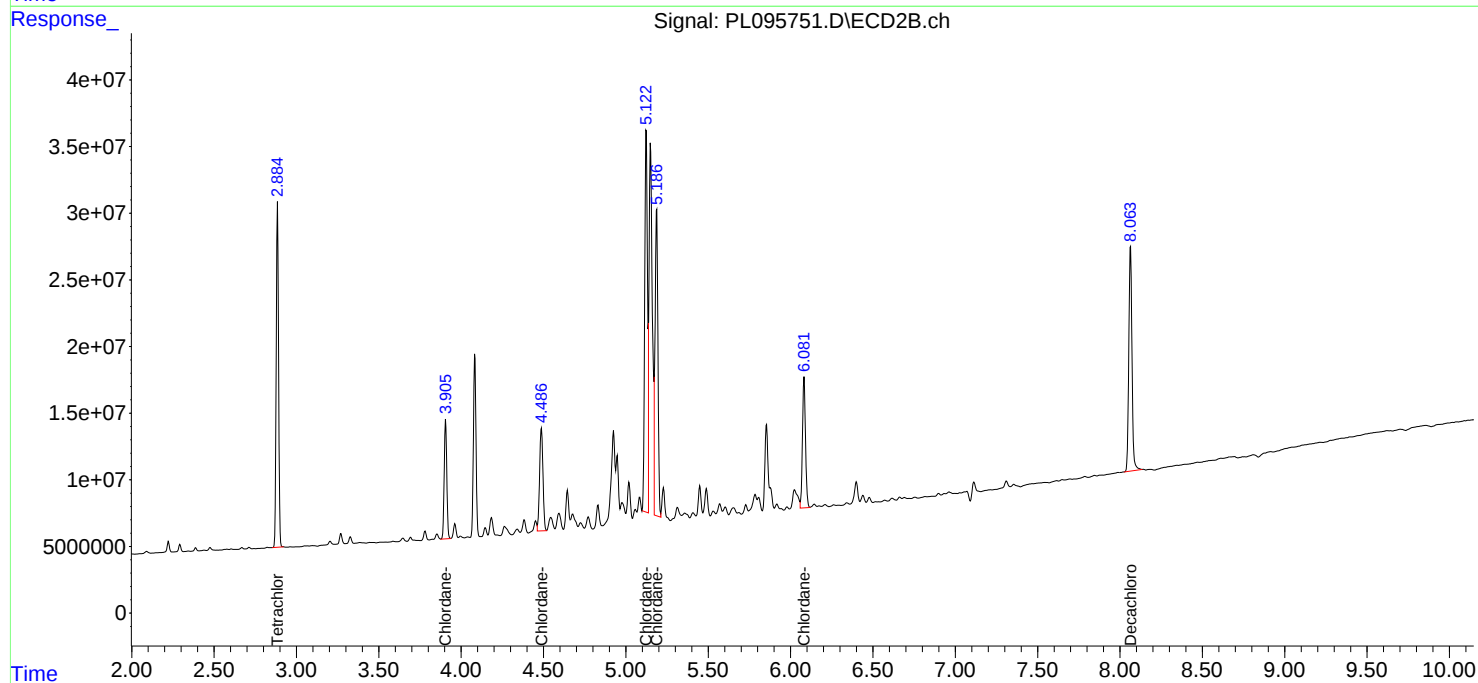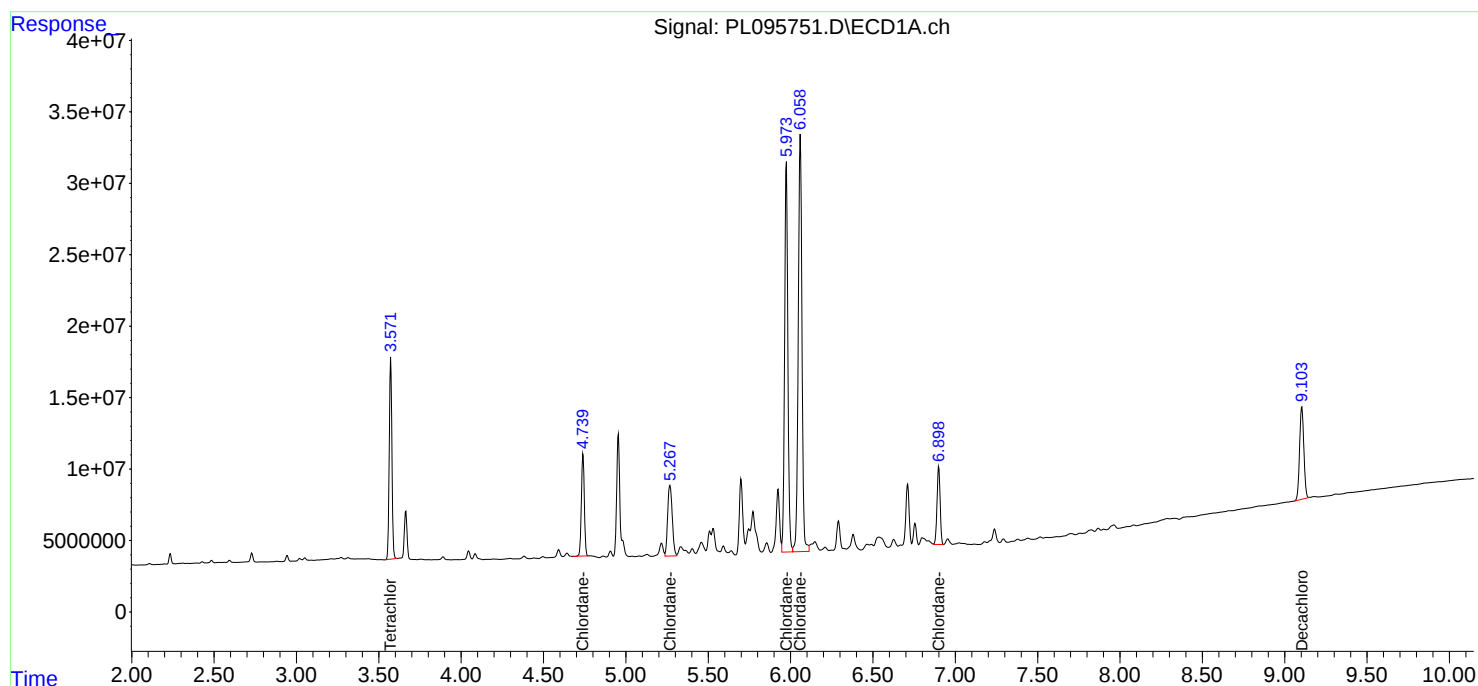


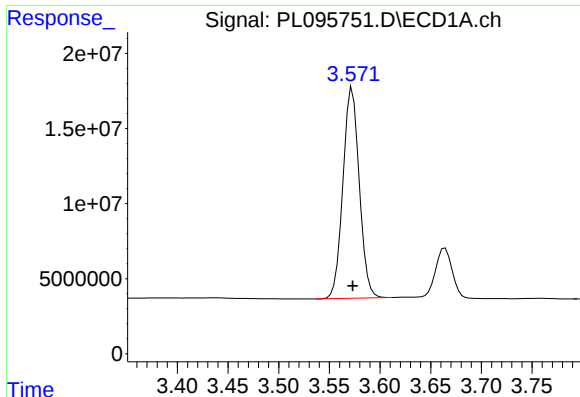

#1 Tetrachloro-m-xylene


R.T.: 3.573 min
Delta R.T.: 0.000 min
Response: 156911848
Conc: 50.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL052125CHLOR

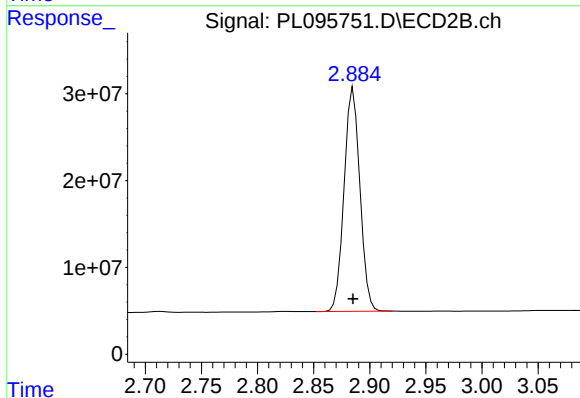


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.000 min
Response: 252709314
Conc: 49.84 ng/ml

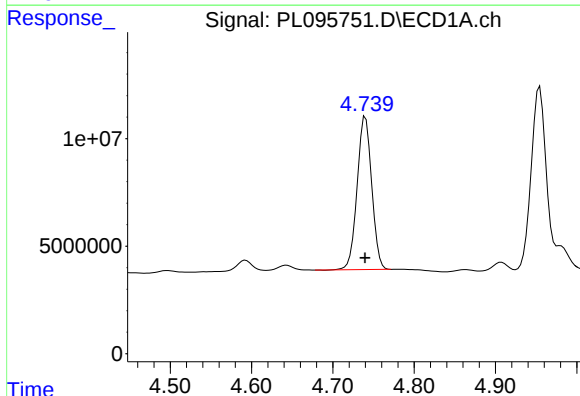


#23 Chlordane-1

R.T.: 4.740 min
Delta R.T.: 0.000 min
Response: 88597152
Conc: 497.30 ng/ml

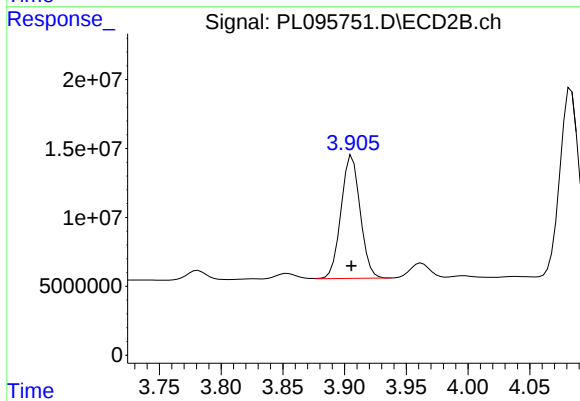

#23 Chlordane-1


R.T.: 3.906 min
Delta R.T.: 0.000 min
Response: 96171041
Conc: 493.23 ng/ml

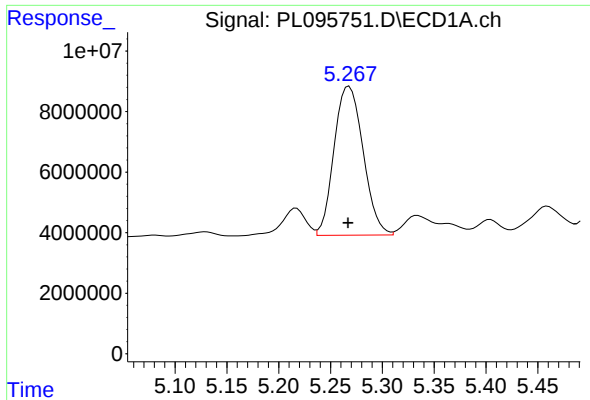

#24 Chlordane-2


R.T.: 5.268 min
Delta R.T.: 0.001 min
Response: 96121246
Conc: 500.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL052125CHLOR

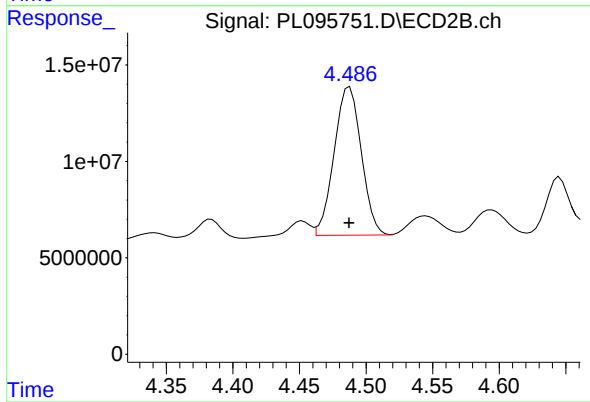


#24 Chlordane-2

R.T.: 4.488 min
Delta R.T.: 0.000 min
Response: 109280725
Conc: 490.59 ng/ml

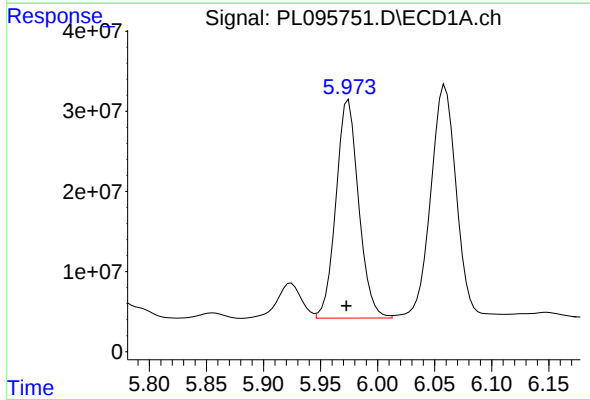


#25 Chlordane-3

R.T.: 5.974 min
Delta R.T.: 0.002 min
Response: 377342003
Conc: 510.59 ng/ml

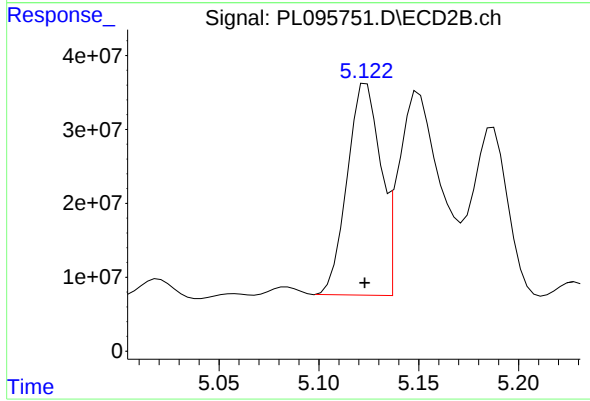

#25 Chlordane-3


R.T.: 5.124 min
Delta R.T.: 0.000 min
Response: 331408650
Conc: 502.97 ng/ml

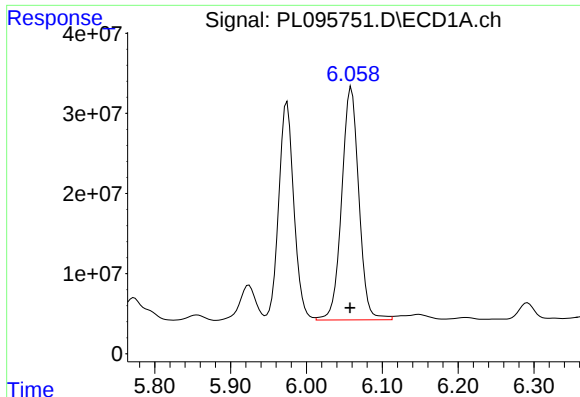

#26 Chlordane-4


R.T.: 6.059 min
Delta R.T.: 0.002 min
Response: 457193182
Conc: 508.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL052125CHLOR

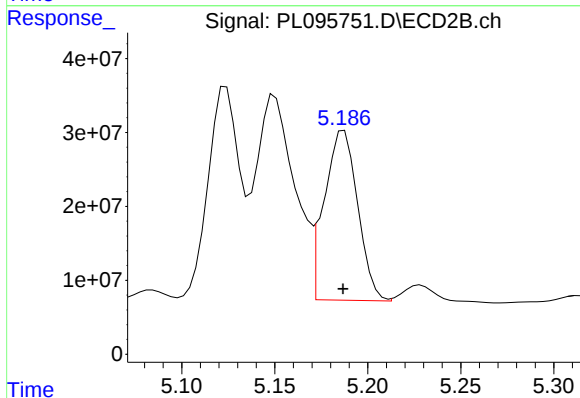


#26 Chlordane-4

R.T.: 5.187 min
Delta R.T.: 0.000 min
Response: 286980441
Conc: 502.67 ng/ml

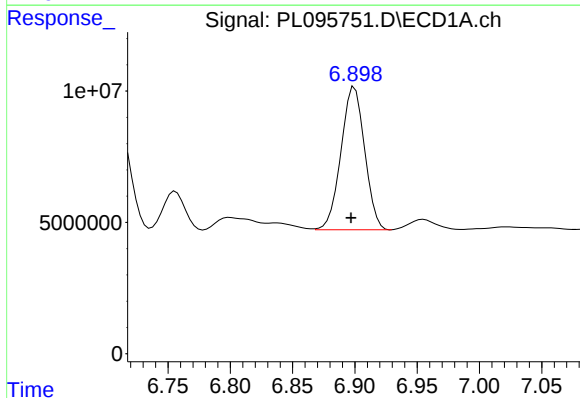


#27 Chlordane-5

R.T.: 6.900 min
Delta R.T.: 0.003 min
Response: 69143587
Conc: 504.90 ng/ml

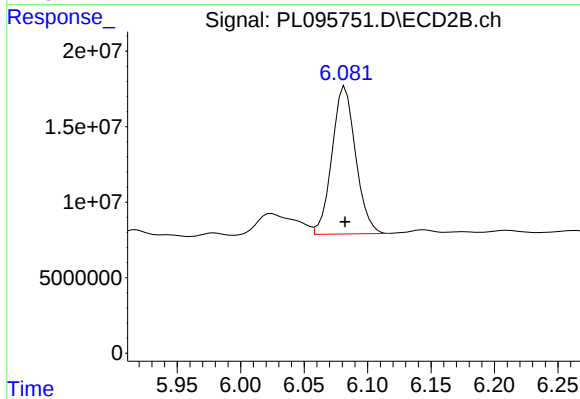

#27 Chlordane-5


R.T.: 6.082 min
Delta R.T.: 0.000 min
Response: 126753637
Conc: 497.20 ng/ml

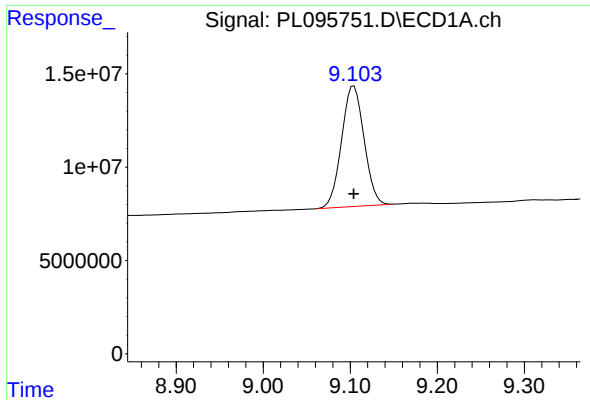

#28 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: 0.000 min
Response: 115945743
Conc: 50.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL052125CHLOR

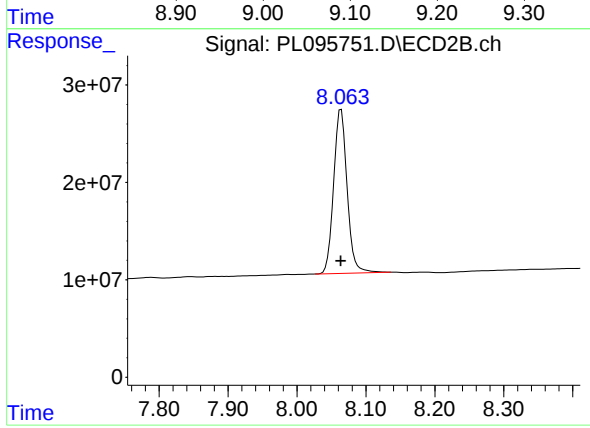

#28 Decachlorobiphenyl

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 229025179
Conc: 51.35 ng/ml