

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052219\
 Data File : PL048826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2019 10:51
 Operator : SM\AJ
 Sample : K2951-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-12-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 01:05:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.326	3.938	88842133	24456273	9.171	9.818
28)	SA Decachlor...	7.992	8.973	121.1E6	36252256	12.048	13.658
Target Compounds							
10)	B gamma-Chl...	5.190f	0.000	4200729	0	0.315	N.D. #
12)	B 4,4'-DDE	0.000	6.265	0	3689421	N.D.	1.336 #
13)	MA Dieldrin	5.559	0.000	14126000	0	1.085	N.D. #
14)	MA Endrin	5.825	6.636	37063053	10081506	3.044	3.866 #
16)	A 4,4'-DDD	0.000	6.761	0	8158061	N.D.	3.635 #
17)	MA 4,4'-DDT	6.176	0.000	17640005	0	1.756	N.D. #
18)	B Endrin al...	6.269	0.000	10352919	0	1.065	N.D. #
19)	B Endosulfa...	6.457	0.000	13702840	0	1.277	N.D. #
20)	A Methoxychlor	6.704f	0.000	43801721	0	8.045	N.D. #
21)	B Endrin ke...	6.974f	0.000	10279549	0	0.882	N.D. #
25)	Chlordane-3	5.190f	0.000	4200729	0	2.668	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052219\
Data File : PL048826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2019 10:51
Operator : SM\AJ
Sample : K2951-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-12-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 01:05:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

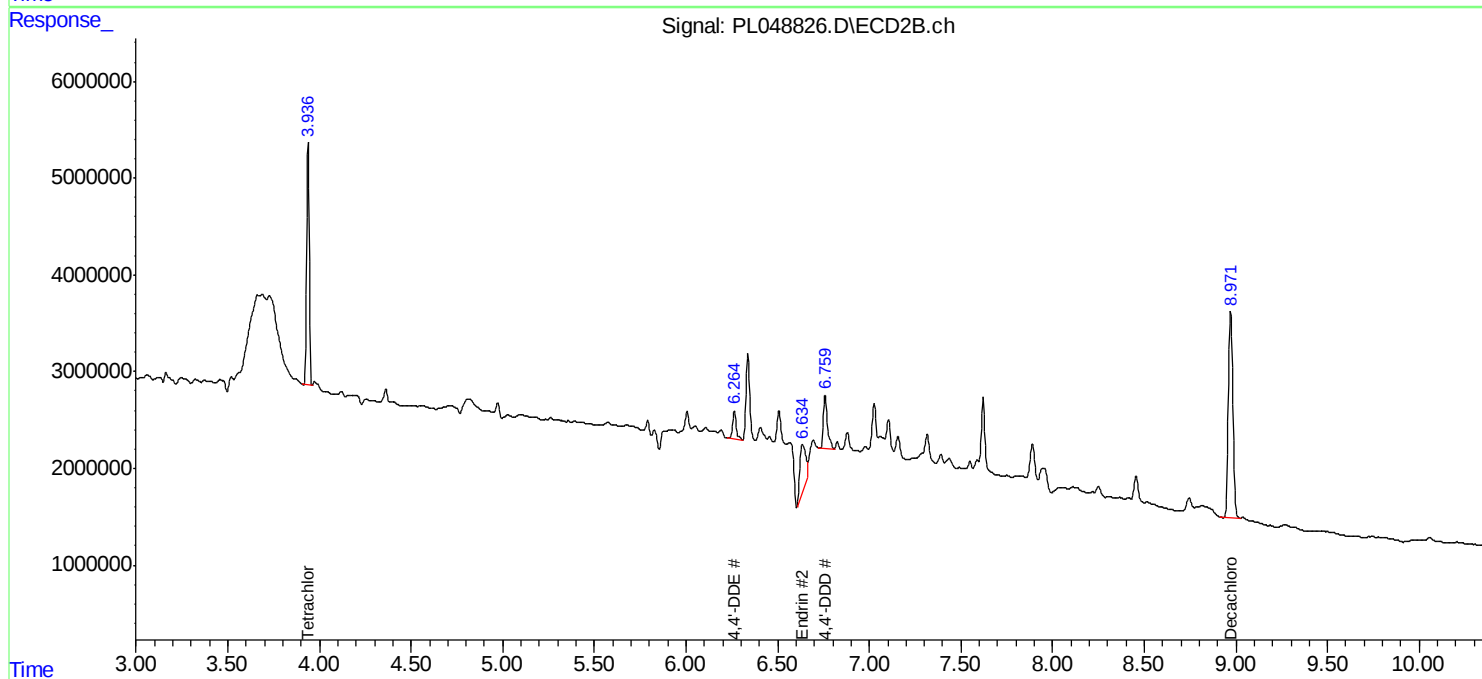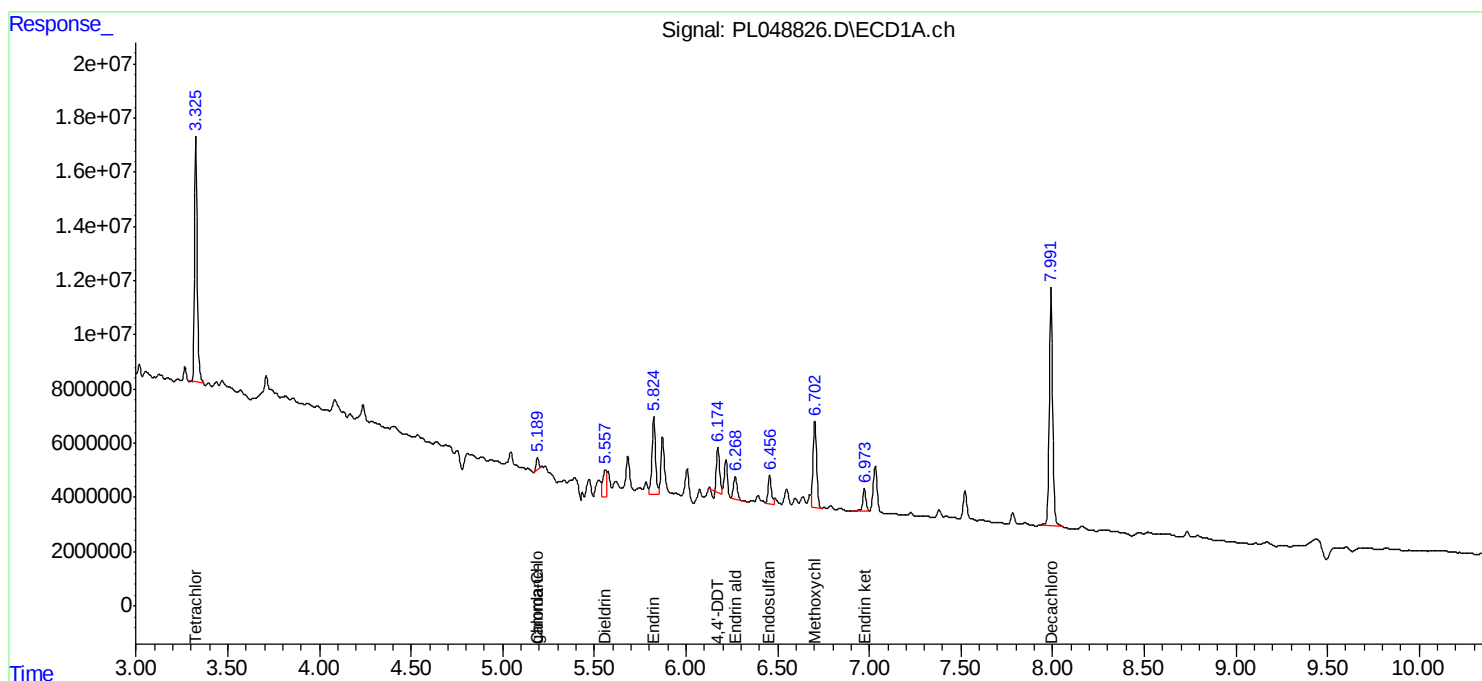


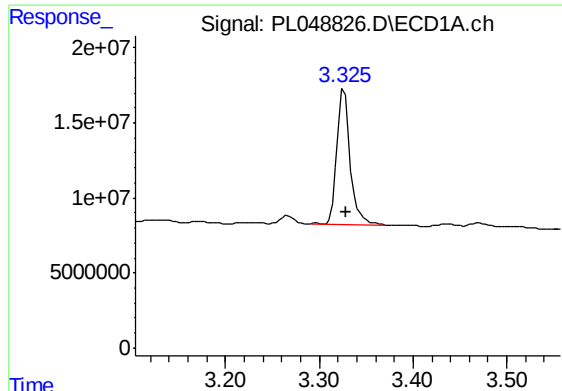

#1 Tetrachloro-m-xylene


R.T.: 3.326 min
Delta R.T.: -0.002 min
Response: 88842133
Conc: 9.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-12-S

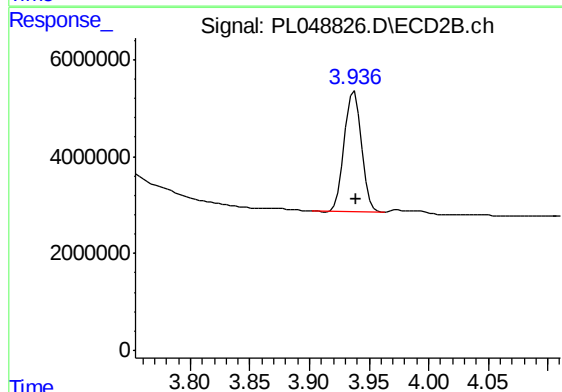


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: -0.002 min
Response: 24456273
Conc: 9.82 ng/ml

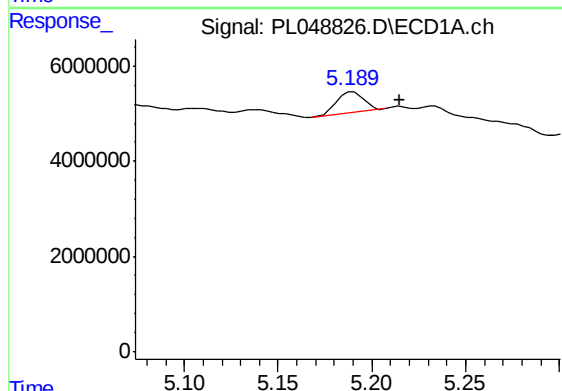


#10 gamma-Chlordane

R.T.: 5.190 min
Delta R.T.: -0.025 min
Response: 4200729
Conc: 0.31 ng/ml

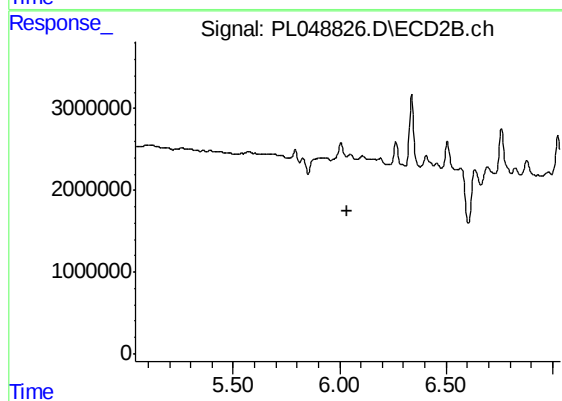

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

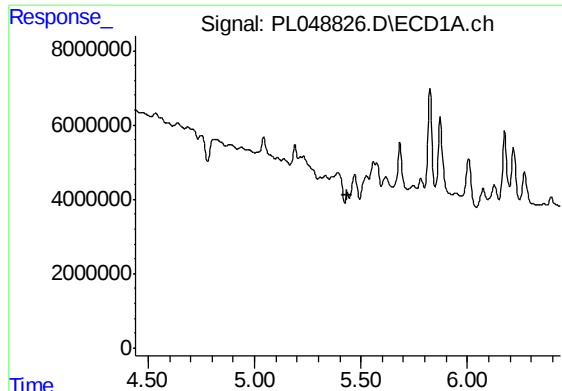

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.439 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-12-S

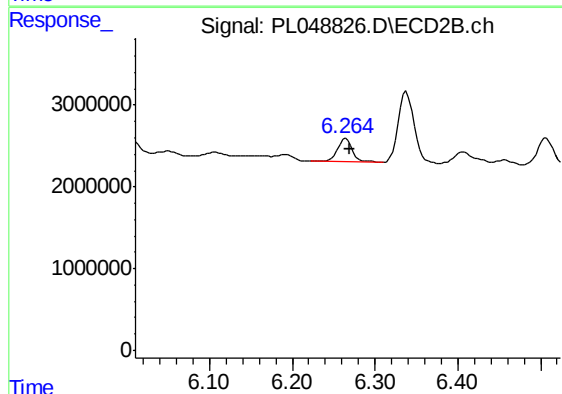


#12 4,4'-DDE

R.T.: 6.265 min
Delta R.T.: -0.004 min
Response: 3689421
Conc: 1.34 ng/ml

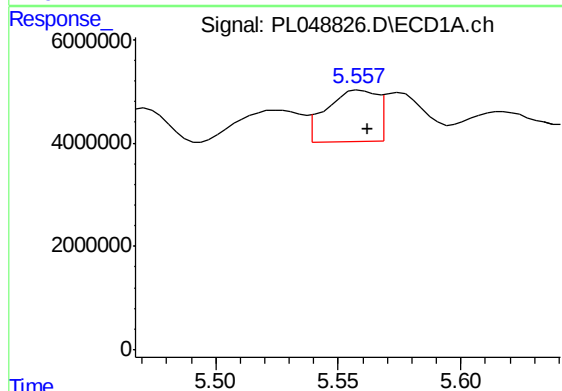


#13 Dieldrin

R.T.: 5.559 min
Delta R.T.: -0.003 min
Response: 14126000
Conc: 1.08 ng/ml

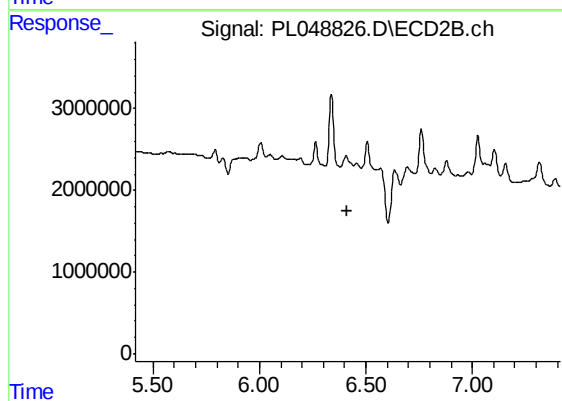

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

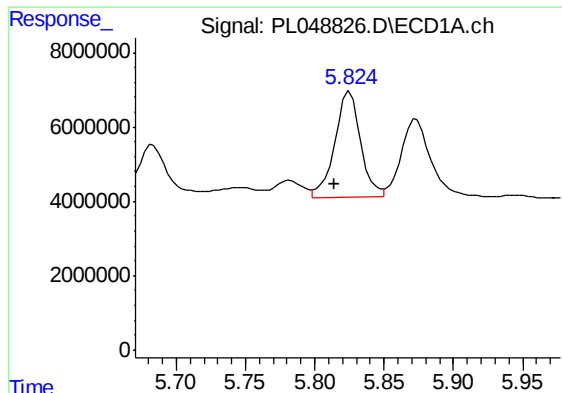

#14 Endrin


R.T.: 5.825 min
Delta R.T.: 0.011 min
Response: 37063053
Conc: 3.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-12-S

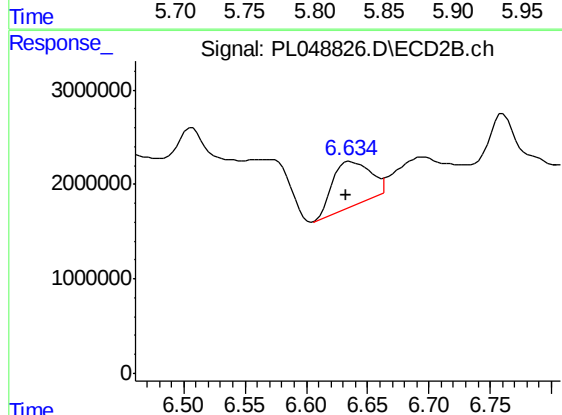


#14 Endrin

R.T.: 6.636 min
Delta R.T.: 0.003 min
Response: 10081506
Conc: 3.87 ng/ml

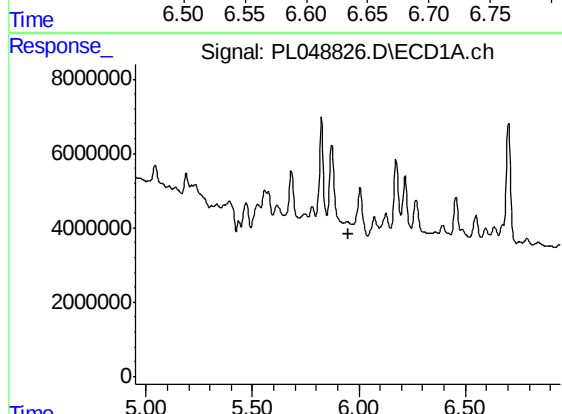


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

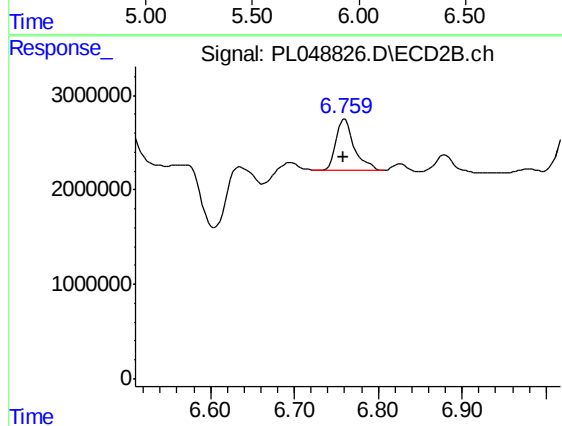

#16 4,4'-DDD


R.T.: 6.761 min
Delta R.T.: 0.001 min
Response: 8158061
Conc: 3.64 ng/ml

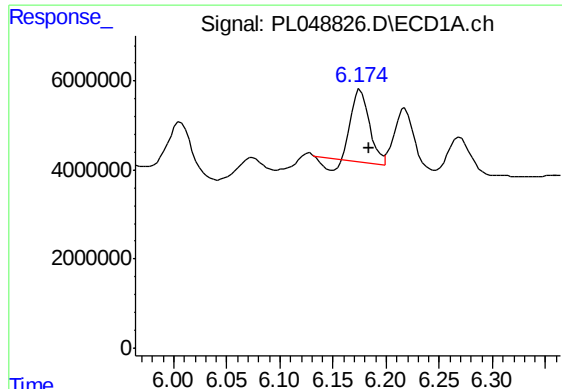

#17 4,4'-DDT


R.T.: 6.176 min
Delta R.T.: -0.008 min
Response: 17640005
Conc: 1.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-12-S

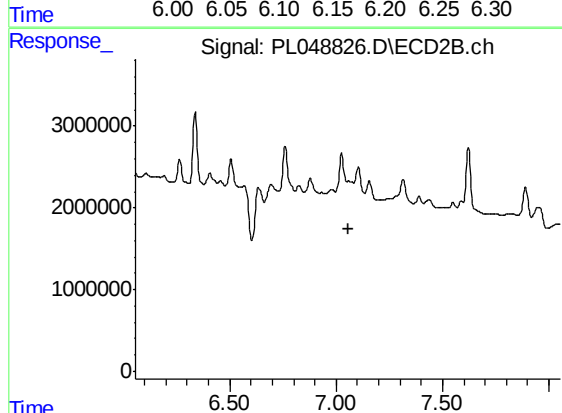


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.057 min
Response: 0
Conc: N.D.

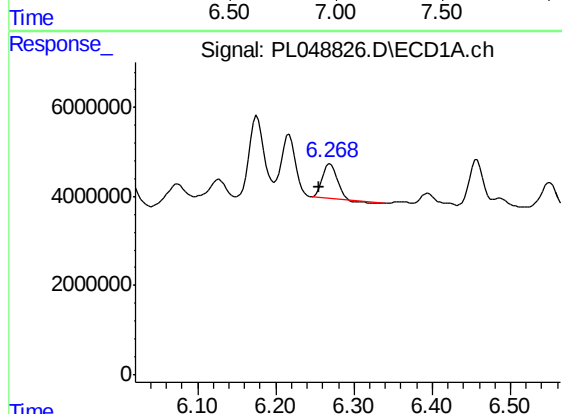


#18 Endrin aldehyde

R.T.: 6.269 min
Delta R.T.: 0.013 min
Response: 10352919
Conc: 1.07 ng/ml

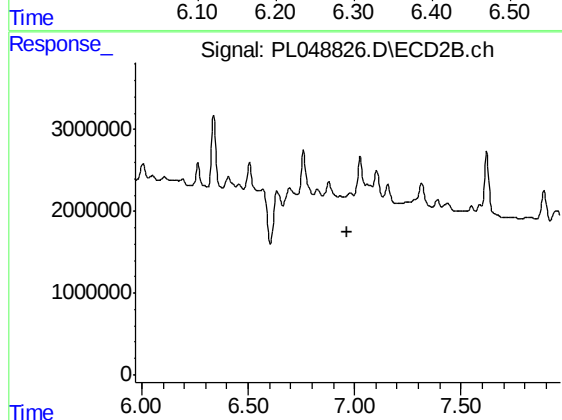

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.967 min
Response: 0
Conc: N.D.

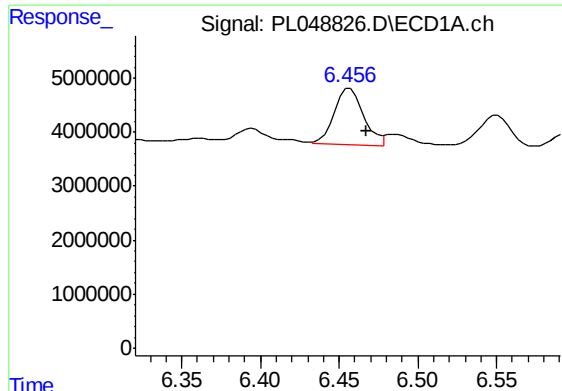

#19 Endosulfan Sulfate


R.T.: 6.457 min
Delta R.T.: -0.011 min
Response: 13702840
Conc: 1.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-12-S

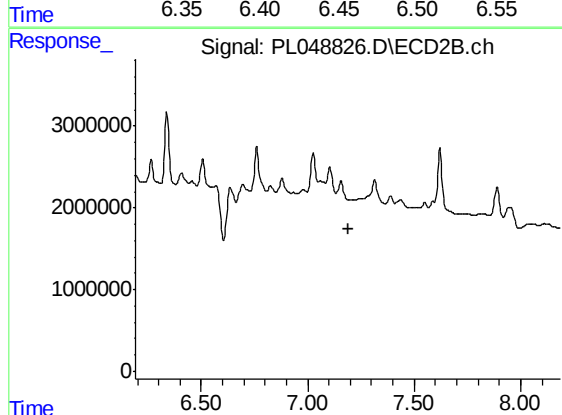


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.190 min
Response: 0
Conc: N.D.

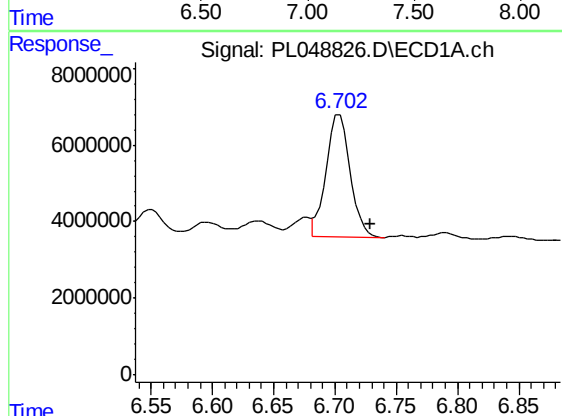


#20 Methoxychlor

R.T.: 6.704 min
Delta R.T.: -0.025 min
Response: 43801721
Conc: 8.04 ng/ml

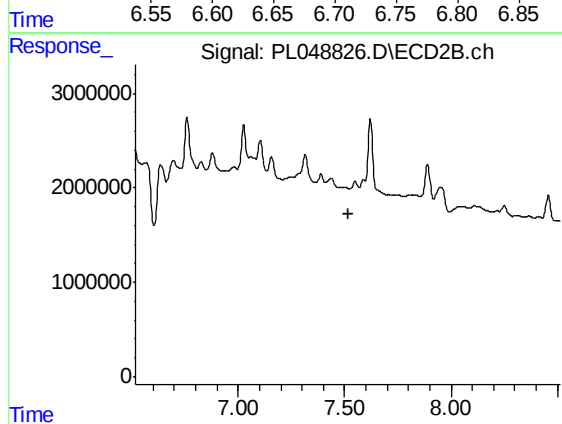

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.516 min
Response: 0
Conc: N.D.

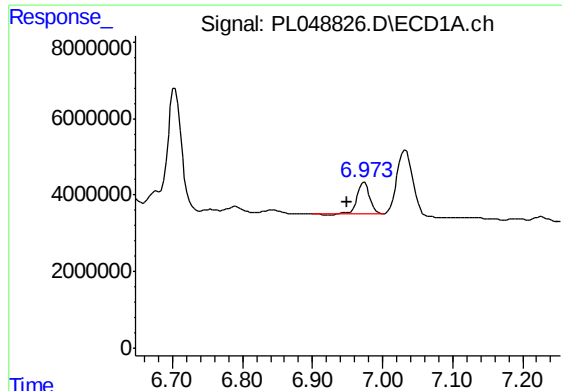

#21 Endrin ketone


R.T.: 6.974 min
Delta R.T.: 0.024 min
Response: 10279549
Conc: 0.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-12-S

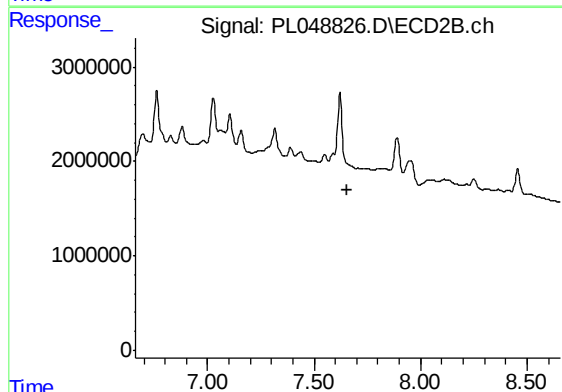


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.658 min
Response: 0
Conc: N.D.

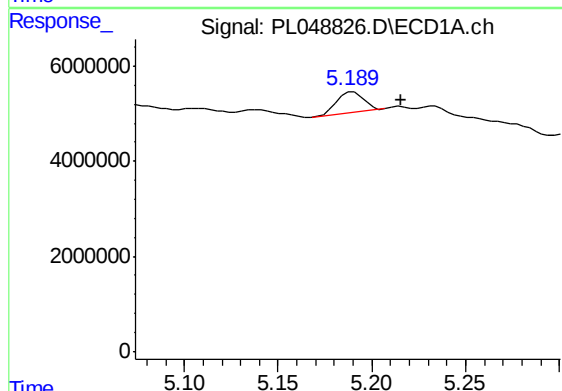


#25 Chlordane-3

R.T.: 5.190 min
Delta R.T.: -0.026 min
Response: 4200729
Conc: 2.67 ng/ml

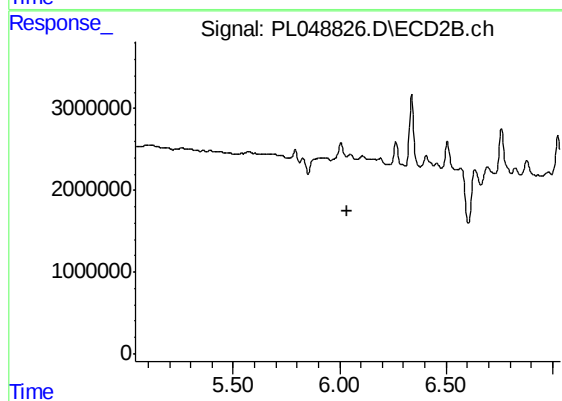

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

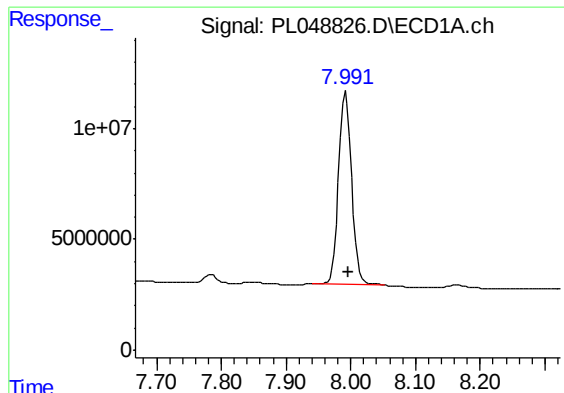

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.004 min
Response: 121128142
Conc: 12.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-12-S

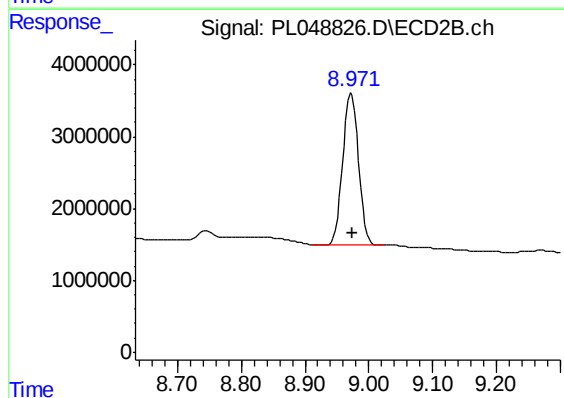

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: -0.002 min
Response: 36252256
Conc: 13.66 ng/ml