

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052219\
 Data File : PL048827.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2019 11:06
 Operator : SM\AJ
 Sample : K2951-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-14-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 01:05:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.326	3.938	75867413	17607820	7.832	7.069
28) SA Decachlor...	7.993	8.972	59344673	18048806	5.902	6.800
Target Compounds						
13) MA Dieldrin	5.555	0.000	8254772	0	0.634	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052219\
Data File : PL048827.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2019 11:06
Operator : SM\AJ
Sample : K2951-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-14-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 01:05:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

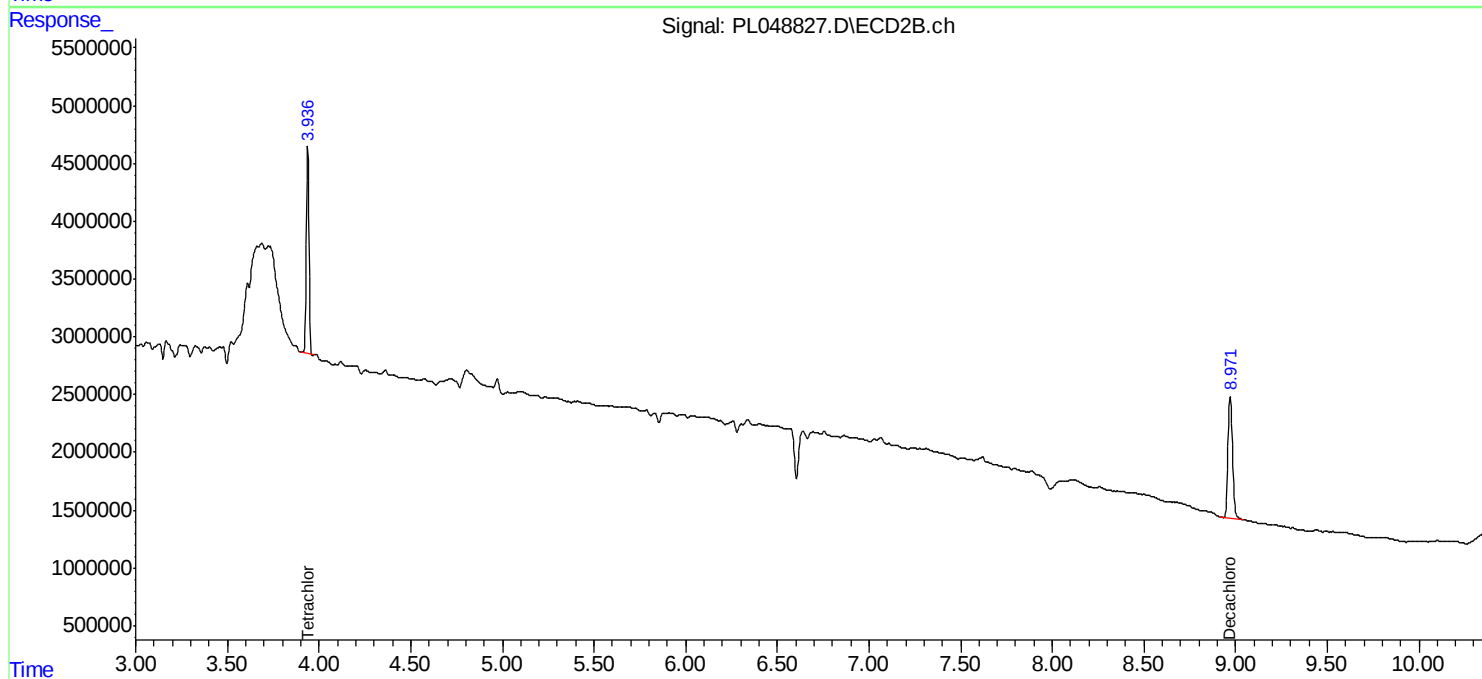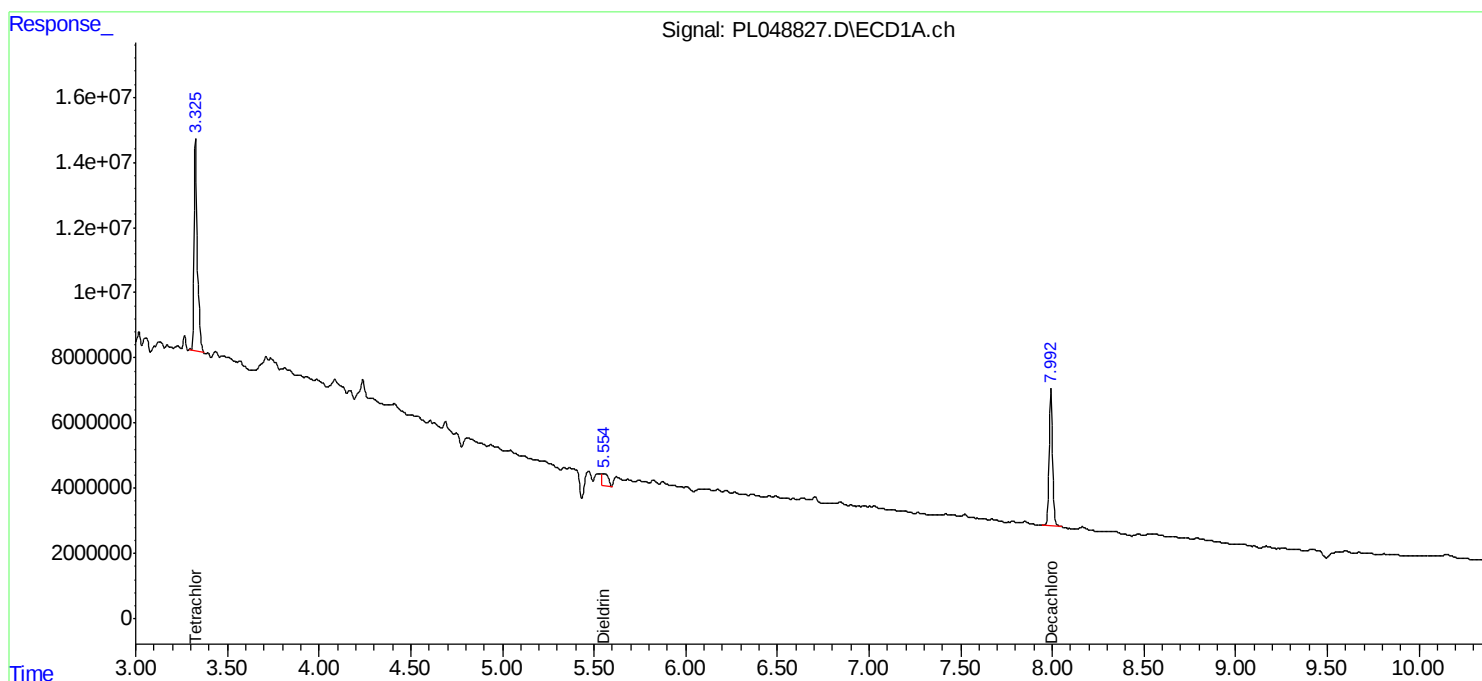


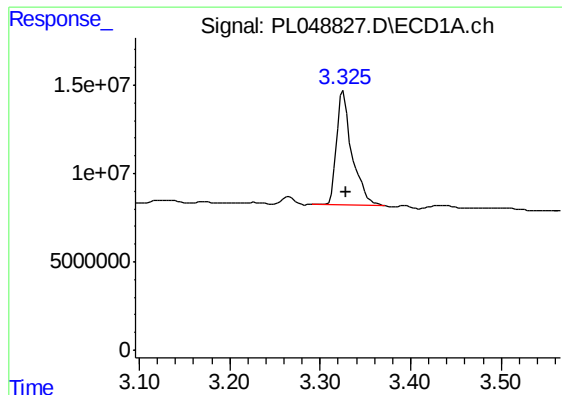

#1 Tetrachloro-m-xylene


R.T.: 3.326 min
Delta R.T.: -0.002 min
Response: 75867413
Conc: 7.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

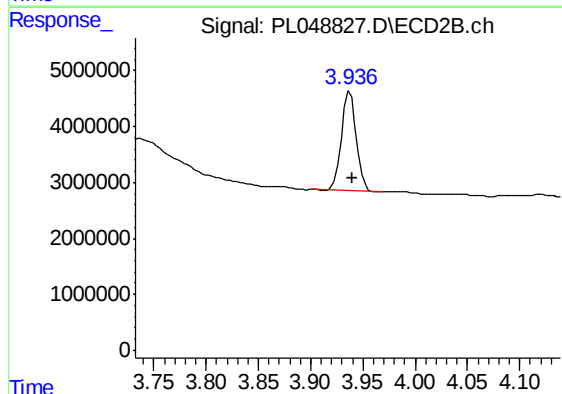


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: -0.002 min
Response: 17607820
Conc: 7.07 ng/ml

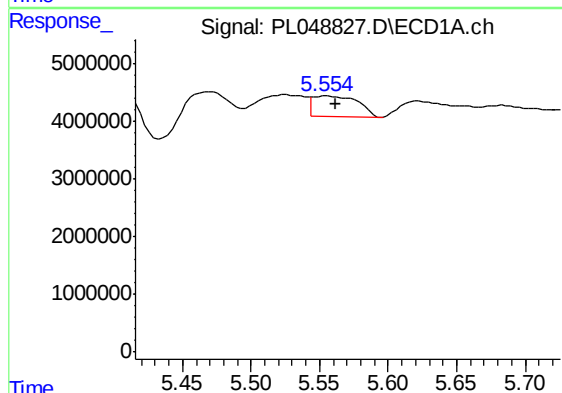


#13 Dieldrin

R.T.: 5.555 min
Delta R.T.: -0.007 min
Response: 8254772
Conc: 0.63 ng/ml

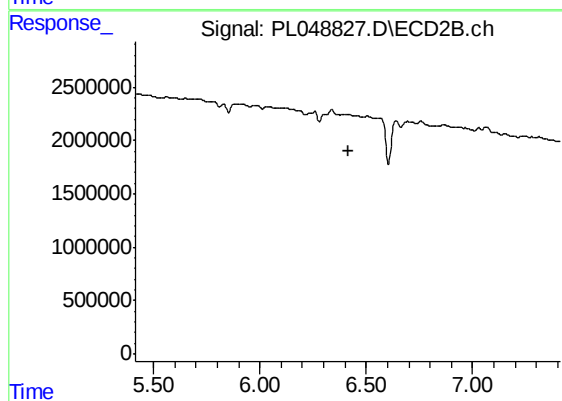

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

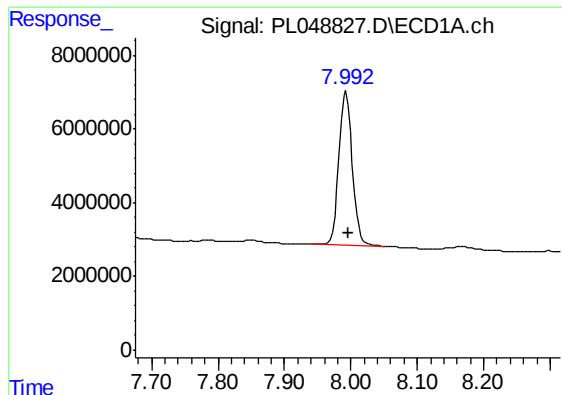

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.003 min
Response: 59344673
Conc: 5.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

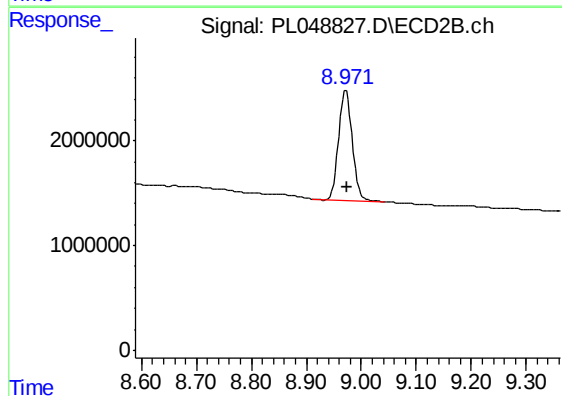

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: -0.003 min
Response: 18048806
Conc: 6.80 ng/ml