

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052219\
 Data File : PL048828.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2019 11:21
 Operator : SM\AJ
 Sample : K2951-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-15-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 01:06:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.326	3.937	85922946	23725336	8.870	9.525
28) SA Decachlor...	7.993	8.972	66895210	20635067	6.653	7.774
Target Compounds						
14) MA Endrin	5.826	6.641	12826425	366469	1.054	0.141 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052219\
Data File : PL048828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2019 11:21
Operator : SM\AJ
Sample : K2951-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-15-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 01:06:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

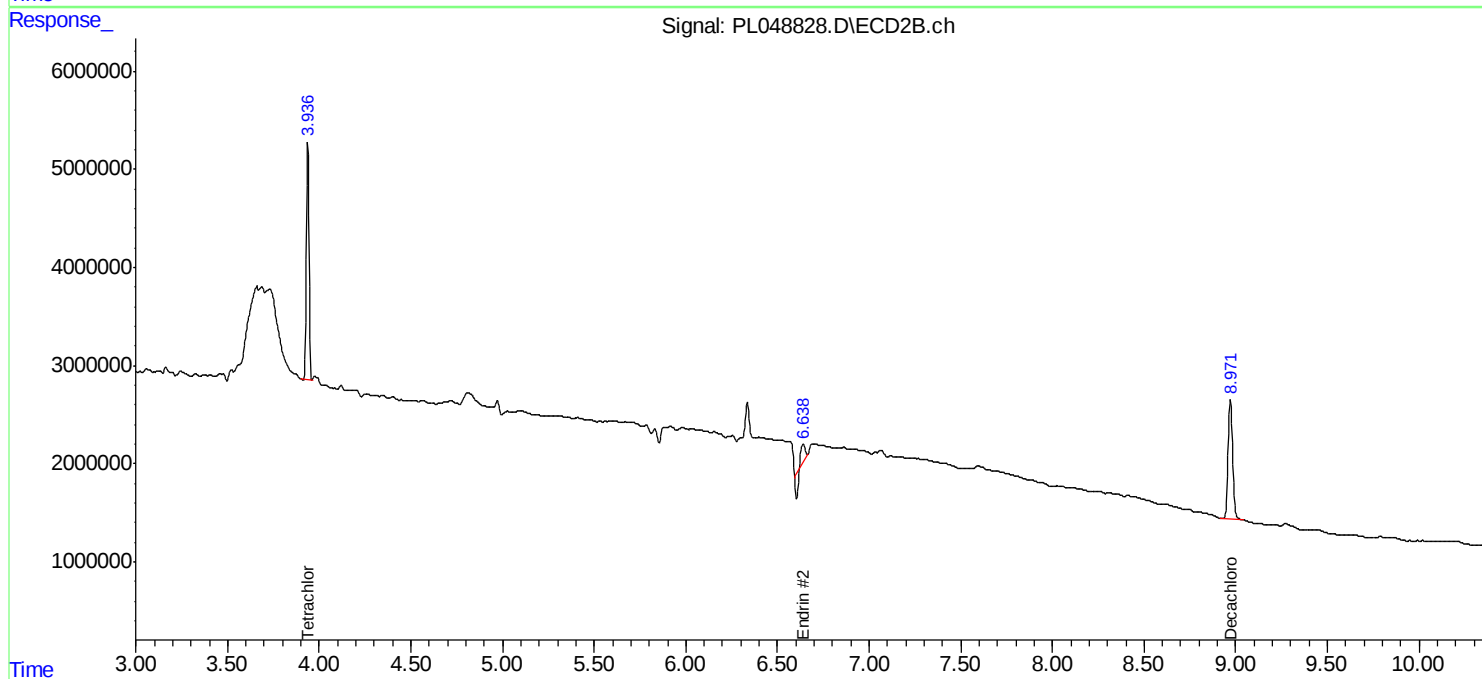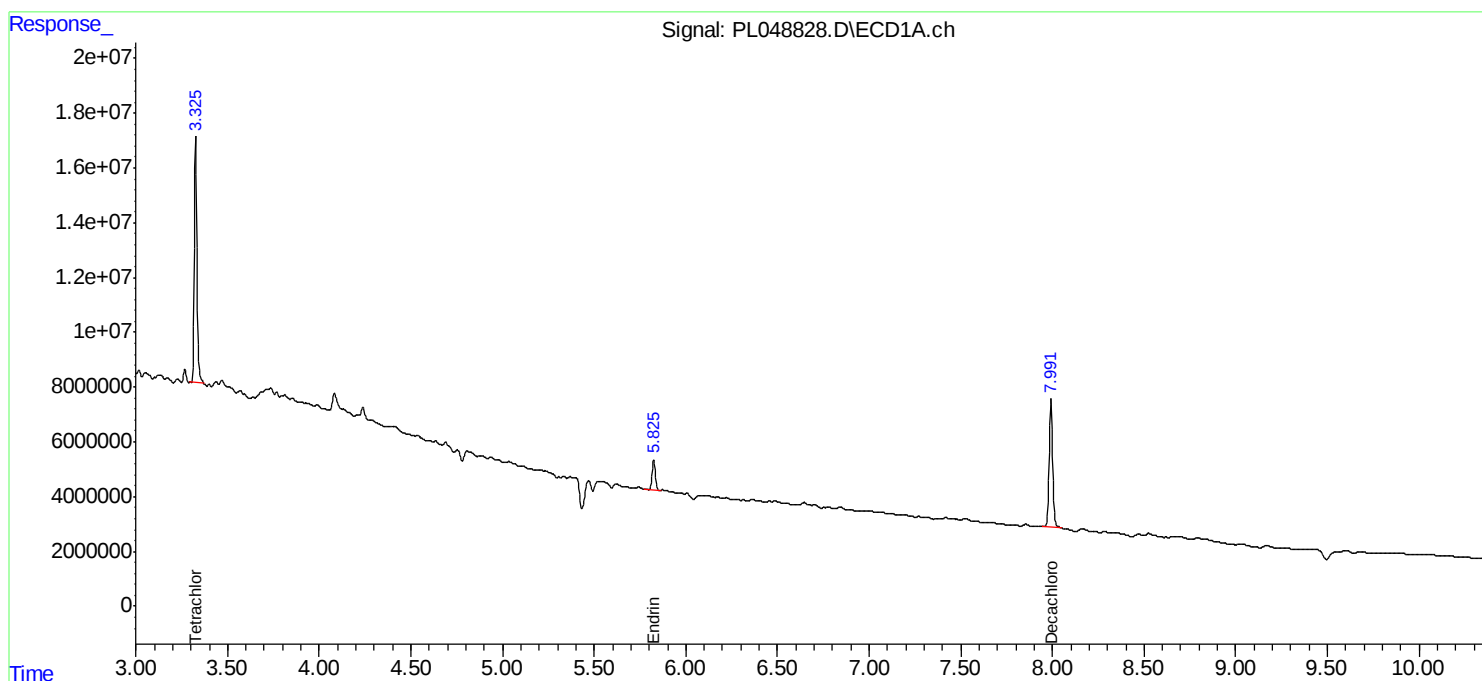


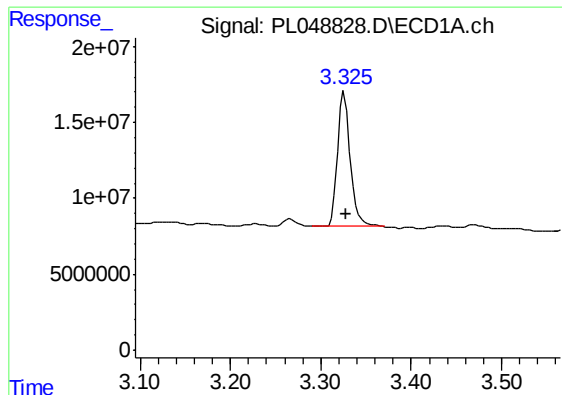

#1 Tetrachloro-m-xylene


R.T.: 3.326 min
Delta R.T.: -0.002 min
Response: 85922946
Conc: 8.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15-S

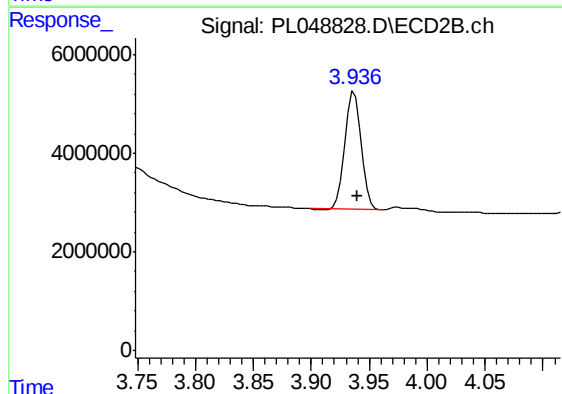


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.002 min
Response: 23725336
Conc: 9.52 ng/ml

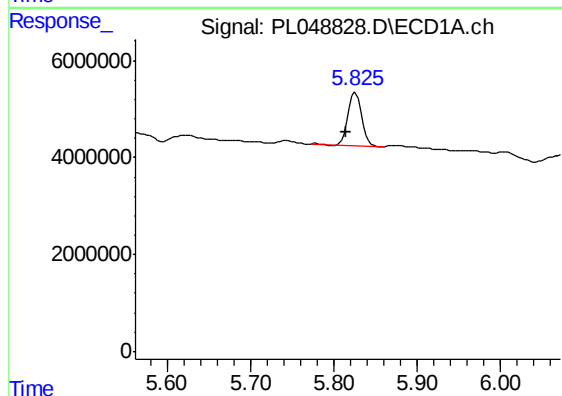


#14 Endrin

R.T.: 5.826 min
Delta R.T.: 0.012 min
Response: 12826425
Conc: 1.05 ng/ml

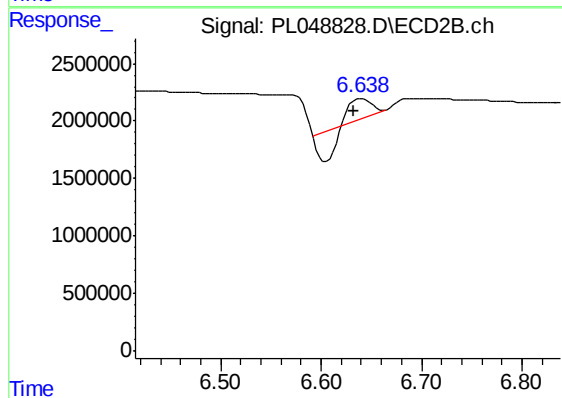

#14 Endrin


R.T.: 6.641 min
Delta R.T.: 0.008 min
Response: 366469
Conc: 0.14 ng/ml

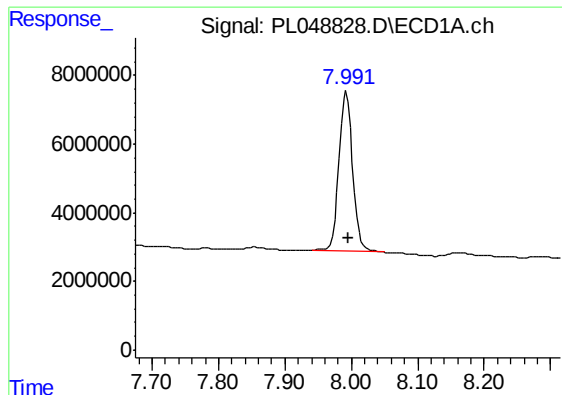

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.003 min
Response: 66895210
Conc: 6.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15-S

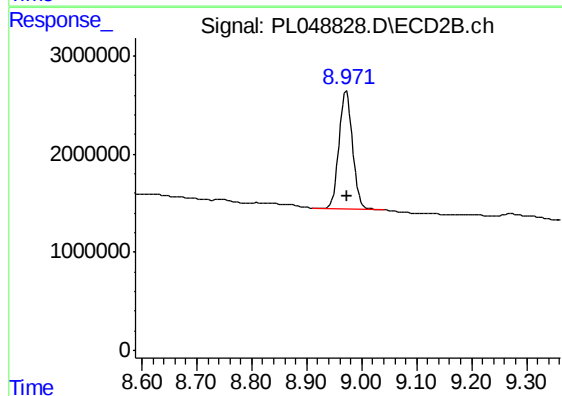

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: -0.003 min
Response: 20635067
Conc: 7.77 ng/ml