

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052219\
 Data File : PL048856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2019 20:04
 Operator : SM\AJ
 Sample : K2970-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-9-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 01:13:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.936	33193704	13298259	3.427	5.339 #
28)	SA Decachlor...	7.990	8.970	54429536	17828302	5.414	6.717
Target Compounds							
3)	MA gamma-BHC...	0.000	4.624	0	6922480	N.D.	2.119 #
4)	MA Heptachlor	4.330	0.000	1862550	0	0.127	N.D. #
5)	MB Aldrin	4.538f	0.000	341.6E6	0	24.928	N.D. #
6)	B beta-BHC	4.293	4.805f	4766355	4305893	0.808	2.767 #
9)	A Endosulfan I	0.000	6.180f	0	6436467	N.D.	2.276 #
12)	B 4,4'-DDE	5.431	6.263	-9479613	3397832	N.D.	1.231
20)	A Methoxychlor	6.702f	0.000	8697019	0	1.597	N.D. #
23)	Chlordane-1	4.172	4.950f	8091716	4200805	18.025	34.391 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052219\
Data File : PL048856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2019 20:04
Operator : SM\AJ
Sample : K2970-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-9-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 01:13:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

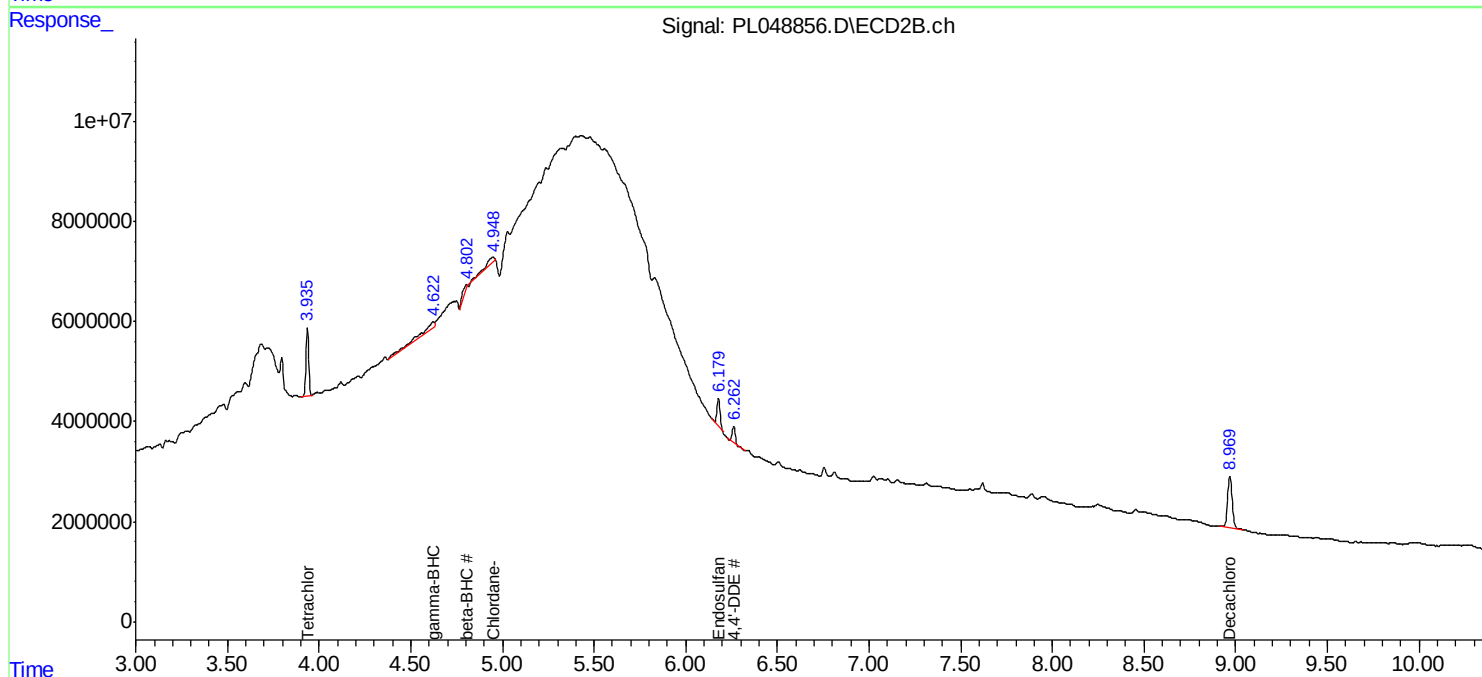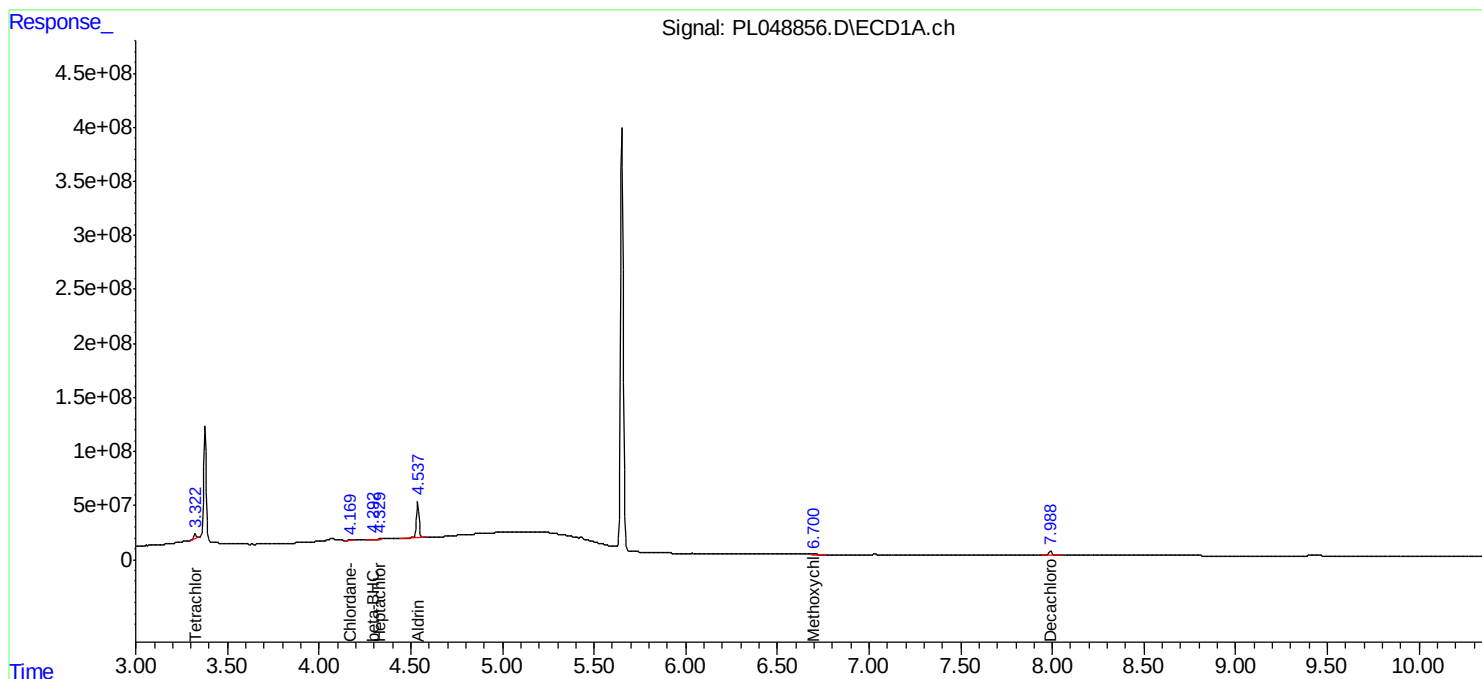


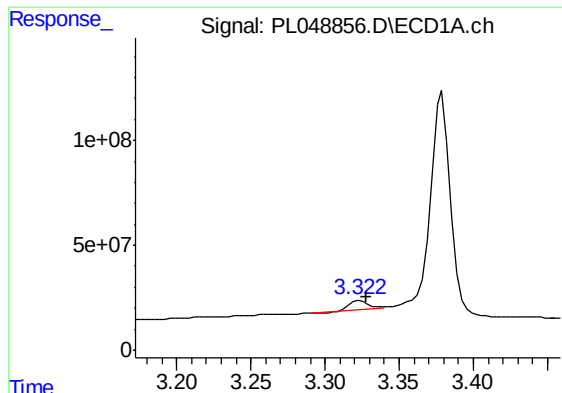

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.004 min
Response: 33193704
Conc: 3.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-9-S

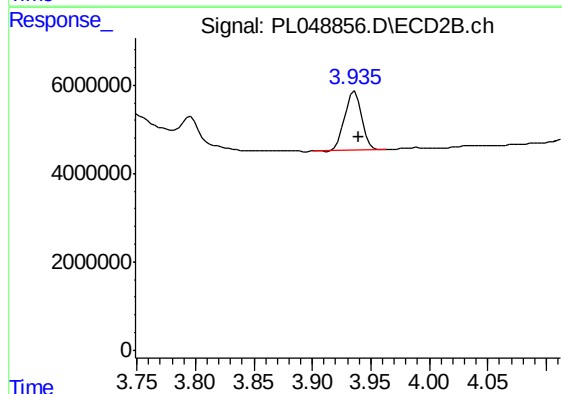


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.004 min
Response: 13298259
Conc: 5.34 ng/ml

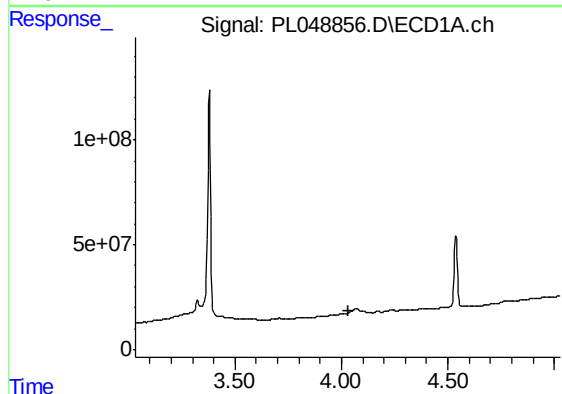


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.032 min
Response: 0
Conc: N.D.

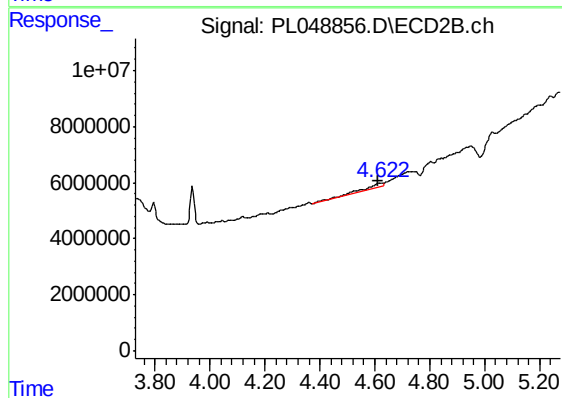

#3 gamma-BHC (Lindane)


R.T.: 4.624 min
Delta R.T.: 0.013 min
Response: 6922480
Conc: 2.12 ng/ml

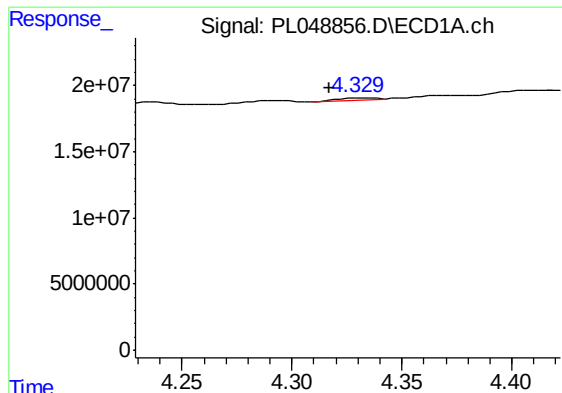

#4 Heptachlor


R.T.: 4.330 min
Delta R.T.: 0.013 min
Response: 1862550
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-9-S

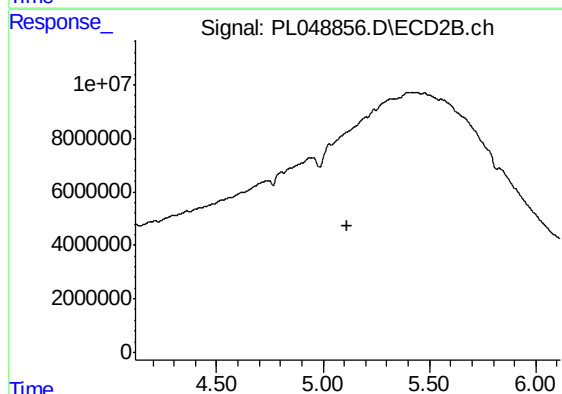


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.116 min
Response: 0
Conc: N.D.

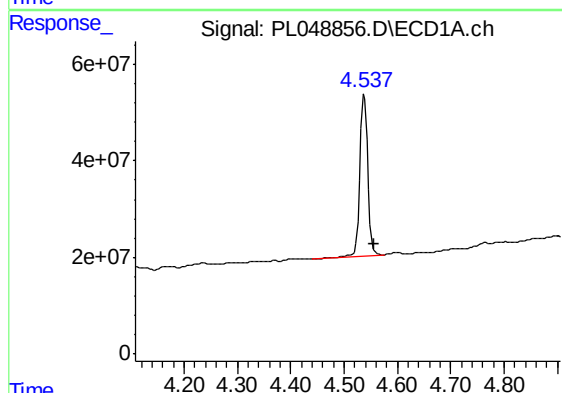


#5 Aldrin

R.T.: 4.538 min
Delta R.T.: -0.018 min
Response: 341558660
Conc: 24.93 ng/ml

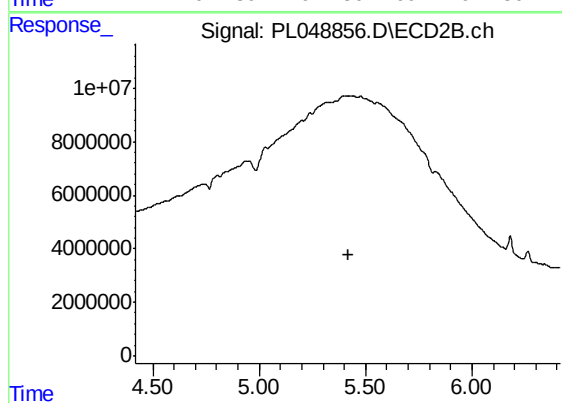

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.418 min
Response: 0
Conc: N.D.

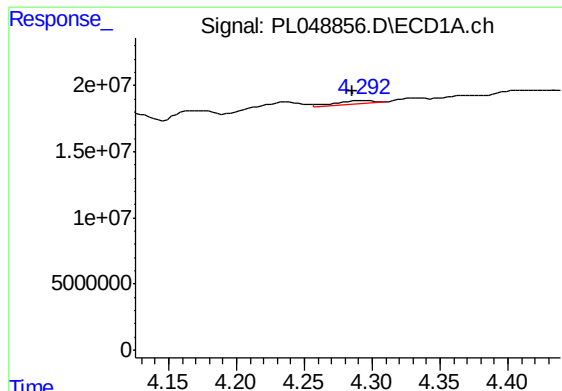

#6 beta-BHC


R.T.: 4.293 min
Delta R.T.: 0.008 min
Response: 4766355
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-9-S

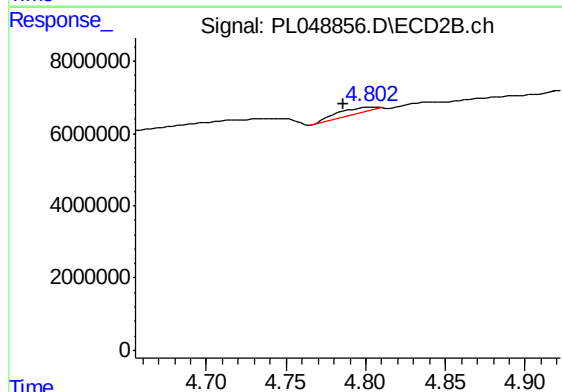


#6 beta-BHC

R.T.: 4.805 min
Delta R.T.: 0.019 min
Response: 4305893
Conc: 2.77 ng/ml

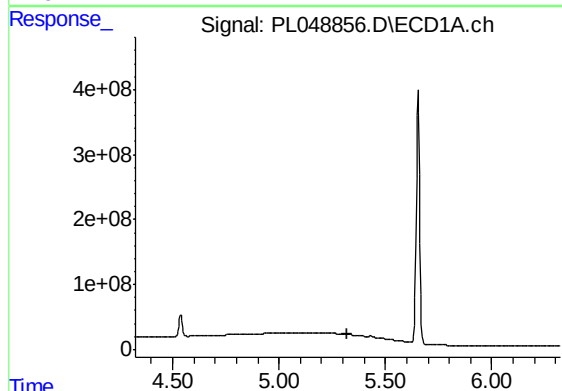


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.323 min
Response: 0
Conc: N.D.

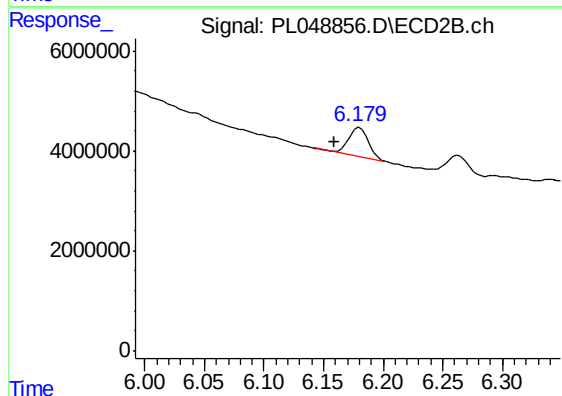

#9 Endosulfan I


R.T.: 6.180 min
Delta R.T.: 0.021 min
Response: 6436467
Conc: 2.28 ng/ml

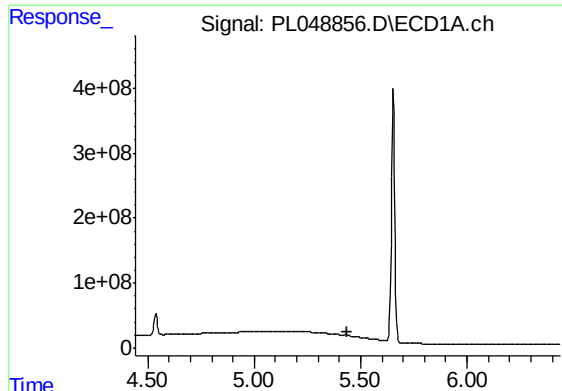

#12 4,4'-DDE


R.T.: 5.431 min
Delta R.T.: -0.008 min
Response: -9479613
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-9-S

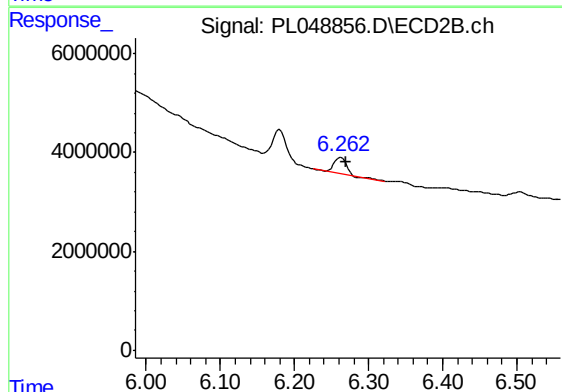


#12 4,4'-DDE

R.T.: 6.263 min
Delta R.T.: -0.006 min
Response: 3397832
Conc: 1.23 ng/ml

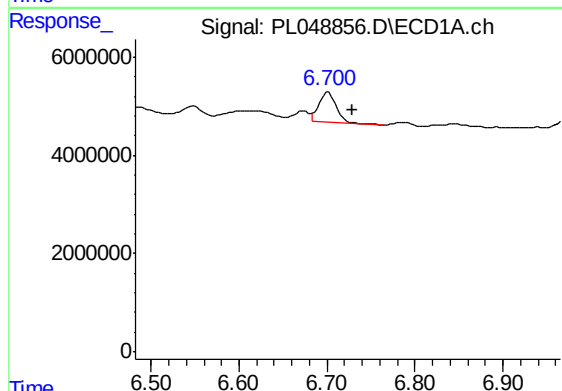


#20 Methoxychlor

R.T.: 6.702 min
Delta R.T.: -0.027 min
Response: 8697019
Conc: 1.60 ng/ml

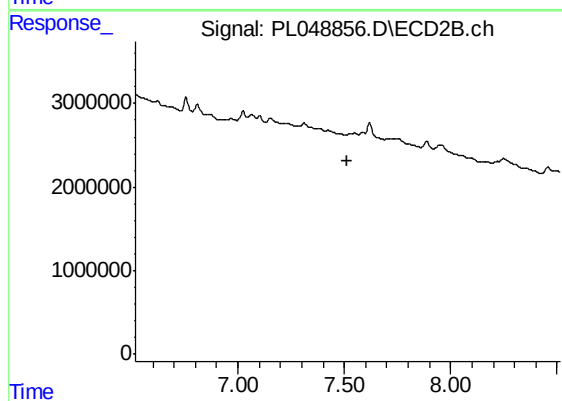

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.516 min
Response: 0
Conc: N.D.

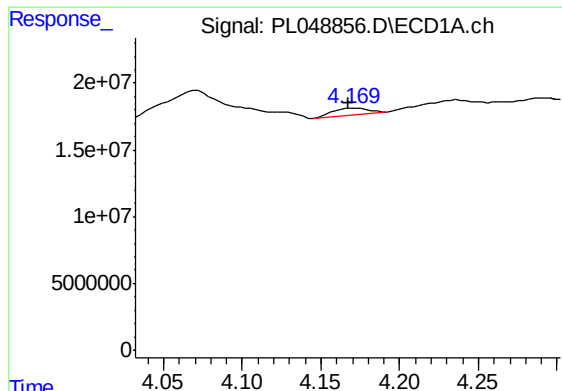

#23 Chlordane-1


R.T.: 4.172 min
Delta R.T.: 0.004 min
Response: 8091716
Conc: 18.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-9-S

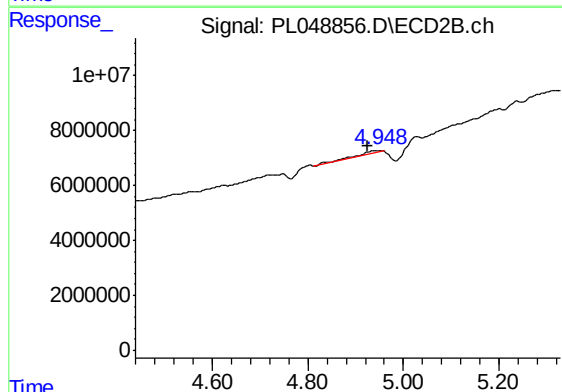


#23 Chlordane-1

R.T.: 4.950 min
Delta R.T.: 0.024 min
Response: 4200805
Conc: 34.39 ng/ml

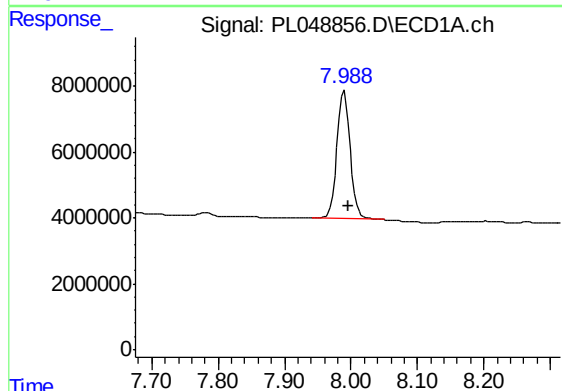

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.006 min
Response: 54429536
Conc: 5.41 ng/ml

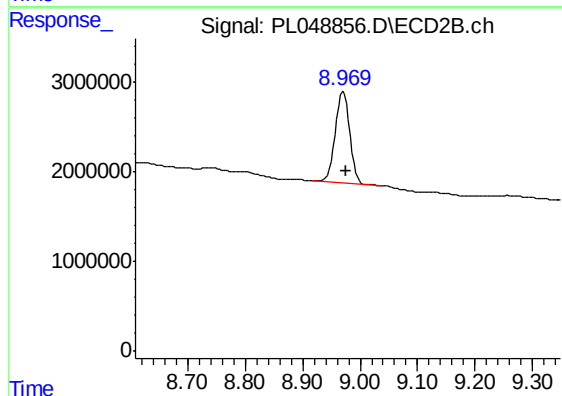

#28 Decachlorobiphenyl

R.T.: 8.970 min
Delta R.T.: -0.005 min
Response: 17828302
Conc: 6.72 ng/ml