

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052219\
 Data File : PL048851.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2019 18:53
 Operator : SM\AJ
 Sample : K2642-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-01-052119

Manual Integrations
 APPROVED

Ankita
 5/23/2019 4:43:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 01:12:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.324	3.936	94864790	22775772	9.793m	9.144
28) SA Decachlor...	7.992	8.971	100.1E6	31750154	9.953	11.962
Target Compounds						
12) B 4,4'-DDE	5.433	6.260	20130736	3501782	1.587m	1.268m
17) MA 4,4'-DDT	6.177	7.052	4157960	2480787	0.414m	1.057m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052219\
Data File : PL048851.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2019 18:53
Operator : SM\AJ
Sample : K2642-05
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-01-052119


Manual Integrations
APPROVED

Ankita
5/23/2019 4:43:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 01:12:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

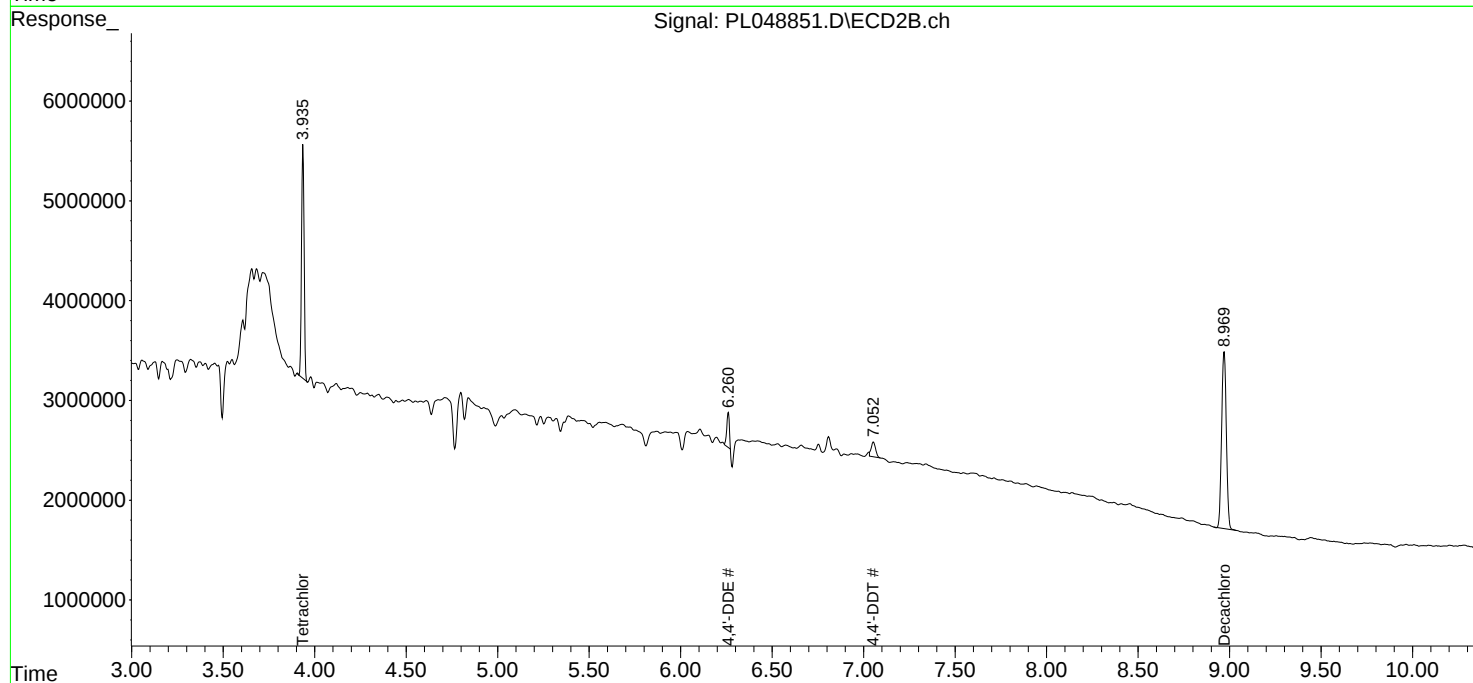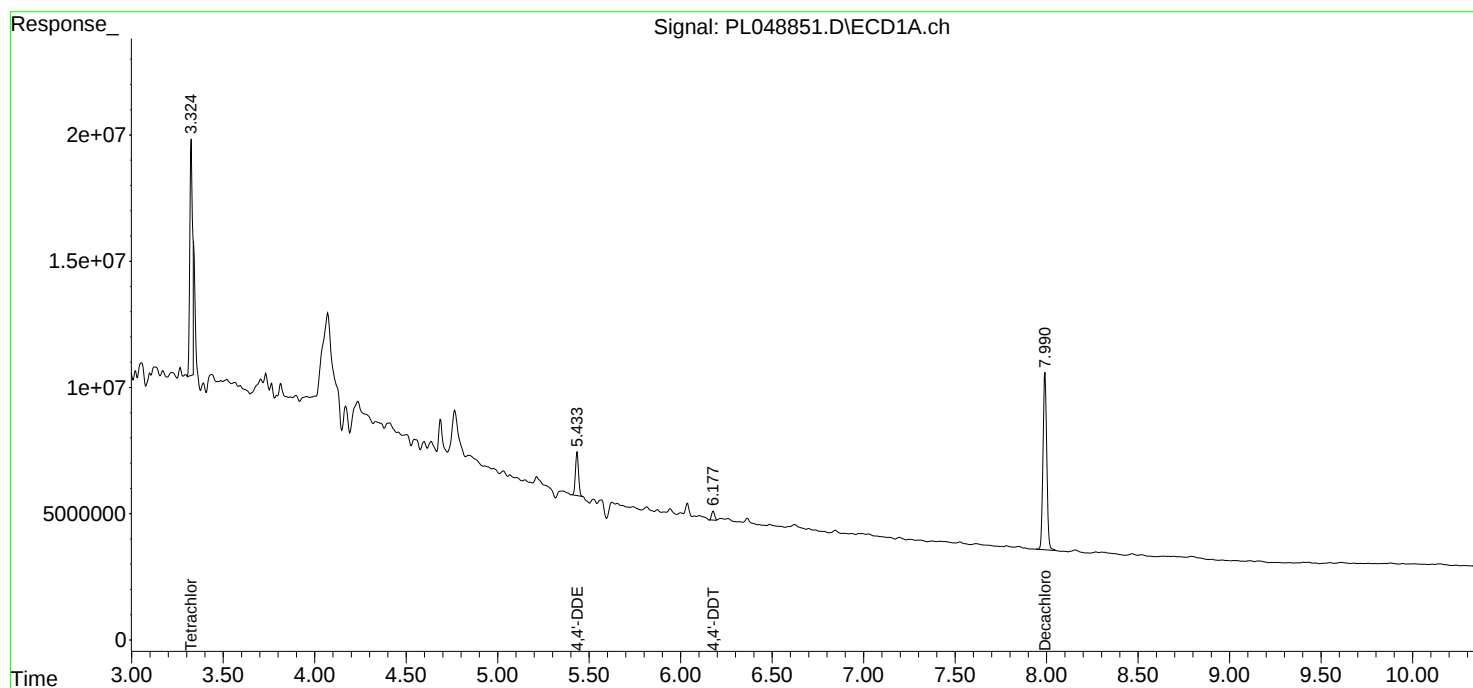

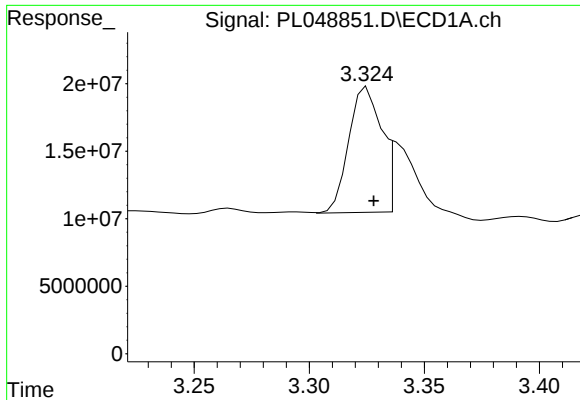


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: -0.004 min
Response: 94864790
Conc: 9.79 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OK-01-052119


Manual Integrations
APPROVED

Ankita
5/23/2019 4:43:05 PM

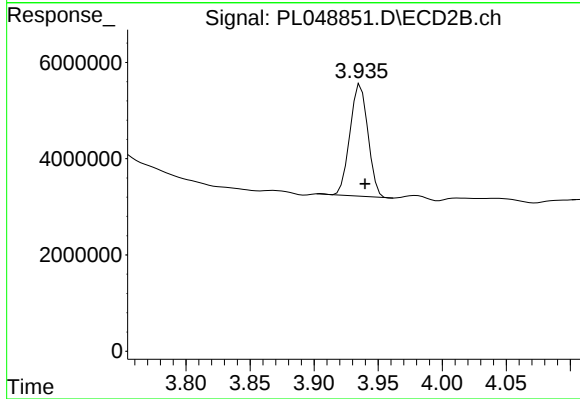


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.003 min
Response: 22775772
Conc: 9.14 ng/ml

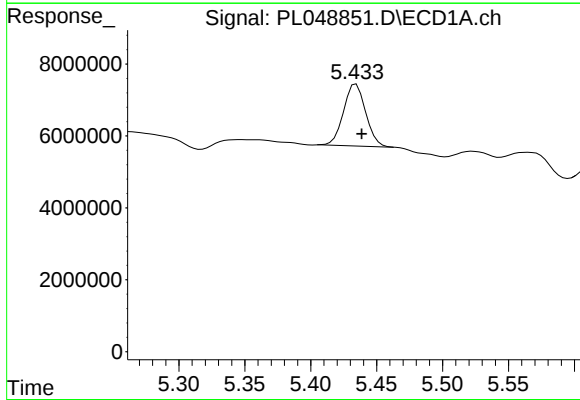


#12 4,4'-DDE

R.T.: 5.433 min
Delta R.T.: -0.006 min
Response: 20130736
Conc: 1.59 ng/ml m

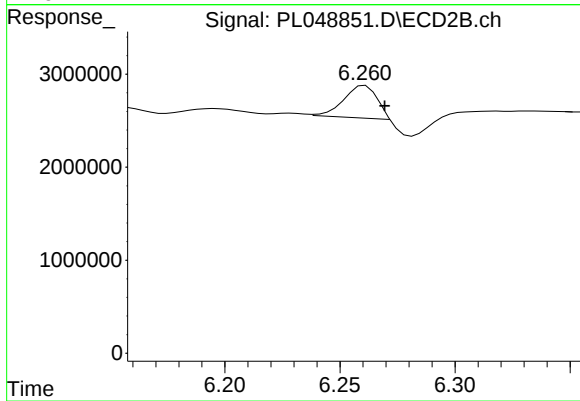

#12 4,4'-DDE

R.T.: 6.260 min
Delta R.T.: -0.010 min
Response: 3501782
Conc: 1.27 ng/ml m

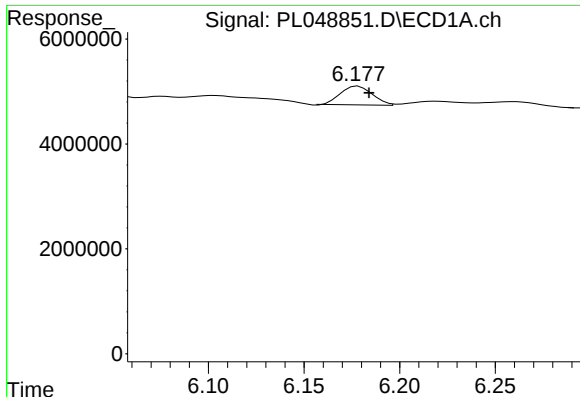


#17 4,4'-DDT

R.T.: 6.177 min
Delta R.T.: -0.007 min
Response: 4157960
Conc: 0.41 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OK-01-052119


Manual Integrations
APPROVED

Ankita
5/23/2019 4:43:05 PM

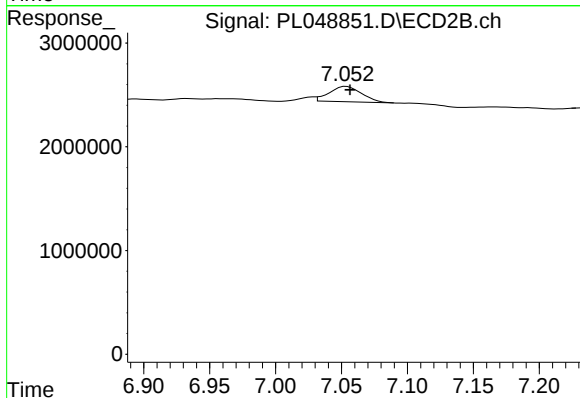


#17 4,4'-DDT

R.T.: 7.052 min
Delta R.T.: -0.004 min
Response: 2480787
Conc: 1.06 ng/ml m

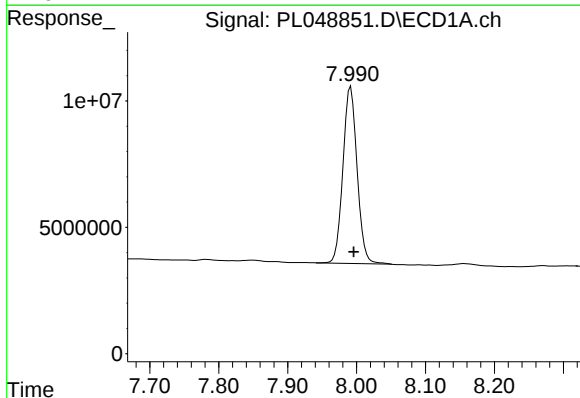

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.004 min
Response: 100069719
Conc: 9.95 ng/ml

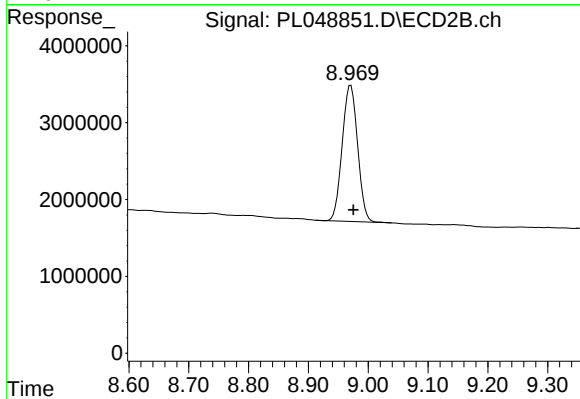

#28 Decachlorobiphenyl

R.T.: 8.971 min
Delta R.T.: -0.004 min
Response: 31750154
Conc: 11.96 ng/ml