

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052219\
 Data File : PL048856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2019 20:04
 Operator : SM\AJ
 Sample : K2970-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-9-S

Manual Integrations
 APPROVED

Ankita
 5/23/2019 10:27:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 01:13:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	3.936	44686199	13298259	4.613m	5.339
28)	SA Decachlor...	7.990	8.970	54429536	17828302	5.414	6.717

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052219\
Data File : PL048856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2019 20:04
Operator : SM\AJ
Sample : K2970-15
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-9-S


Manual Integrations
APPROVED

Ankita
5/23/2019 10:27:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 01:13:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

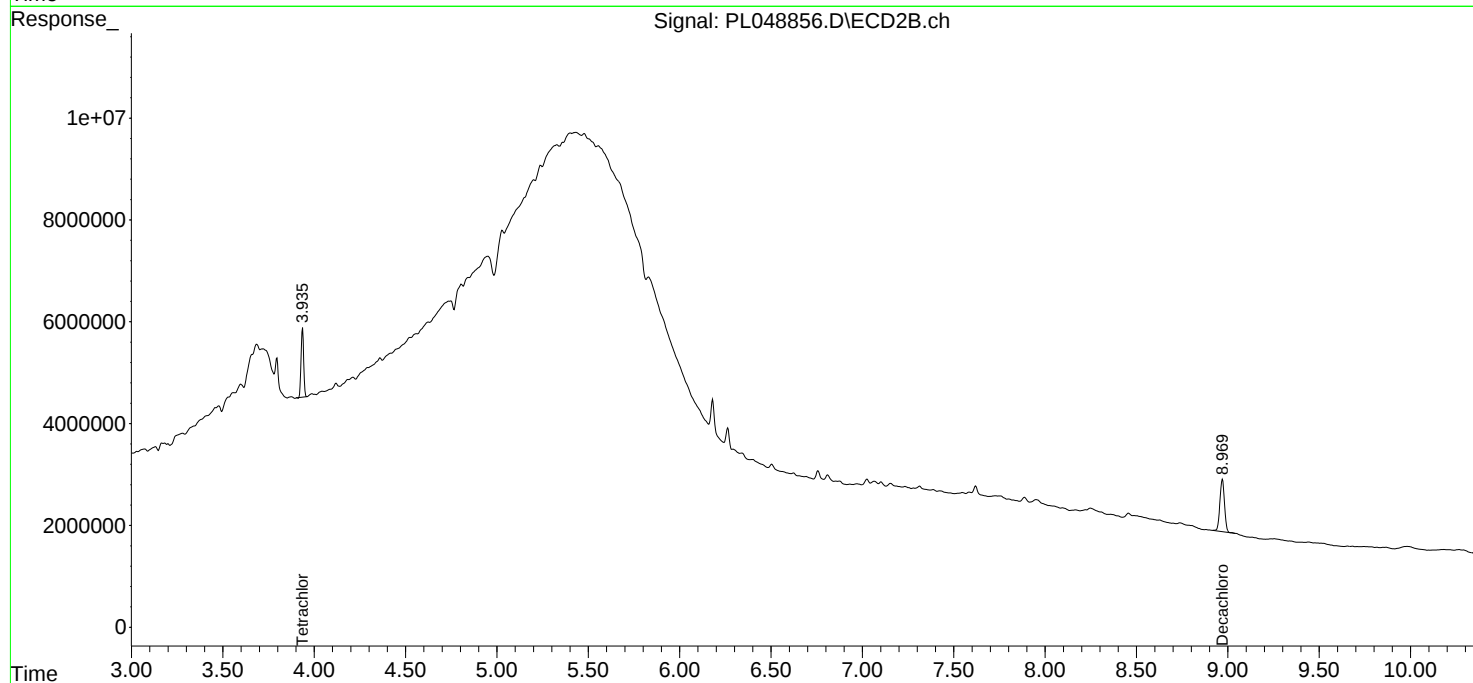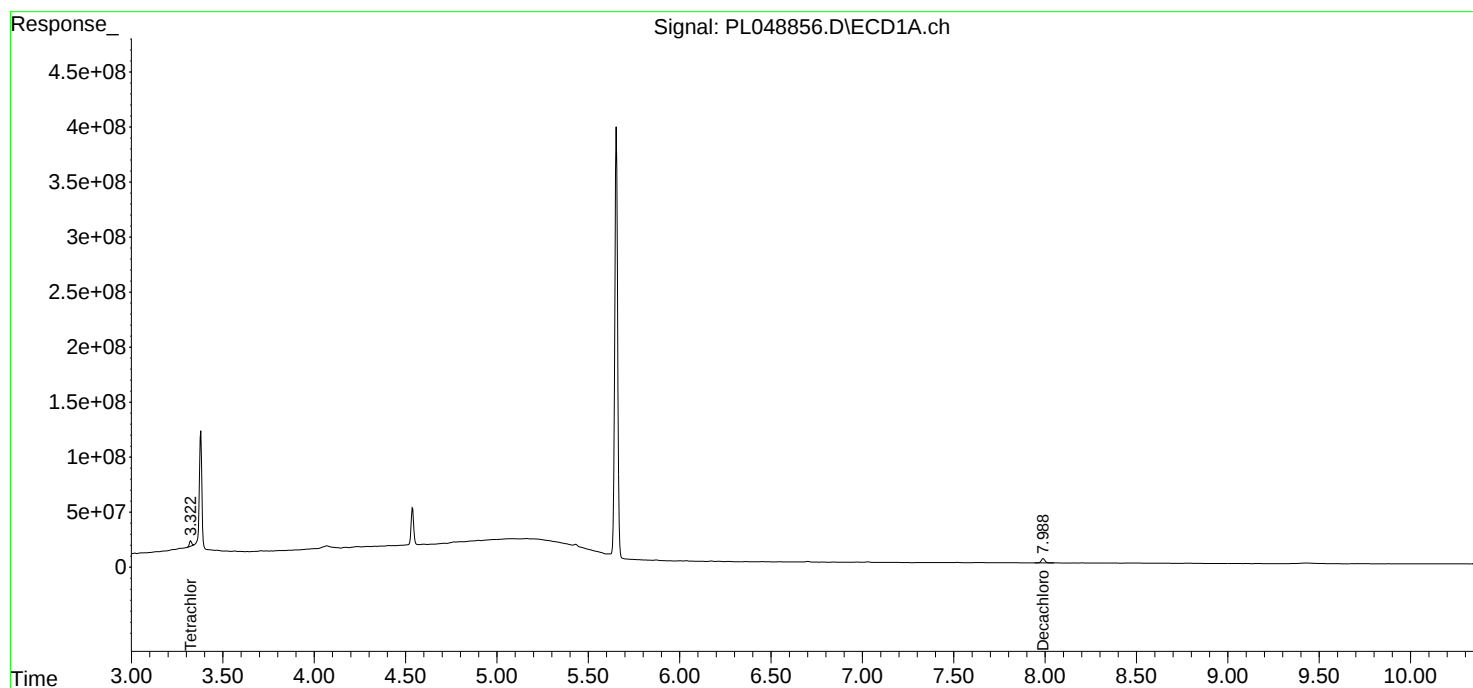

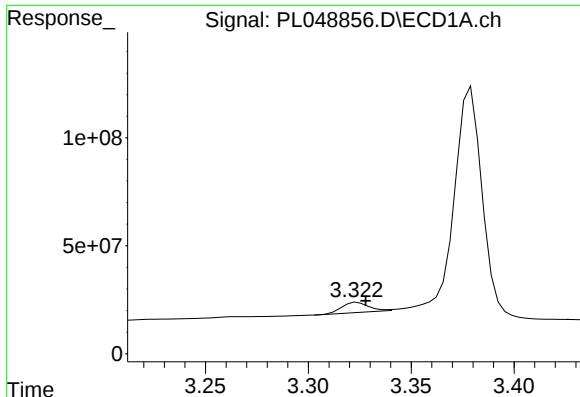


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: -0.006 min
Response: 44686199
Conc: 4.61 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-9-S


Manual Integrations
APPROVED

Ankita
5/23/2019 10:27:05 AM

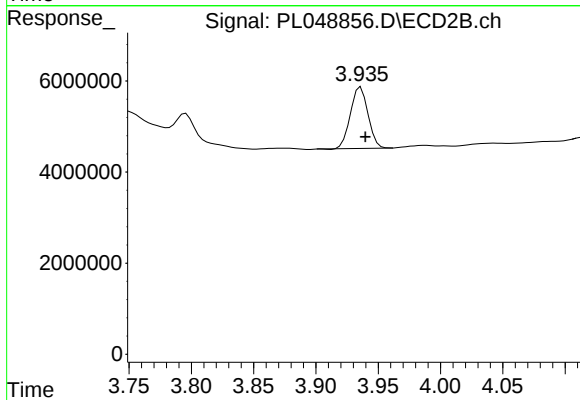


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.004 min
Response: 13298259
Conc: 5.34 ng/ml

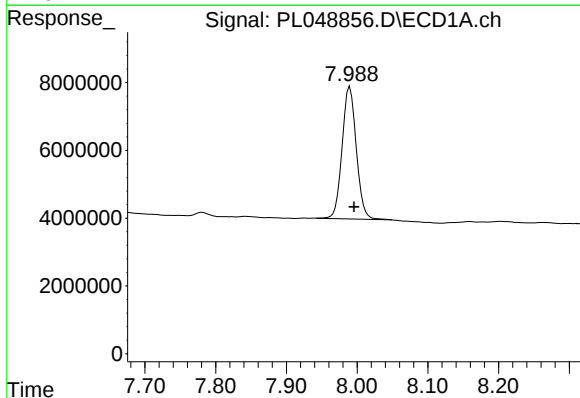

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.006 min
Response: 54429536
Conc: 5.41 ng/ml

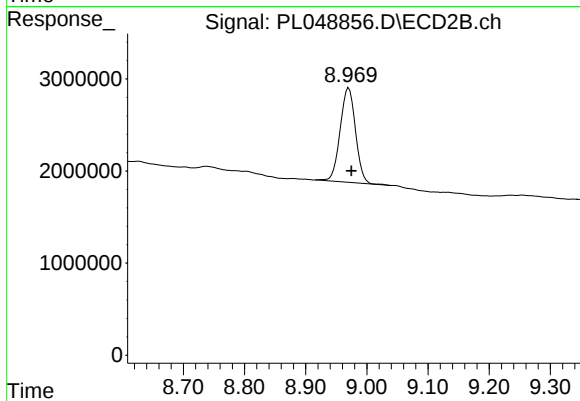

#28 Decachlorobiphenyl

R.T.: 8.970 min
Delta R.T.: -0.005 min
Response: 17828302
Conc: 6.72 ng/ml