

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052223\
 Data File : PL082878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2023 16:03
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 21:42:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	2.638	126.6E6	135.3E6	43.075	52.126
28)	SA Decachlor...	8.736	7.746	86009421	100.7E6	41.009	40.505
Target Compounds							
23)	Chlordane-1	4.460	3.621	56410287	42344684	515.632	513.187
24)	Chlordane-2	4.987	4.194	59142870	45011265	536.891	505.579
25)	Chlordane-3	5.692	4.820	217.0E6	139.8E6	522.992	524.384
26)	Chlordane-4	5.773	4.881	260.8E6	142.5E6	515.110	505.729
27)	Chlordane-5	6.614	5.773	42745915	46561371	520.865	479.291



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052223\
Data File : PL082878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2023 16:03
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 21:42:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

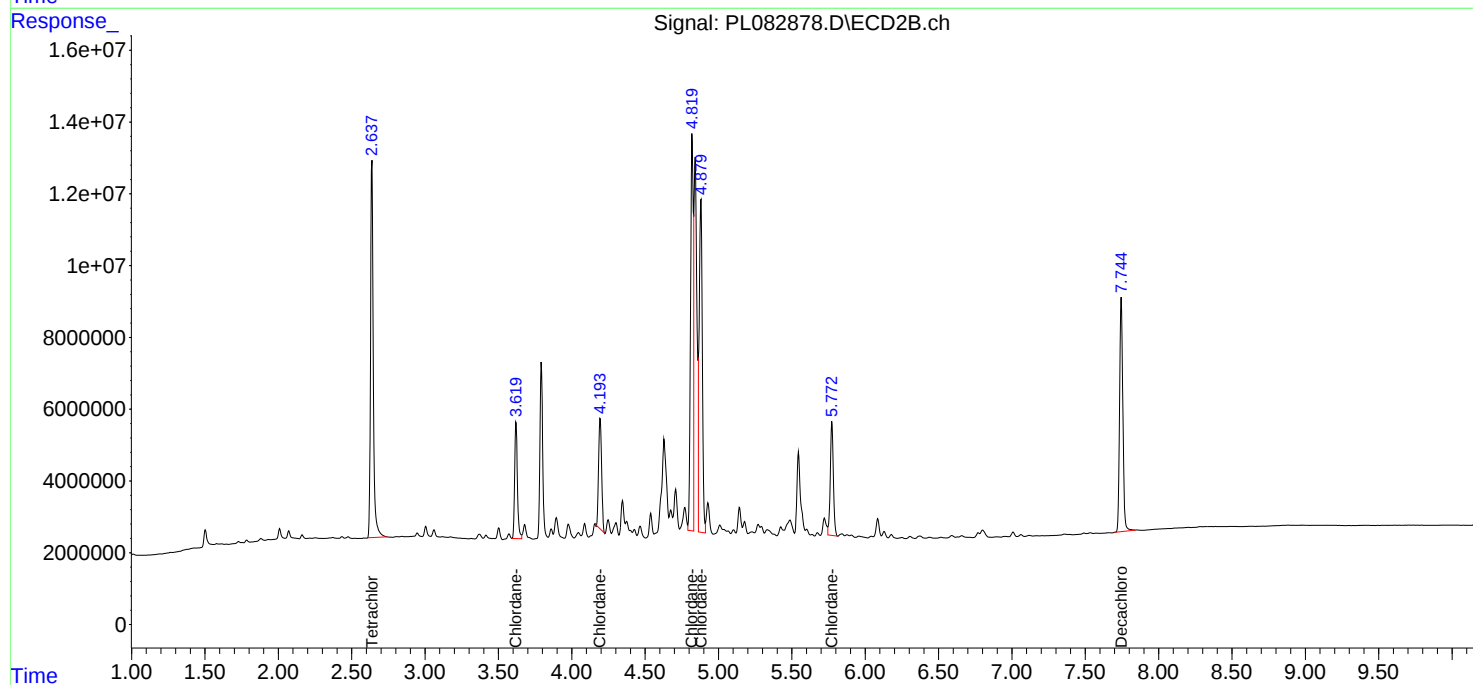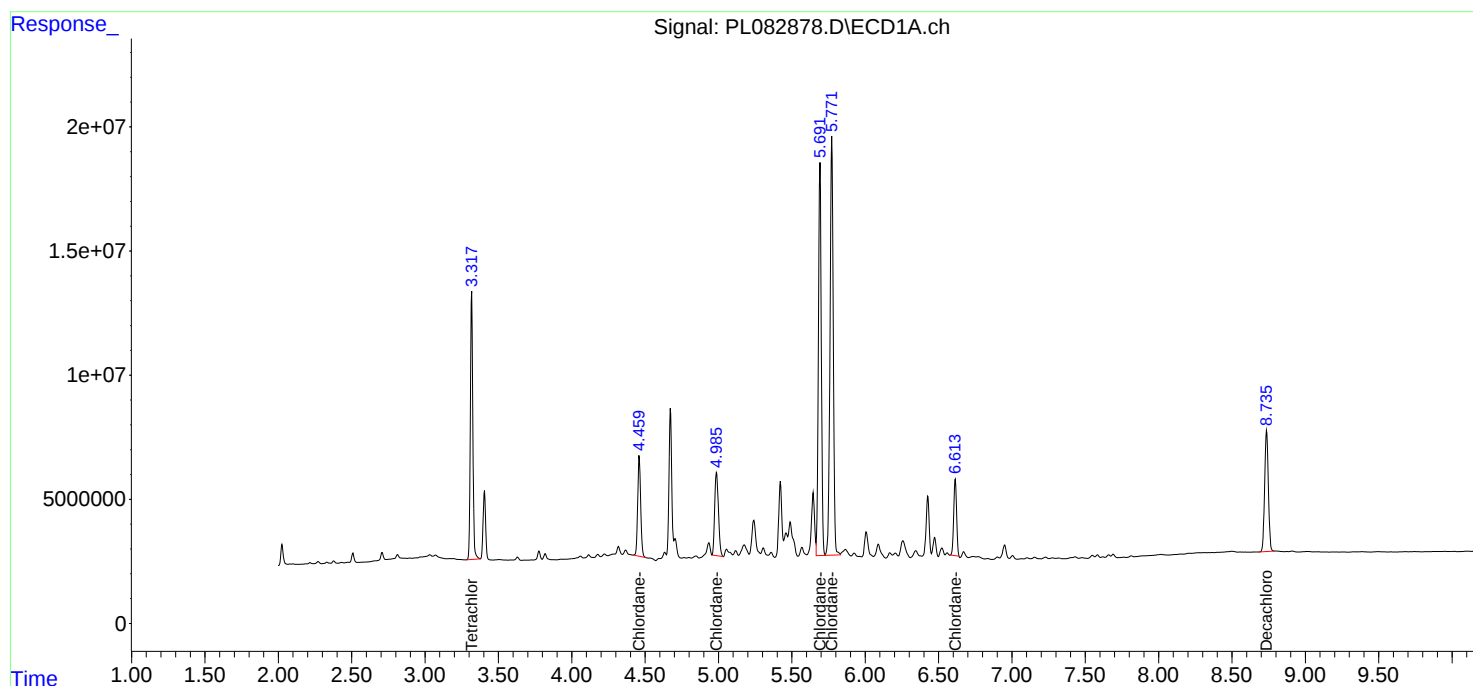


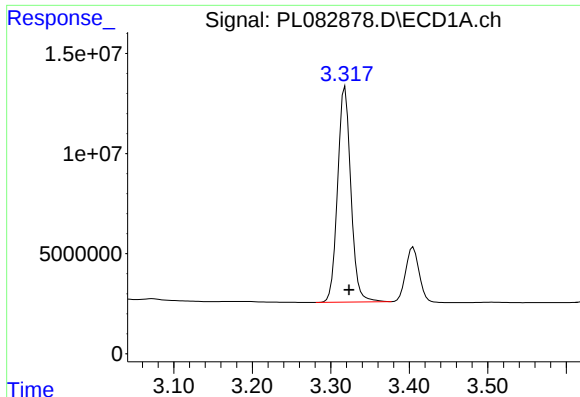

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: -0.005 min
Response: 126597351
Conc: 43.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

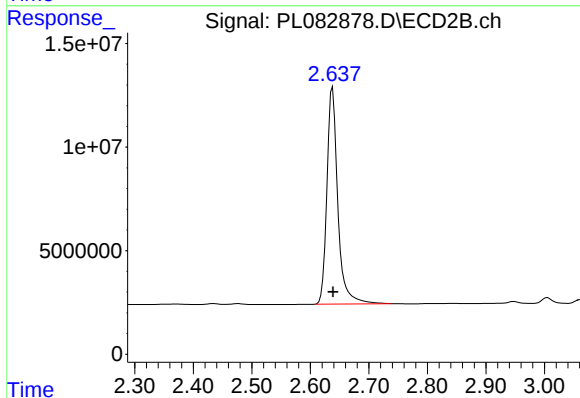


#1 Tetrachloro-m-xylene

R.T.: 2.638 min
Delta R.T.: 0.000 min
Response: 135324449
Conc: 52.13 ng/ml

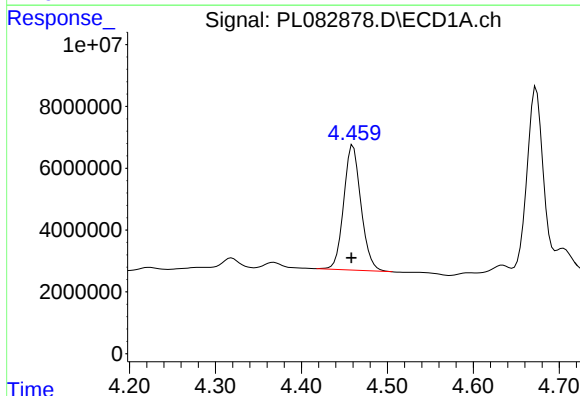


#23 Chlordane-1

R.T.: 4.460 min
Delta R.T.: 0.002 min
Response: 56410287
Conc: 515.63 ng/ml

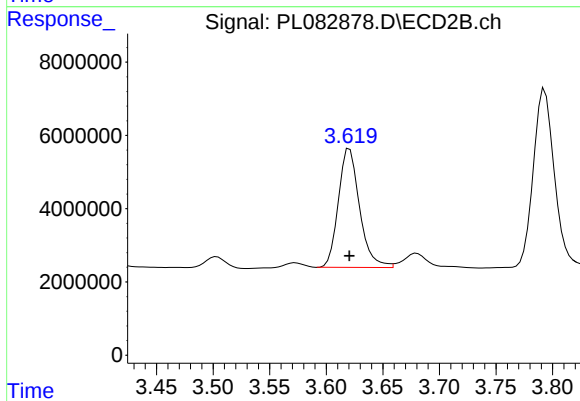

#23 Chlordane-1


R.T.: 3.621 min
Delta R.T.: 0.000 min
Response: 42344684
Conc: 513.19 ng/ml

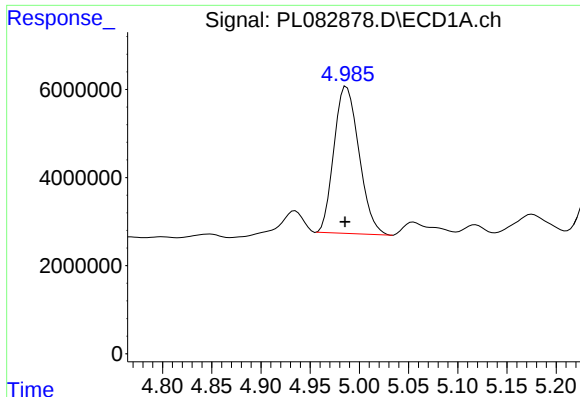

#24 Chlordane-2


R.T.: 4.987 min
Delta R.T.: 0.002 min
Response: 59142870
Conc: 536.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

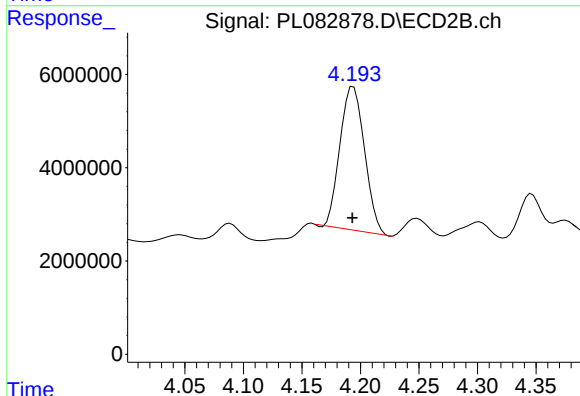


#24 Chlordane-2

R.T.: 4.194 min
Delta R.T.: 0.000 min
Response: 45011265
Conc: 505.58 ng/ml

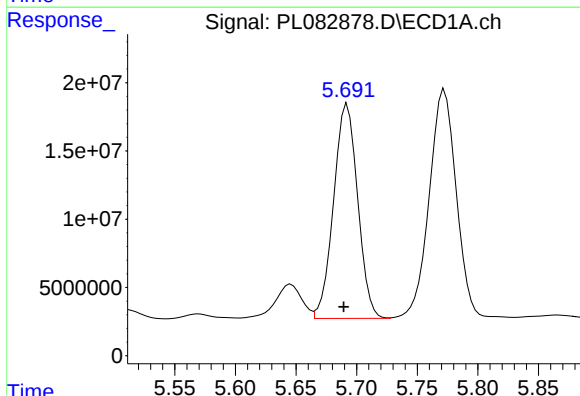


#25 Chlordane-3

R.T.: 5.692 min
Delta R.T.: 0.003 min
Response: 216990928
Conc: 522.99 ng/ml

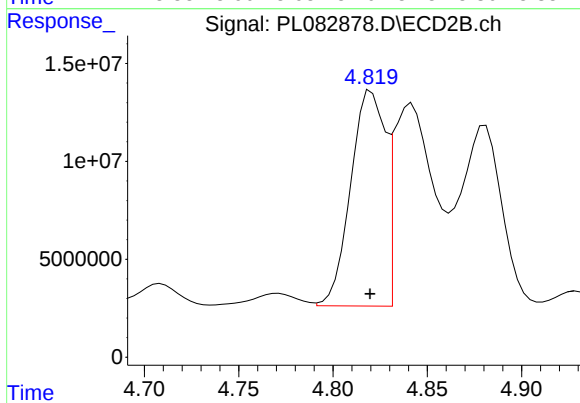

#25 Chlordane-3


R.T.: 4.820 min
Delta R.T.: 0.000 min
Response: 139750719
Conc: 524.38 ng/ml

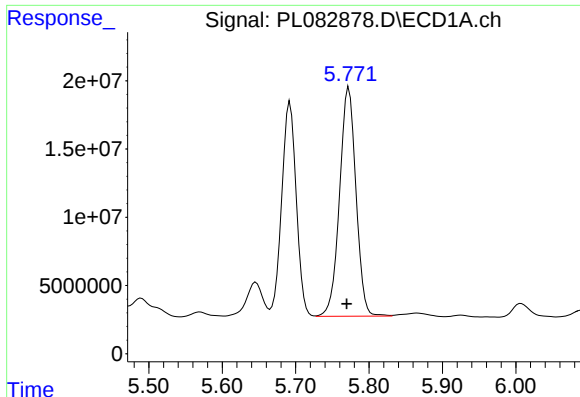

#26 Chlordane-4


R.T.: 5.773 min
Delta R.T.: 0.003 min
Response: 260840043
Conc: 515.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

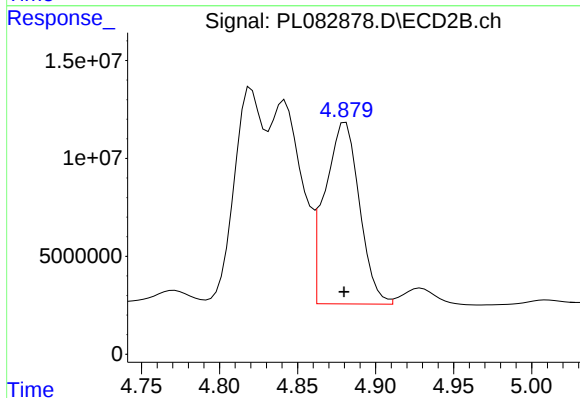


#26 Chlordane-4

R.T.: 4.881 min
Delta R.T.: 0.001 min
Response: 142489815
Conc: 505.73 ng/ml

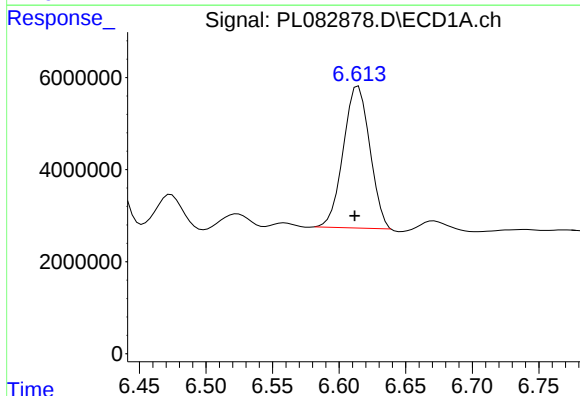


#27 Chlordane-5

R.T.: 6.614 min
Delta R.T.: 0.003 min
Response: 42745915
Conc: 520.87 ng/ml

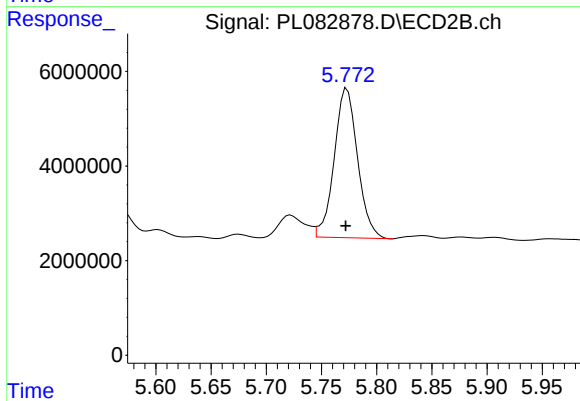

#27 Chlordane-5


R.T.: 5.773 min
Delta R.T.: 0.001 min
Response: 46561371
Conc: 479.29 ng/ml

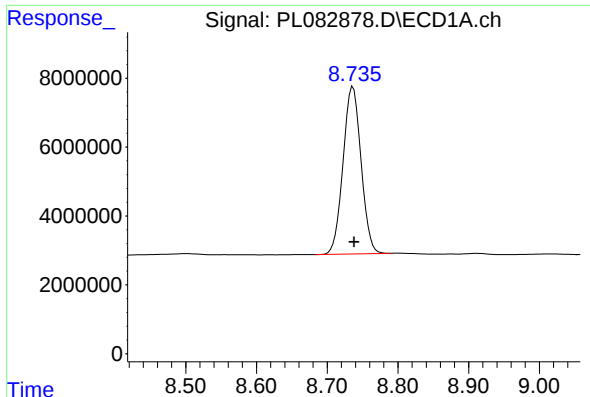

#28 Decachlorobiphenyl

R.T.: 8.736 min
Delta R.T.: -0.002 min
Response: 86009421
Conc: 41.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

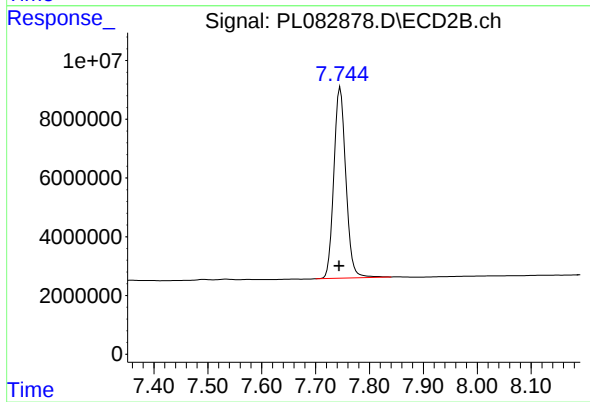

#28 Decachlorobiphenyl

R.T.: 7.746 min
Delta R.T.: 0.002 min
Response: 100718116
Conc: 40.51 ng/ml