

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052224\
 Data File : PL0895686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2024 17:36
 Operator : AR\AJ
 Sample : P2558-01 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/23/2024
 Supervised By :Ankita Jodhani 05/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 01:57:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 26 19:27:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.548	2.788	1410467	1662383	0.700m	1.296m#
28) SA Decachlor...	9.066	7.943	2217389	1874308	1.585m	1.393

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052224\
Data File : PL0895686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2024 17:36
Operator : AR\AJ
Sample : P2558-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/23/2024
Supervised By : Ankita Jodhani 05/23/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 01:57:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
Quant Title : GC Extractables
QLast Update : Fri Apr 26 19:27:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

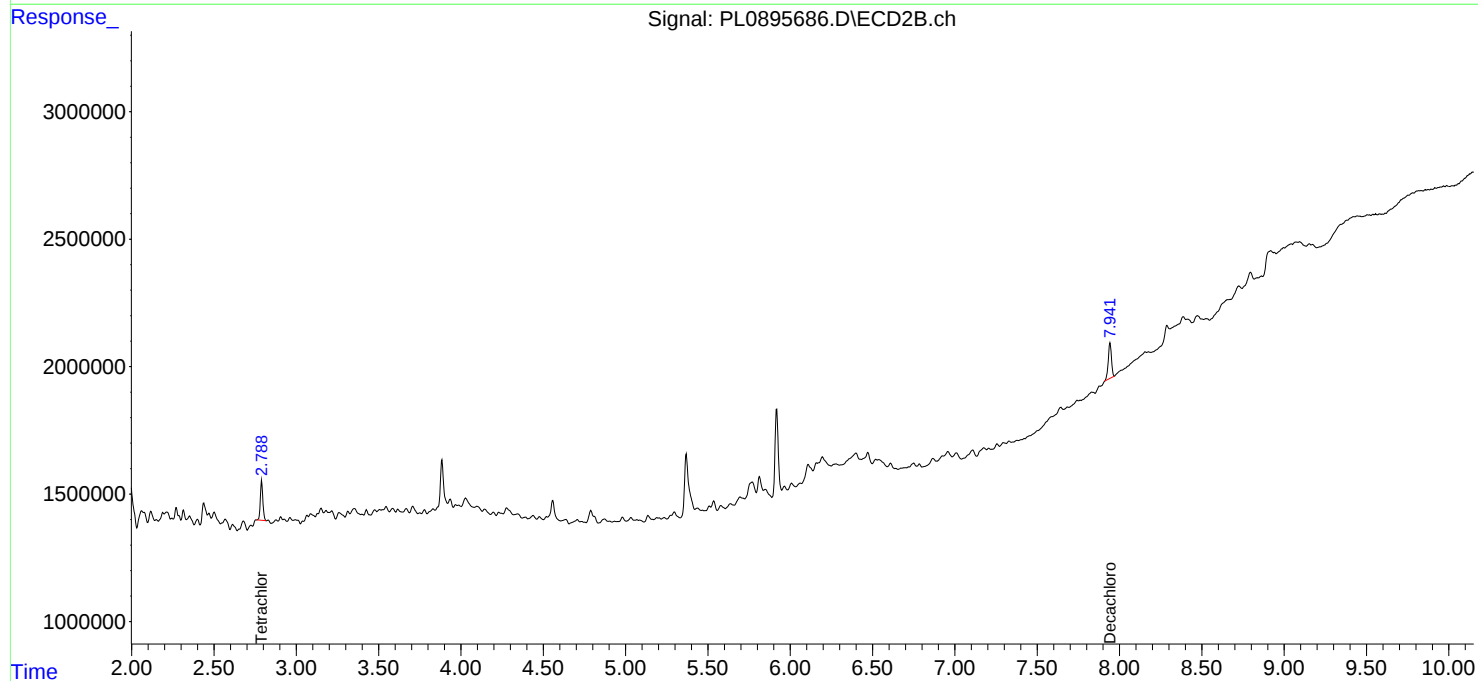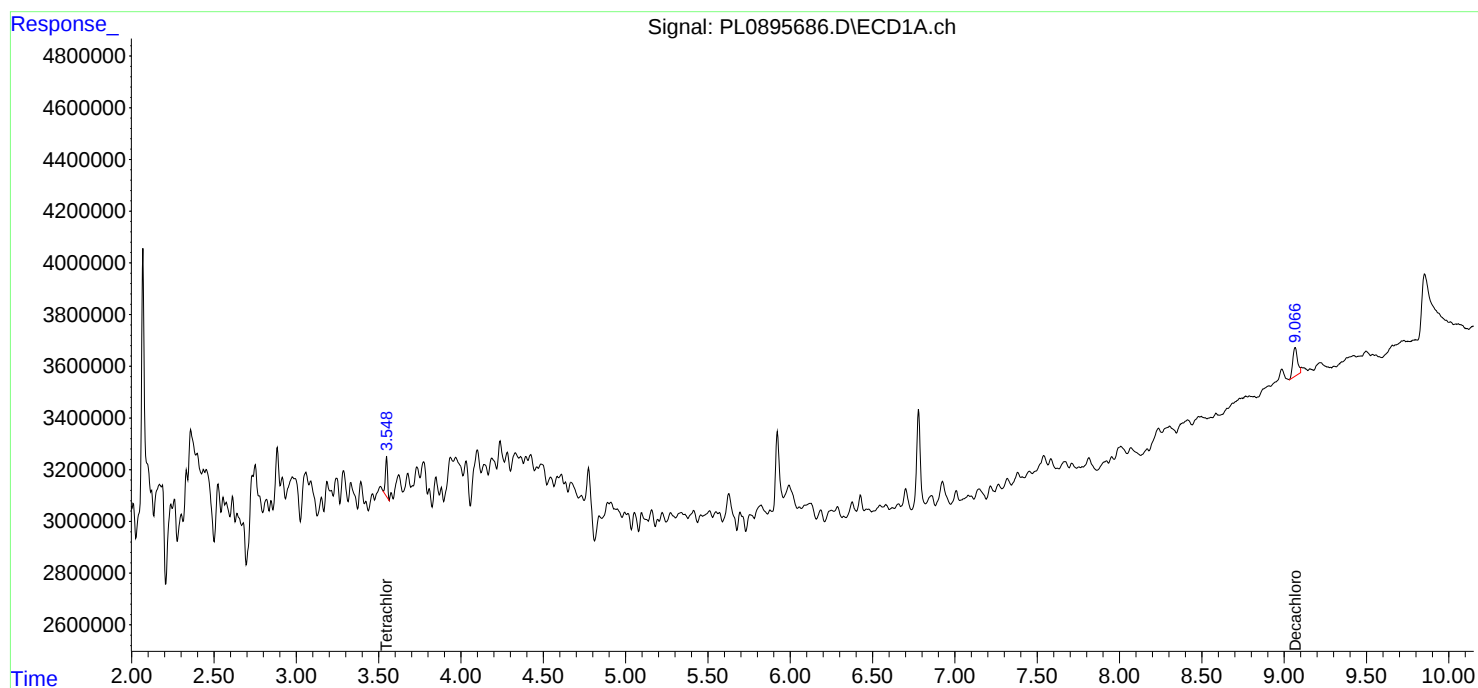

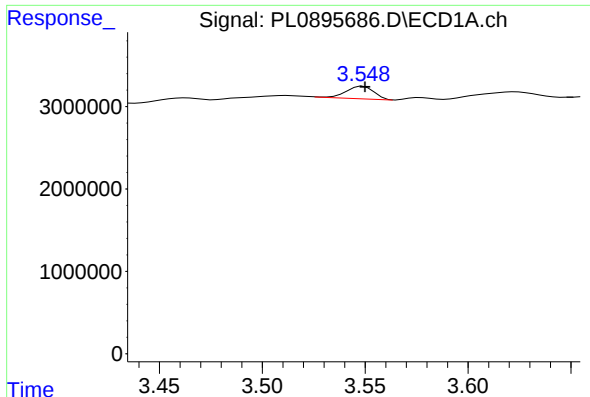


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: -0.002 min
Response: 1410467
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/23/2024
Supervised By :Ankita Jodhani 05/23/2024

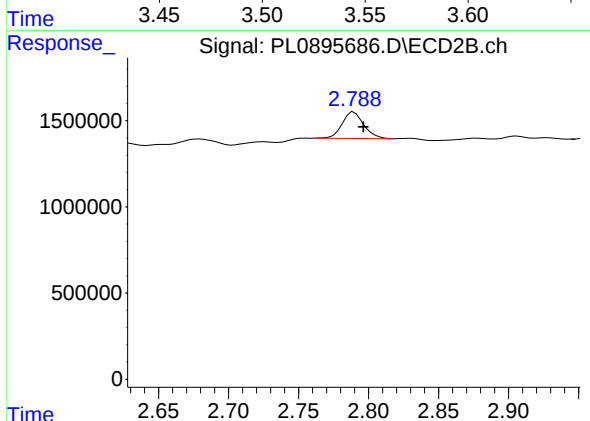


#1 Tetrachloro-m-xylene

R.T.: 2.788 min
Delta R.T.: -0.008 min
Response: 1662383
Conc: 1.30 ng/ml m

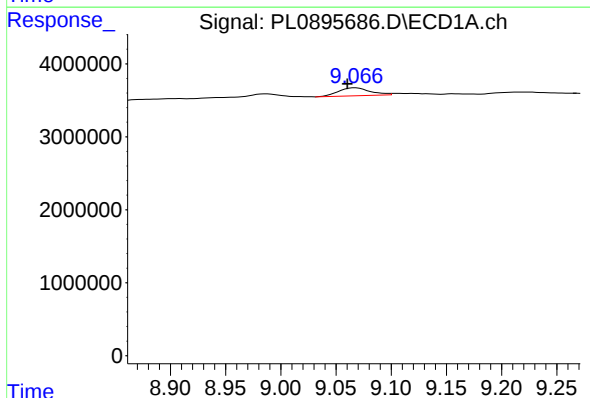

#28 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: 0.006 min
Response: 2217389
Conc: 1.58 ng/ml m

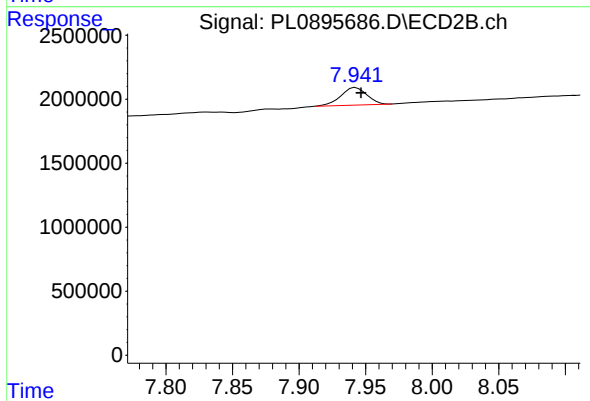

#28 Decachlorobiphenyl

R.T.: 7.943 min
Delta R.T.: -0.004 min
Response: 1874308
Conc: 1.39 ng/ml