

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052225\
 Data File : PL095769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2025 13:49
 Operator : AR\AJ
 Sample : Q2078-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-A1-06A-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 22:40:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.573	2.885	56880977	68248892	18.027	17.437
28)	SA Decachlor...	9.102	8.063	43395216	85148605	18.416	19.465
Target Compounds							
23)	Chlordane-1	0.000	3.900	0	12409402	N.D.	63.644 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052225\
Data File : PL095769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2025 13:49
Operator : AR\AJ
Sample : Q2078-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WC-A1-06A-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 22:40:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

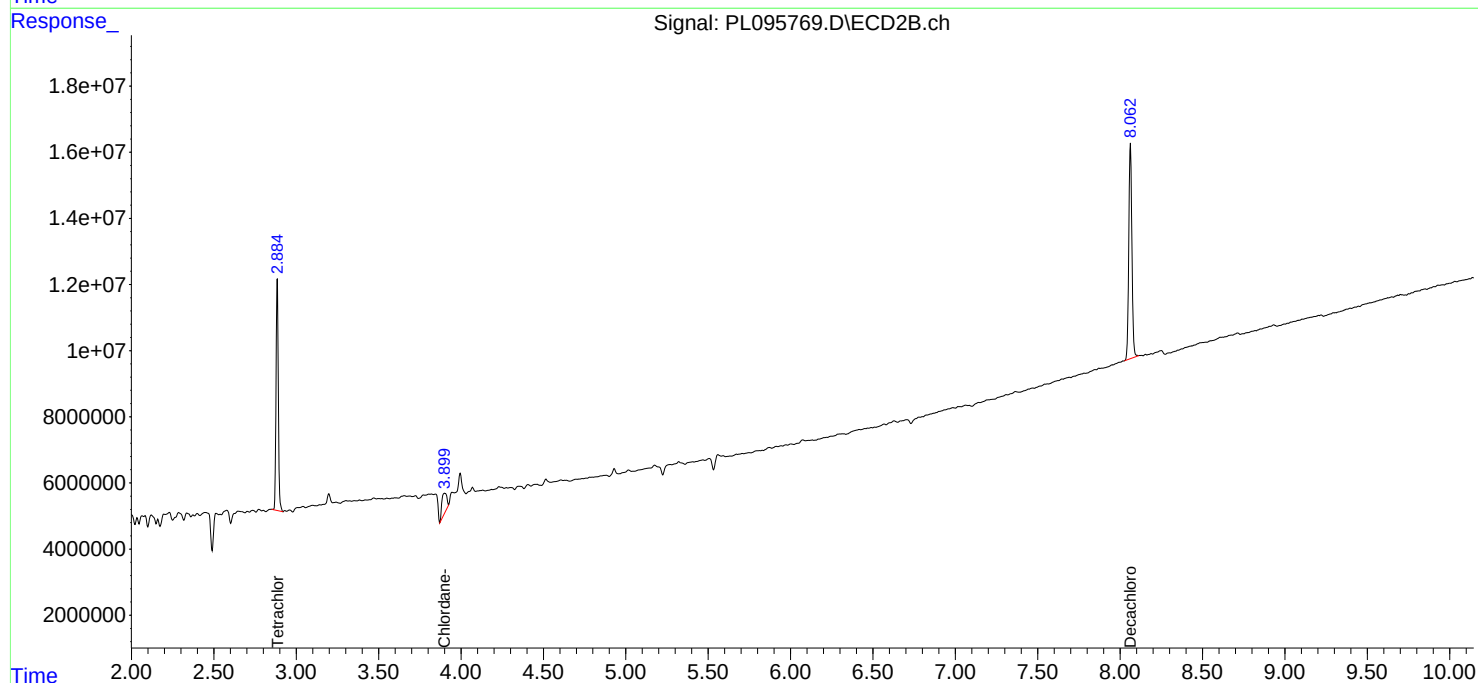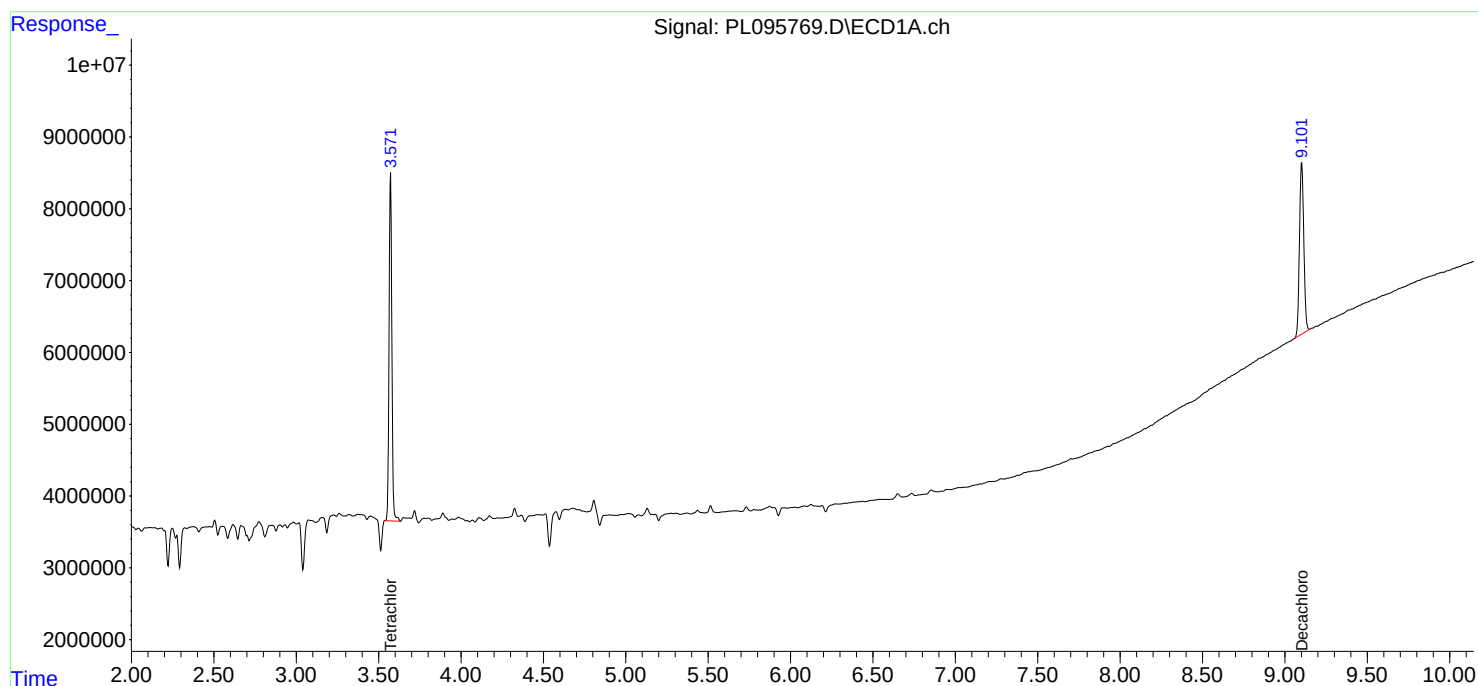


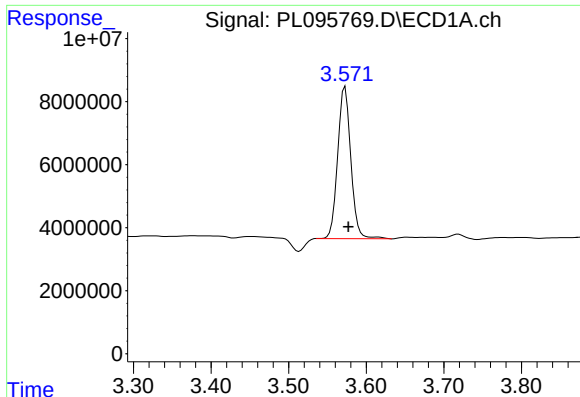

#1 Tetrachloro-m-xylene


R.T.: 3.573 min
Delta R.T.: -0.004 min
Response: 56880977
Conc: 18.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-A1-06A-C

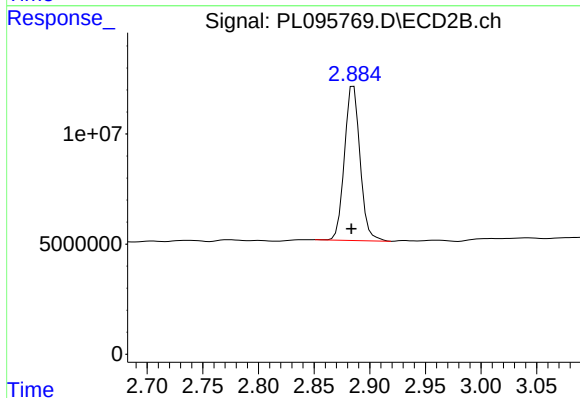


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.002 min
Response: 68248892
Conc: 17.44 ng/ml

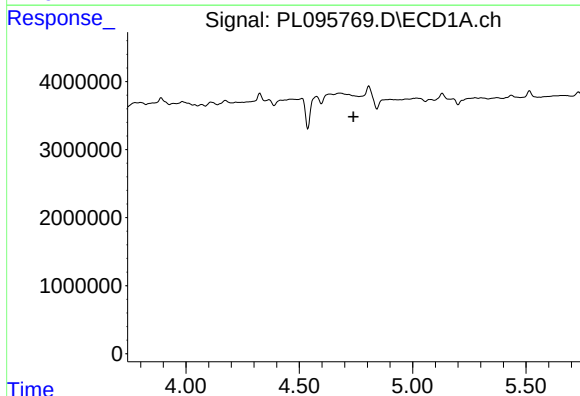


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.739 min
Response: 0
Conc: N.D.

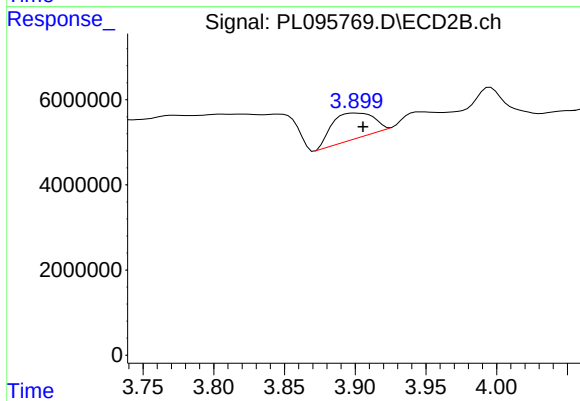

#23 Chlordane-1

R.T.: 3.900 min
Delta R.T.: -0.005 min
Response: 12409402
Conc: 63.64 ng/ml

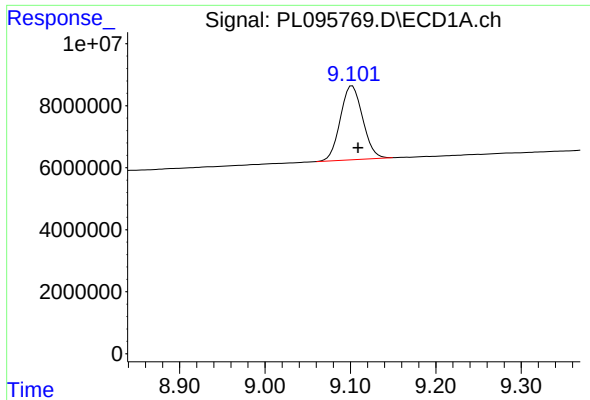

#28 Decachlorobiphenyl


R.T.: 9.102 min

Delta R.T.: -0.007 min

Response: 43395216

Conc: 18.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-A1-06A-C

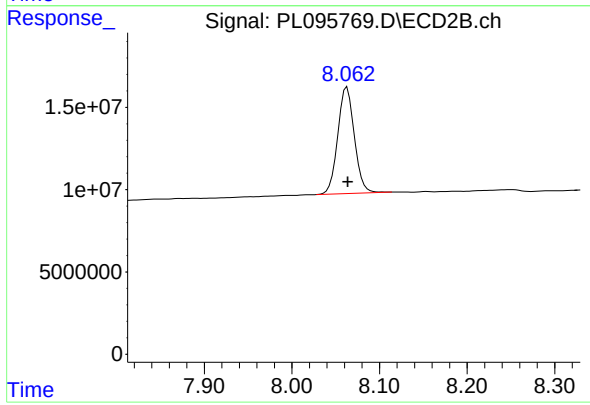

#28 Decachlorobiphenyl

R.T.: 8.063 min

Delta R.T.: 0.000 min

Response: 85148605

Conc: 19.46 ng/ml