

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052225\
 Data File : PL095771.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2025 14:16
 Operator : AR\AJ
 Sample : Q2078-19
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-A4-06-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 22:40:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.573	2.886	63493056	73015909	20.123	18.655
28)	SA Decachlor...	9.103	8.063	46988812	94610970	19.941	21.628
Target Compounds							
23)	Chlordane-1	0.000	3.902	0	17406255	N.D.	89.271 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052225\
Data File : PL095771.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2025 14:16
Operator : AR\AJ
Sample : Q2078-19
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WC-A4-06-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 22:40:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

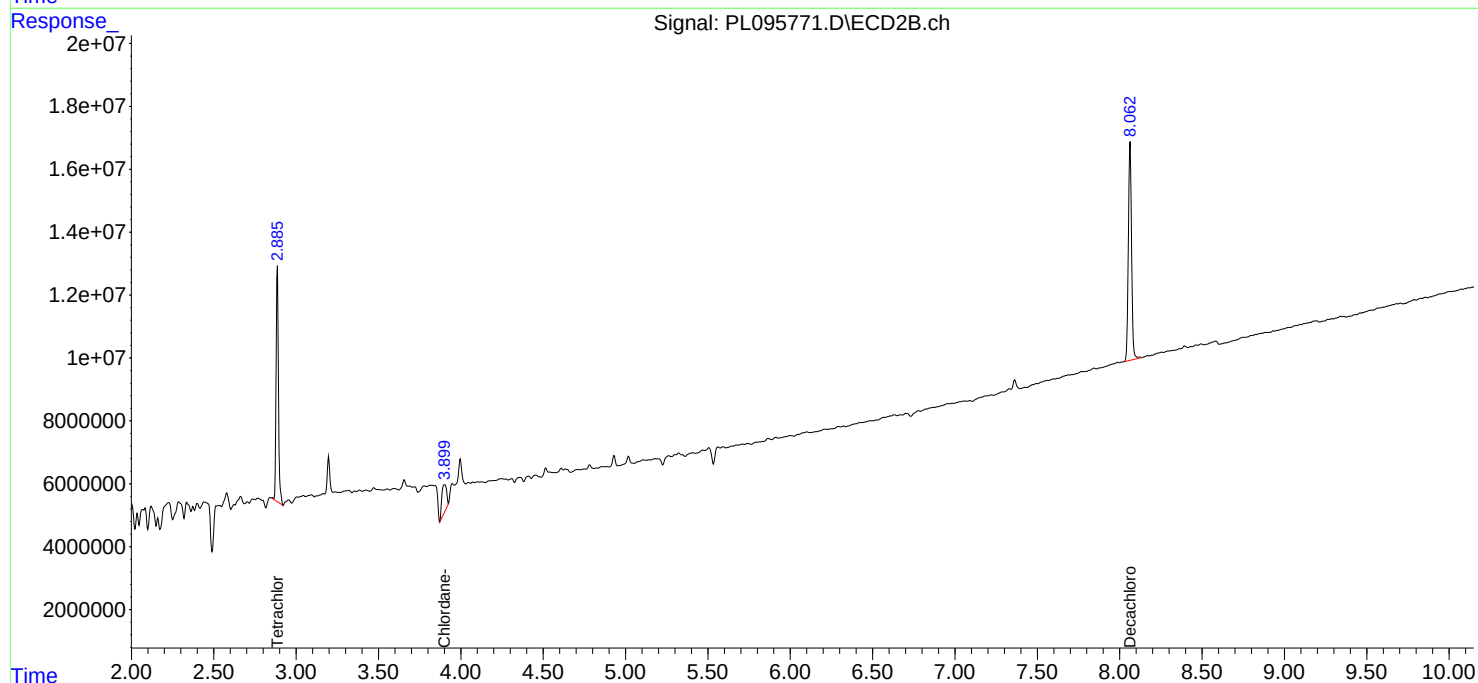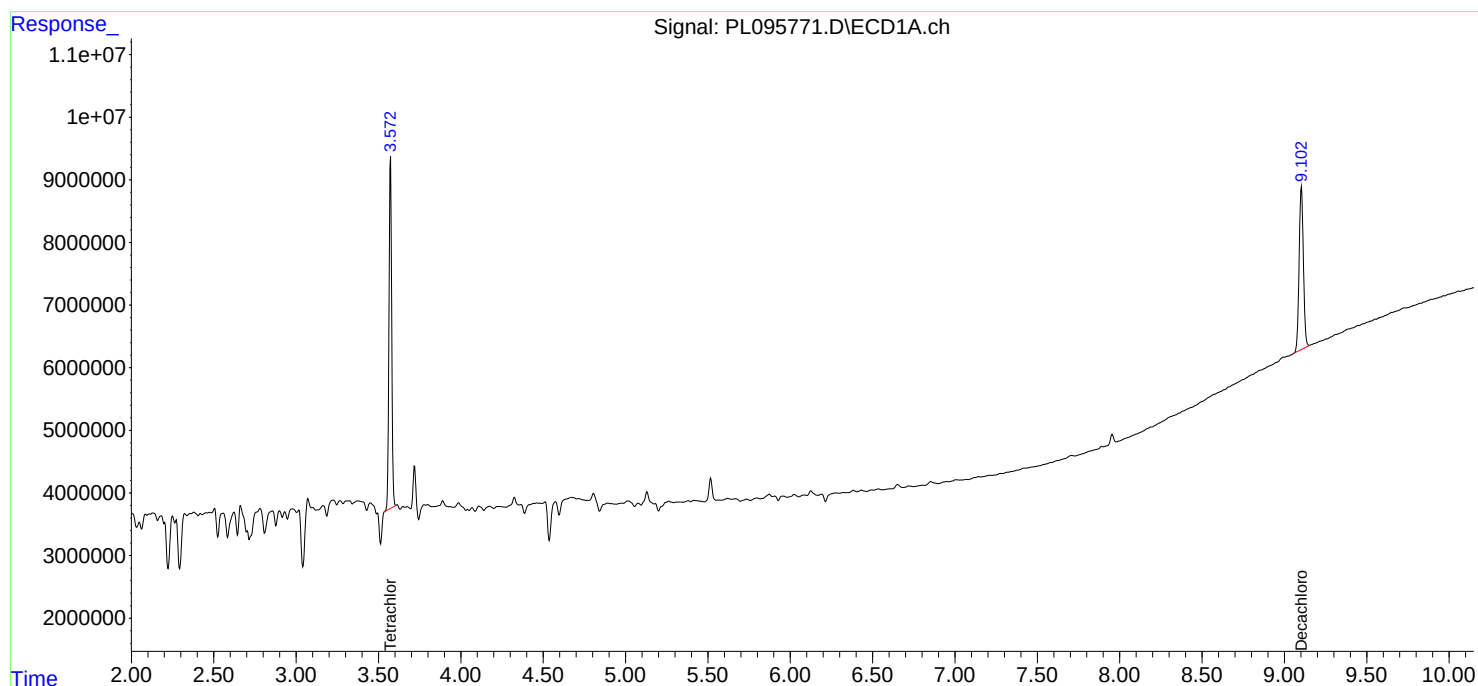


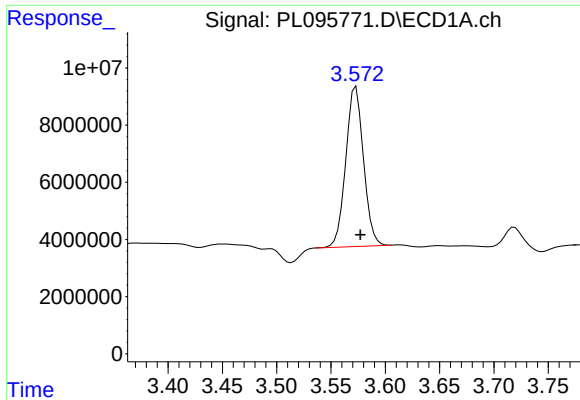

#1 Tetrachloro-m-xylene


R.T.: 3.573 min
Delta R.T.: -0.004 min
Response: 63493056
Conc: 20.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-A4-06-C

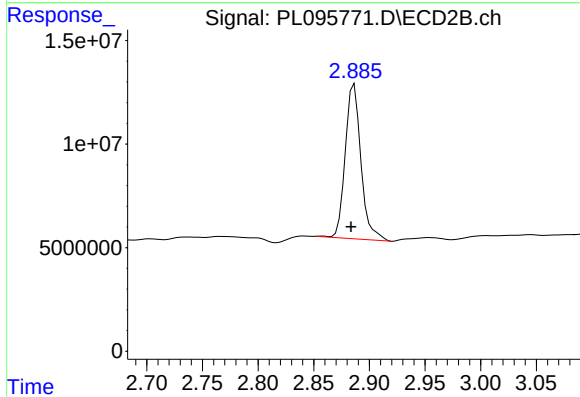


#1 Tetrachloro-m-xylene

R.T.: 2.886 min
Delta R.T.: 0.003 min
Response: 73015909
Conc: 18.66 ng/ml

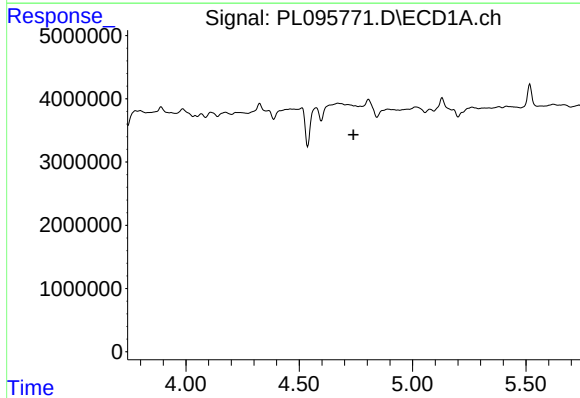


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.739 min
Response: 0
Conc: N.D.

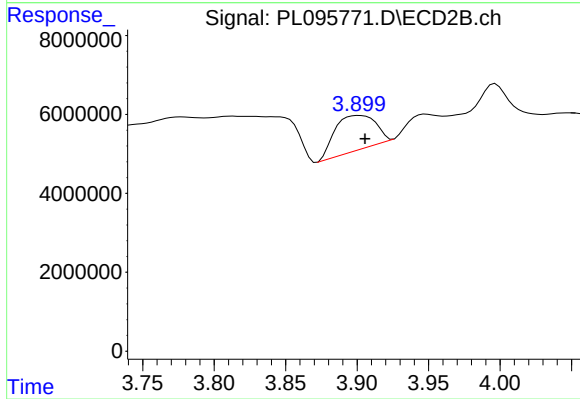

#23 Chlordane-1


R.T.: 3.902 min
Delta R.T.: -0.004 min
Response: 17406255
Conc: 89.27 ng/ml

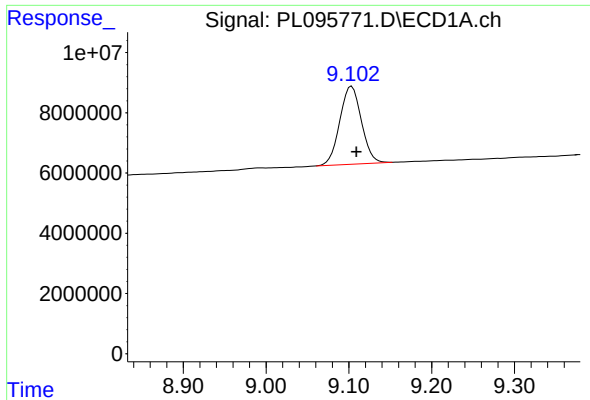

#28 Decachlorobiphenyl

R.T.: 9.103 min
Delta R.T.: -0.006 min
Response: 46988812
Conc: 19.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-A4-06-C

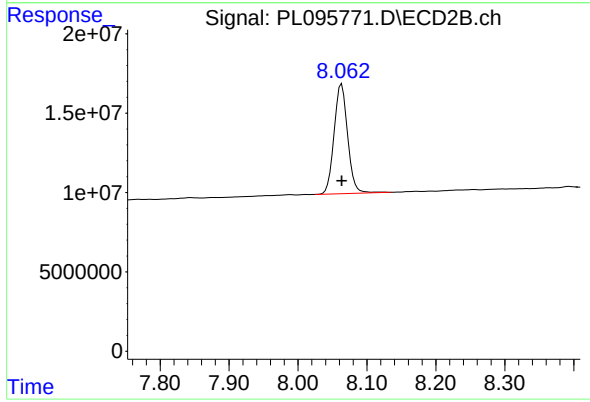

#28 Decachlorobiphenyl

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 94610970
Conc: 21.63 ng/ml