

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052319\
 Data File : PL048865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2019 09:37
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 00:59:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
Target Compounds							
8) B	Heptachlo...	0.000	5.800	0	29160102	N.D.	9.998 #
9) A	Endosulfan I	5.338f	0.000	5485424	0	0.456	N.D. #
12) B	4,4'-DDE	5.416f	0.000	152.6E6	0	12.027	N.D. #
13) MA	Dieldrin	5.544f	0.000	154.6E6	0	11.876	N.D. #
14) MA	Endrin	5.834f	0.000	17175208	0	1.411	N.D. #
15) B	Endosulfa...	6.079	0.000	51659419	0	4.476	N.D. #
16) A	4,4'-DDD	5.953	0.000	11673133	0	1.199	N.D. #
17) MA	4,4'-DDT	6.187	0.000	130.7E6	0	13.008	N.D. #
18) B	Endrin al...	6.276f	0.000	135.0E6	0	13.888	N.D. #
19) B	Endosulfa...	0.000	7.164f	0	4417223	N.D.	1.707 #
20) A	Methoxychlor	6.740	0.000	195.2E6	0	35.849	N.D. #
27)	Chlordane-5	6.079	0.000	51659419	0	110.018	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052319\
Data File : PL048865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2019 09:37
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 00:59:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

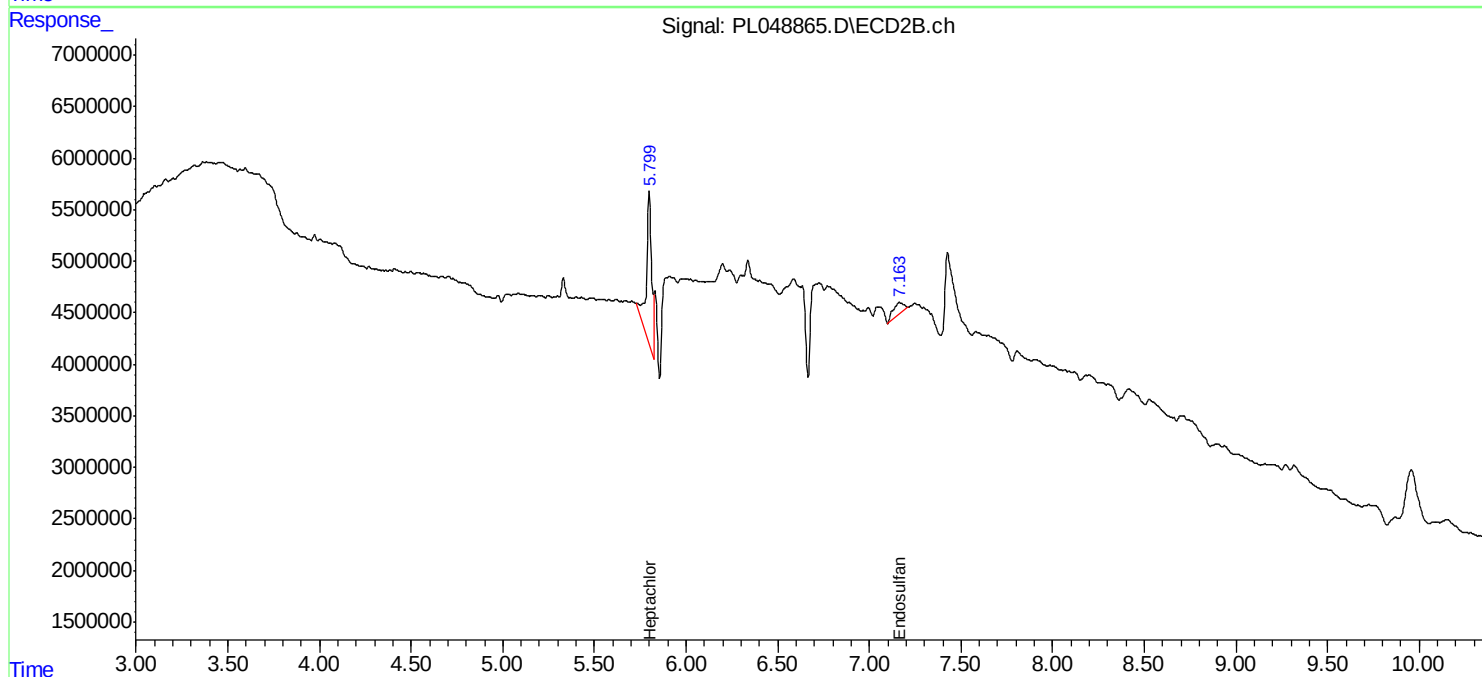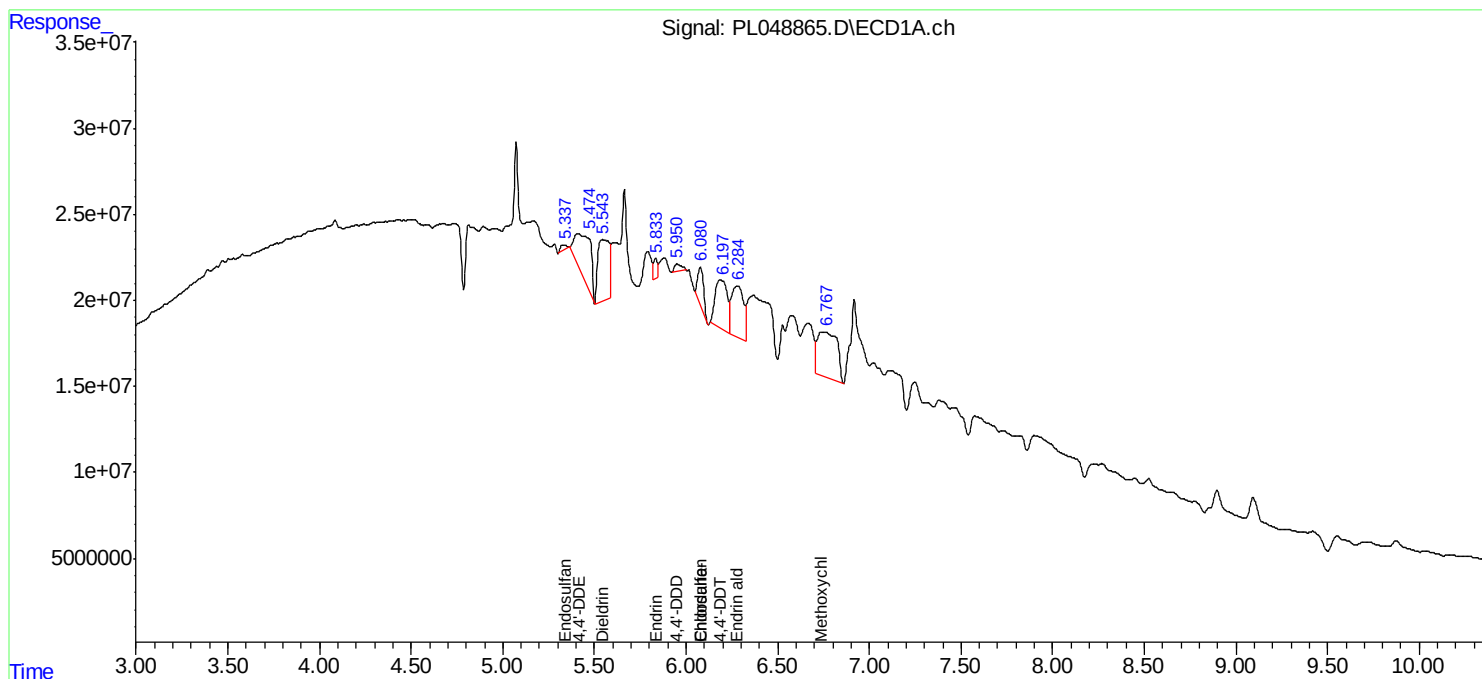


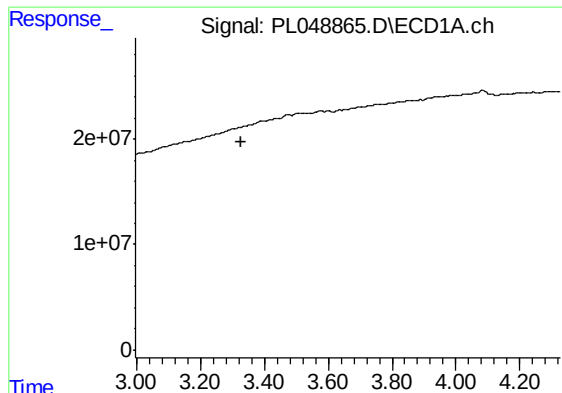

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

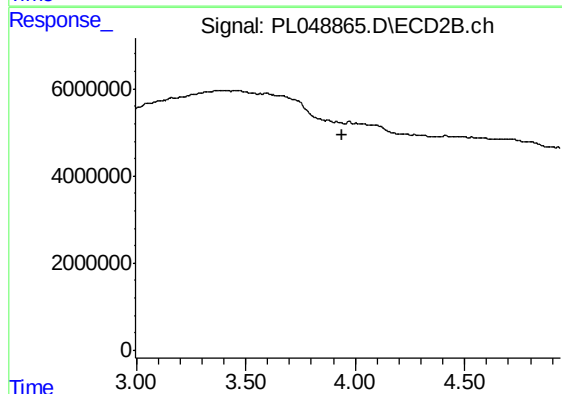


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.940 min
Response: 0
Conc: N.D.

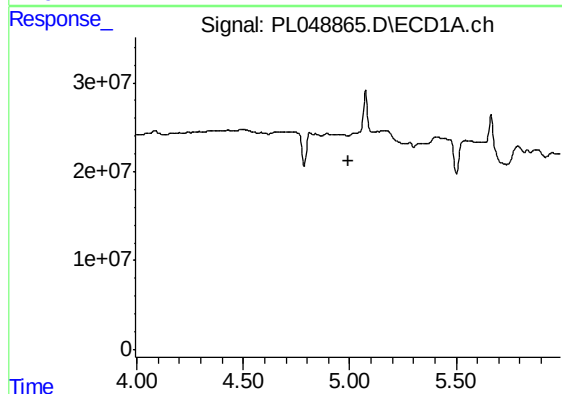


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.992 min
Response: 0
Conc: N.D.

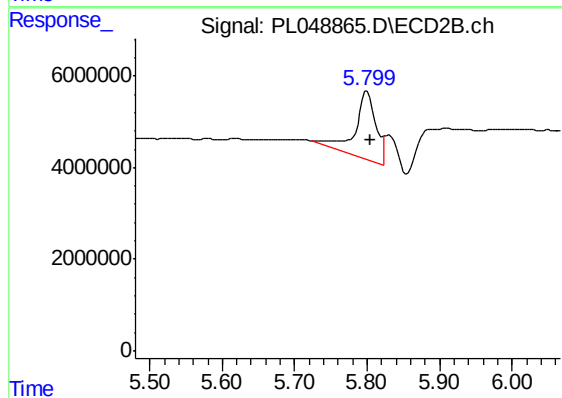

#8 Heptachlor epoxide


R.T.: 5.800 min
Delta R.T.: -0.004 min
Response: 29160102
Conc: 10.00 ng/ml

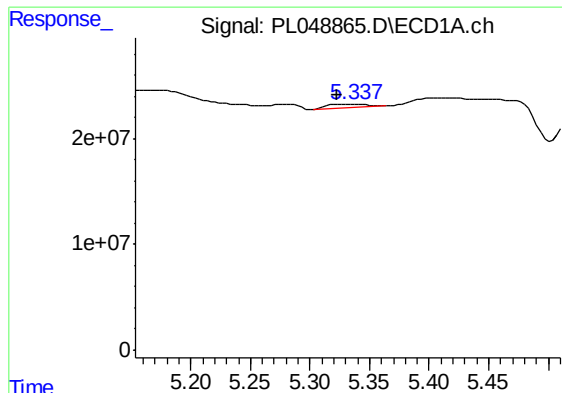

#9 Endosulfan I


R.T.: 5.338 min
Delta R.T.: 0.015 min
Response: 5485424
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

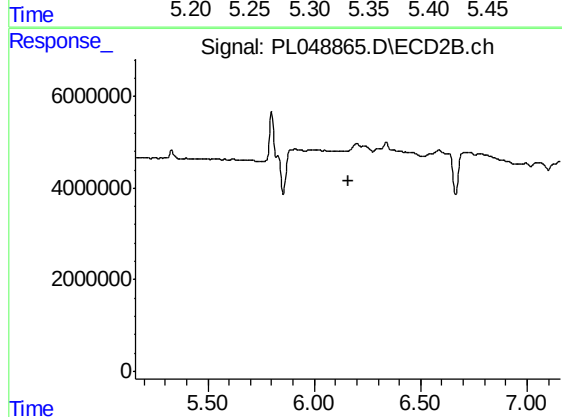


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.159 min
Response: 0
Conc: N.D.

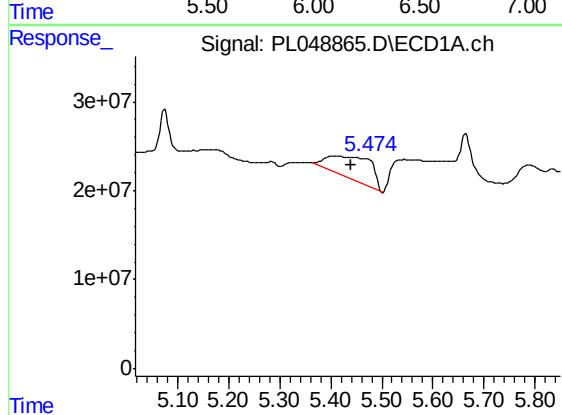


#12 4,4'-DDE

R.T.: 5.416 min
Delta R.T.: -0.023 min
Response: 152562164
Conc: 12.03 ng/ml

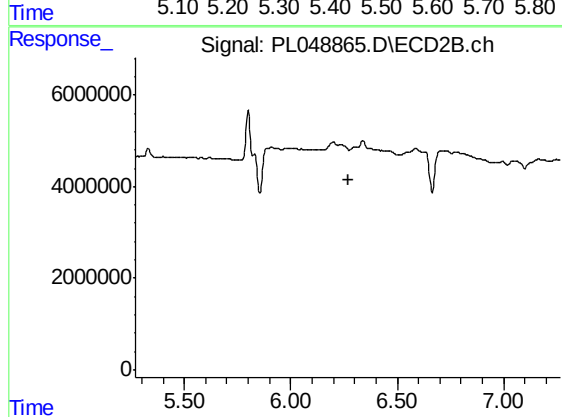

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.269 min
Response: 0
Conc: N.D.

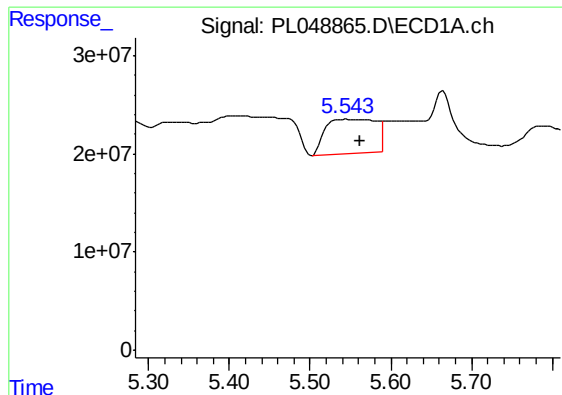

#13 Dieldrin


R.T.: 5.544 min
Delta R.T.: -0.018 min
Response: 154640292
Conc: 11.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

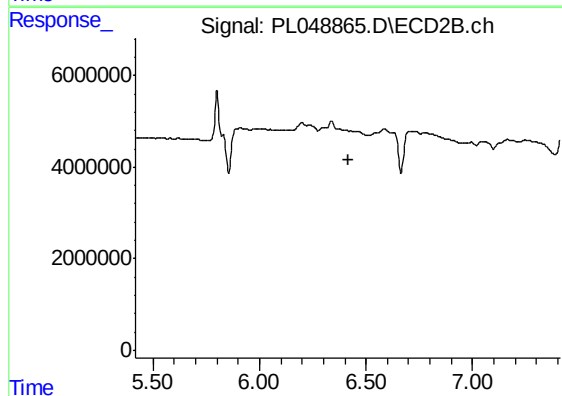


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

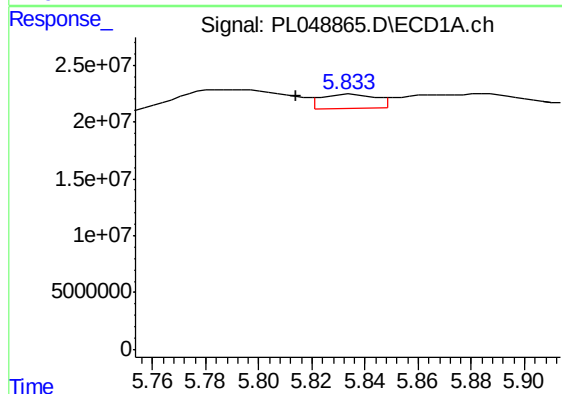


#14 Endrin

R.T.: 5.834 min
Delta R.T.: 0.020 min
Response: 17175208
Conc: 1.41 ng/ml

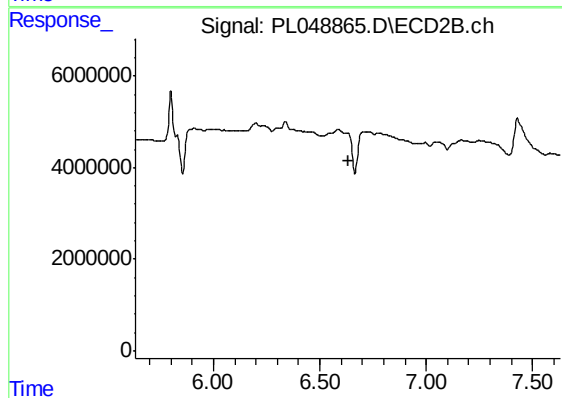

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

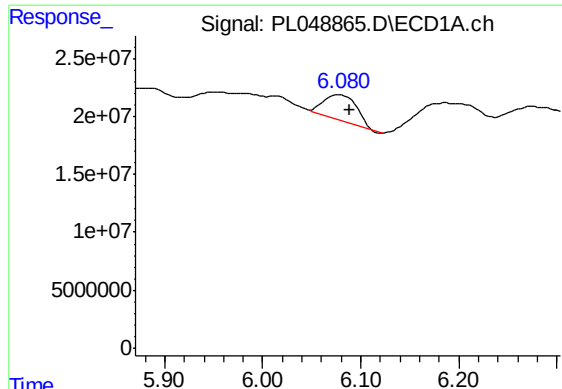

#15 Endosulfan II


R.T.: 6.079 min
Delta R.T.: -0.011 min
Response: 51659419
Conc: 4.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

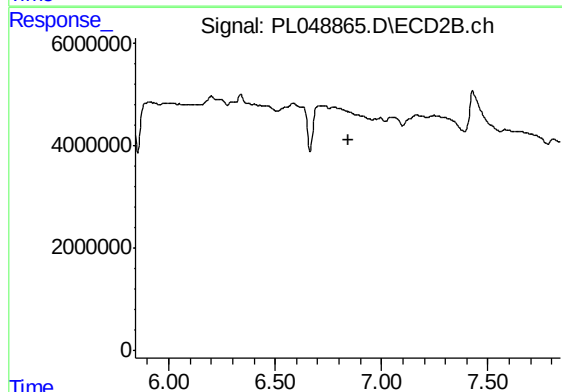


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.843 min
Response: 0
Conc: N.D.

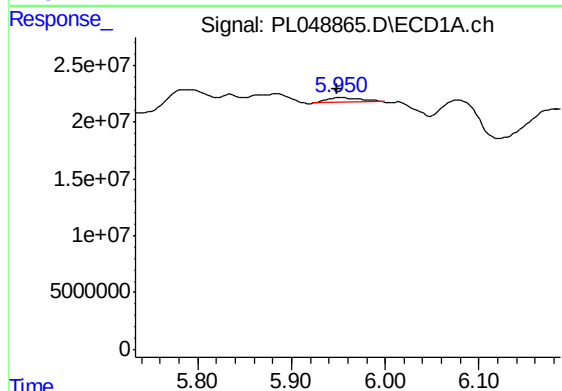


#16 4,4'-DDD

R.T.: 5.953 min
Delta R.T.: 0.004 min
Response: 11673133
Conc: 1.20 ng/ml

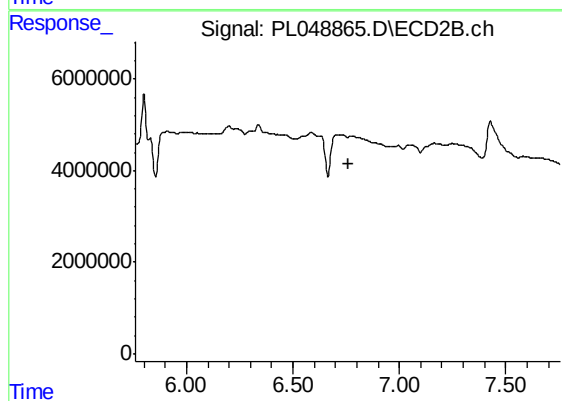

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

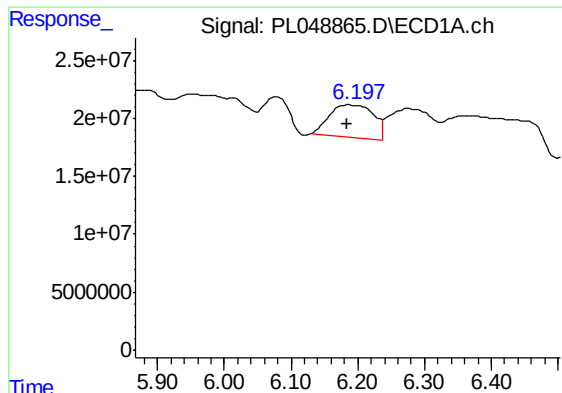

#17 4,4'-DDT


R.T.: 6.187 min
Delta R.T.: 0.003 min
Response: 130680134
Conc: 13.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

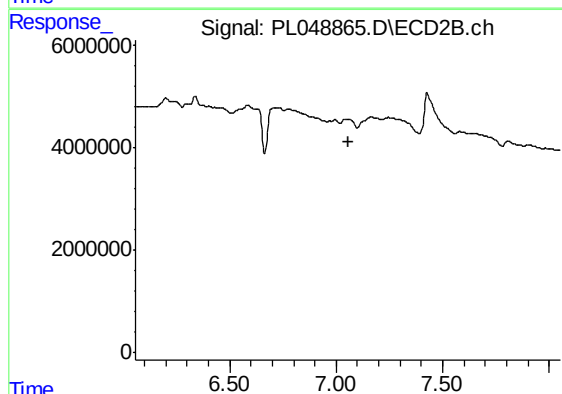


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.057 min
Response: 0
Conc: N.D.

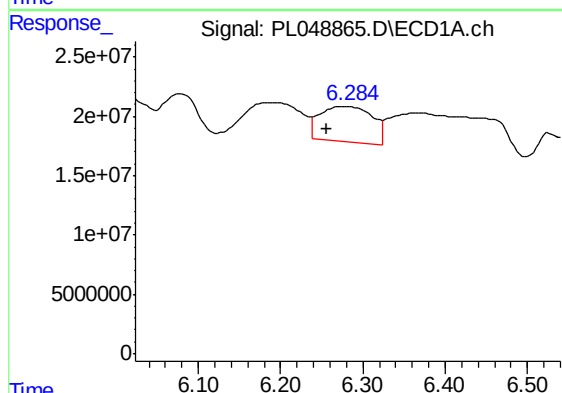


#18 Endrin aldehyde

R.T.: 6.276 min
Delta R.T.: 0.020 min
Response: 134971969
Conc: 13.89 ng/ml

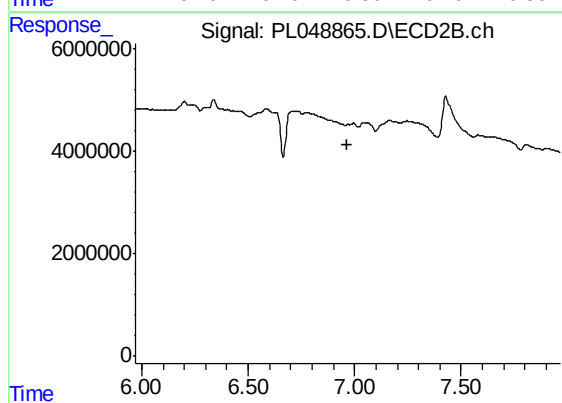

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.967 min
Response: 0
Conc: N.D.

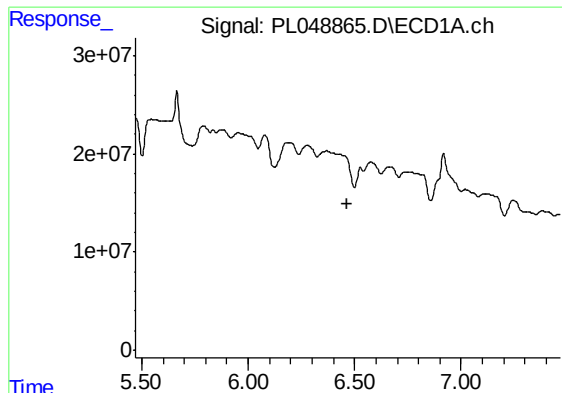

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.468 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

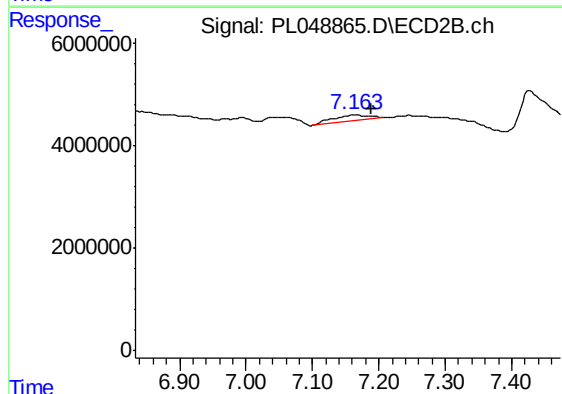


#19 Endosulfan Sulfate

R.T.: 7.164 min
Delta R.T.: -0.026 min
Response: 4417223
Conc: 1.71 ng/ml

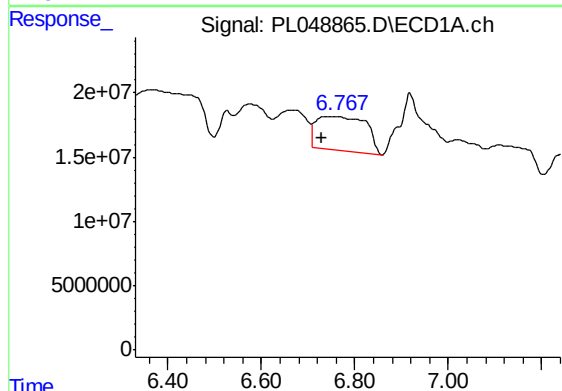


#20 Methoxychlor

R.T.: 6.740 min
Delta R.T.: 0.011 min
Response: 195190283
Conc: 35.85 ng/ml

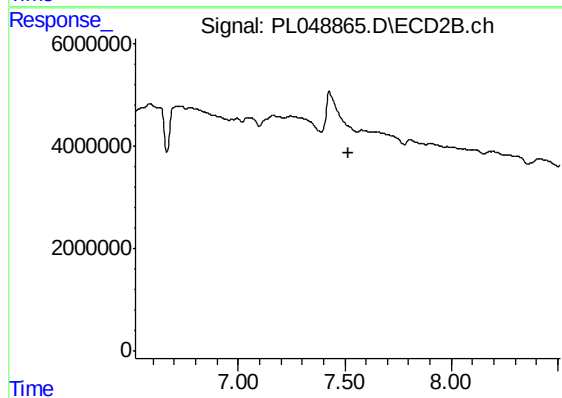

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.516 min
Response: 0
Conc: N.D.

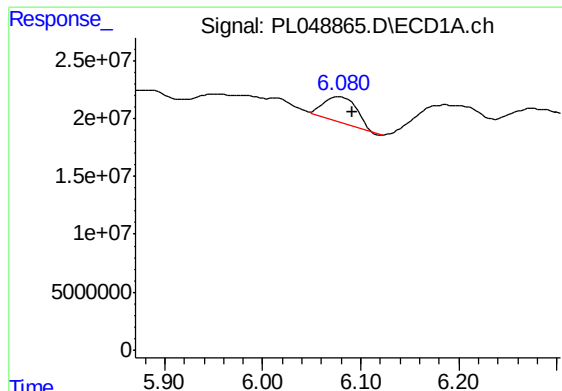

#27 Chlordane-5


R.T.: 6.079 min
Delta R.T.: -0.013 min
Response: 51659419
Conc: 110.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

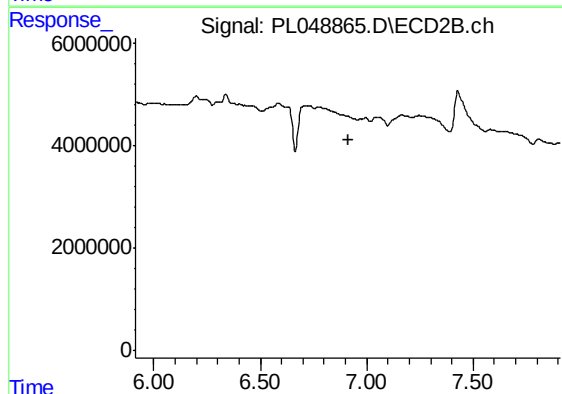


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.913 min
Response: 0
Conc: N.D.

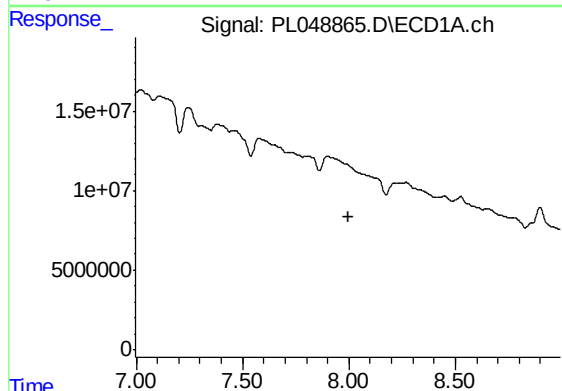

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.996 min
Response: 0
Conc: N.D.

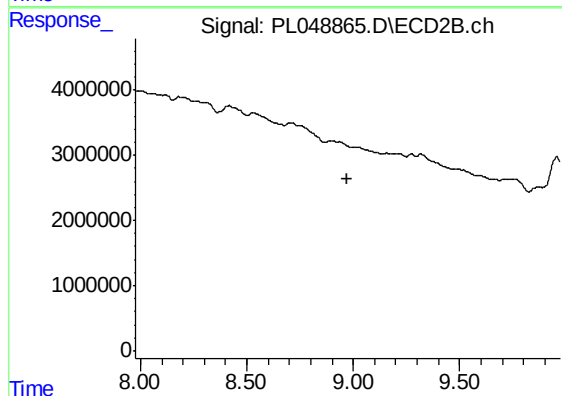

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.975 min
Response: 0
Conc: N.D.