

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052319\
 Data File : PL048871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2019 12:13
 Operator : SM\AJ
 Sample : K2970-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-9-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 01:01:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.326	3.938	56937753	14147895	5.878	5.680
28) SA Decachlor...	7.993	8.973	55256629	18298205	5.496	6.894 #
Target Compounds						
12) B 4,4'-DDE	5.436	6.266	15670729	4107519	1.235	1.488
17) MA 4,4'-DDT	6.176	0.000	3848444	0	0.383	N.D. #
20) A Methoxychlor	6.705f	0.000	9499675	0	1.745	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052319\
Data File : PL048871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2019 12:13
Operator : SM\AJ
Sample : K2970-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-9-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 01:01:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

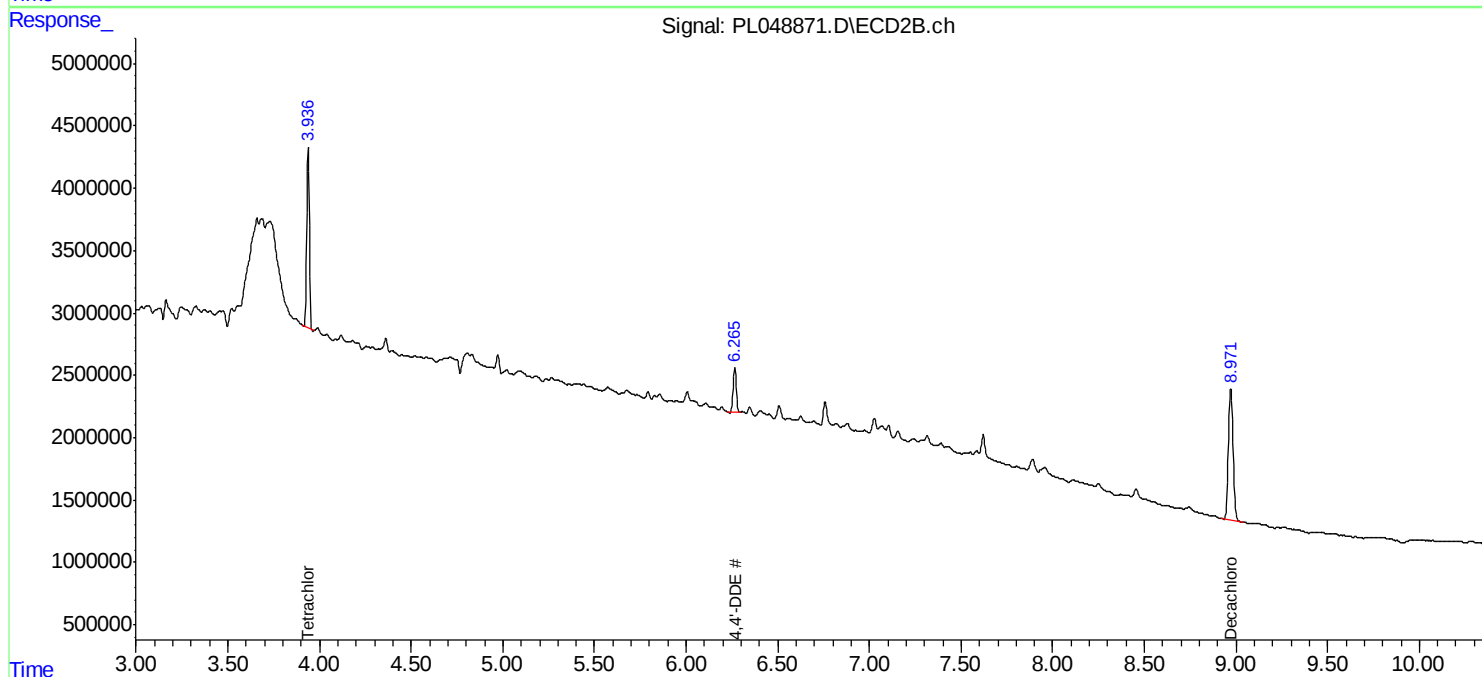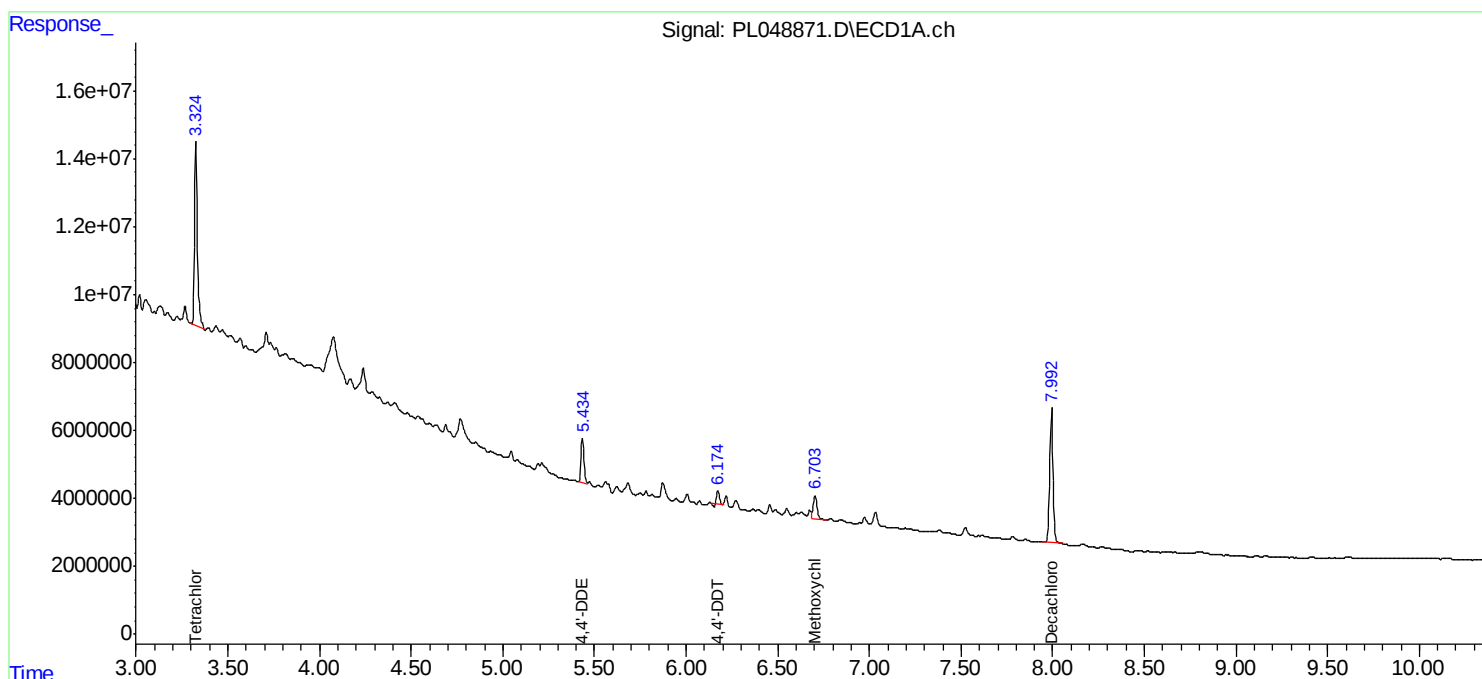


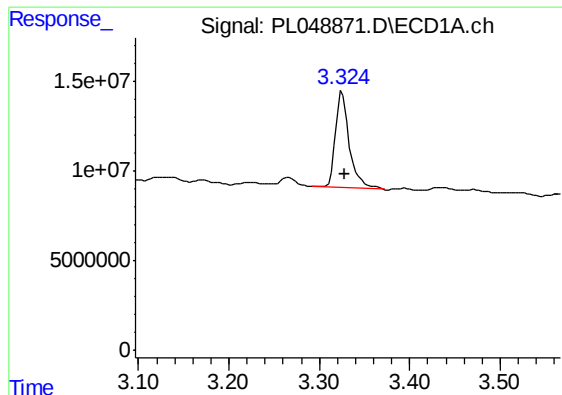

#1 Tetrachloro-m-xylene


R.T.: 3.326 min
Delta R.T.: -0.002 min
Response: 56937753
Conc: 5.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-9-S

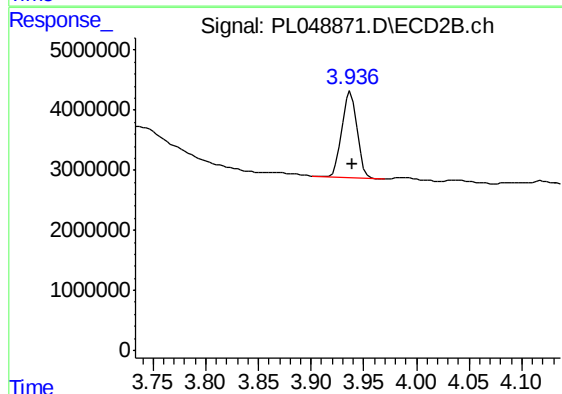


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: -0.002 min
Response: 14147895
Conc: 5.68 ng/ml

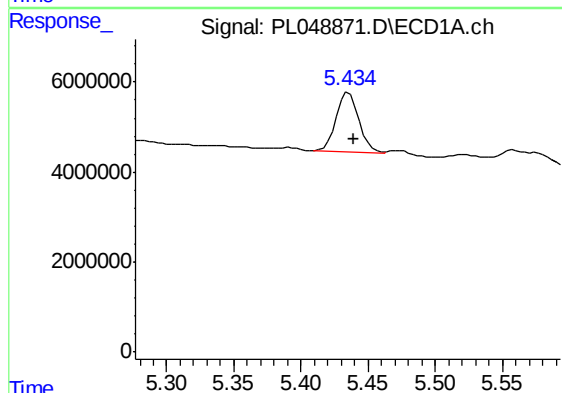


#12 4,4'-DDE

R.T.: 5.436 min
Delta R.T.: -0.003 min
Response: 15670729
Conc: 1.24 ng/ml

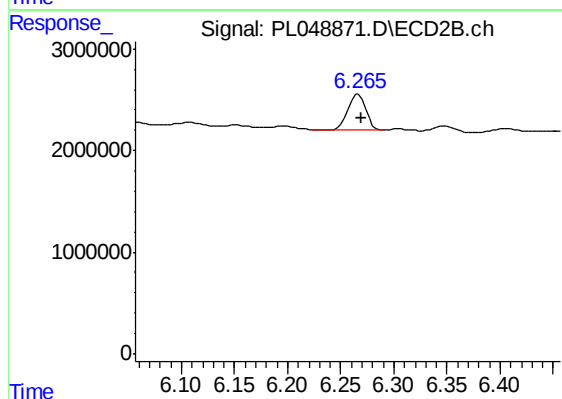

#12 4,4'-DDE


R.T.: 6.266 min
Delta R.T.: -0.003 min
Response: 4107519
Conc: 1.49 ng/ml

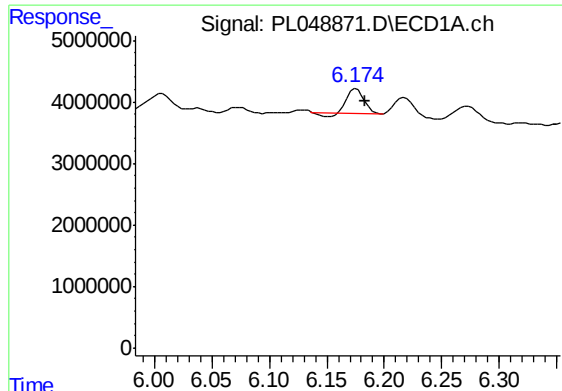

#17 4,4'-DDT


R.T.: 6.176 min
Delta R.T.: -0.008 min
Response: 3848444
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-9-S

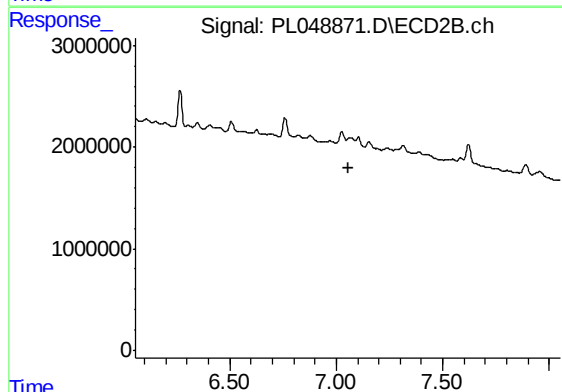


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.057 min
Response: 0
Conc: N.D.

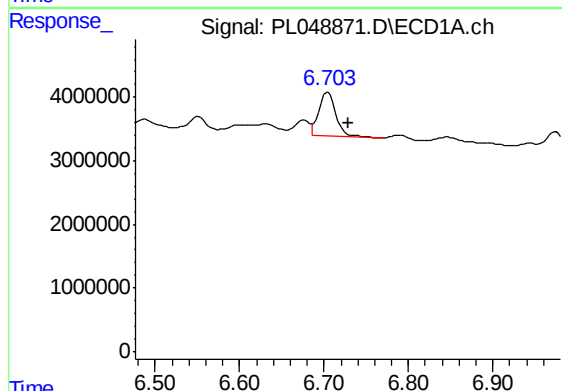


#20 Methoxychlor

R.T.: 6.705 min
Delta R.T.: -0.024 min
Response: 9499675
Conc: 1.74 ng/ml

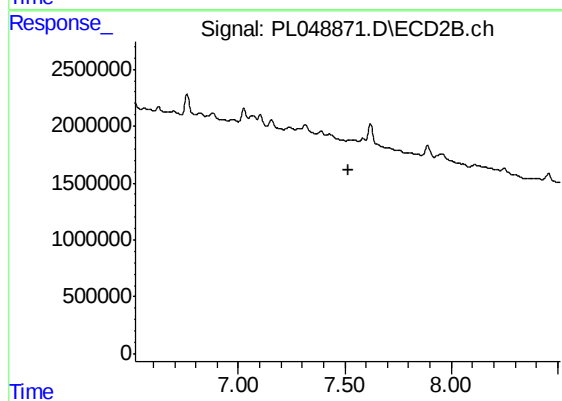

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.516 min
Response: 0
Conc: N.D.

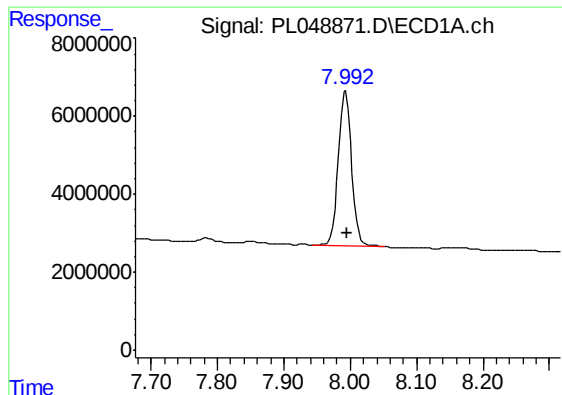

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.002 min
Response: 55256629
Conc: 5.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-9-S

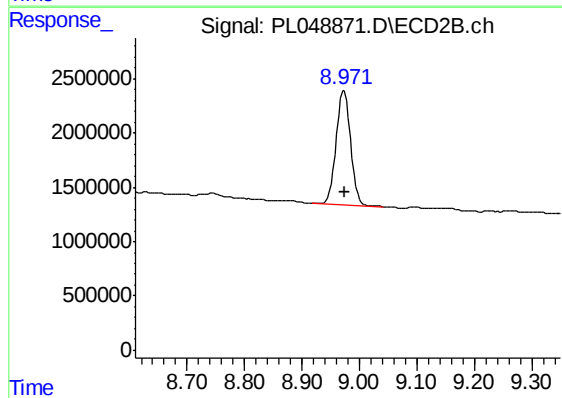

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: -0.002 min
Response: 18298205
Conc: 6.89 ng/ml