

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052319\
 Data File : PL048891.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2019 18:41
 Operator : SM\AJ
 Sample : K3008-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-20

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 01:06:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.325	3.938	186.2E6	50907438	19.219	20.437
28) SA Decachlor...	7.992	8.973	186.3E6	55491264	18.528	20.906
Target Compounds						
3) MA gamma-BHC...	4.037	0.000	16061618	0	1.130	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052319\
Data File : PL048891.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2019 18:41
Operator : SM\AJ
Sample : K3008-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-20

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 01:06:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

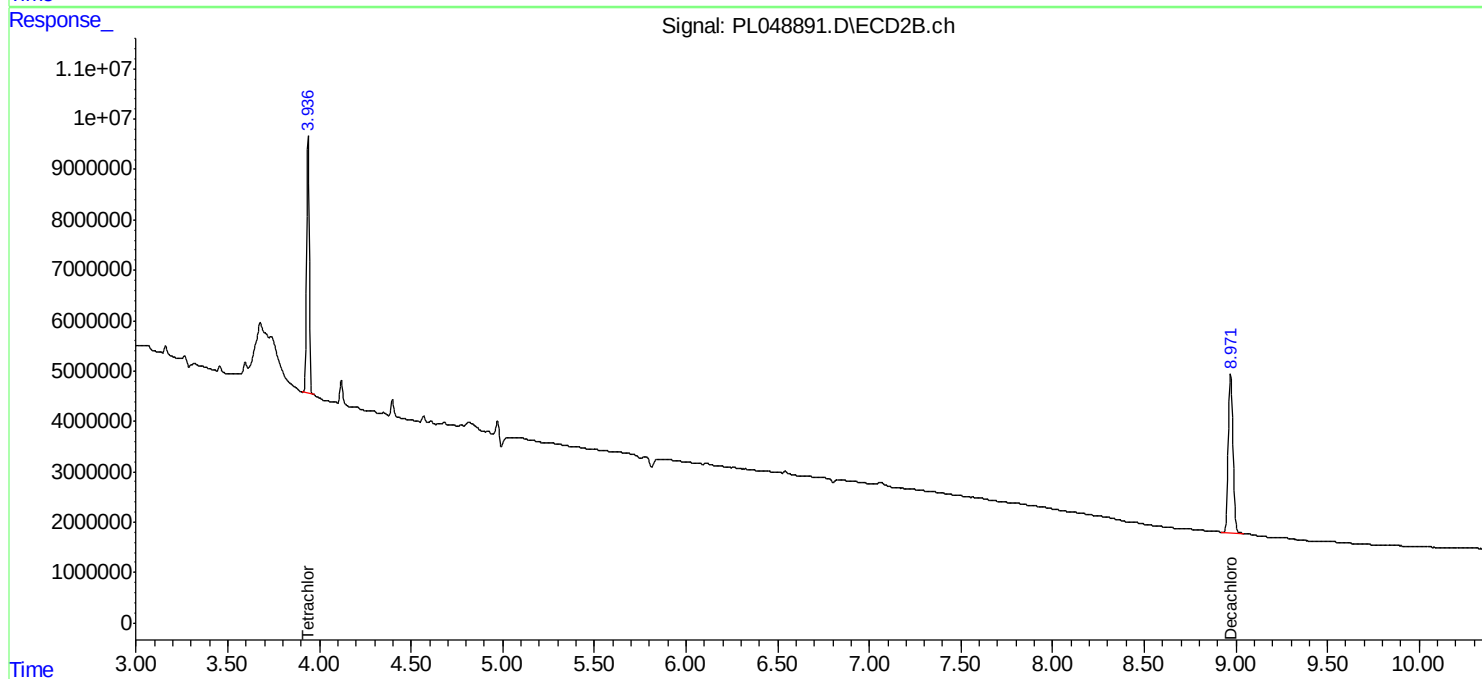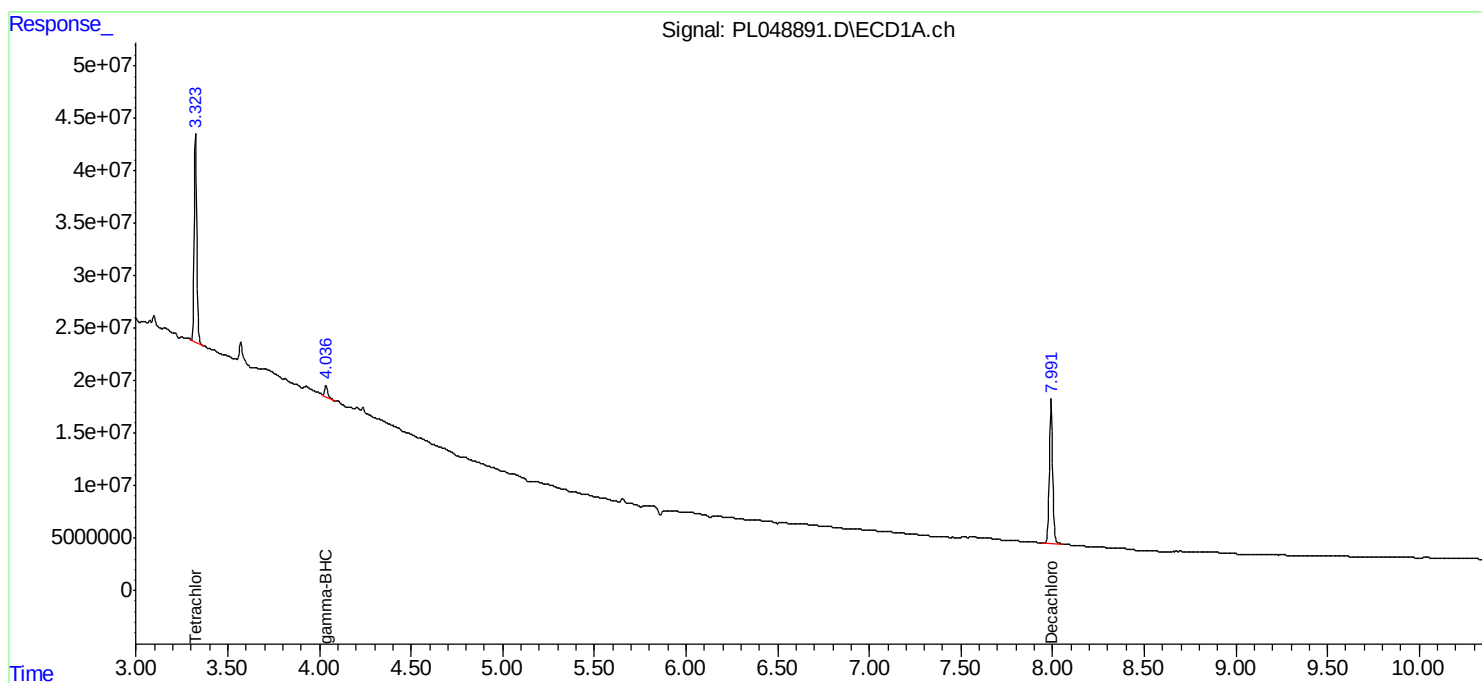


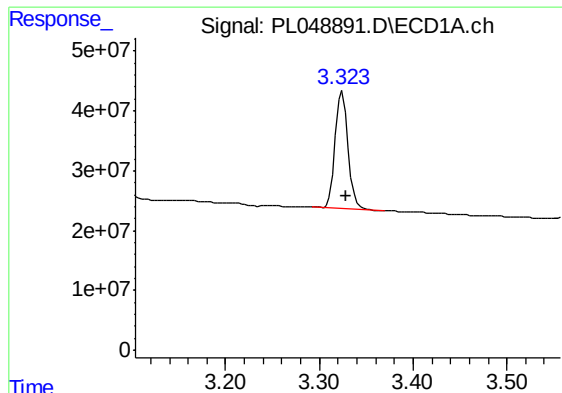

#1 Tetrachloro-m-xylene


R.T.: 3.325 min
Delta R.T.: -0.003 min
Response: 186168224
Conc: 19.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-20

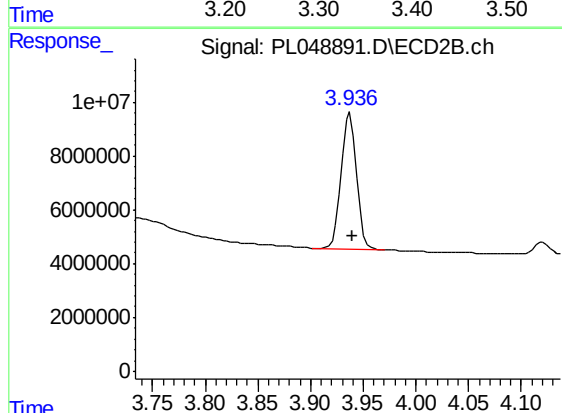


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: -0.002 min
Response: 50907438
Conc: 20.44 ng/ml

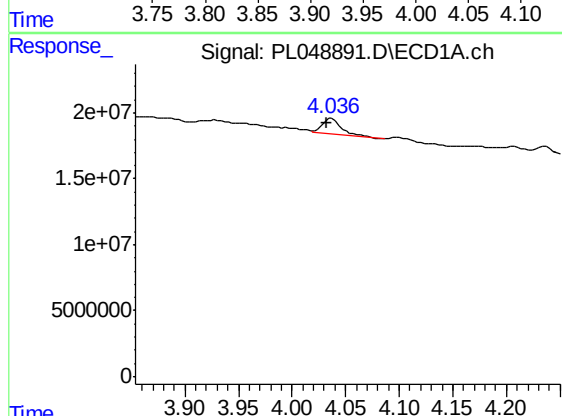


#3 gamma-BHC (Lindane)

R.T.: 4.037 min
Delta R.T.: 0.005 min
Response: 16061618
Conc: 1.13 ng/ml

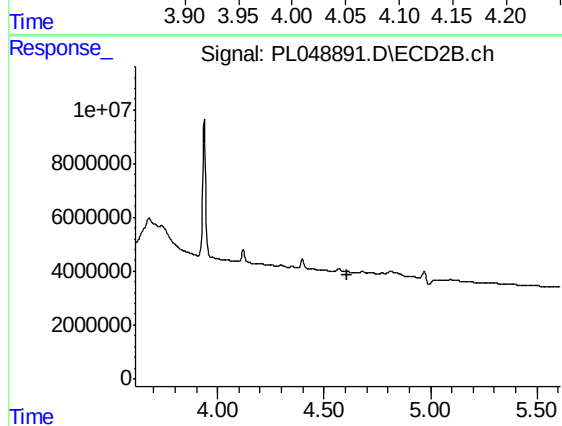

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.612 min
Response: 0
Conc: N.D.

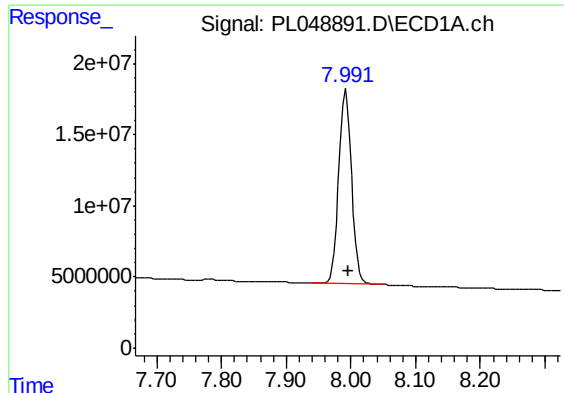

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.004 min
Response: 186282329
Conc: 18.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-20

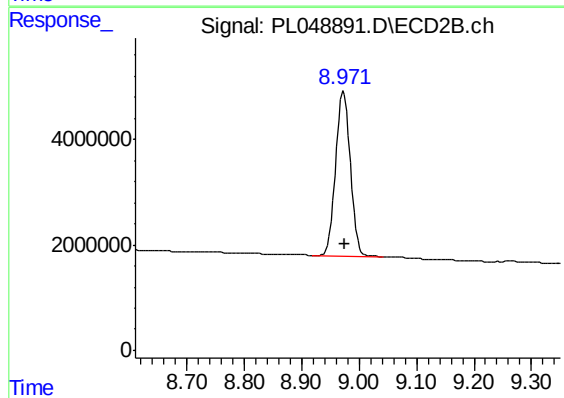

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: -0.002 min
Response: 55491264
Conc: 20.91 ng/ml