

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052319\
 Data File : PS004755.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2019 02:50
 Operator : SM\AJ
 Sample : K3008-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-19

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 04:40:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.579	5.289	530.7E6	369.9E6	378.605	383.378
Target Compounds							
1) T	Dalapon	2.080	0.000	57978162	0	34.975	N.D. #
2) T	3,5-DICHL...	4.999	4.608	11692840	285.8E6	6.780	231.974 #
3) T	4-Nitroph...	5.492	4.993	44457947	17407012	71.303	36.730 #
5) T	DICAMBA	5.770	5.396	16716980	18614491	3.148	5.039 #
6) T	MCPD	5.934	0.000	13235225	0	3.179	N.D. #
7) T	MCPA	0.000	5.771	0	72477420	N.D.	17.713
9) T	2,4-D	6.666	0.000	20255154	0	14.807	N.D. #
10) T	Pentachlo...	6.943	0.000	16681285	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	6.944	0	190.3E6	N.D.	36.990



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052319\
Data File : PS004755.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2019 02:50
Operator : SM\AJ
Sample : K3008-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-19

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 04:40:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

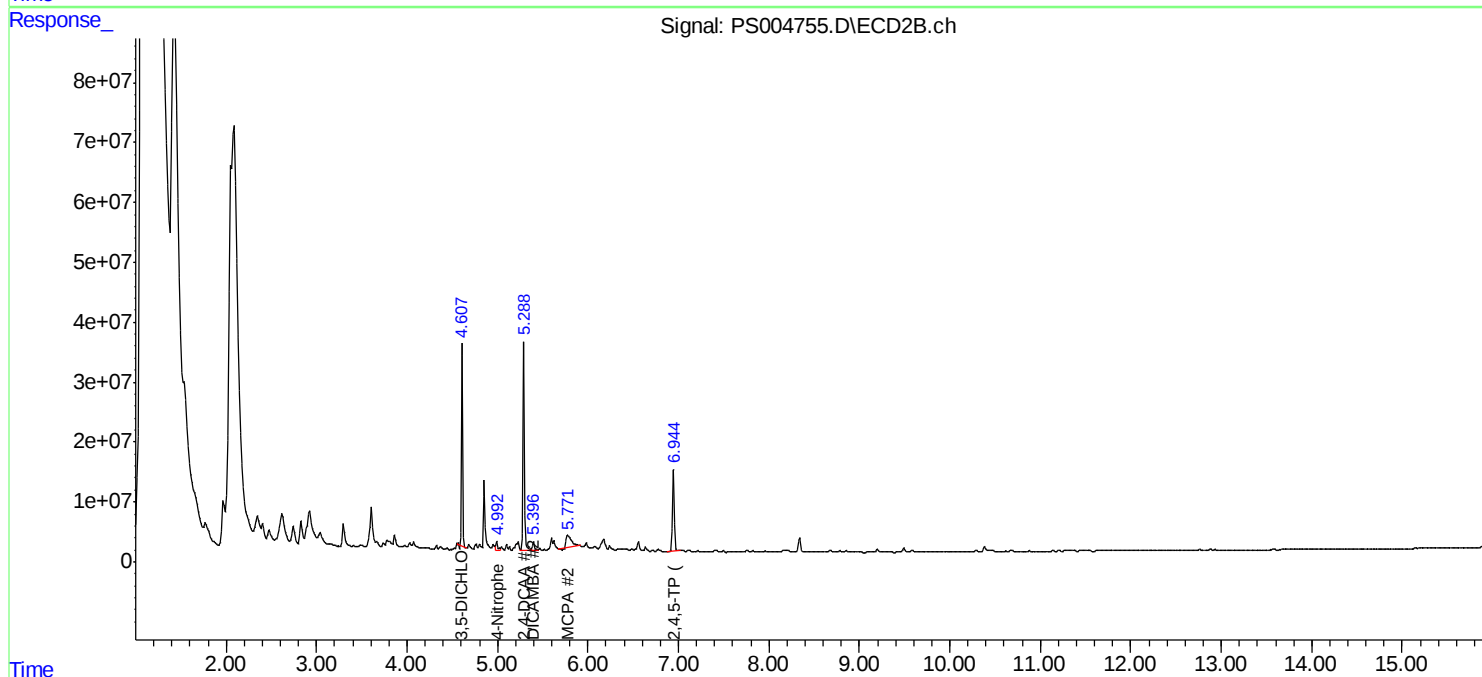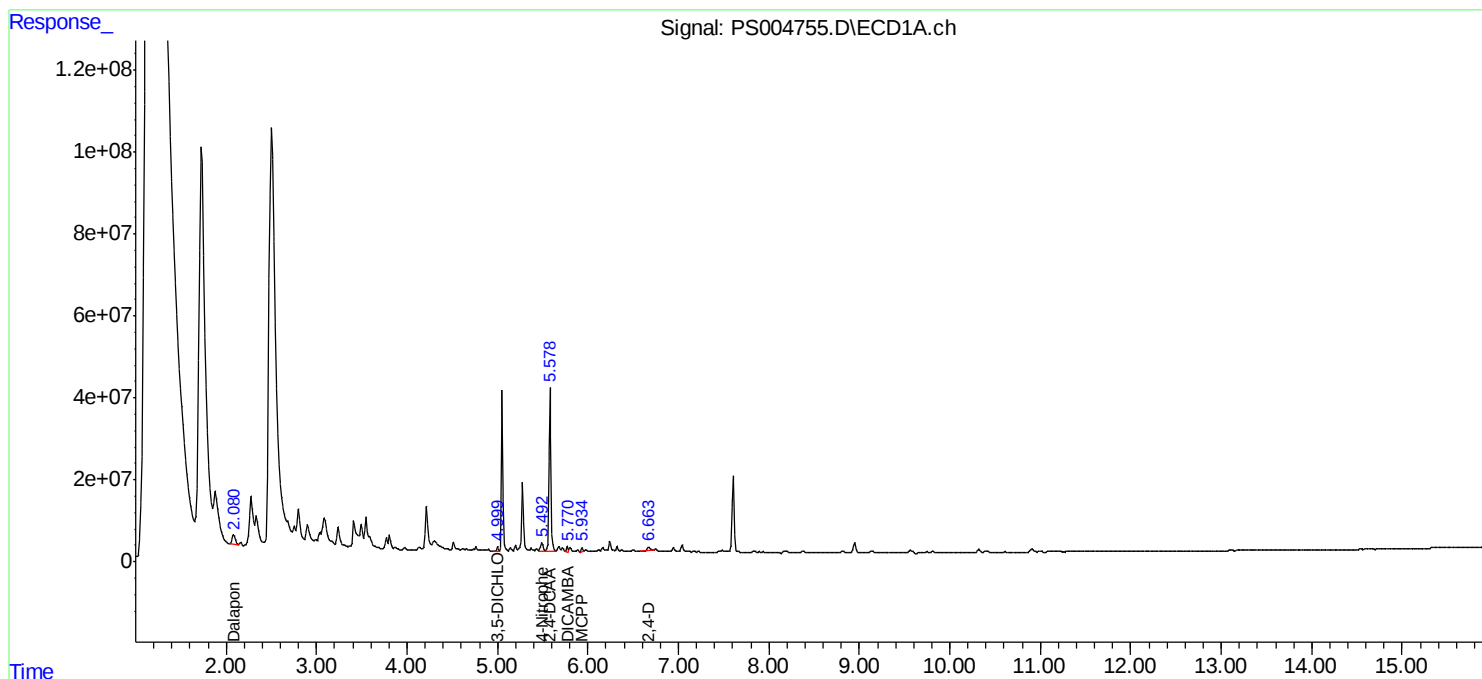


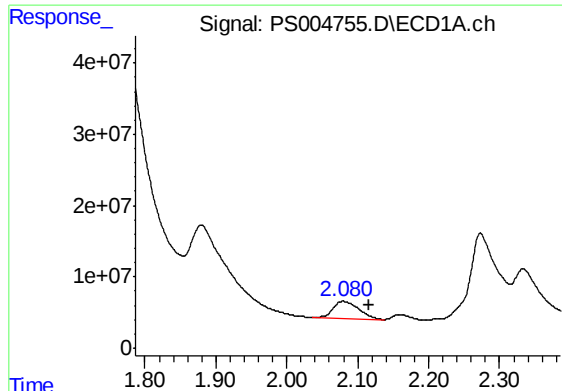

#1 Dalapon


R.T.: 2.080 min
Delta R.T.: -0.036 min
Response: 57978162
Conc: 34.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-19

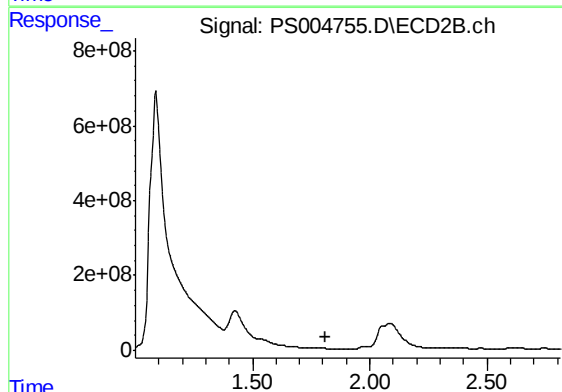


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

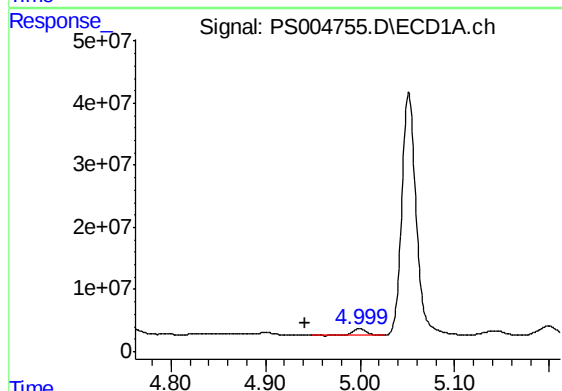


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.999 min
Delta R.T.: 0.057 min
Response: 11692840
Conc: 6.78 ng/ml

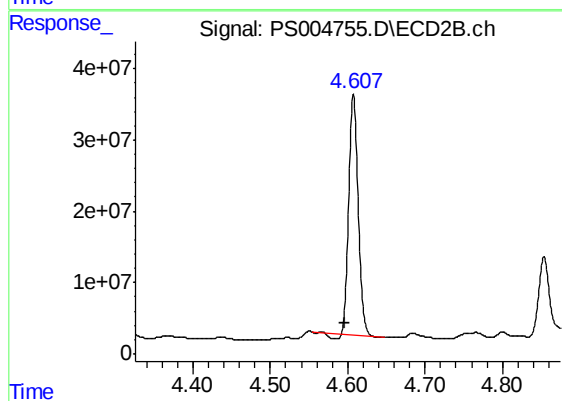

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.608 min
Delta R.T.: 0.012 min
Response: 285821144
Conc: 231.97 ng/ml

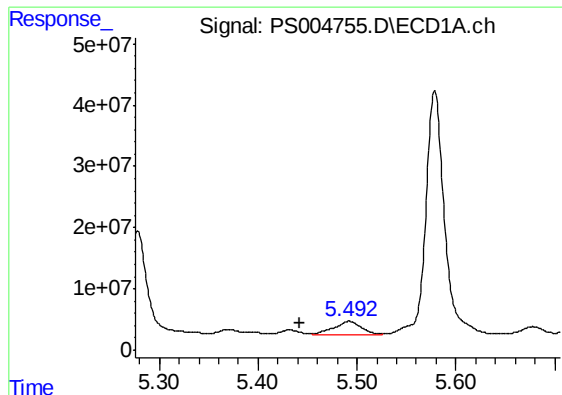

#3 4-Nitrophenol


R.T.: 5.492 min
Delta R.T.: 0.049 min
Response: 44457947
Conc: 71.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-19

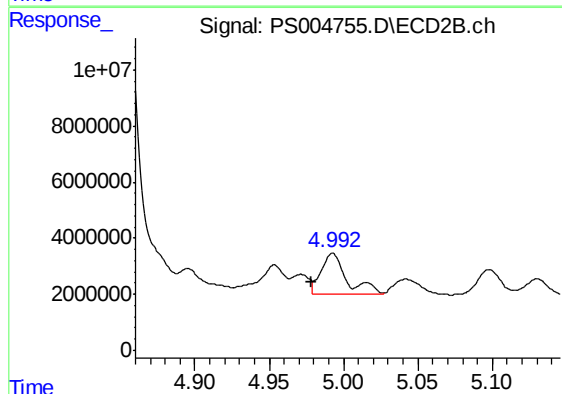


#3 4-Nitrophenol

R.T.: 4.993 min
Delta R.T.: 0.014 min
Response: 17407012
Conc: 36.73 ng/ml

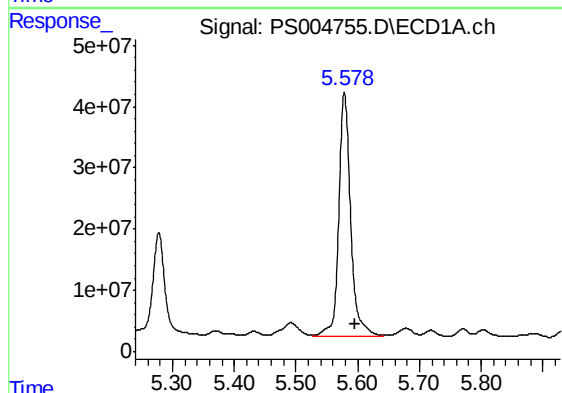


#4 2,4-DCAA

R.T.: 5.579 min
Delta R.T.: -0.016 min
Response: 530712416
Conc: 378.61 ng/ml

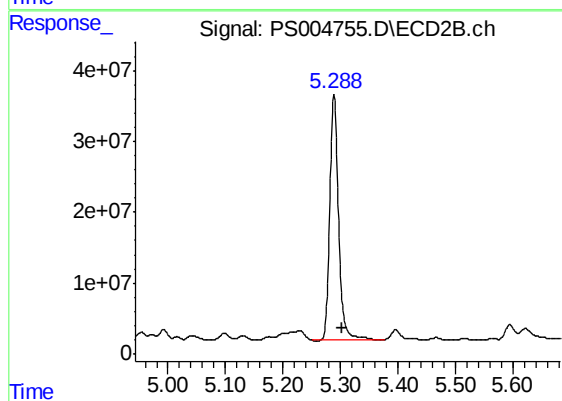

#4 2,4-DCAA


R.T.: 5.289 min
Delta R.T.: -0.015 min
Response: 369896855
Conc: 383.38 ng/ml

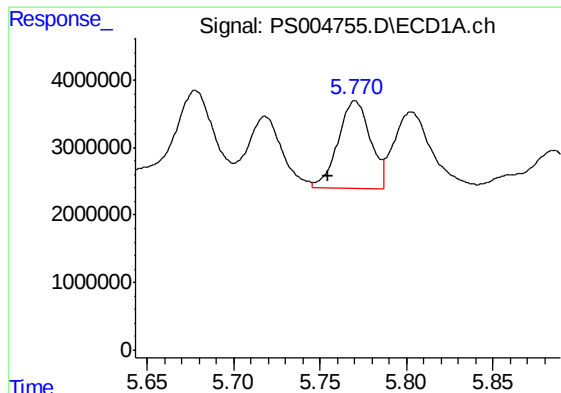

#5 DICAMBA


R.T.: 5.770 min
Delta R.T.: 0.015 min
Response: 16716980
Conc: 3.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-19

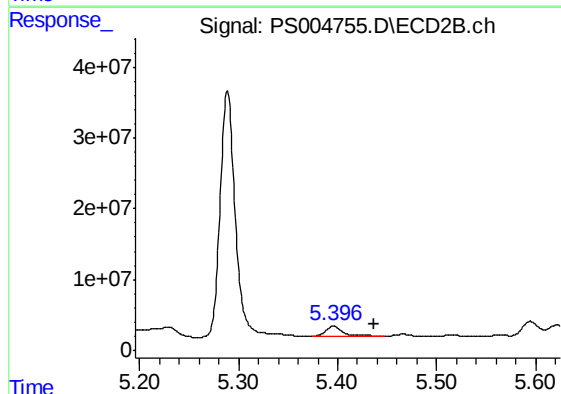


#5 DICAMBA

R.T.: 5.396 min
Delta R.T.: -0.041 min
Response: 18614491
Conc: 5.04 ng/ml

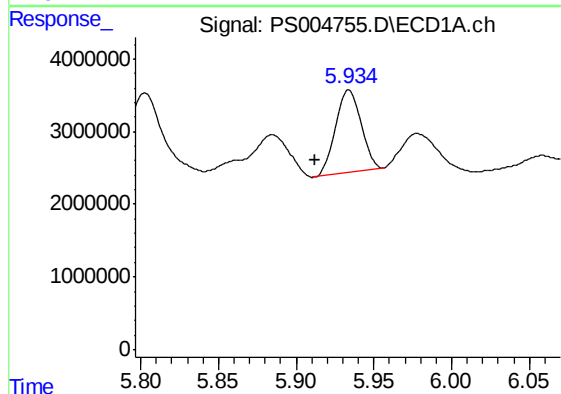


#6 MCP

R.T.: 5.934 min
Delta R.T.: 0.021 min
Response: 13235225
Conc: 3.18 ug/ml

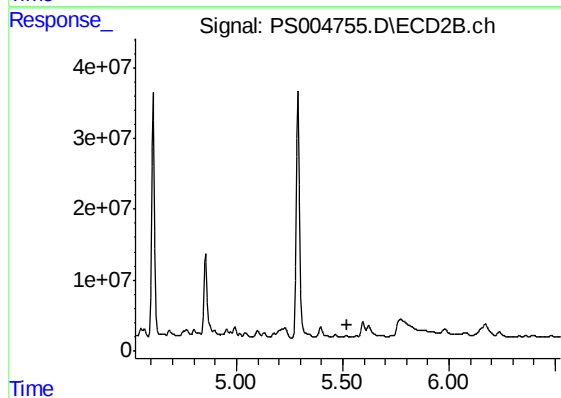

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

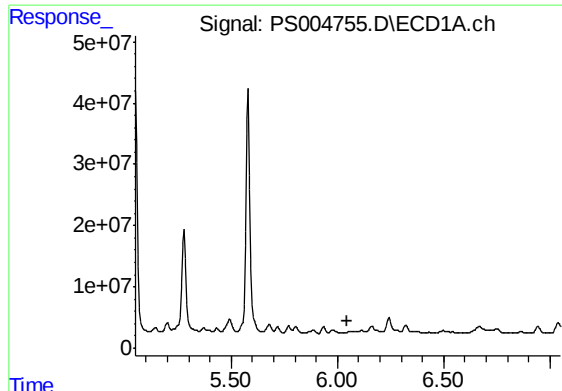

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-19

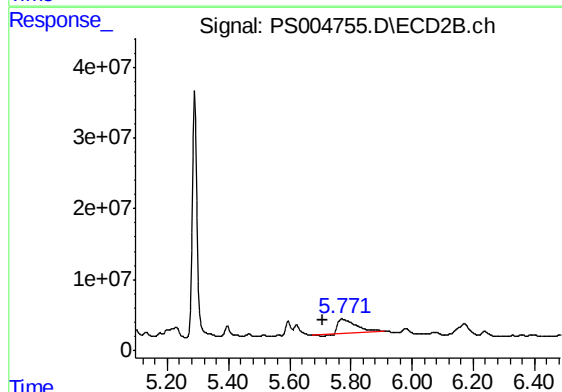


#7 MCPA

R.T.: 5.771 min
Delta R.T.: 0.061 min
Response: 72477420
Conc: 17.71 ug/ml

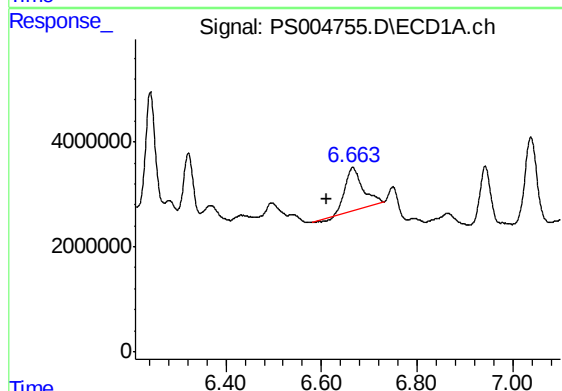


#9 2,4-D

R.T.: 6.666 min
Delta R.T.: 0.054 min
Response: 20255154
Conc: 14.81 ng/ml

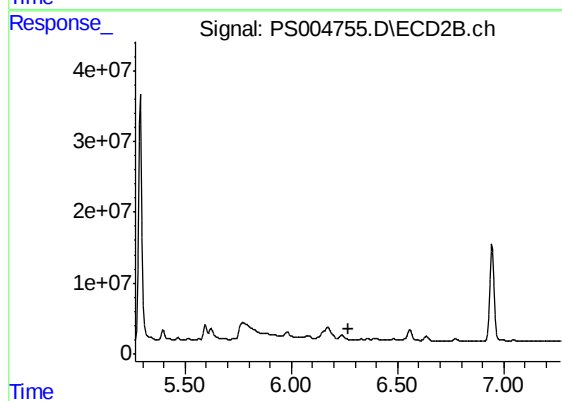

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

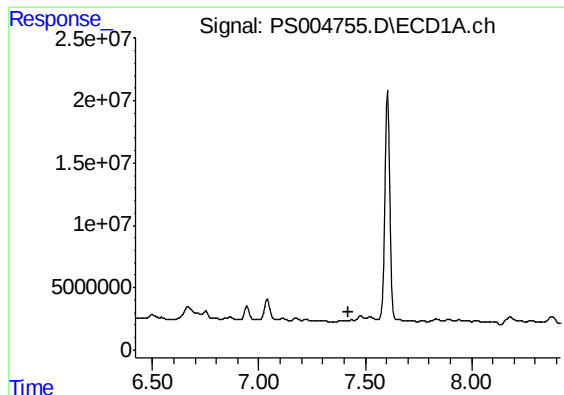

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-19

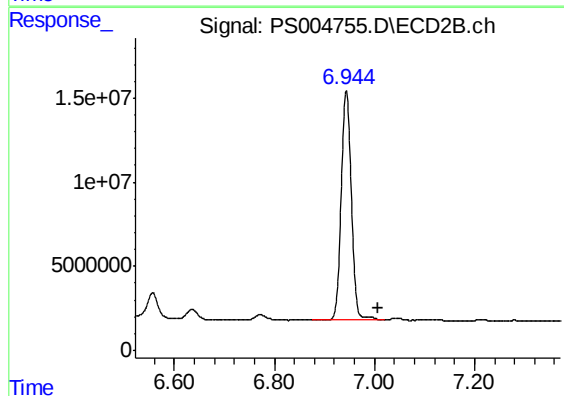

#11 2,4,5-TP (SILVEX)

R.T.: 6.944 min
Delta R.T.: -0.062 min
Response: 190326606
Conc: 36.99 ng/ml