

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052319\
 Data File : PS004756.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2019 03:12
 Operator : SM\AJ
 Sample : K3008-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-20

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 04:40:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.557	5.284	645.0E6	442.9E6	460.161	459.003
Target Compounds							
1) T	Dalapon	2.057	0.000	45664351	0	27.547	N.D. #
2) T	3,5-DICHL...	4.978	4.603	10934215	316.9E6	6.340	257.200 #
3) T	4-Nitroph...	5.471	4.988	65182374	27055977	104.542	57.090 #
5) T	DICAMBA	5.748	5.391	25467205	18450228	4.796	4.994
6) T	MCPD	5.913	5.590	13885710	20457350	3.335	7.466 #
7) T	MCPA	0.000	5.764	0	98370967	N.D.	24.042
9) T	2,4-D	6.644	0.000	19066940	0	13.939	N.D. #
10) T	Pentachlo...	6.922	0.000	17325032	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	6.939	0	200.9E6	N.D.	39.044



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052319\
Data File : PS004756.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2019 03:12
Operator : SM\AJ
Sample : K3008-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-20

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 04:40:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

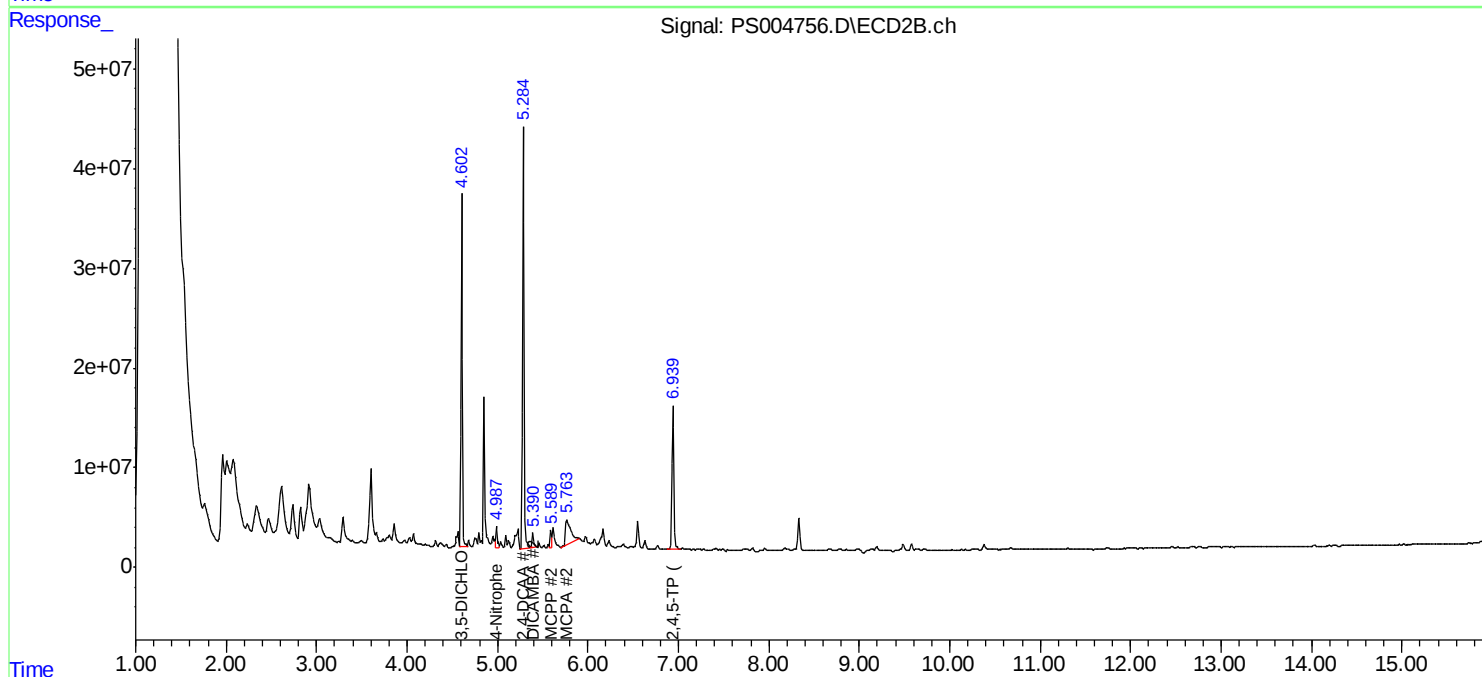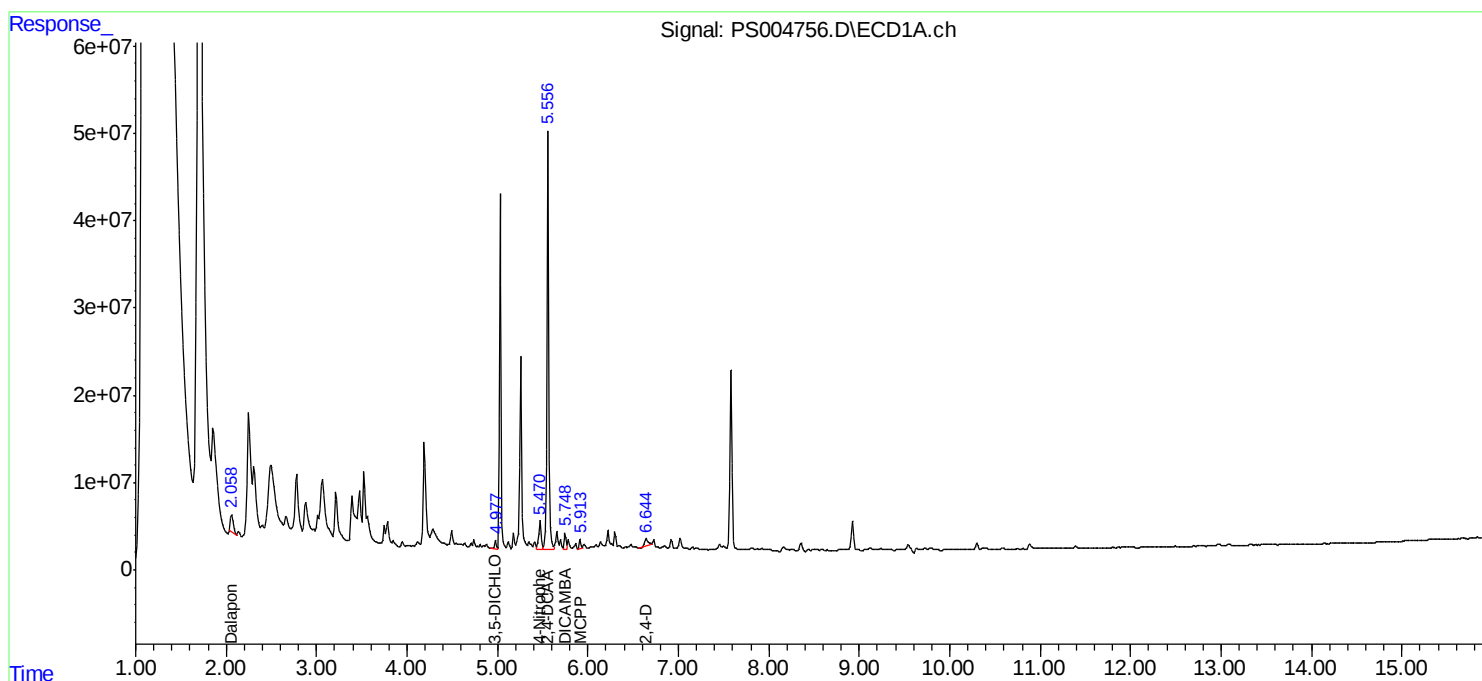


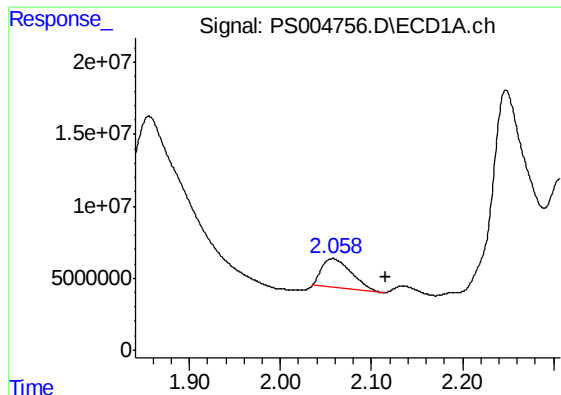

#1 Dalapon


R.T.: 2.057 min
Delta R.T.: -0.059 min
Response: 45664351
Conc: 27.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-20

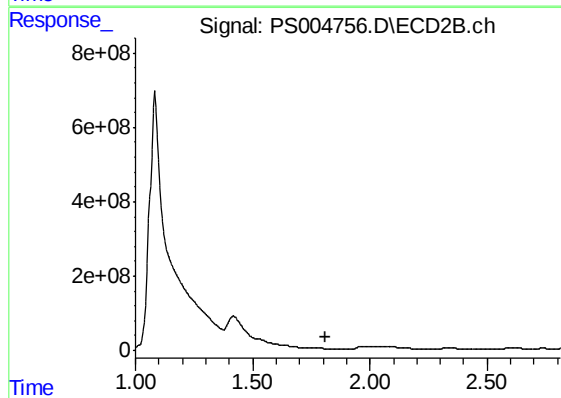


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

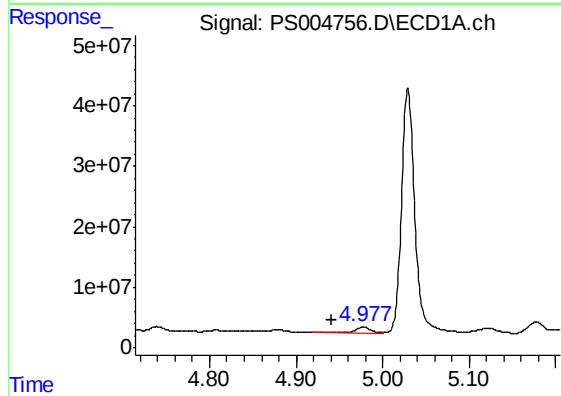


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.978 min
Delta R.T.: 0.036 min
Response: 10934215
Conc: 6.34 ng/ml

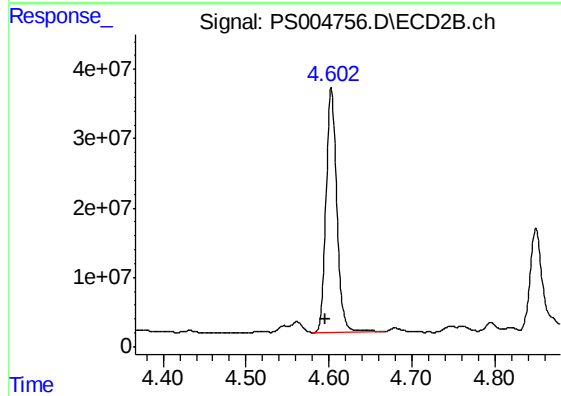

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.603 min
Delta R.T.: 0.008 min
Response: 316903650
Conc: 257.20 ng/ml

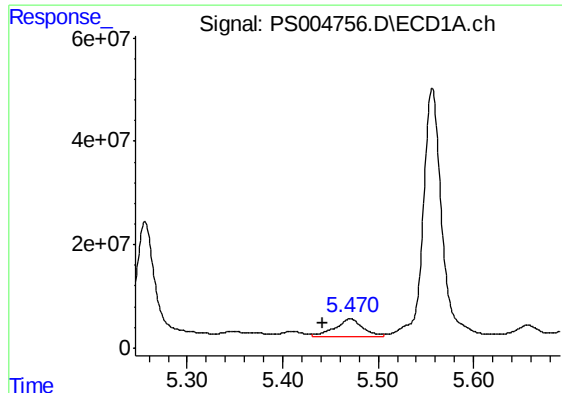

#3 4-Nitrophenol


R.T.: 5.471 min
Delta R.T.: 0.028 min
Response: 65182374
Conc: 104.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-20

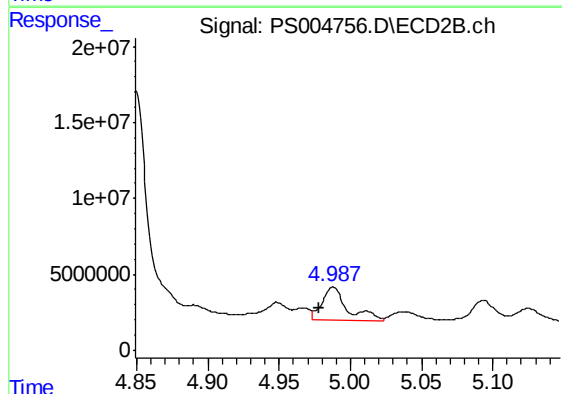


#3 4-Nitrophenol

R.T.: 4.988 min
Delta R.T.: 0.009 min
Response: 27055977
Conc: 57.09 ng/ml

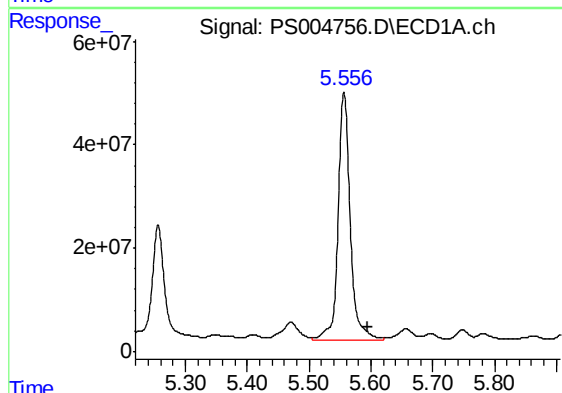


#4 2,4-DCAA

R.T.: 5.557 min
Delta R.T.: -0.038 min
Response: 645034082
Conc: 460.16 ng/ml

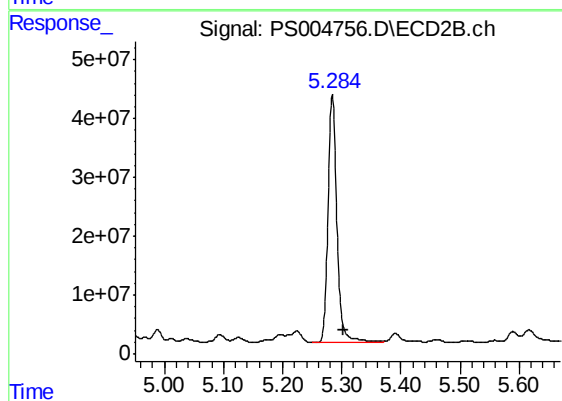

#4 2,4-DCAA


R.T.: 5.284 min
Delta R.T.: -0.020 min
Response: 442862797
Conc: 459.00 ng/ml

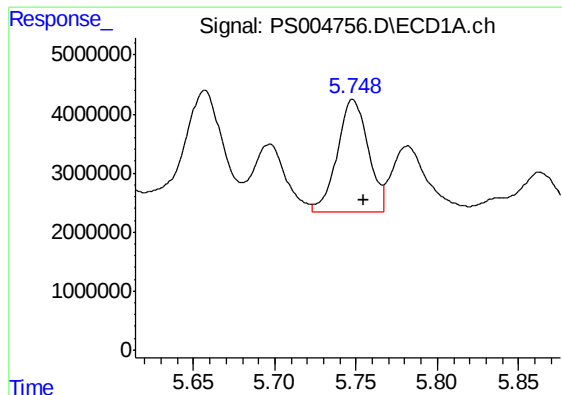

#5 DICAMBA


R.T.: 5.748 min
Delta R.T.: -0.007 min
Response: 25467205
Conc: 4.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-20

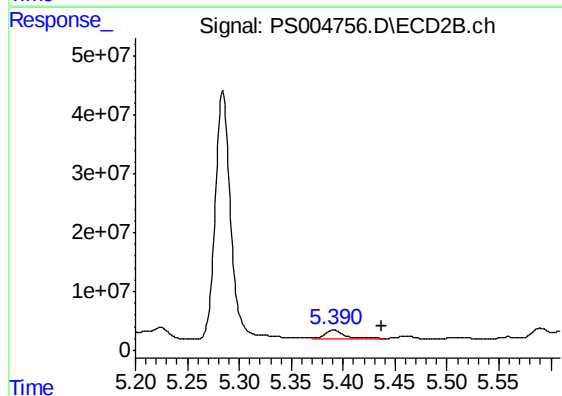


#5 DICAMBA

R.T.: 5.391 min
Delta R.T.: -0.046 min
Response: 18450228
Conc: 4.99 ng/ml

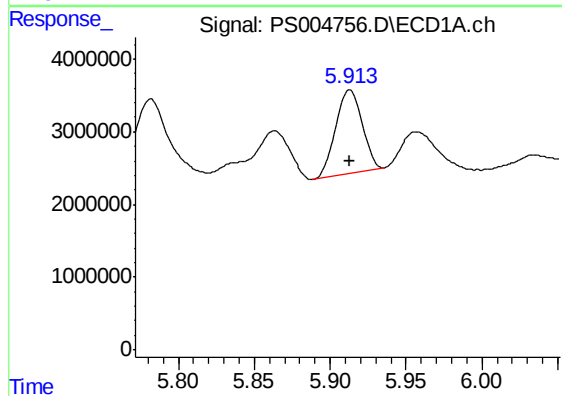


#6 MCPP

R.T.: 5.913 min
Delta R.T.: 0.000 min
Response: 13885710
Conc: 3.34 ug/ml

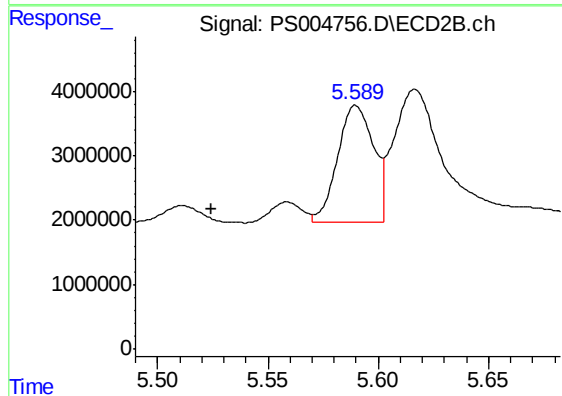

#6 MCPP


R.T.: 5.590 min
Delta R.T.: 0.066 min
Response: 20457350
Conc: 7.47 ug/ml

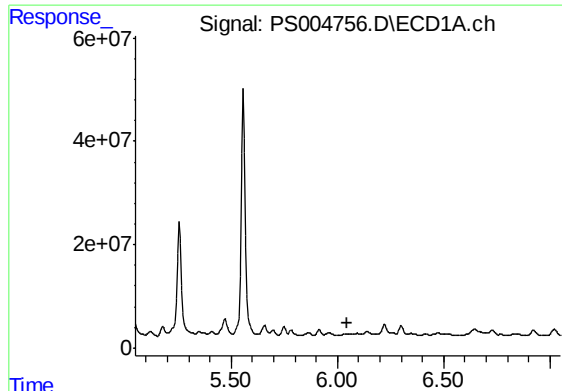

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-20

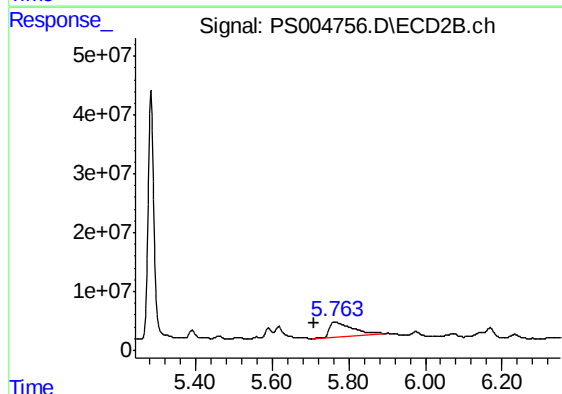


#7 MCPA

R.T.: 5.764 min
Delta R.T.: 0.055 min
Response: 98370967
Conc: 24.04 ug/ml

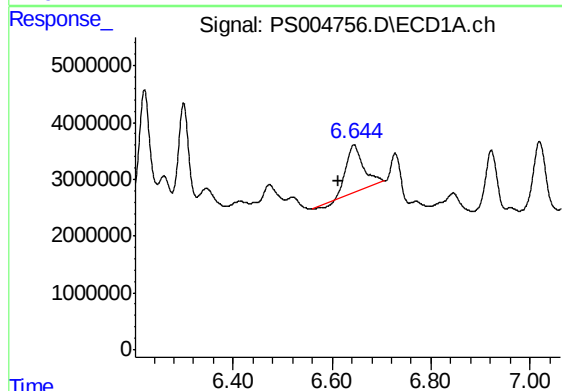


#9 2,4-D

R.T.: 6.644 min
Delta R.T.: 0.032 min
Response: 19066940
Conc: 13.94 ng/ml

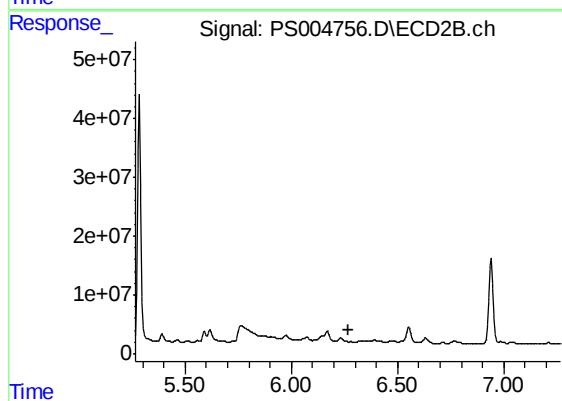

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

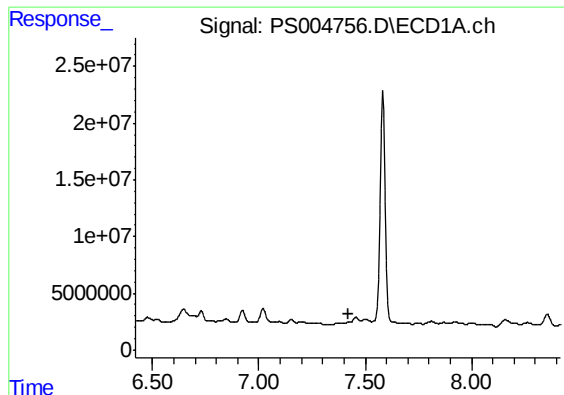

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-20

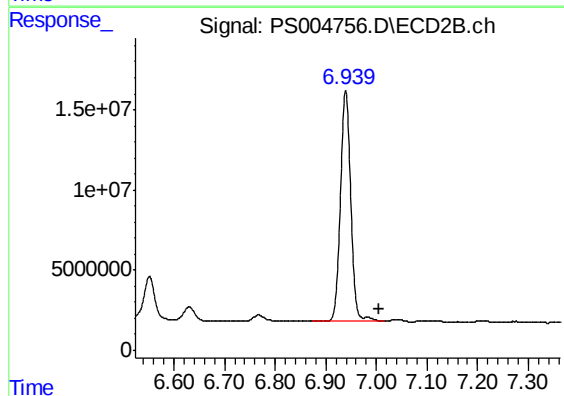

#11 2,4,5-TP (SILVEX)

R.T.: 6.939 min
Delta R.T.: -0.067 min
Response: 200895012
Conc: 39.04 ng/ml