

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052319\
 Data File : PS004757.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2019 03:34
 Operator : SM\AJ
 Sample : K3008-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-21

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 04:40:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.575	5.285	610.6E6	424.7E6	435.573	440.146
Target Compounds							
1) T	Dalapon	2.078	0.000	61408744	0	37.045	N.D. #
2) T	3,5-DICHL...	4.995	4.604	16190992	301.6E6	9.388	244.761 #
3) T	4-Nitroph...	5.488	4.988	61069147	28850359	97.945	60.876 #
5) T	DICAMBA	5.767	5.392	24315346	21965005	4.579	5.946 #
6) T	MCPD	5.930	5.591	13289890	23722022	3.192	8.658 #
7) T	MCPA	6.037	5.748	37435344	309.3E6	6.463	75.588 #
8) T	DICHLORPROP	0.000	5.974	0	18851230	N.D.	19.994
9) T	2,4-D	6.662	0.000	39697191	0	29.020	N.D. #
10) T	Pentachlo...	6.939	0.000	17648399	0	1.005	N.D. #
11) T	2,4,5-TP ...	0.000	6.940	0	182.6E6	N.D.	35.481



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052319\
Data File : PS004757.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2019 03:34
Operator : SM\AJ
Sample : K3008-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
COMP-21

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 04:40:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

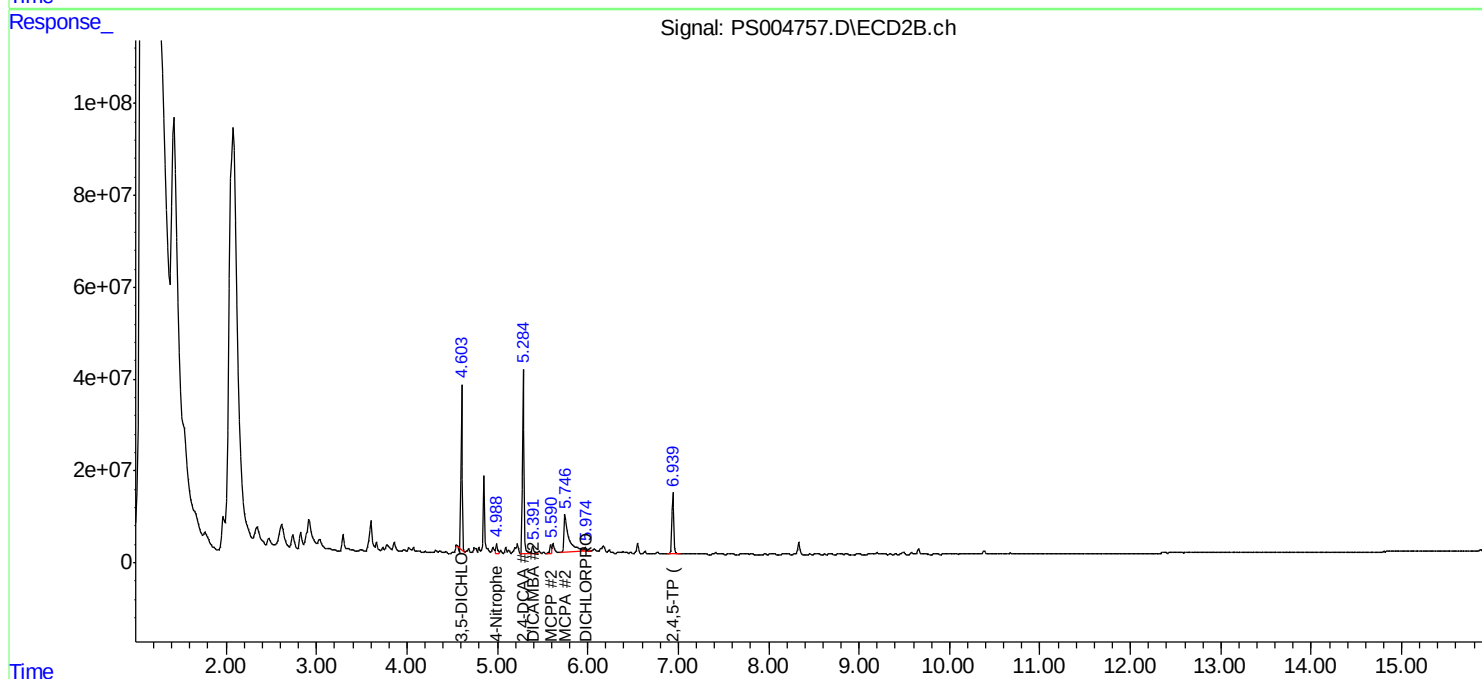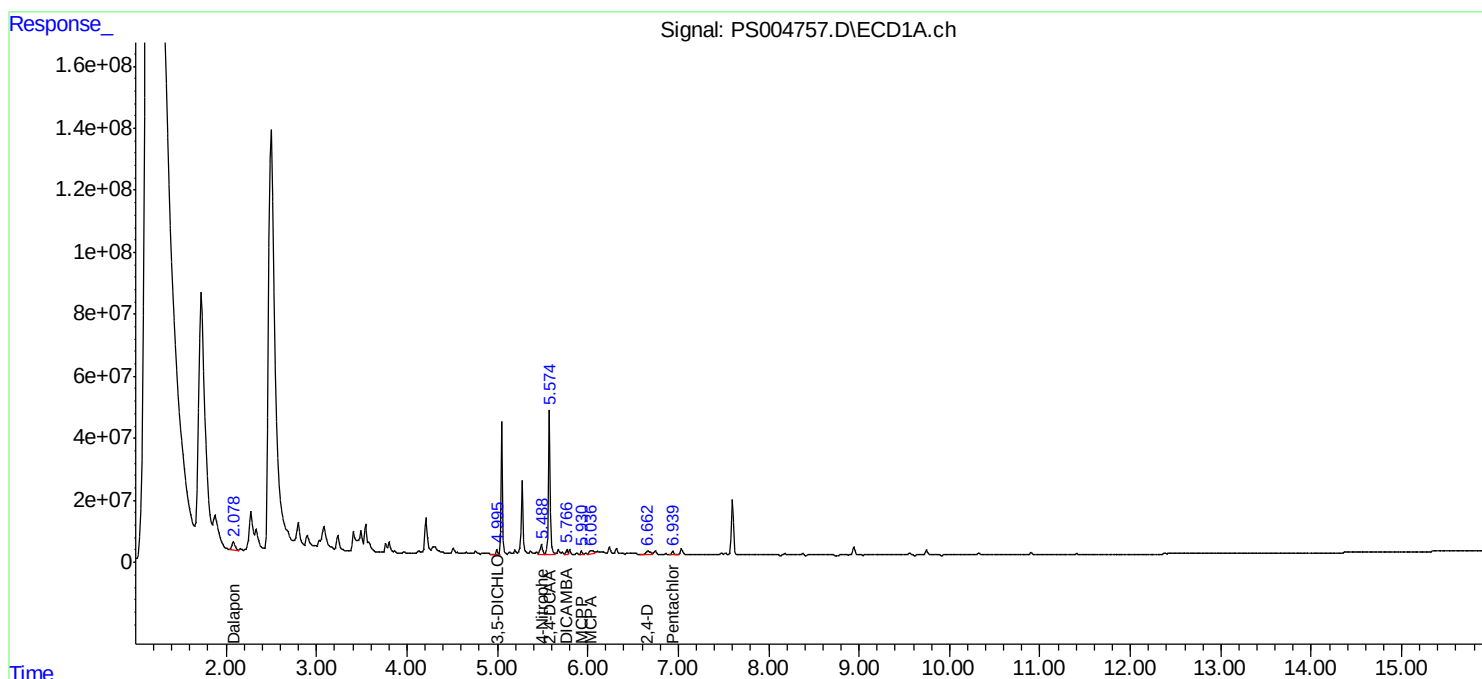


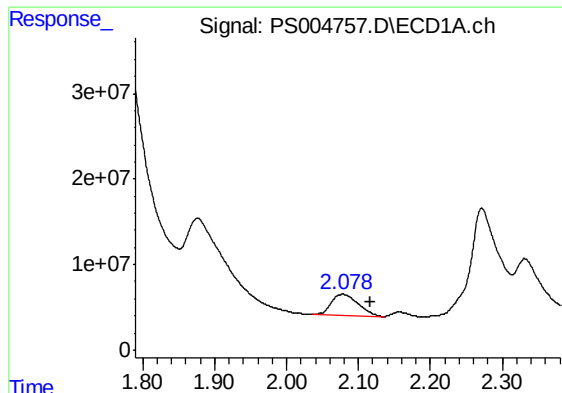

#1 Dalapon


R.T.: 2.078 min
Delta R.T.: -0.038 min
Response: 61408744
Conc: 37.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-21

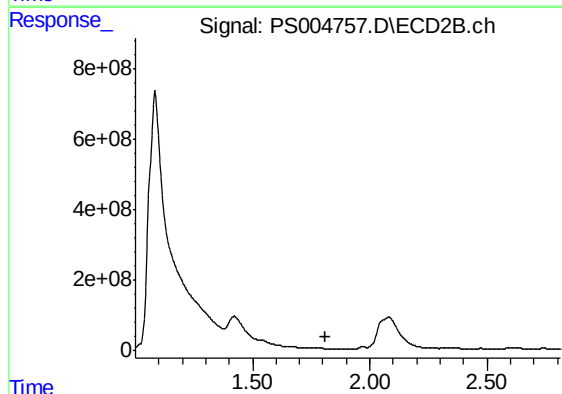


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

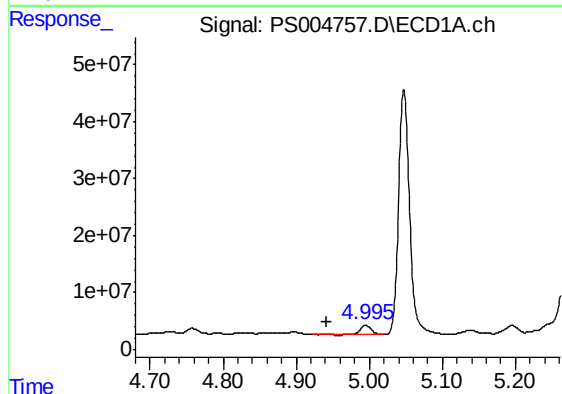


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.995 min
Delta R.T.: 0.053 min
Response: 16190992
Conc: 9.39 ng/ml

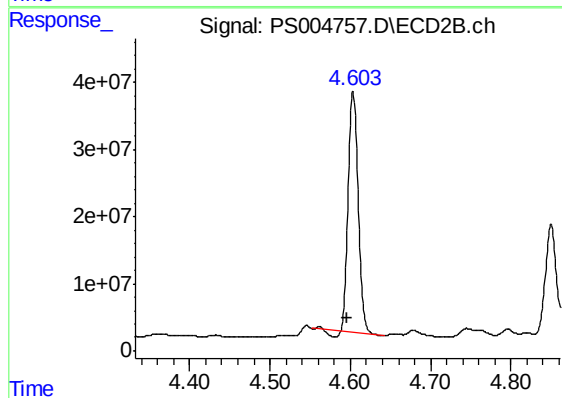

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.604 min
Delta R.T.: 0.008 min
Response: 301576823
Conc: 244.76 ng/ml

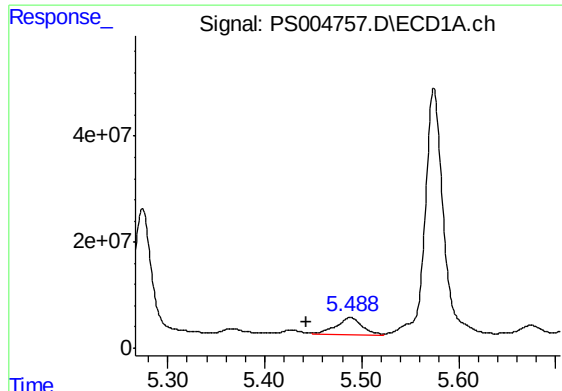

#3 4-Nitrophenol


R.T.: 5.488 min
Delta R.T.: 0.046 min
Response: 61069147
Conc: 97.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-21

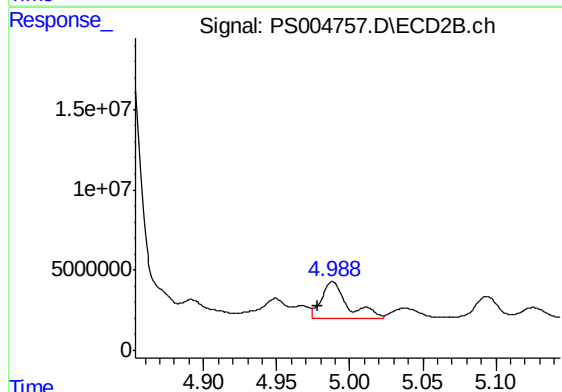


#3 4-Nitrophenol

R.T.: 4.988 min
Delta R.T.: 0.010 min
Response: 28850359
Conc: 60.88 ng/ml

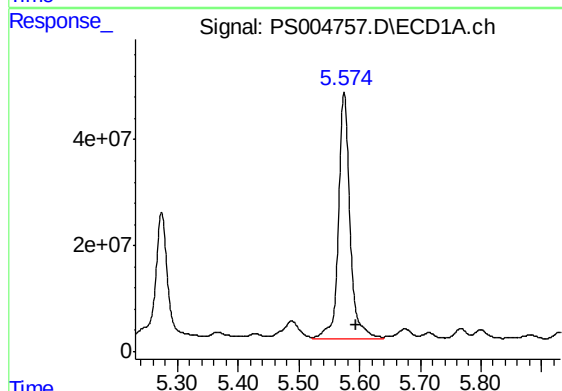


#4 2,4-DCAA

R.T.: 5.575 min
Delta R.T.: -0.020 min
Response: 610567210
Conc: 435.57 ng/ml

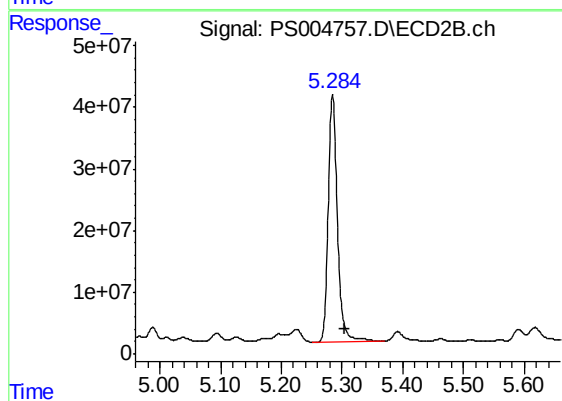

#4 2,4-DCAA


R.T.: 5.285 min
Delta R.T.: -0.019 min
Response: 424668630
Conc: 440.15 ng/ml

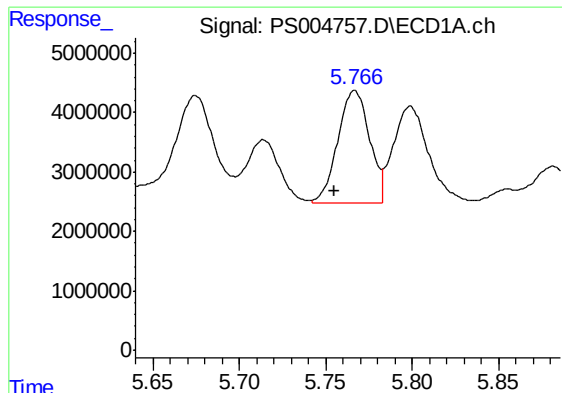

#5 DICAMBA


R.T.: 5.767 min
Delta R.T.: 0.012 min
Response: 24315346
Conc: 4.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-21

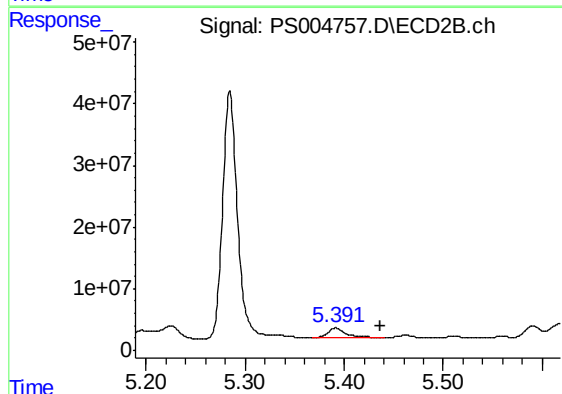


#5 DICAMBA

R.T.: 5.392 min
Delta R.T.: -0.046 min
Response: 21965005
Conc: 5.95 ng/ml

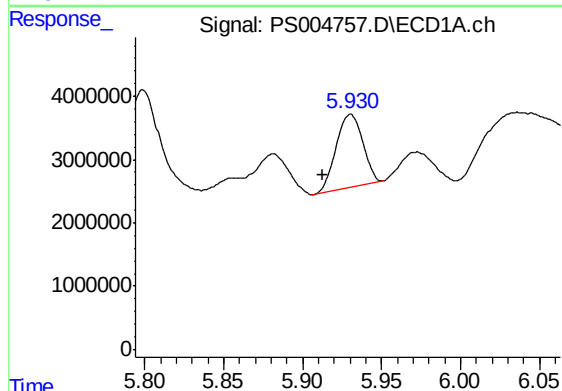


#6 MCPP

R.T.: 5.930 min
Delta R.T.: 0.018 min
Response: 13289890
Conc: 3.19 ug/ml

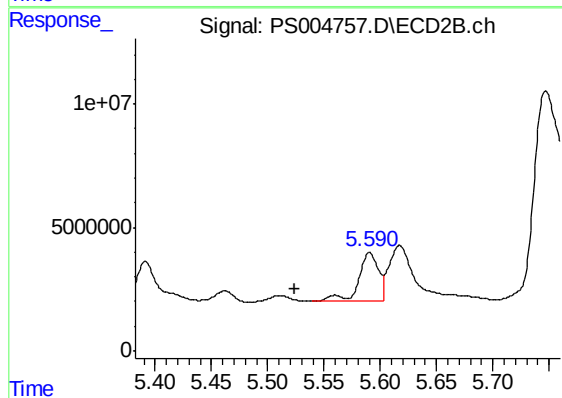

#6 MCPP


R.T.: 5.591 min
Delta R.T.: 0.066 min
Response: 23722022
Conc: 8.66 ug/ml

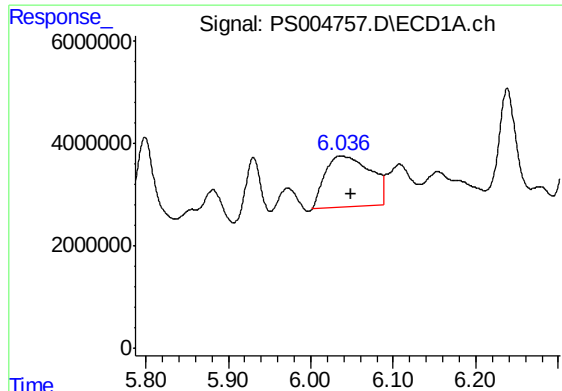

#7 MCPA


R.T.: 6.037 min
Delta R.T.: -0.012 min
Response: 37435344
Conc: 6.46 ug/ml

Instrument :
ECD_L
ClientSampleId :
COMP-21

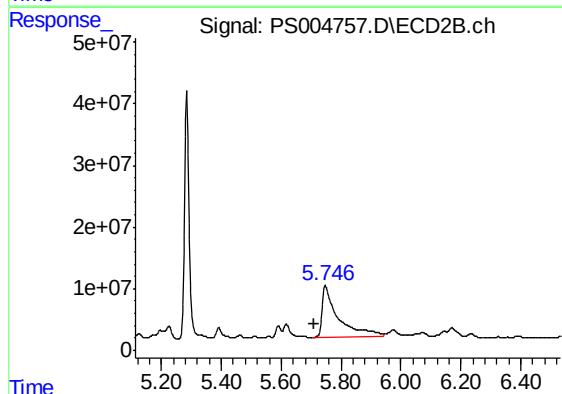


#7 MCPA

R.T.: 5.748 min
Delta R.T.: 0.038 min
Response: 309281389
Conc: 75.59 ug/ml

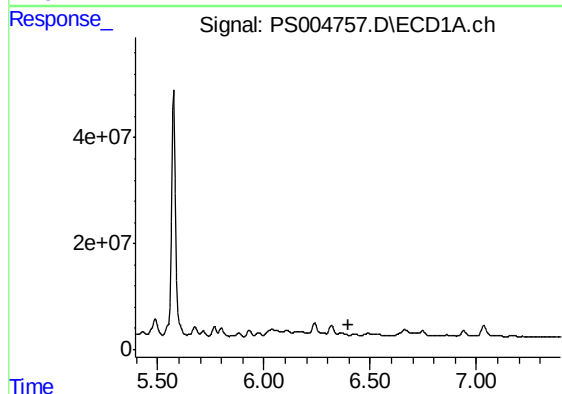


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

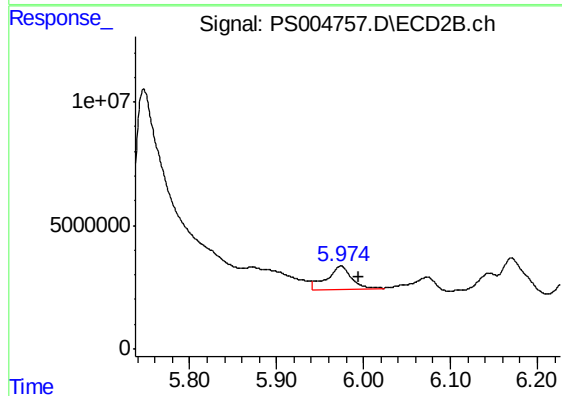

#8 DICHLORPROP


R.T.: 5.974 min
Delta R.T.: -0.020 min
Response: 18851230
Conc: 19.99 ng/ml

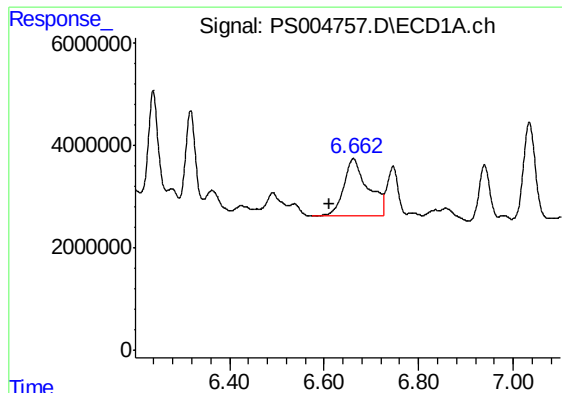

#9 2,4-D


R.T.: 6.662 min
Delta R.T.: 0.050 min
Response: 39697191
Conc: 29.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-21

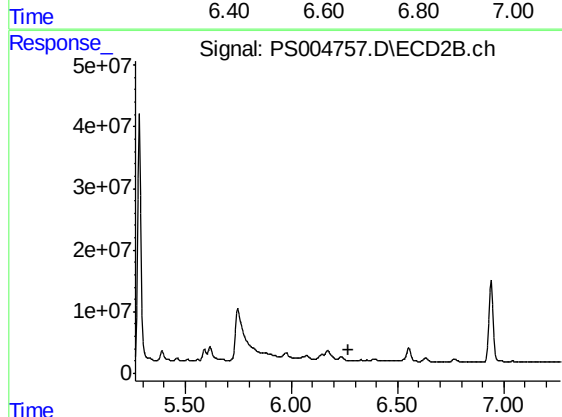


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

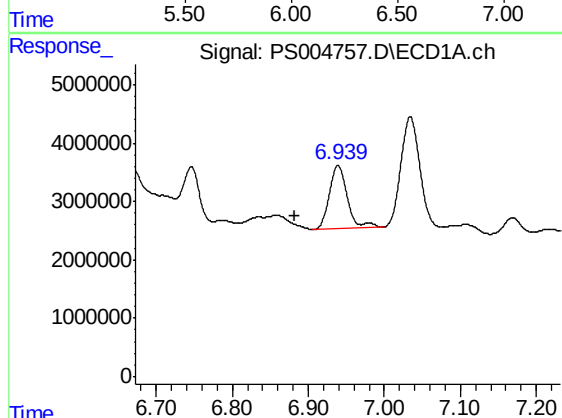


#10 Pentachlorophenol

R.T.: 6.939 min
Delta R.T.: 0.057 min
Response: 17648399
Conc: 1.00 ng/ml

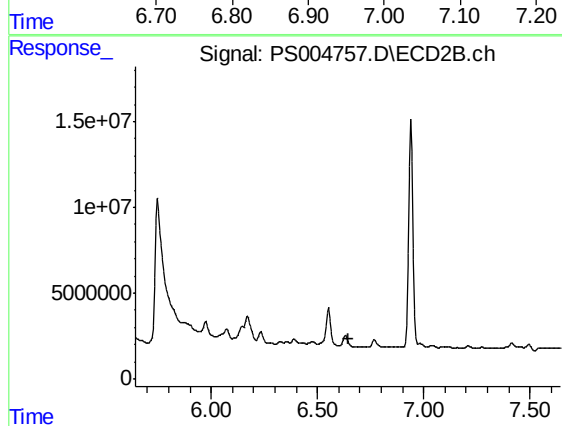

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.644 min
Response: 0
Conc: N.D.

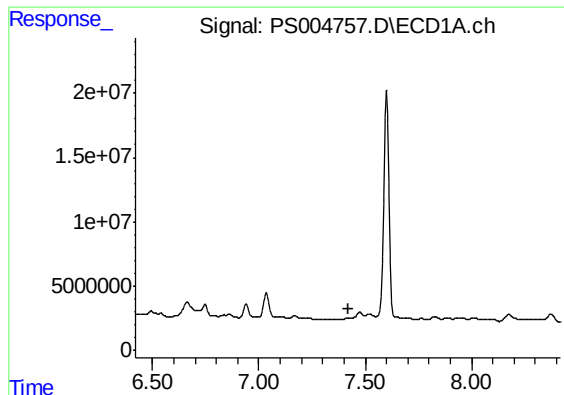

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-21

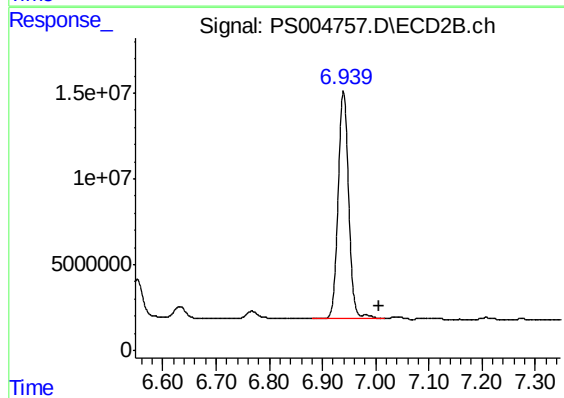

#11 2,4,5-TP (SILVEX)

R.T.: 6.940 min
Delta R.T.: -0.067 min
Response: 182559756
Conc: 35.48 ng/ml