

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052319\
 Data File : PL048876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2019 15:01
 Operator : SM\AJ
 Sample : K2994-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6-S

Manual Integrations
 APPROVED

Ankita
 5/24/2019 10:02:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 01:02:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.937	85444191	22407012	8.821m	8.996
28)	SA Decachlor...	7.996	8.973	94774639	30948578	9.426	11.660
Target Compounds							
12)	B 4,4'-DDE	5.436	6.265	71204566	15672257	5.613m	5.676m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052319\
Data File : PL048876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2019 15:01
Operator : SM\AJ
Sample : K2994-15
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-6-S


Manual Integrations
APPROVED

Ankita
5/24/2019 10:02:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 01:02:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

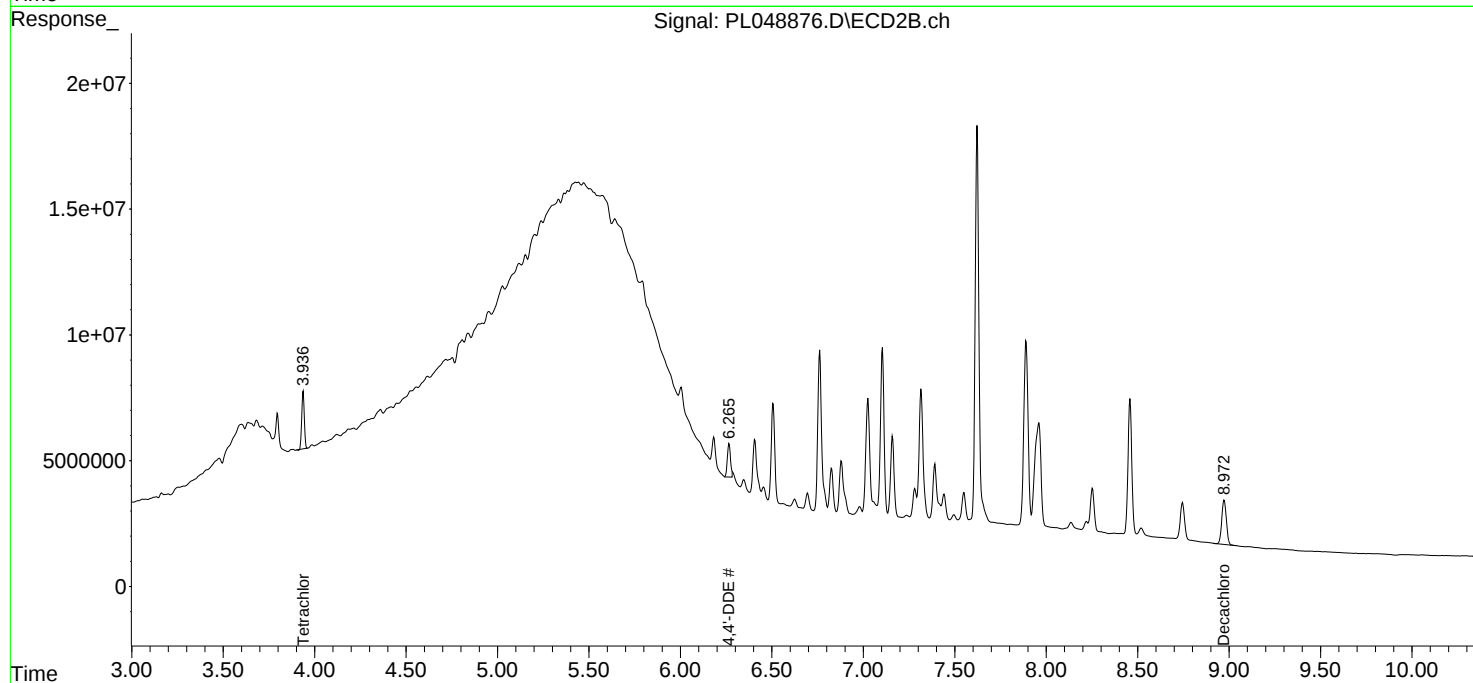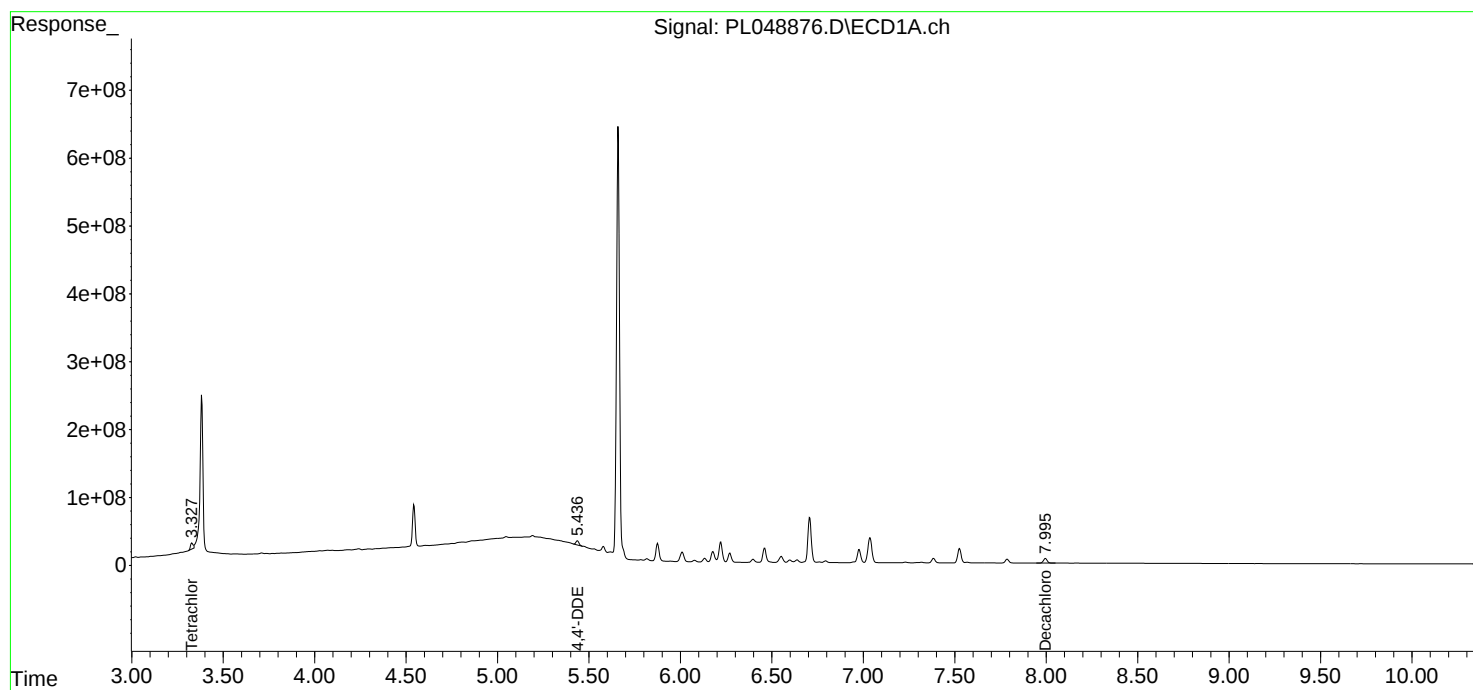

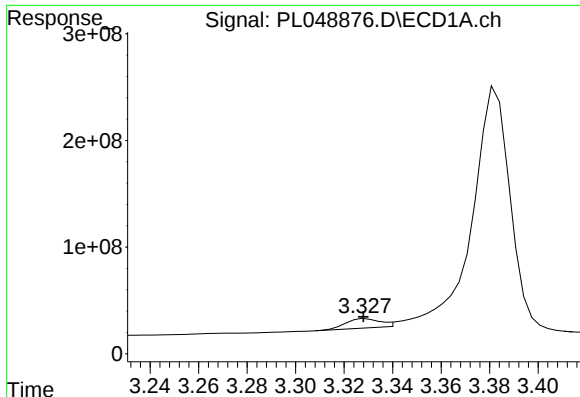


#1 Tetrachloro-m-xylene

R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 85444191
Conc: 8.82 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-6-S


Manual Integrations
APPROVED

Ankita
5/24/2019 10:02:21 AM

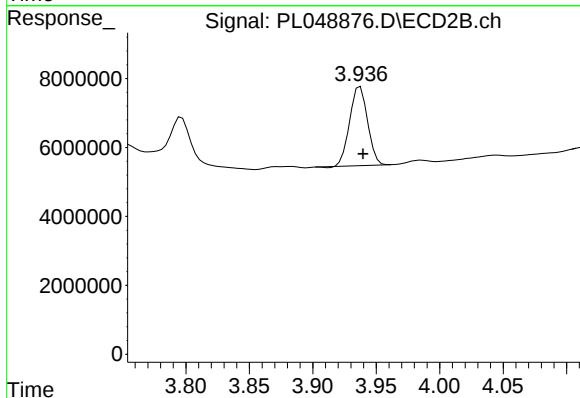


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.002 min
Response: 22407012
Conc: 9.00 ng/ml

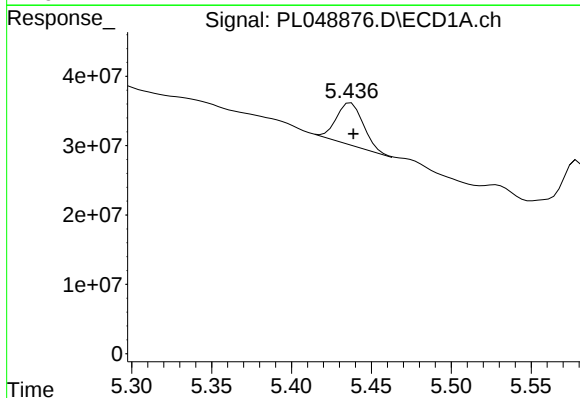


#12 4,4'-DDE

R.T.: 5.436 min
Delta R.T.: -0.003 min
Response: 71204566
Conc: 5.61 ng/ml m

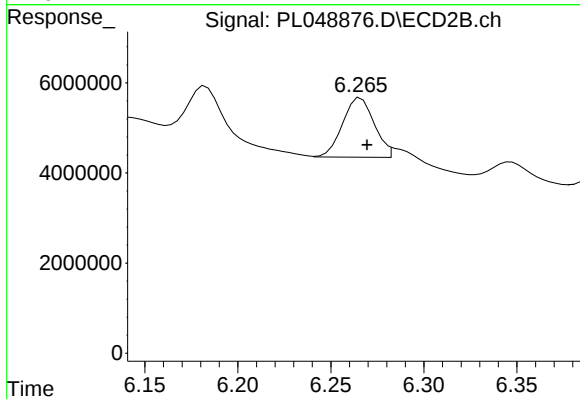

#12 4,4'-DDE

R.T.: 6.265 min
Delta R.T.: -0.005 min
Response: 15672257
Conc: 5.68 ng/ml m

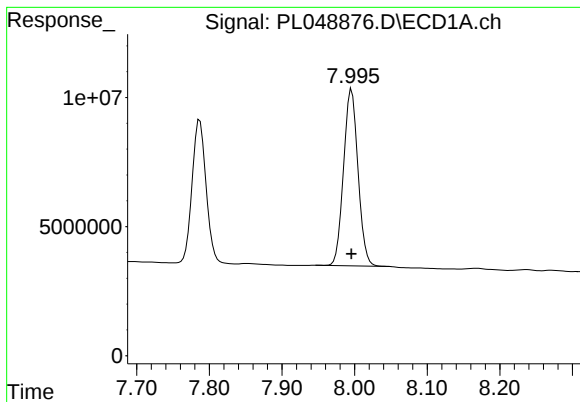

#28 Decachlorobiphenyl

R.T.: 7.996 min

Delta R.T.: 0.000 min


Response: 94774639

Conc: 9.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-S

Manual Integrations
APPROVED

Ankita
5/24/2019 10:02:21 AM

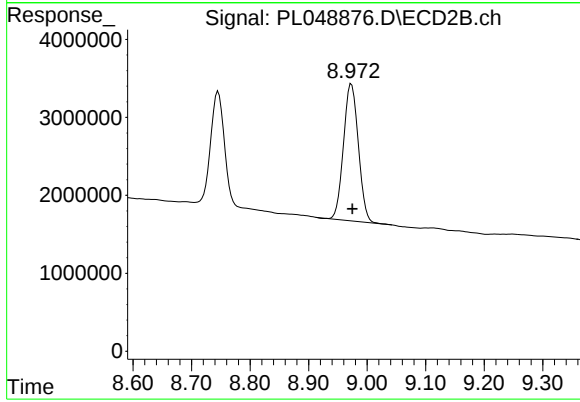

#28 Decachlorobiphenyl

R.T.: 8.973 min

Delta R.T.: -0.002 min

Response: 30948578

Conc: 11.66 ng/ml