

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052322\
 Data File : PL074941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2022 11:17
 Operator : AR\AJ
 Sample : N2874-10RE 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P007-SS002-2430-01RE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/24/2022
 Supervised By :Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 02:39:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.653	4.648	198460	447805	0.391m	0.326m
2) SA Decachlor...	11.649	10.402	1508000	3292964	3.377	3.208

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052322\
Data File : PL074941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2022 11:17
Operator : AR\AJ
Sample : N2874-10RE 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
P007-SS002-2430-01RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/24/2022
Supervised By : Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:39:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

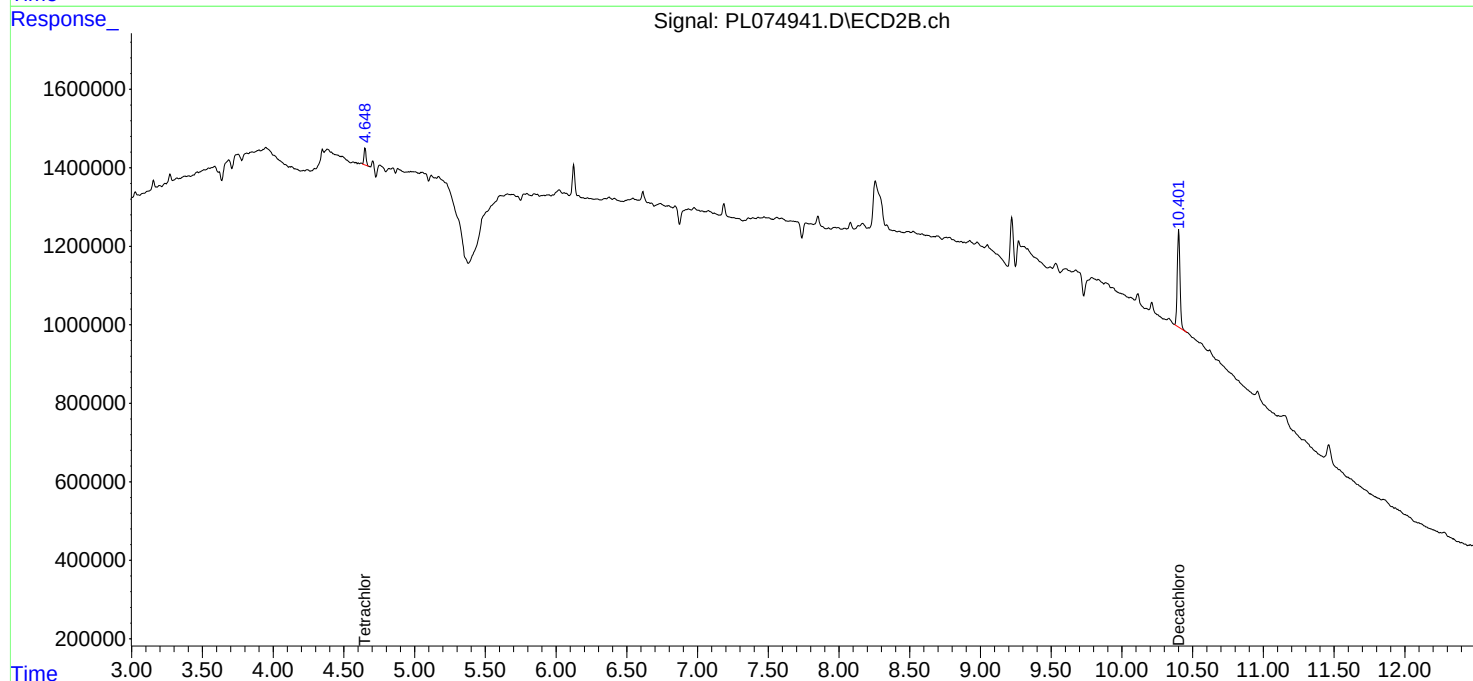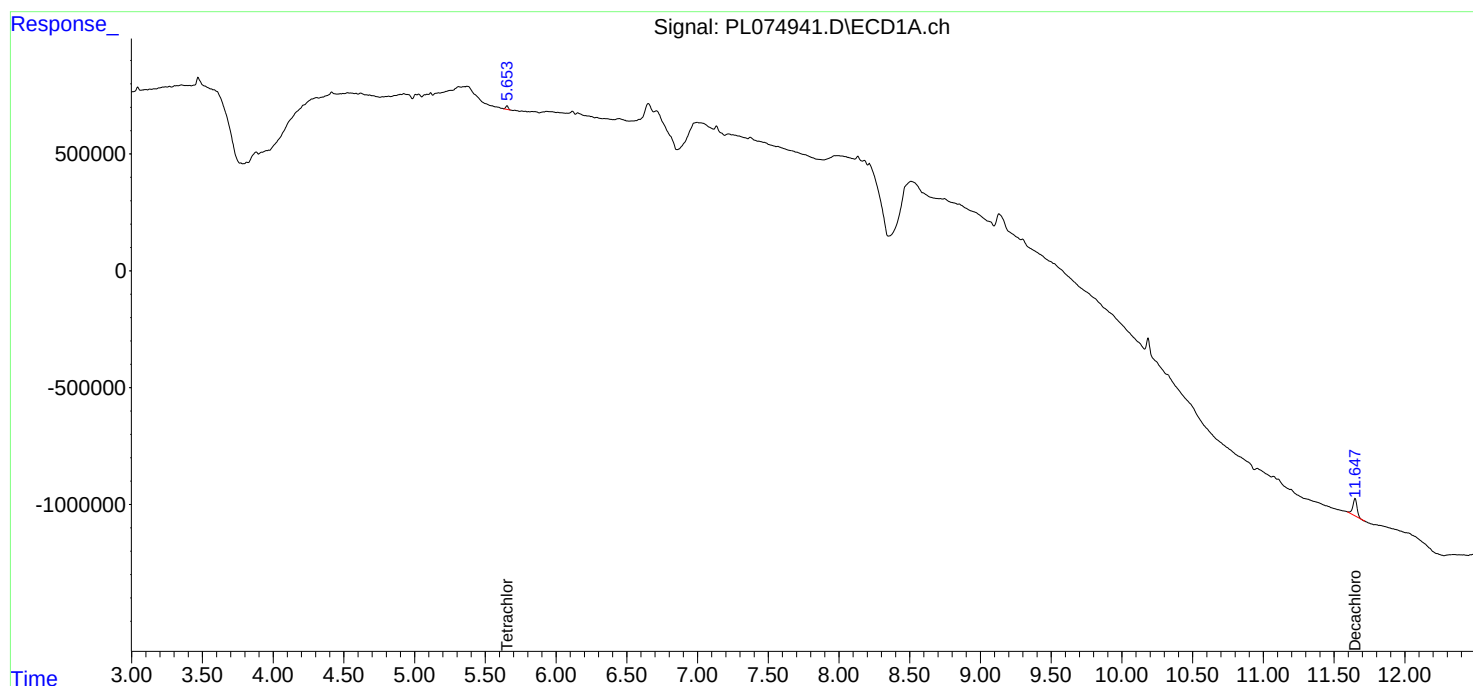

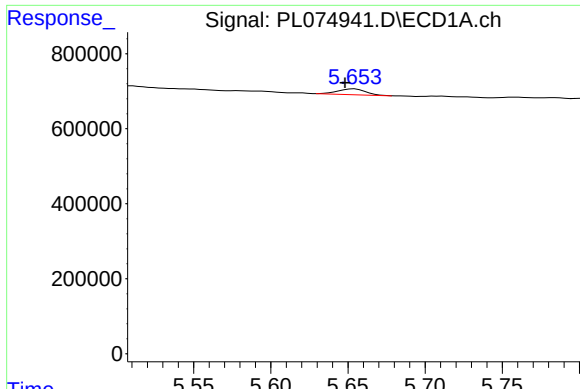


#1 Tetrachloro-m-xylene

R.T.: 5.653 min
Delta R.T.: 0.005 min
Response: 198460
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
P007-SS002-2430-01RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

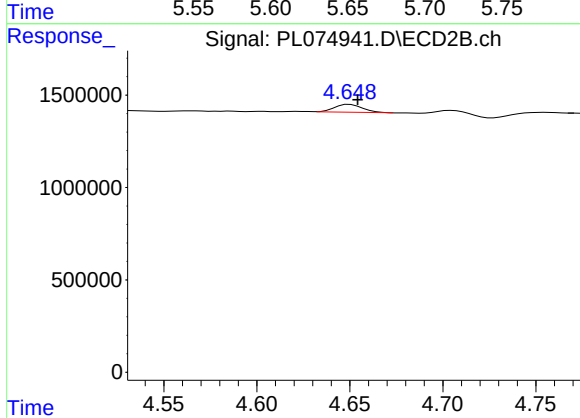


#1 Tetrachloro-m-xylene

R.T.: 4.648 min
Delta R.T.: -0.006 min
Response: 447805
Conc: 0.33 ng/ml m

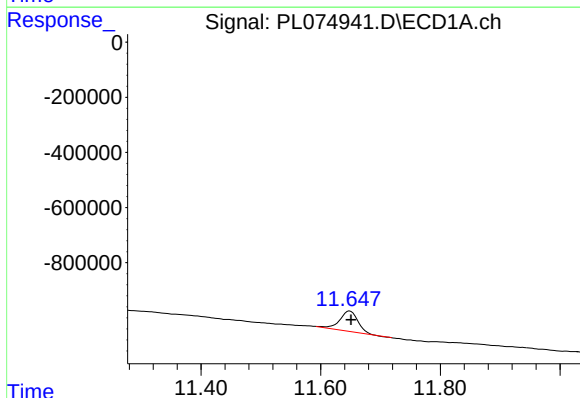

#28 Decachlorobiphenyl

R.T.: 11.649 min
Delta R.T.: -0.002 min
Response: 1508000
Conc: 3.38 ng/ml

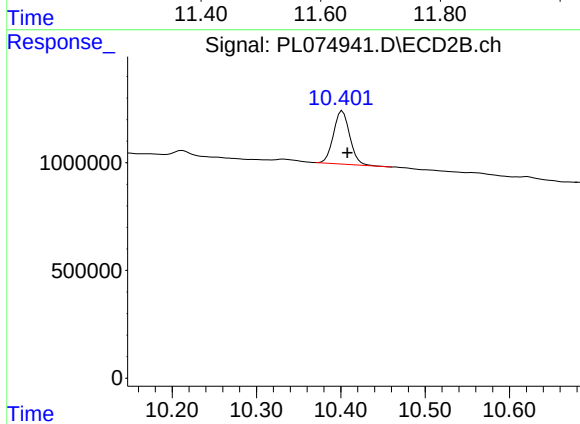

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: -0.006 min
Response: 3292964
Conc: 3.21 ng/ml