

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052322\
 Data File : PL074946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2022 15:55
 Operator : AR\AJ
 Sample : N2877-02 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P007-SS015-0006-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/24/2022
 Supervised By : Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 02:41:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.643	4.646	806612	2305784	1.589	1.680
2) SA Decachlor...	11.636f	10.395	1178534	2632797	2.639m	2.565

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052322\
Data File : PL074946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2022 15:55
Operator : AR\AJ
Sample : N2877-02 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
P007-SS015-0006-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/24/2022
Supervised By : Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:41:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

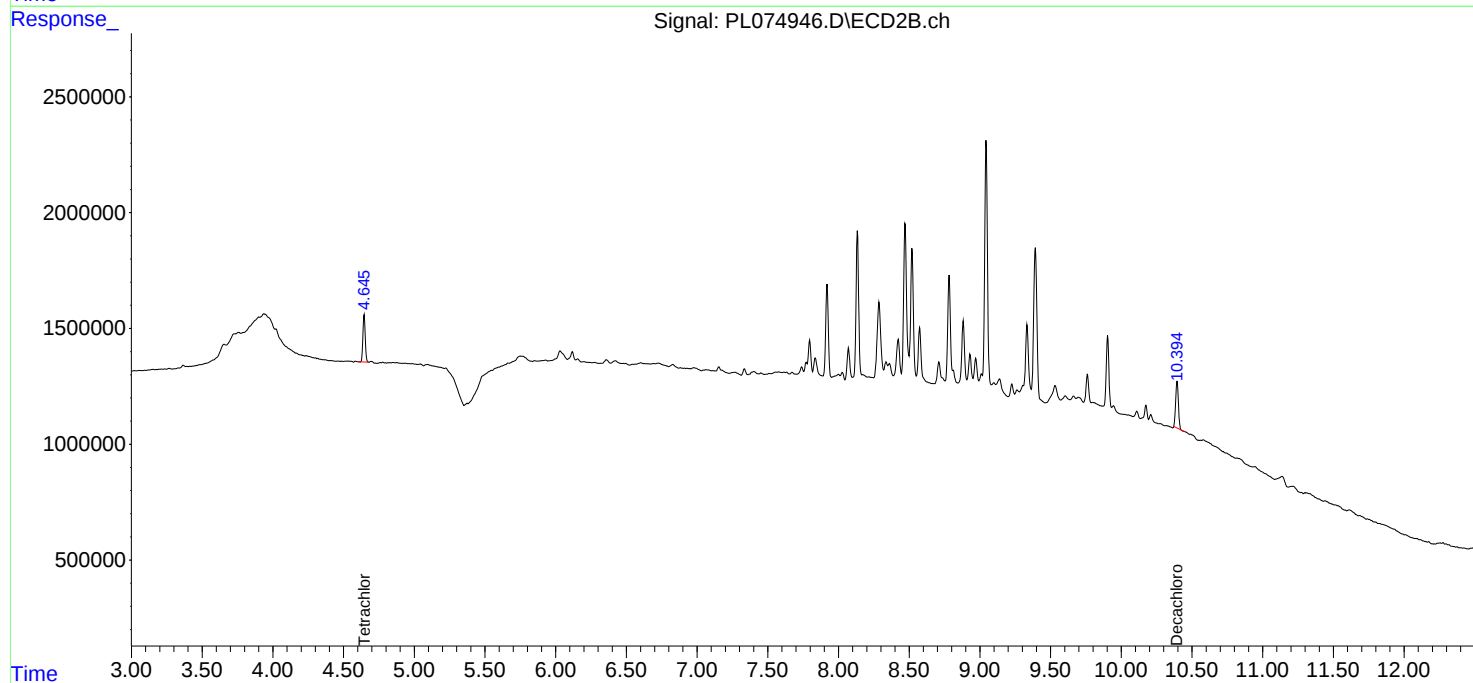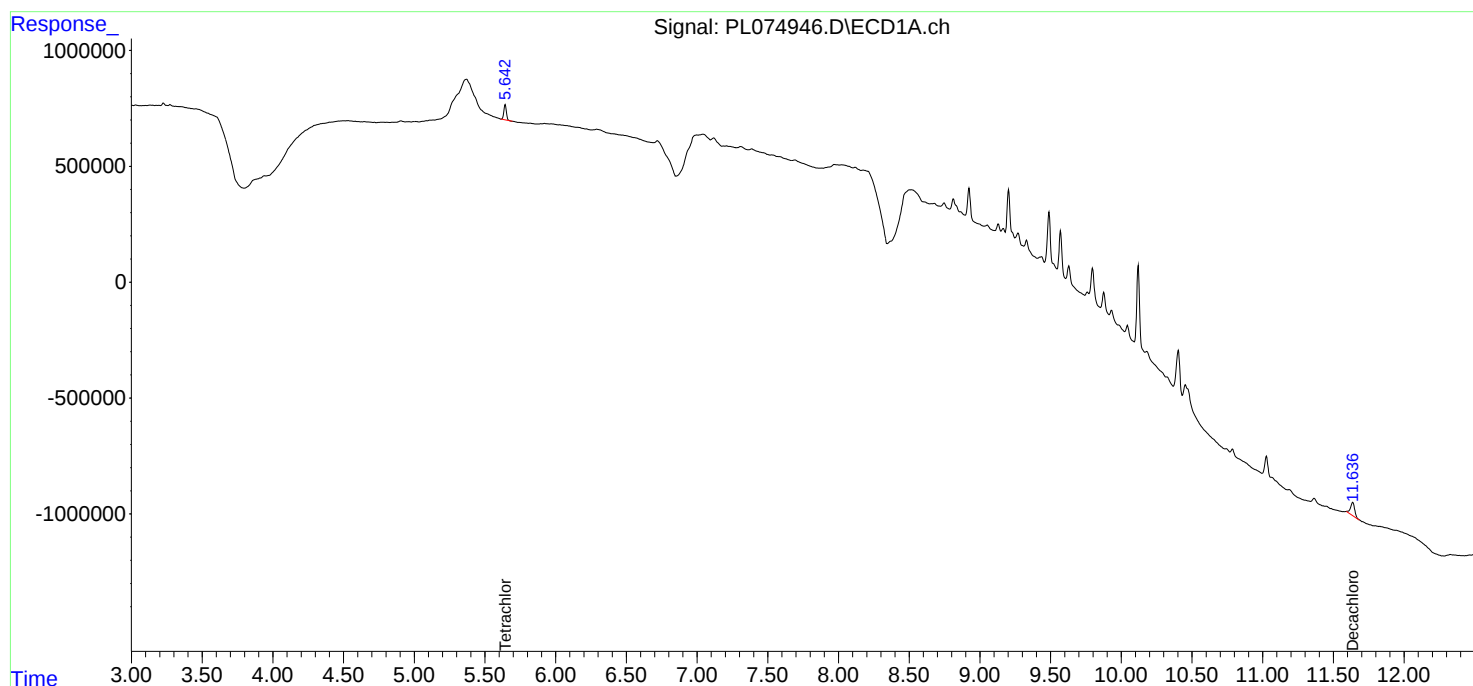

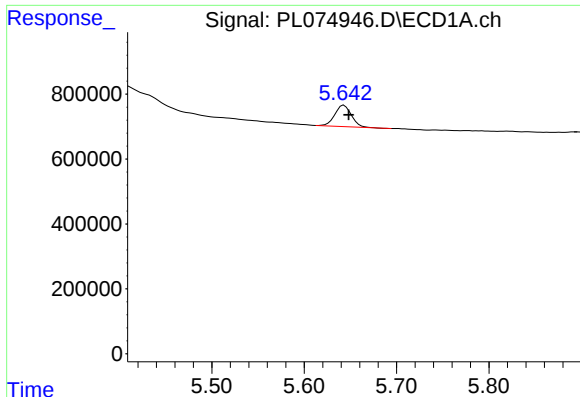

#1 Tetrachloro-m-xylene

R.T.: 5.643 min
Delta R.T.: -0.005 min
Response: 806612
Conc: 1.59 ng/ml


Instrument :
ECD_L
ClientSampleId :
P007-SS015-0006-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2022
Supervised By :Ankita Jodhani 05/24/2022

#1 Tetrachloro-m-xylene

R.T.: 4.646 min
Delta R.T.: -0.008 min
Response: 2305784
Conc: 1.68 ng/ml

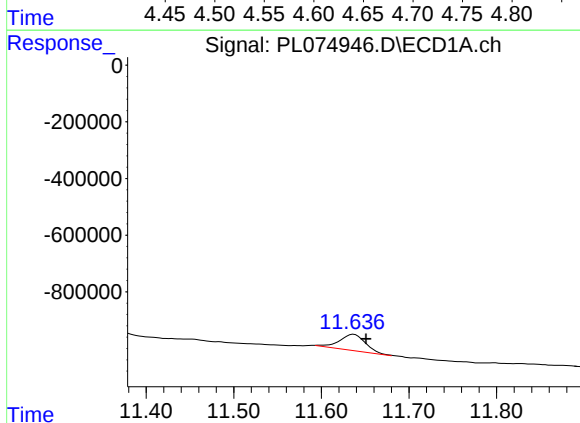

#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: -0.015 min
Response: 1178534
Conc: 2.64 ng/ml m

#28 Decachlorobiphenyl

R.T.: 10.395 min
Delta R.T.: -0.013 min
Response: 2632797
Conc: 2.57 ng/ml