

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052323\
 Data File : PL082916.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2023 09:43
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 21:07:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	2.637	142.1E6	149.7E6	48.338	57.663
28)	SA Decachlor...	8.733	7.742	91544268	111.9E6	43.648	44.987
Target Compounds							
23)	Chlordane-1	4.459	3.619	63368668	47013508	579.236	569.769
24)	Chlordane-2	4.986	4.192	65563206	49961904	595.174	561.186
25)	Chlordane-3	5.691	4.818	243.3E6	153.2E6	586.374	574.823
26)	Chlordane-4	5.771	4.879	292.3E6	161.0E6	577.289	571.538
27)	Chlordane-5	6.613	5.771	47520507	51724648	579.045	532.441



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052323\
Data File : PL082916.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2023 09:43
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 21:07:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

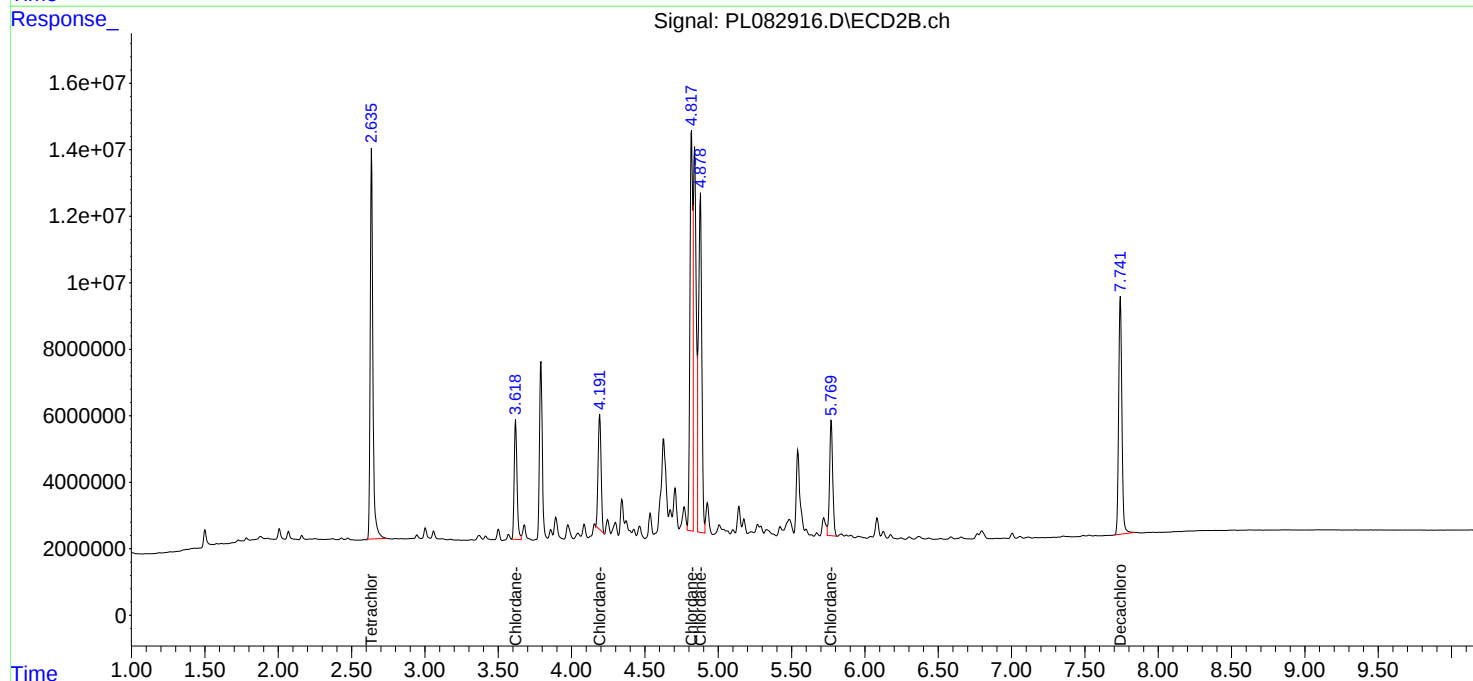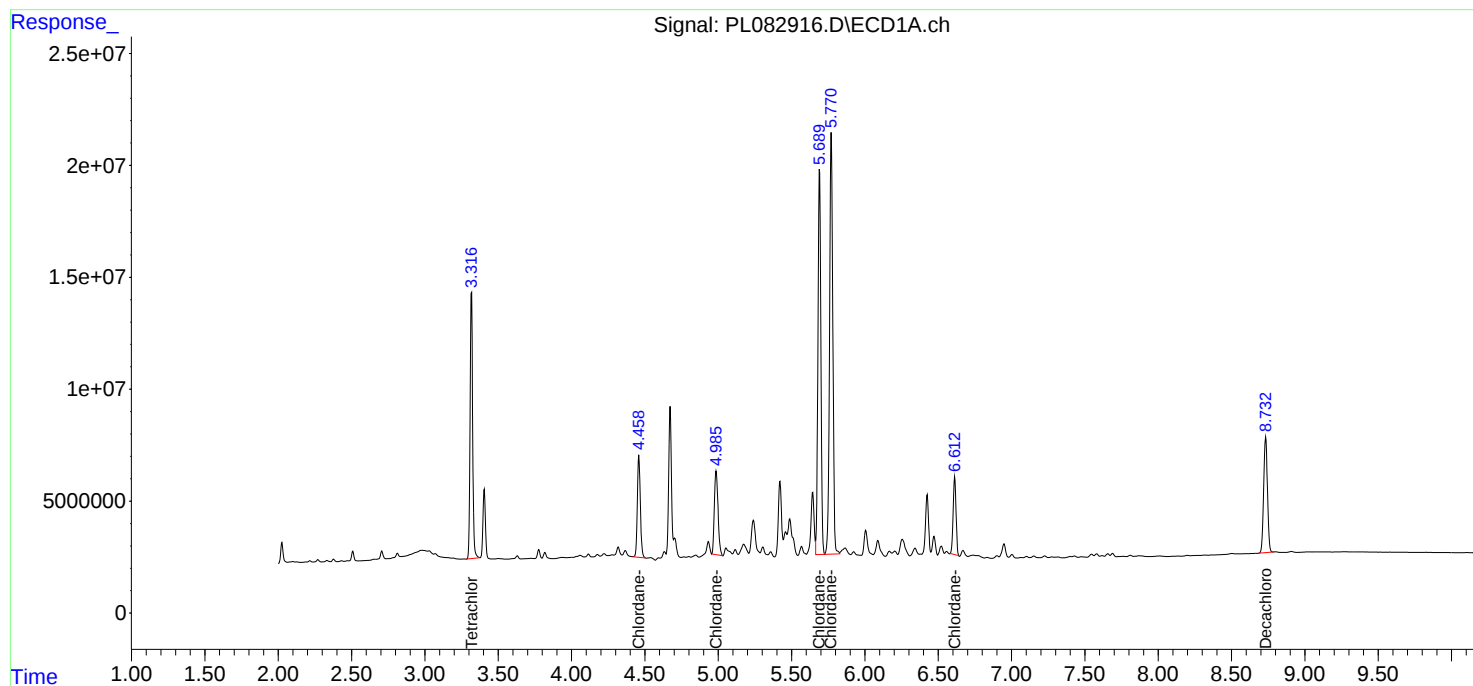


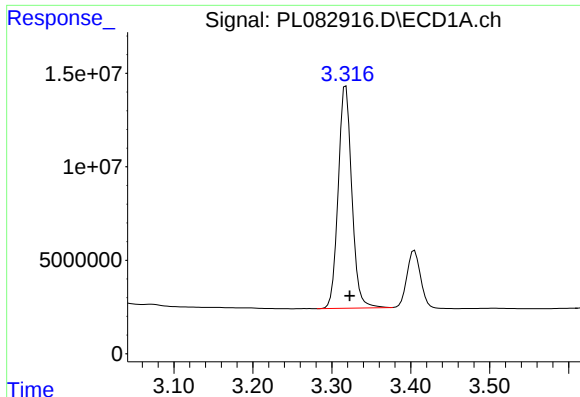

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: -0.005 min
Response: 142066724
Conc: 48.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

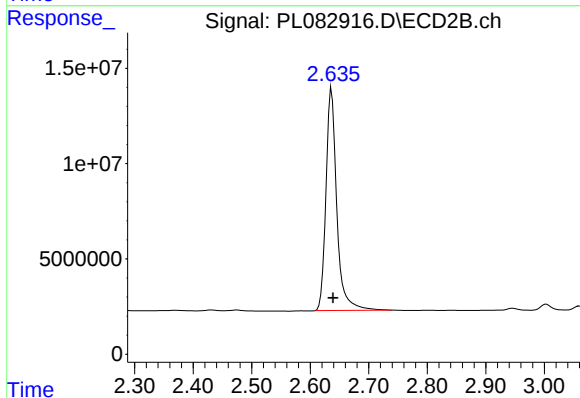


#1 Tetrachloro-m-xylene

R.T.: 2.637 min
Delta R.T.: -0.002 min
Response: 149697636
Conc: 57.66 ng/ml

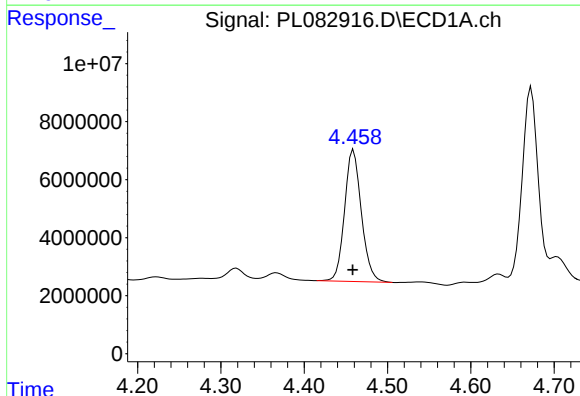


#23 Chlordane-1

R.T.: 4.459 min
Delta R.T.: 0.001 min
Response: 63368668
Conc: 579.24 ng/ml

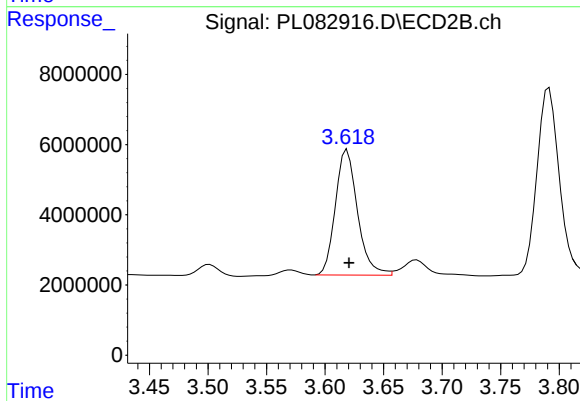

#23 Chlordane-1


R.T.: 3.619 min
Delta R.T.: -0.001 min
Response: 47013508
Conc: 569.77 ng/ml

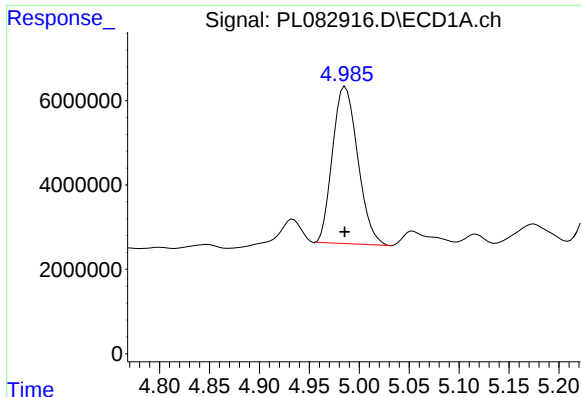

#24 Chlordane-2


R.T.: 4.986 min
Delta R.T.: 0.000 min
Response: 65563206
Conc: 595.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

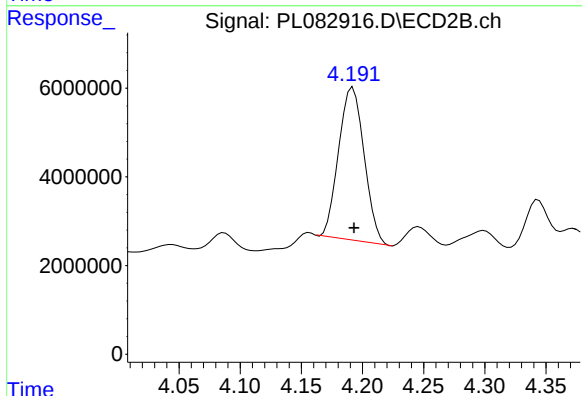


#24 Chlordane-2

R.T.: 4.192 min
Delta R.T.: 0.000 min
Response: 49961904
Conc: 561.19 ng/ml

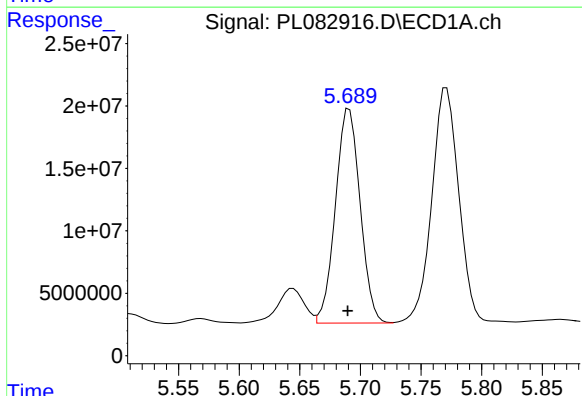


#25 Chlordane-3

R.T.: 5.691 min
Delta R.T.: 0.001 min
Response: 243288218
Conc: 586.37 ng/ml

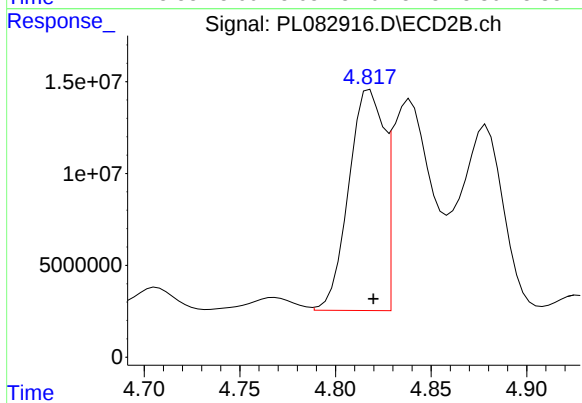

#25 Chlordane-3


R.T.: 4.818 min
Delta R.T.: -0.002 min
Response: 153193118
Conc: 574.82 ng/ml

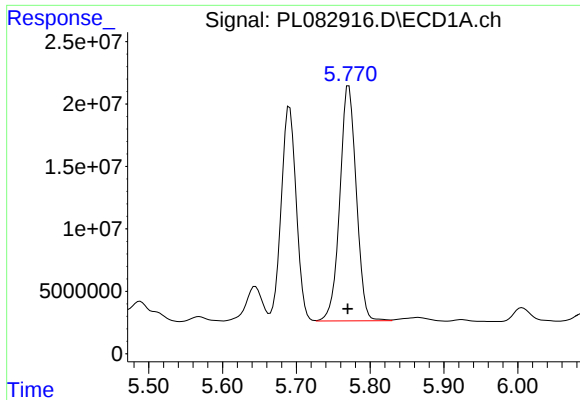

#26 Chlordane-4


R.T.: 5.771 min
Delta R.T.: 0.001 min
Response: 292325842
Conc: 577.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

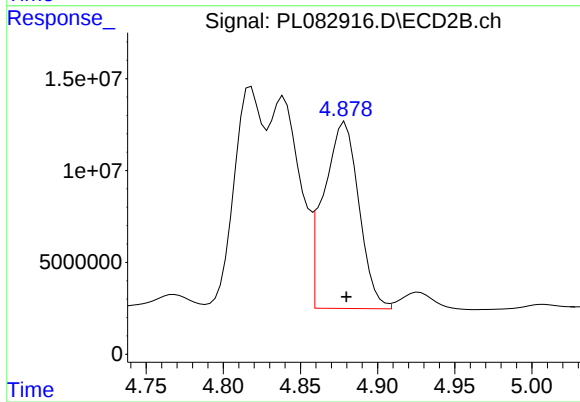


#26 Chlordane-4

R.T.: 4.879 min
Delta R.T.: 0.000 min
Response: 161031473
Conc: 571.54 ng/ml

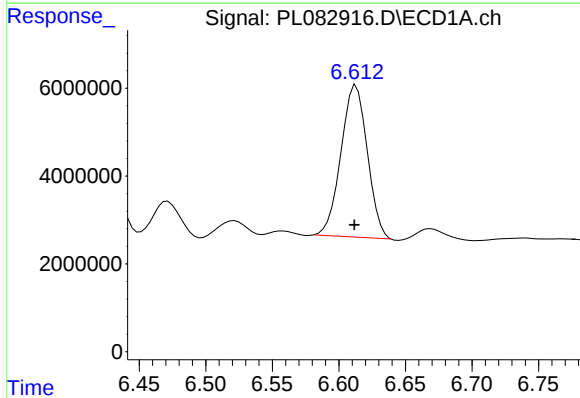


#27 Chlordane-5

R.T.: 6.613 min
Delta R.T.: 0.001 min
Response: 47520507
Conc: 579.04 ng/ml

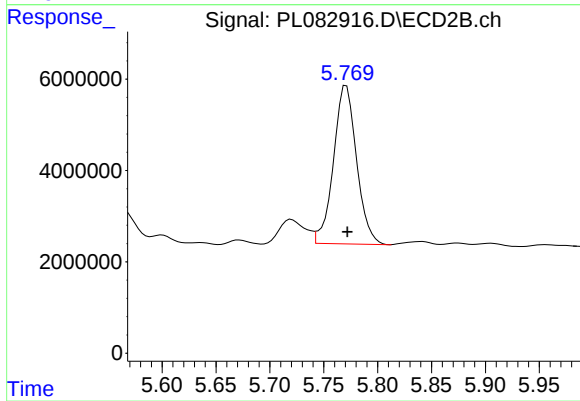

#27 Chlordane-5


R.T.: 5.771 min
Delta R.T.: -0.001 min
Response: 51724648
Conc: 532.44 ng/ml

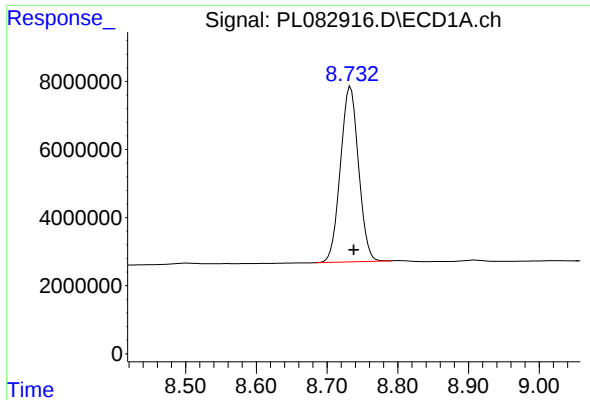

#28 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: -0.005 min
Response: 91544268
Conc: 43.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

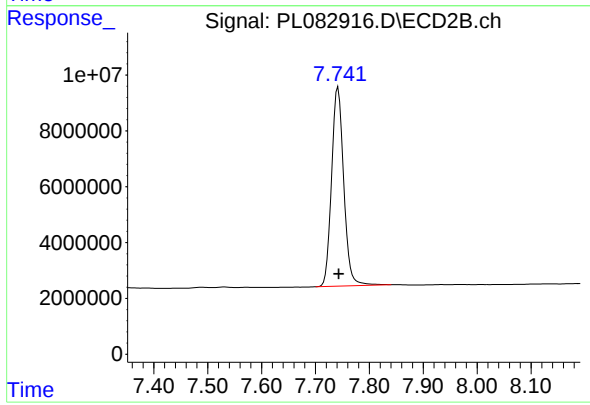

#28 Decachlorobiphenyl

R.T.: 7.742 min
Delta R.T.: -0.002 min
Response: 111862731
Conc: 44.99 ng/ml