

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052323\
 Data File : PL082920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2023 10:55
 Operator : AR\AJ
 Sample : PB152720BS
 Misc : CH-BS
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB152720BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 21:10:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	2.636	53591606	57498702	18.235	22.148
28)	SA Decachlor...	8.732	7.742	37819750	46276901	18.032	18.611
Target Compounds							
23)	Chlordane-1	4.458	3.619	24225768	18376243	221.441	222.707
24)	Chlordane-2	4.985	4.192	26112101	20225980	237.042	227.184
25)	Chlordane-3	5.690	4.818	90588837	57167421	218.337	214.508
26)	Chlordane-4	5.770	4.878	111.1E6	60409980	219.365	214.409
27)	Chlordane-5	6.612	5.770	18526158	19796067	225.744	203.776



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052323\
Data File : PL082920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2023 10:55
Operator : AR\AJ
Sample : PB152720BS
Misc : CH-BS
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB152720BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 21:10:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

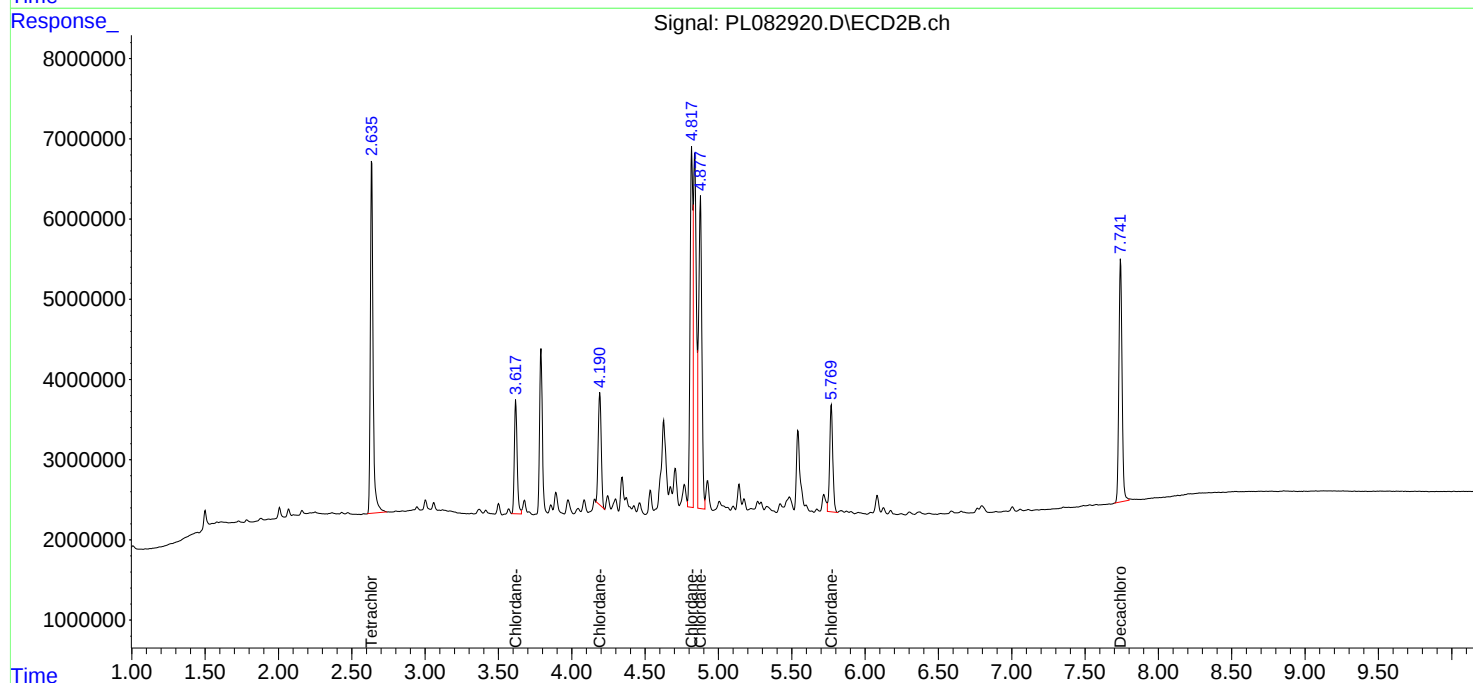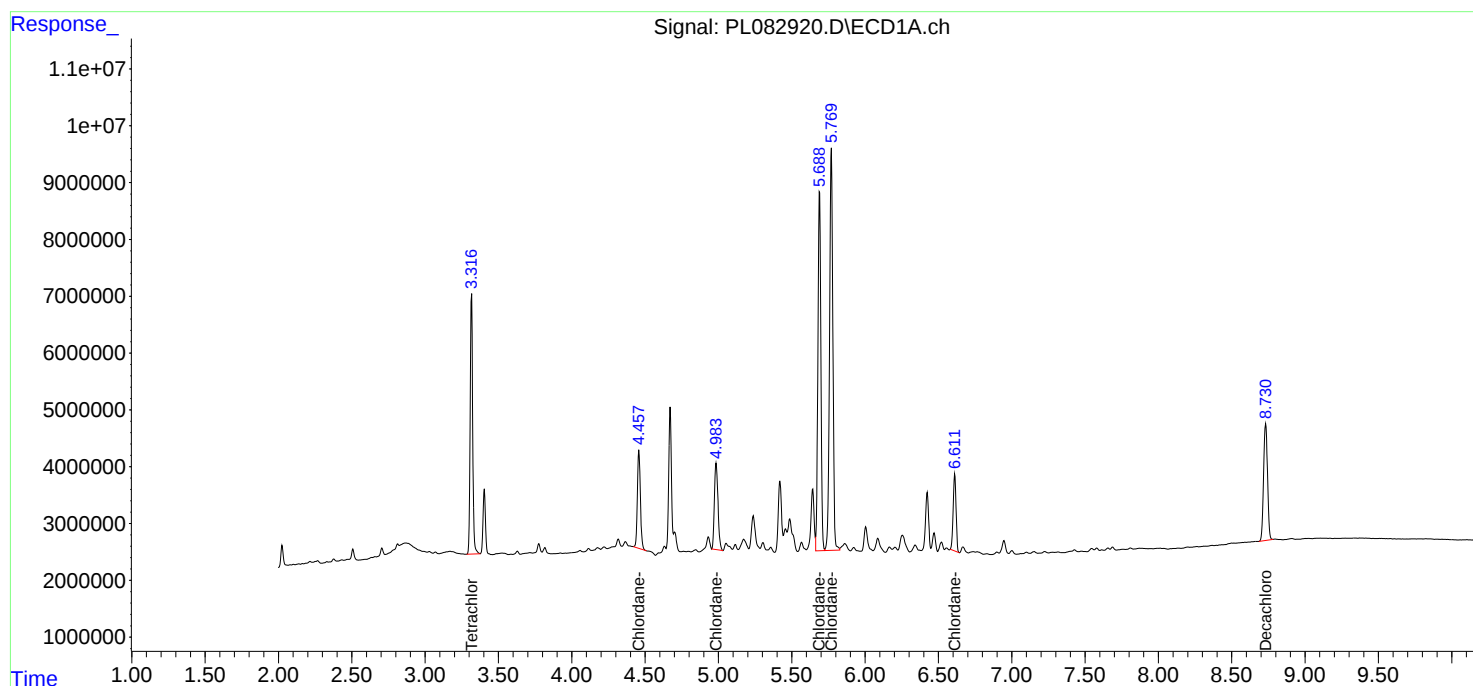


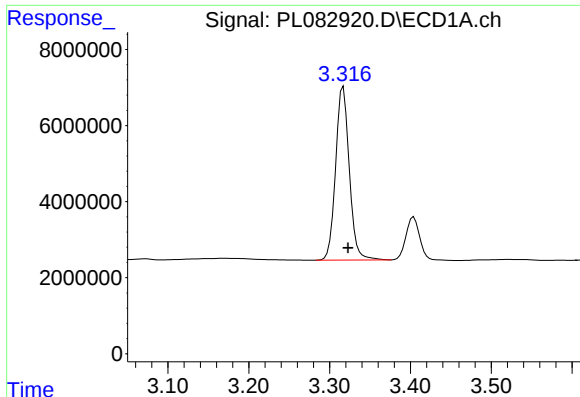

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: -0.006 min
Response: 53591606
Conc: 18.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152720BS

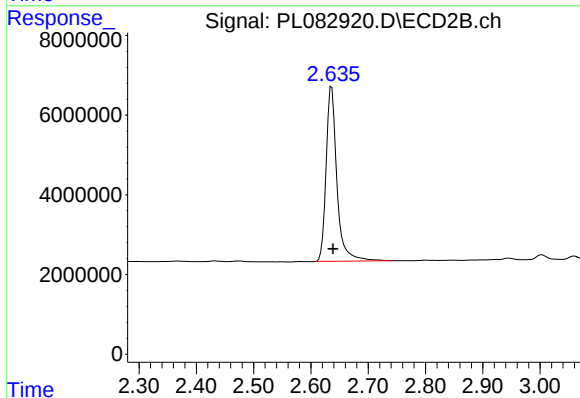


#1 Tetrachloro-m-xylene

R.T.: 2.636 min
Delta R.T.: -0.003 min
Response: 57498702
Conc: 22.15 ng/ml

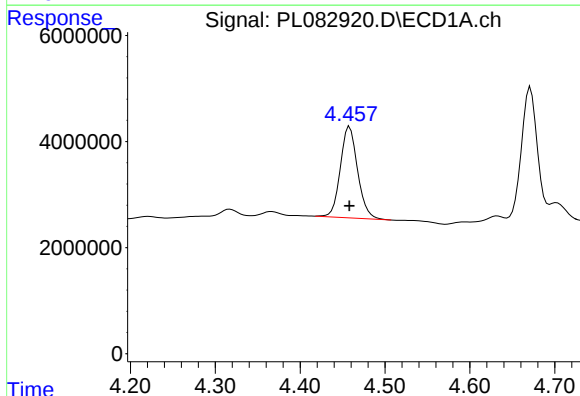


#23 Chlordane-1

R.T.: 4.458 min
Delta R.T.: 0.000 min
Response: 24225768
Conc: 221.44 ng/ml

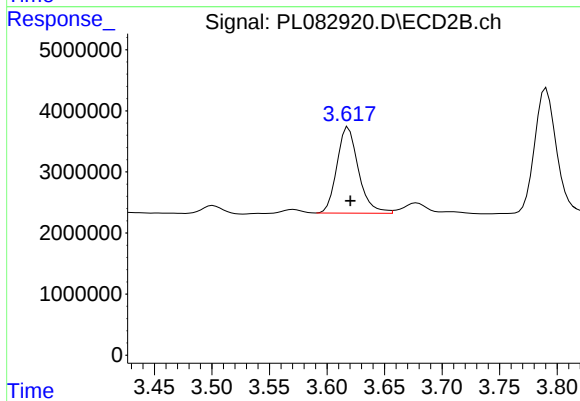

#23 Chlordane-1


R.T.: 3.619 min
Delta R.T.: -0.002 min
Response: 18376243
Conc: 222.71 ng/ml

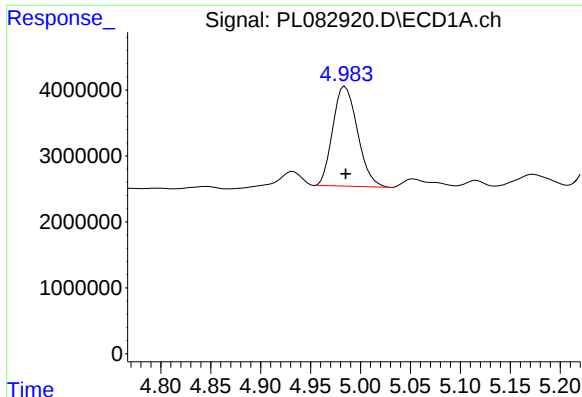

#24 Chlordane-2


R.T.: 4.985 min
Delta R.T.: 0.000 min
Response: 26112101
Conc: 237.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152720BS

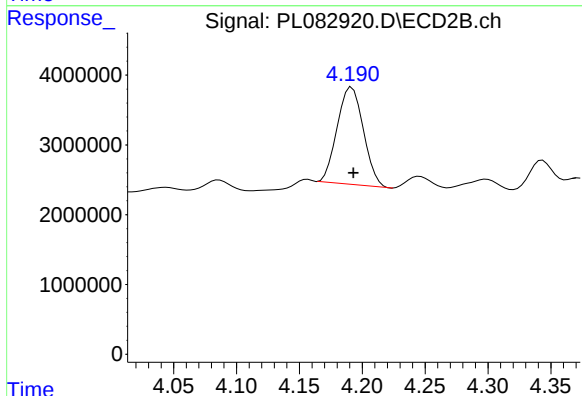


#24 Chlordane-2

R.T.: 4.192 min
Delta R.T.: -0.001 min
Response: 20225980
Conc: 227.18 ng/ml

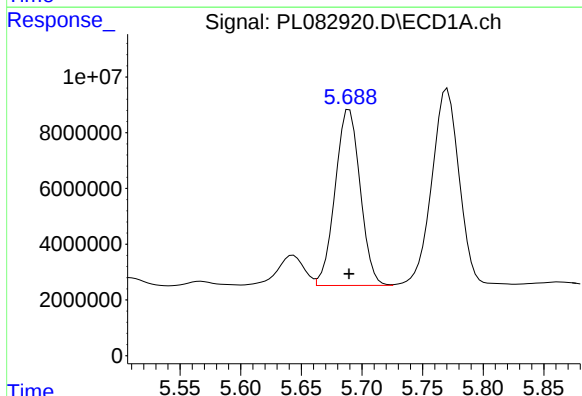


#25 Chlordane-3

R.T.: 5.690 min
Delta R.T.: 0.000 min
Response: 90588837
Conc: 218.34 ng/ml

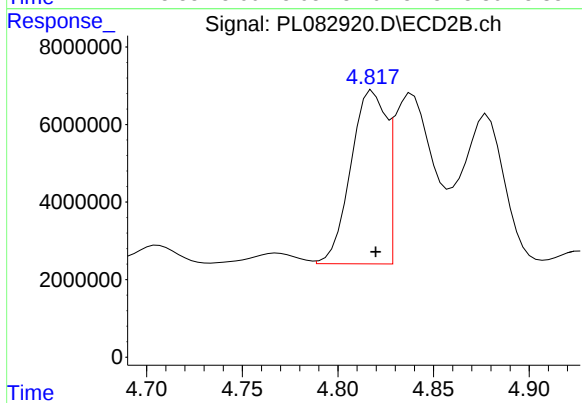

#25 Chlordane-3


R.T.: 4.818 min
Delta R.T.: -0.001 min
Response: 57167421
Conc: 214.51 ng/ml

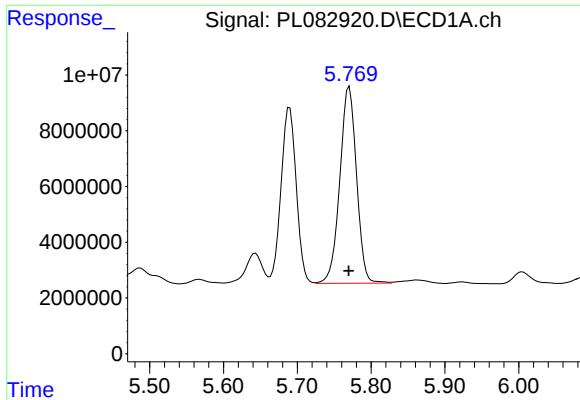

#26 Chlordane-4


R.T.: 5.770 min
Delta R.T.: 0.000 min
Response: 111081195
Conc: 219.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152720BS

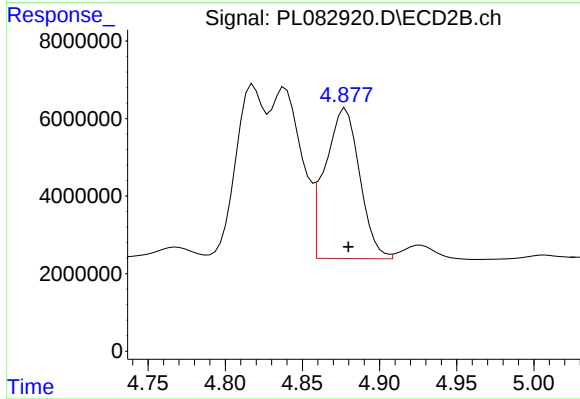


#26 Chlordane-4

R.T.: 4.878 min
Delta R.T.: -0.002 min
Response: 60409980
Conc: 214.41 ng/ml

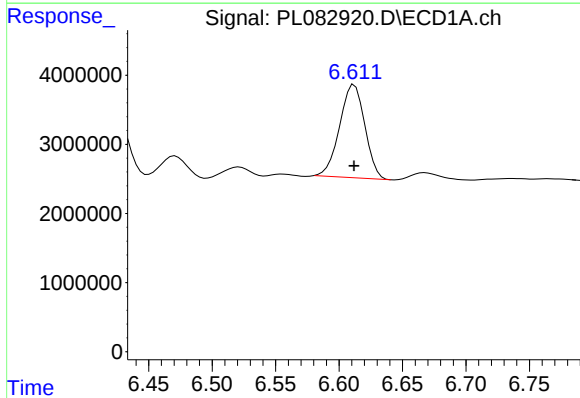


#27 Chlordane-5

R.T.: 6.612 min
Delta R.T.: 0.000 min
Response: 18526158
Conc: 225.74 ng/ml

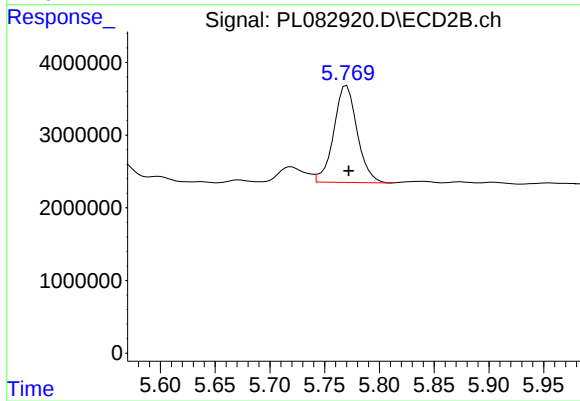

#27 Chlordane-5


R.T.: 5.770 min
Delta R.T.: -0.002 min
Response: 19796067
Conc: 203.78 ng/ml

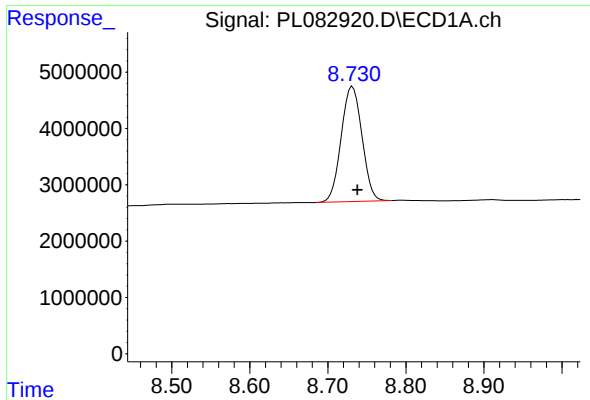

#28 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.006 min
Response: 37819750
Conc: 18.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152720BS

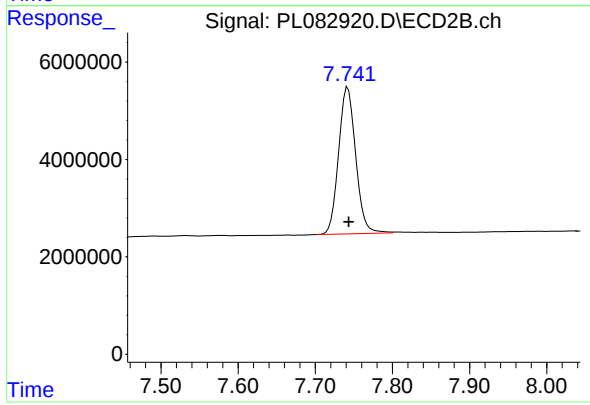

#28 Decachlorobiphenyl

R.T.: 7.742 min
Delta R.T.: -0.001 min
Response: 46276901
Conc: 18.61 ng/ml