

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052323\
 Data File : PL082939.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2023 16:53
 Operator : AR\AJ
 Sample : 02888-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FS-SB-20(ELEV-28-26)

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/24/2023
 Supervised By : Ankita Jodhani 05/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 21:23:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.318	2.638	51694805	42468012	17.589	16.358
28) SA Decachlor...	8.735	7.743	41663908	42533945	19.865	17.106m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052323\
Data File : PL082939.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2023 16:53
Operator : AR\AJ
Sample : 02888-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FS-SB-20(ELEV-28-26)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2023
Supervised By :Ankita Jodhani 05/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 21:23:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

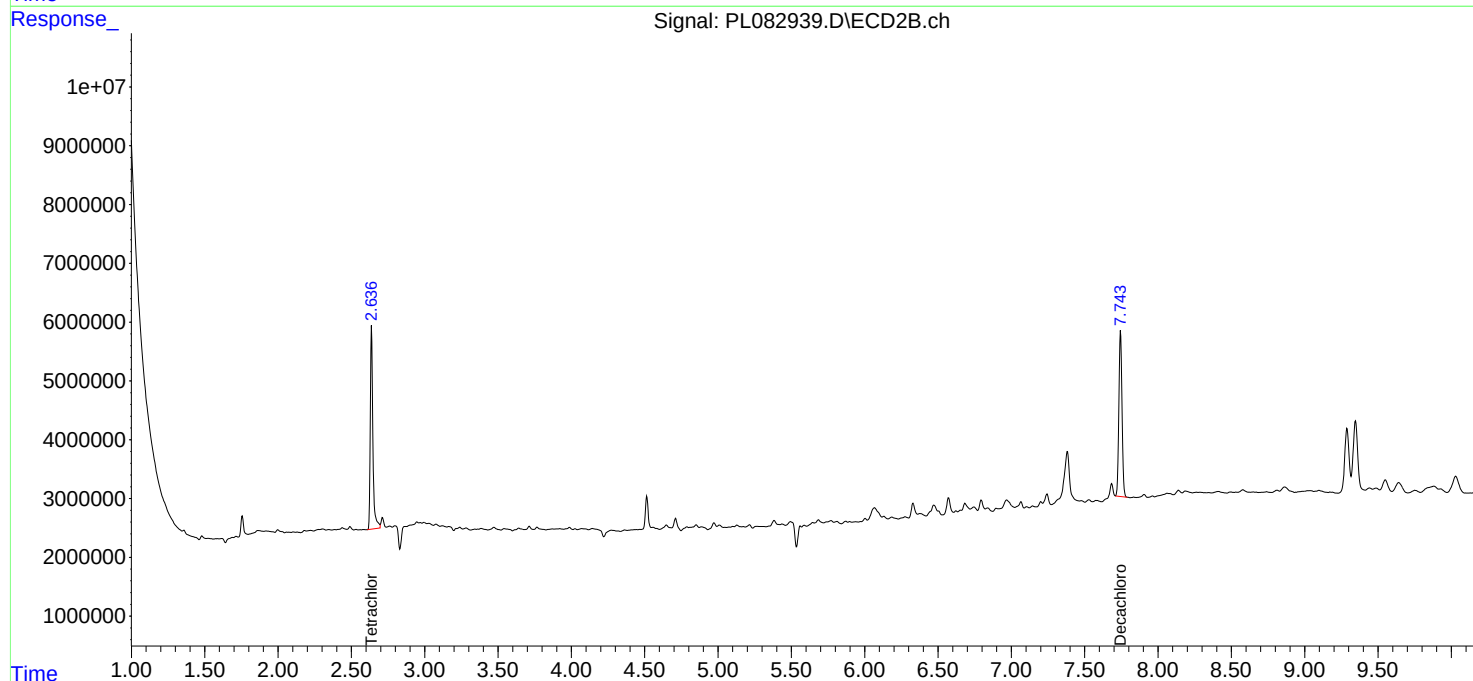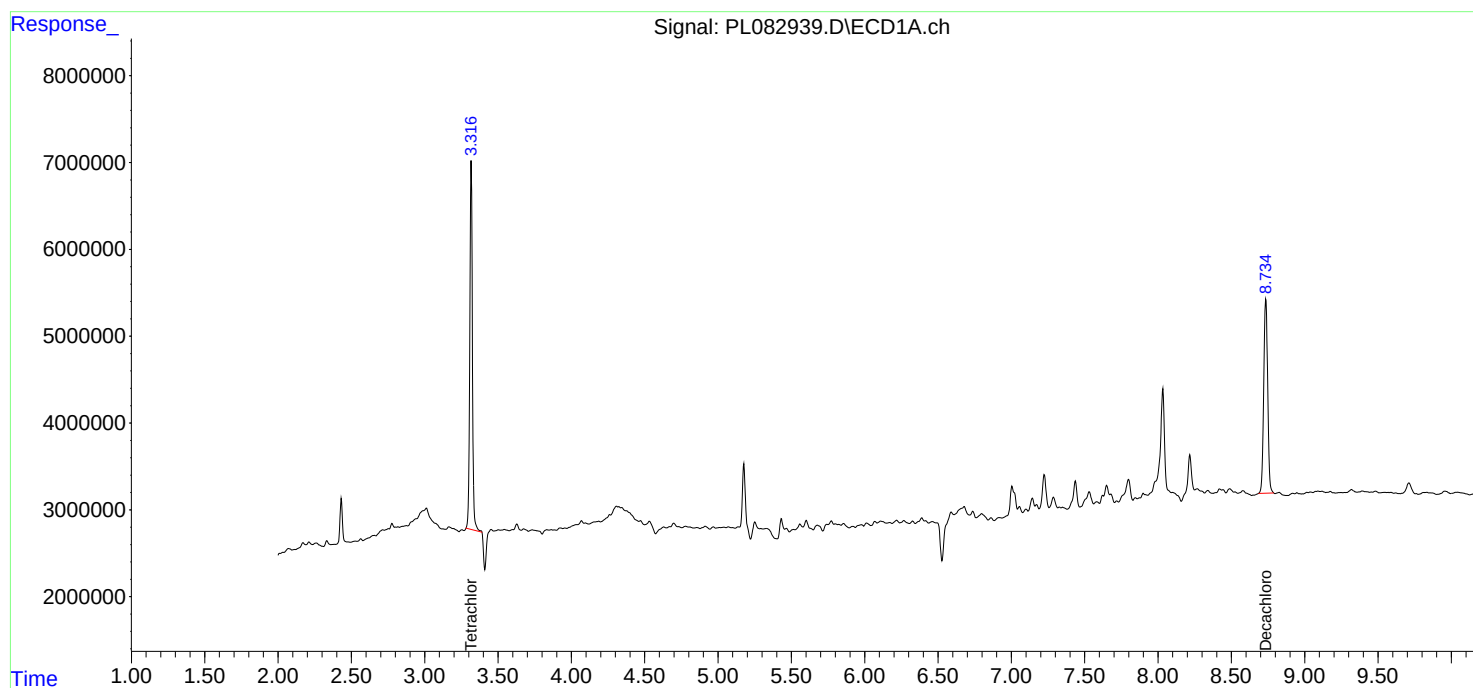

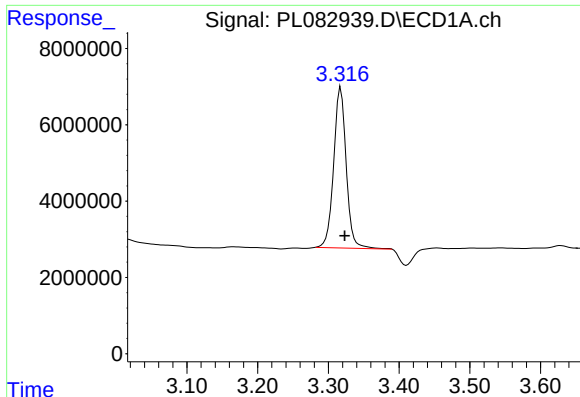


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: -0.005 min
Response: 51694805
Conc: 17.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
FS-SB-20(ELEV-28-26)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2023
Supervised By :Ankita Jodhani 05/24/2023

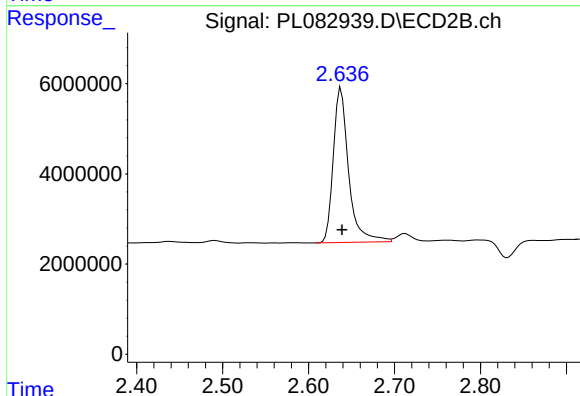


#1 Tetrachloro-m-xylene

R.T.: 2.638 min
Delta R.T.: -0.001 min
Response: 42468012
Conc: 16.36 ng/ml

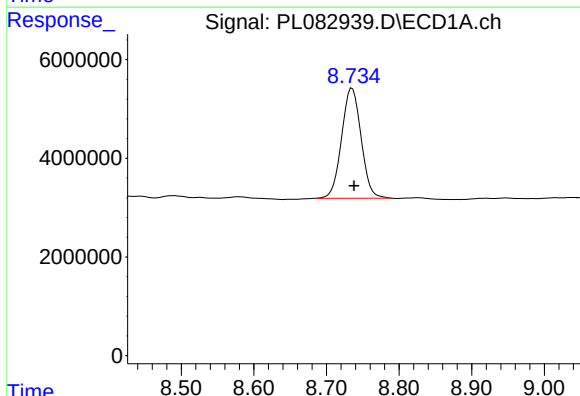

#28 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.003 min
Response: 41663908
Conc: 19.87 ng/ml

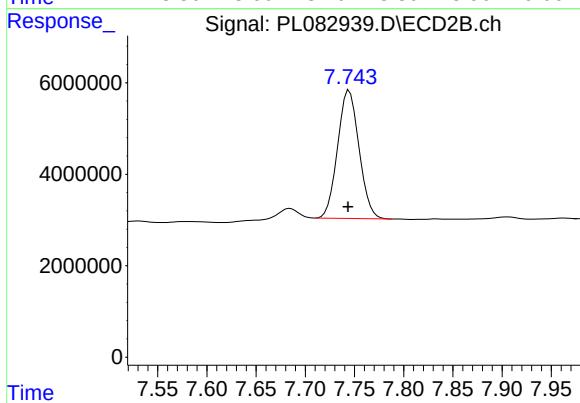

#28 Decachlorobiphenyl

R.T.: 7.743 min
Delta R.T.: 0.000 min
Response: 42533945
Conc: 17.11 ng/ml m