

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052323\
 Data File : PL082948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2023 19:26
 Operator : AR\AJ
 Sample : 02892-10
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-32

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/24/2023
 Supervised By : Ankita Jodhani 05/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 21:28:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	2.635	20964676	23423914	7.133m	9.023m#
28)	SA Decachlor...	8.732	7.741	24852174	29066199	11.849	11.689

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052323\
Data File : PL082948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2023 19:26
Operator : AR\AJ
Sample : 02892-10
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-32


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/24/2023
Supervised By : Ankita Jodhani 05/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 21:28:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

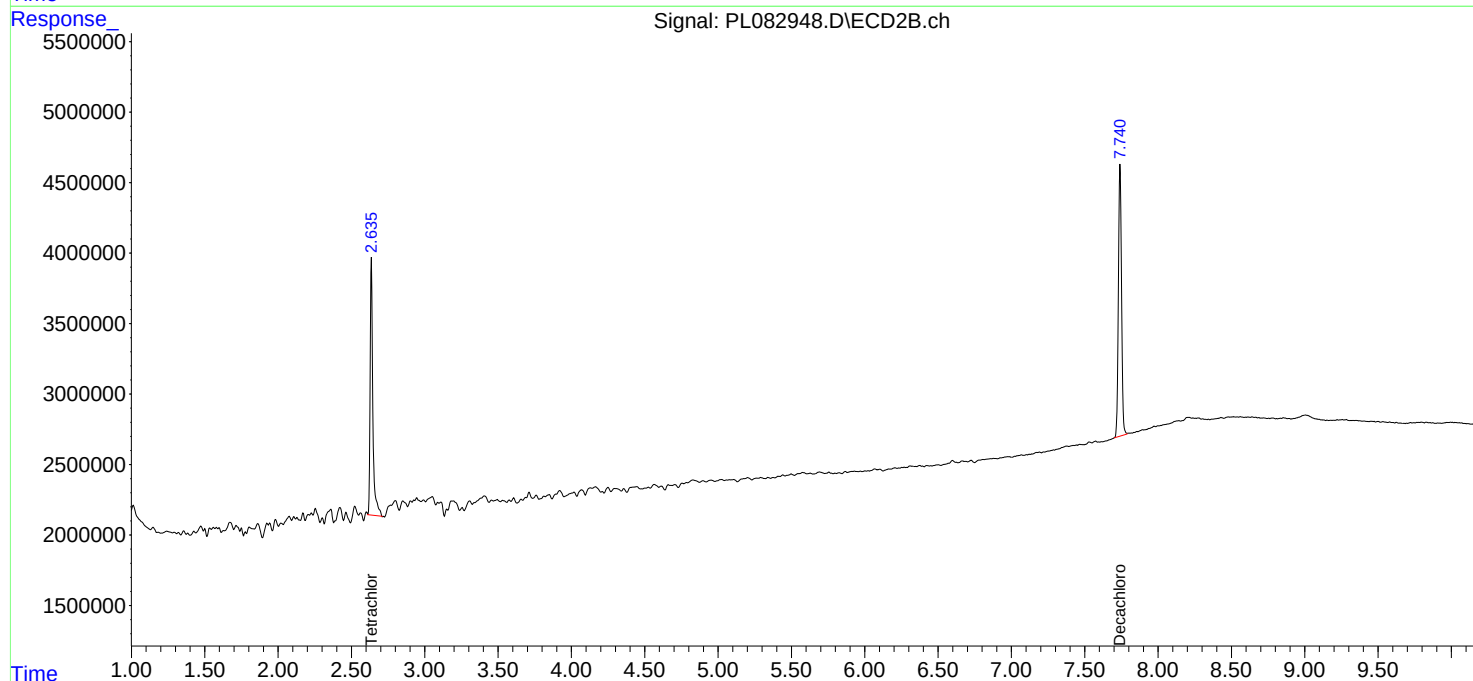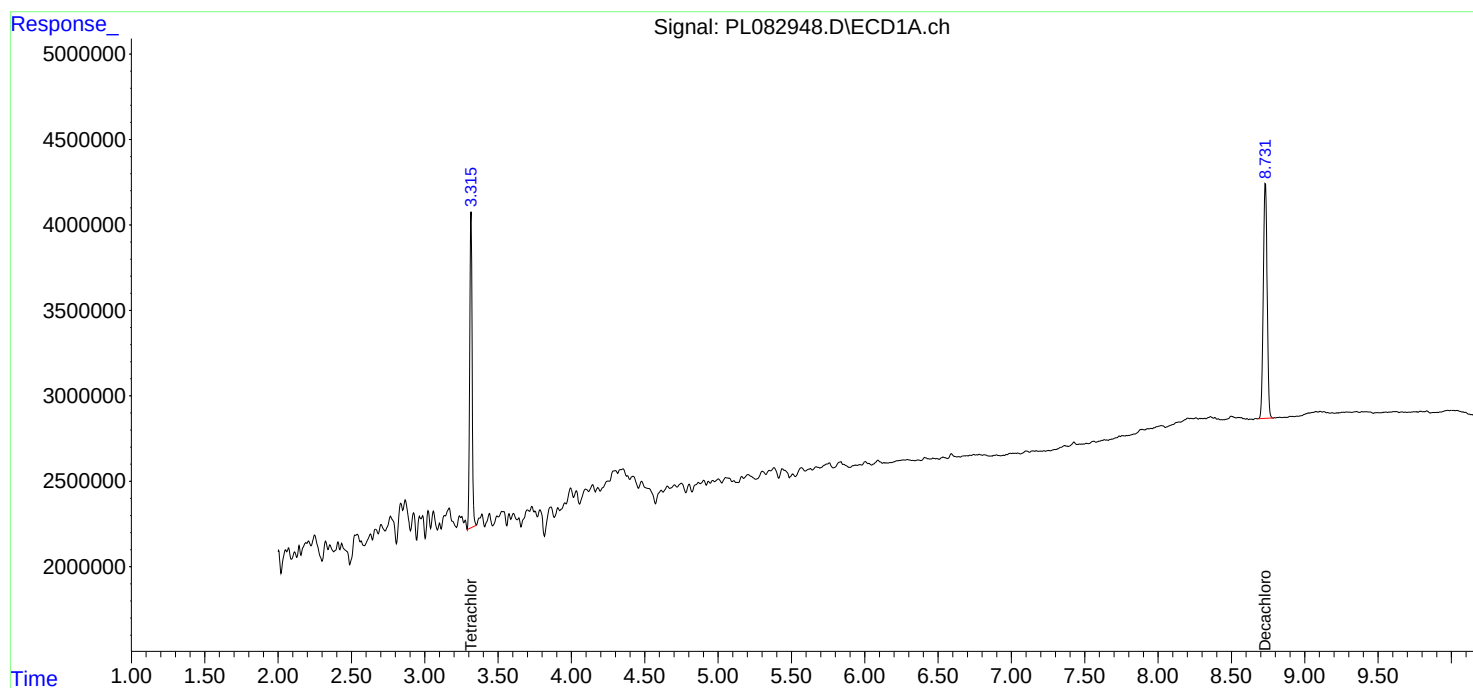

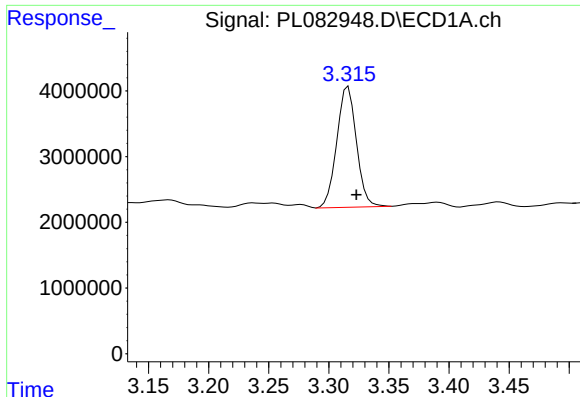


#1 Tetrachloro-m-xylene

R.T.: 3.315 min
Delta R.T.: -0.008 min
Response: 20964676
Conc: 7.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-32


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/24/2023
Supervised By :Ankita Jodhani 05/24/2023

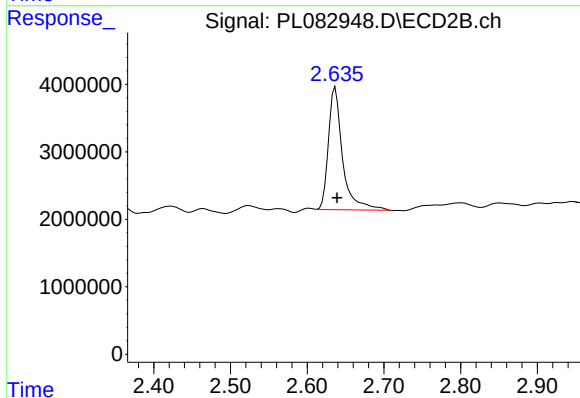


#1 Tetrachloro-m-xylene

R.T.: 2.635 min
Delta R.T.: -0.004 min
Response: 23423914
Conc: 9.02 ng/ml m

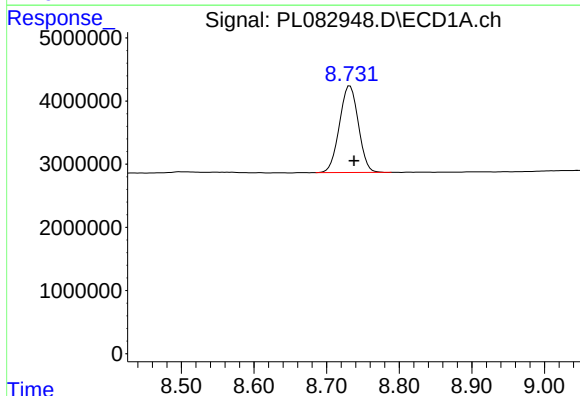

#28 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.006 min
Response: 24852174
Conc: 11.85 ng/ml

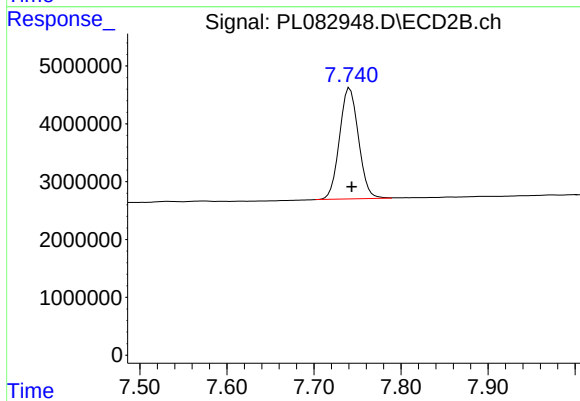

#28 Decachlorobiphenyl

R.T.: 7.741 min
Delta R.T.: -0.002 min
Response: 29066199
Conc: 11.69 ng/ml