

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
 Data File : PL048922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2019 13:50
 Operator : SM\AJ
 Sample : K3004-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-26835

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 22:17:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.338	3.937	213.5E6	16852262	22.038	6.766 #
28)	SA Decachlor...	7.993	8.974	103.6E6	35412602	10.309	13.342 #
Target Compounds							
5)	MB Aldrin	4.548	0.000	9907227	0	0.723	N.D. #
6)	B beta-BHC	4.284	4.798	7743998	4099533	1.312	2.635 #
10)	B gamma-Chl...	5.230f	6.037	5534295	4420929	0.414	1.436 #
11)	B alpha-Chl...	0.000	6.108	0	6508024	N.D.	2.121 #
23)	Chlordane-1	4.168	4.925	11070465	1816903	24.661	14.875 #
24)	Chlordane-2	4.639f	0.000	2411905	0	4.662	N.D. #
25)	Chlordane-3	5.230	6.037	5534295	4420929	3.515	10.088 #
26)	Chlordane-4	0.000	6.108	0	6508024	N.D.	12.406 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
Data File : PL048922.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2019 13:50
Operator : SM\AJ
Sample : K3004-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
CHRT-26835

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 22:17:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

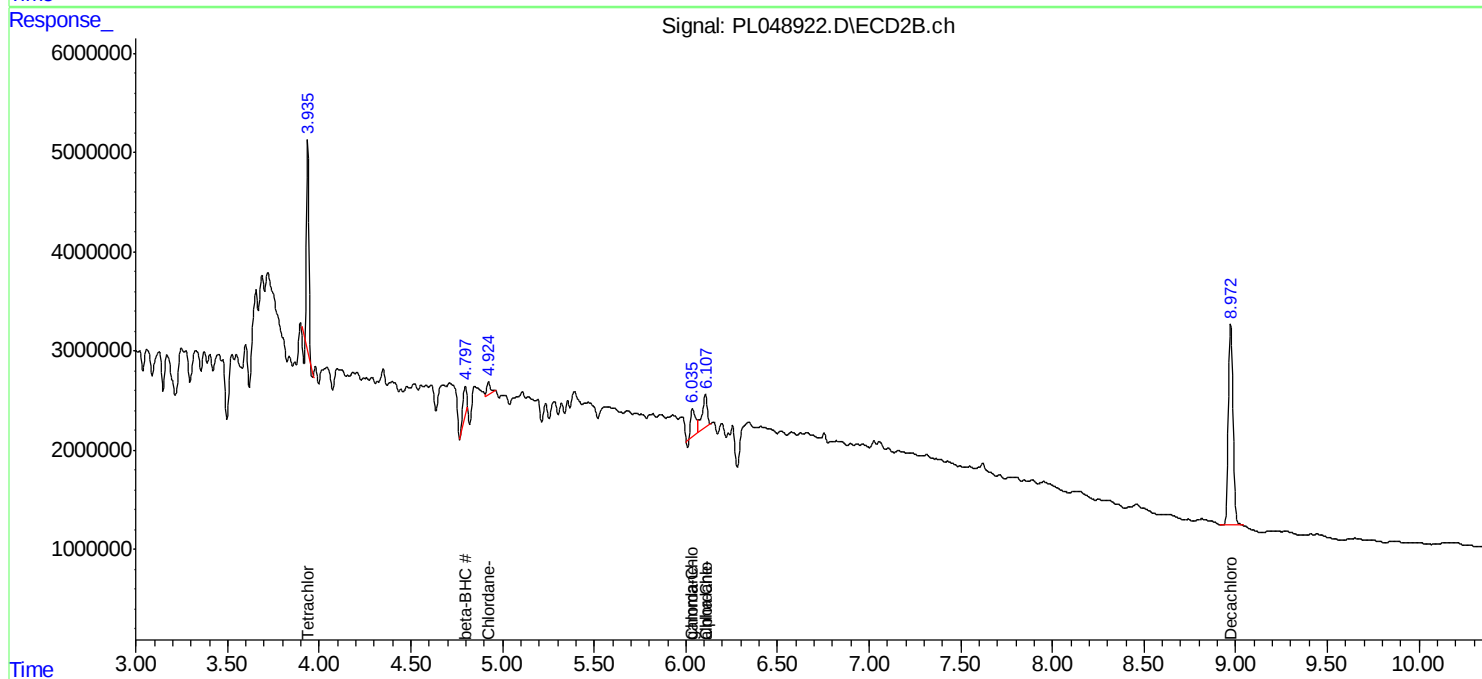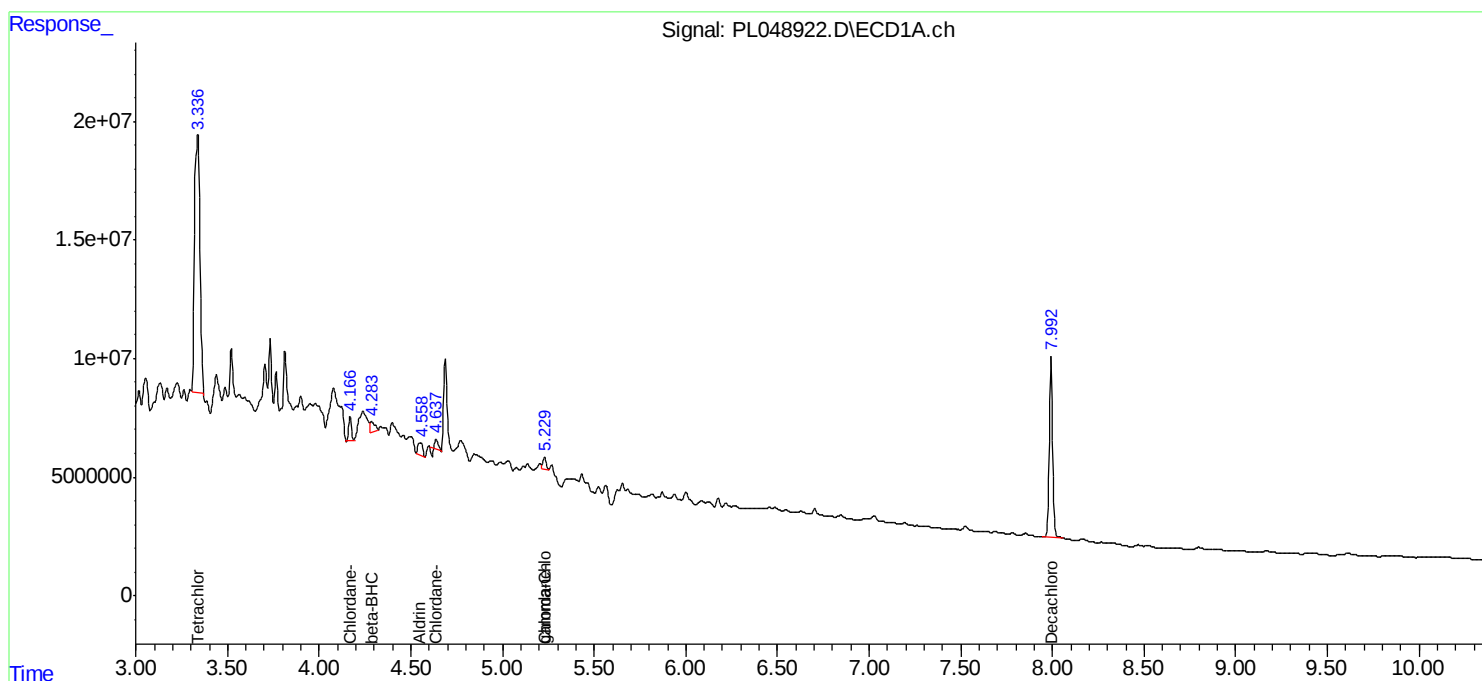


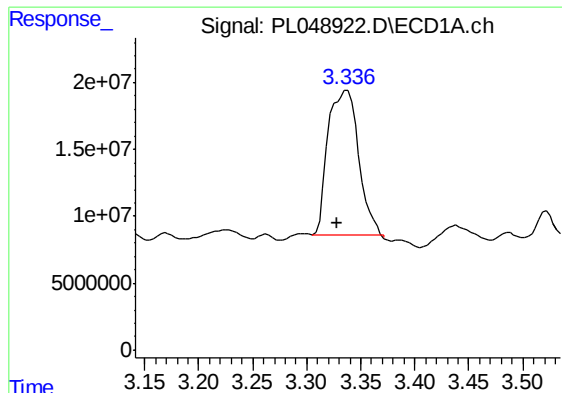

#1 Tetrachloro-m-xylene


R.T.: 3.338 min
Delta R.T.: 0.010 min
Response: 213482344
Conc: 22.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-26835

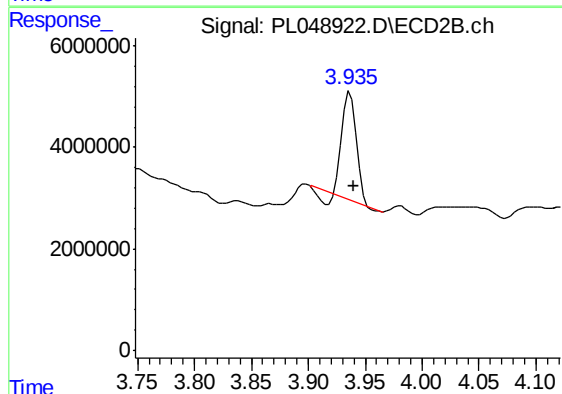


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.003 min
Response: 16852262
Conc: 6.77 ng/ml

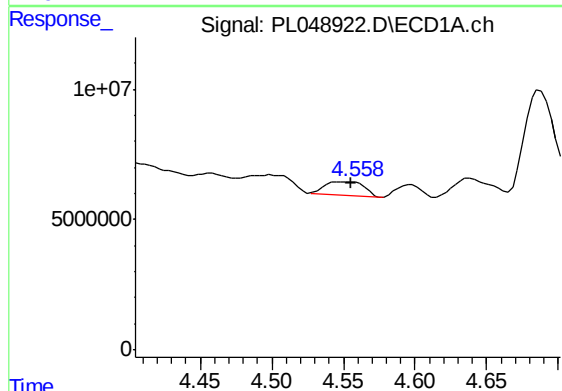


#5 Aldrin

R.T.: 4.548 min
Delta R.T.: -0.008 min
Response: 9907227
Conc: 0.72 ng/ml

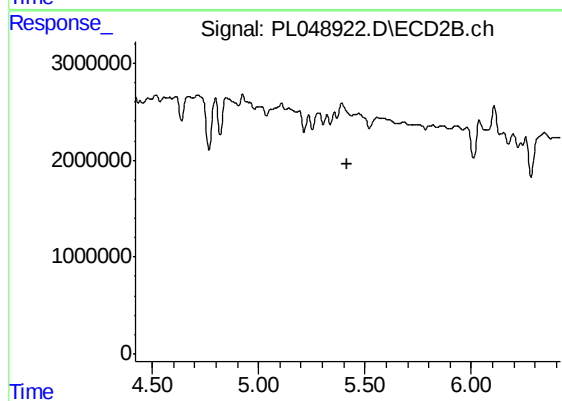

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.418 min
Response: 0
Conc: N.D.

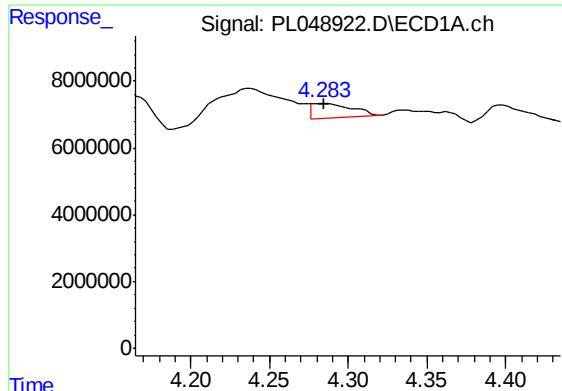

#6 beta-BHC


R.T.: 4.284 min
Delta R.T.: 0.000 min
Response: 7743998
Conc: 1.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-26835

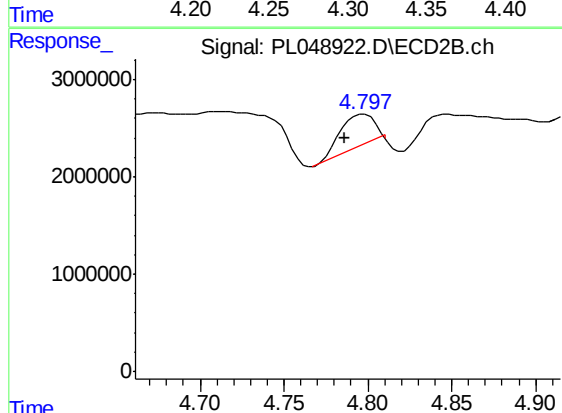


#6 beta-BHC

R.T.: 4.798 min
Delta R.T.: 0.012 min
Response: 4099533
Conc: 2.63 ng/ml

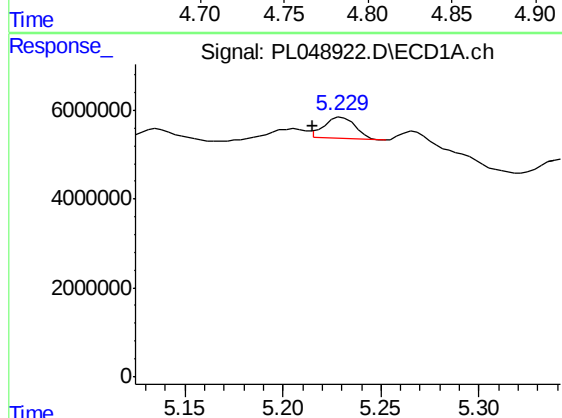


#10 gamma-Chlordane

R.T.: 5.230 min
Delta R.T.: 0.015 min
Response: 5534295
Conc: 0.41 ng/ml

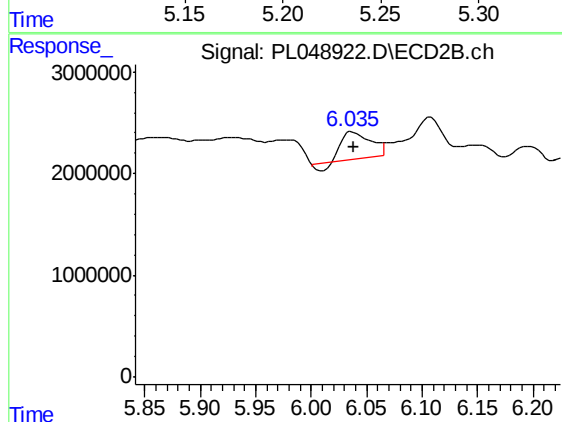

#10 gamma-Chlordane


R.T.: 6.037 min
Delta R.T.: -0.001 min
Response: 4420929
Conc: 1.44 ng/ml

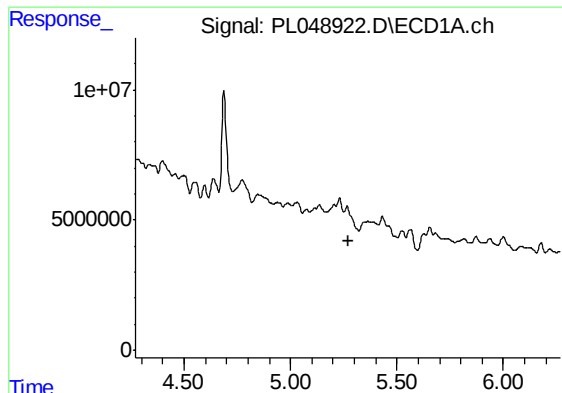

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.271 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CHRT-26835

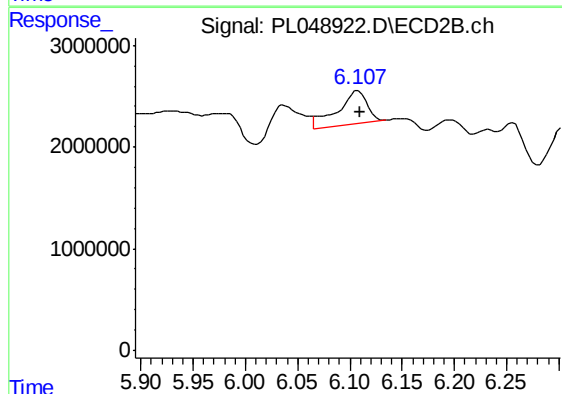


#11 alpha-Chlordane

R.T.: 6.108 min
Delta R.T.: -0.001 min
Response: 6508024
Conc: 2.12 ng/ml

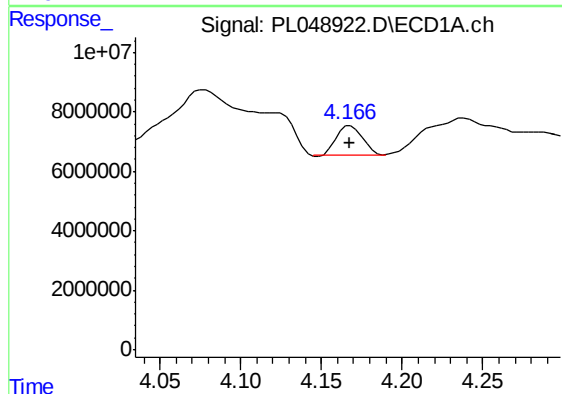


#23 Chlordane-1

R.T.: 4.168 min
Delta R.T.: 0.000 min
Response: 11070465
Conc: 24.66 ng/ml

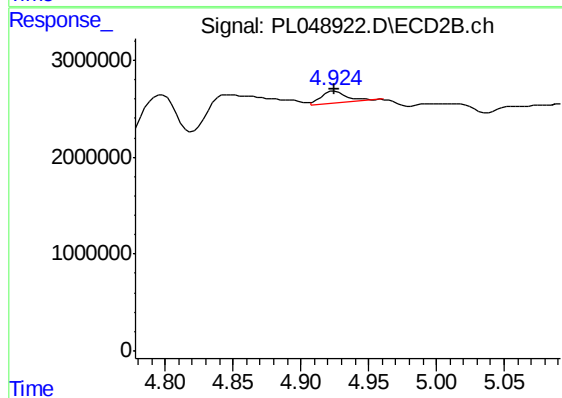

#23 Chlordane-1


R.T.: 4.925 min
Delta R.T.: 0.000 min
Response: 1816903
Conc: 14.87 ng/ml

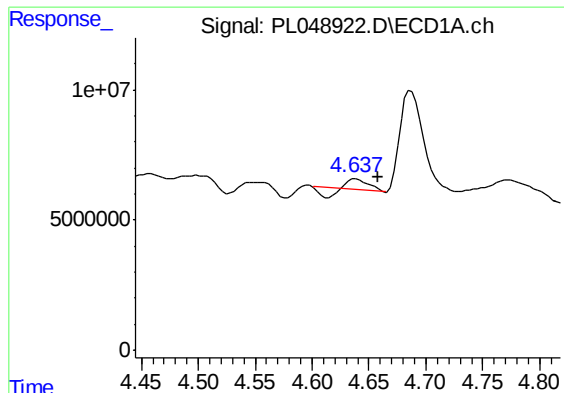

#24 Chlordane-2


R.T.: 4.639 min
Delta R.T.: -0.020 min
Response: 2411905
Conc: 4.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-26835

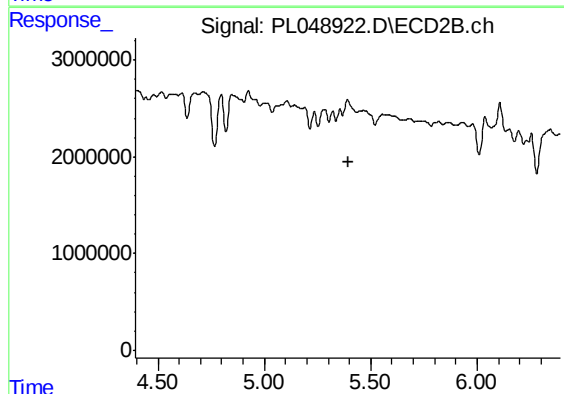


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.394 min
Response: 0
Conc: N.D.

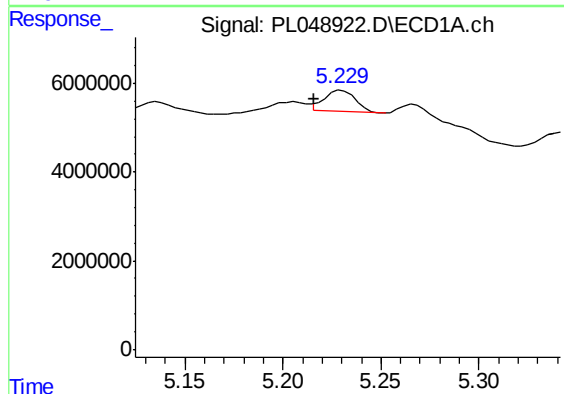


#25 Chlordane-3

R.T.: 5.230 min
Delta R.T.: 0.015 min
Response: 5534295
Conc: 3.51 ng/ml

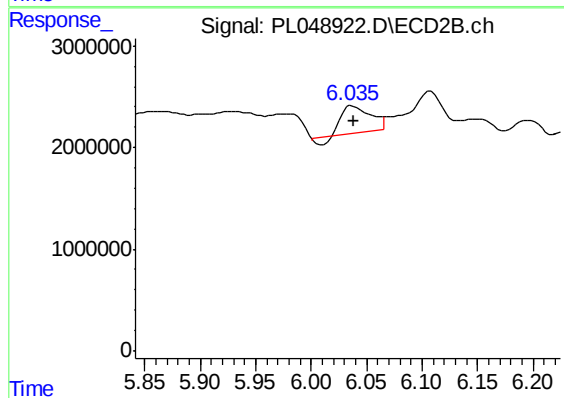

#25 Chlordane-3


R.T.: 6.037 min
Delta R.T.: 0.000 min
Response: 4420929
Conc: 10.09 ng/ml

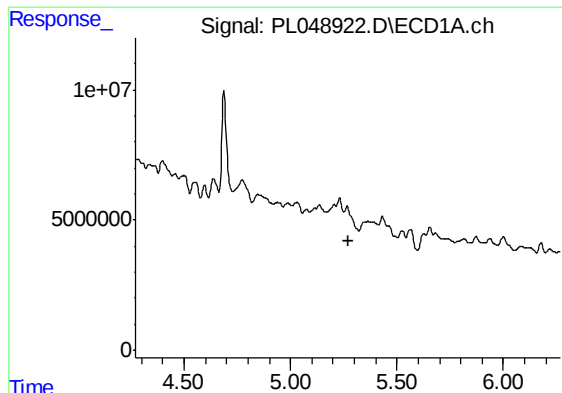

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.270 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CHRT-26835

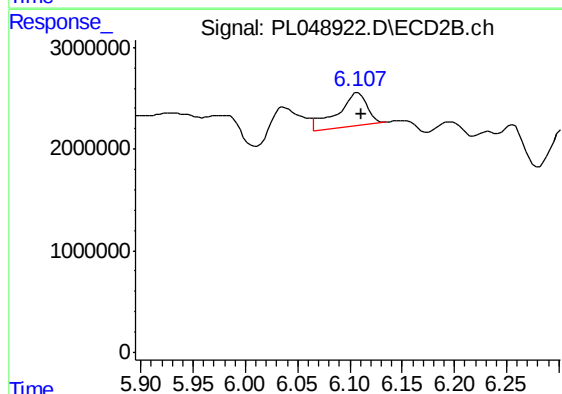


#26 Chlordane-4

R.T.: 6.108 min
Delta R.T.: -0.003 min
Response: 6508024
Conc: 12.41 ng/ml

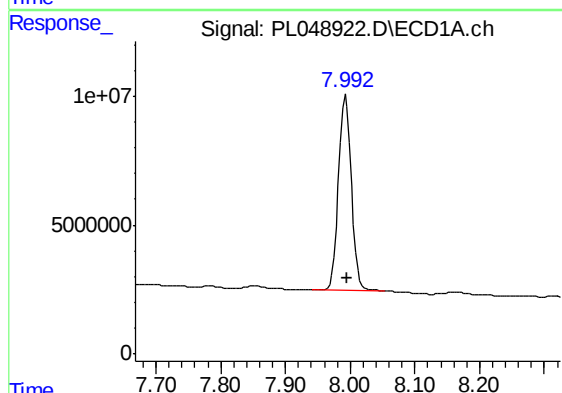

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.003 min
Response: 103649908
Conc: 10.31 ng/ml

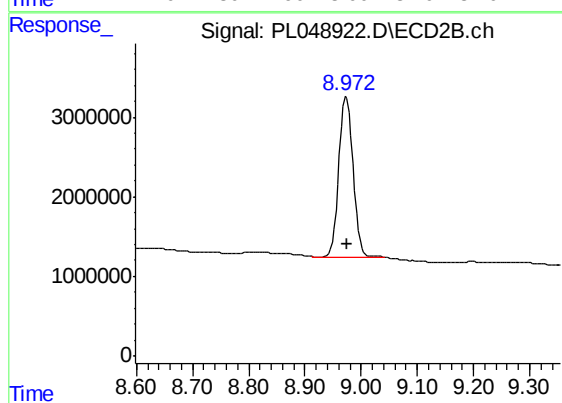

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: -0.001 min
Response: 35412602
Conc: 13.34 ng/ml