

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
 Data File : PL048943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2019 19:57
 Operator : SM\AJ
 Sample : K3026-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-5-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 22:22:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.937	91623854	23612436	9.459	9.480
28)	SA Decachlor...	7.991	8.971	81324115	26343104	8.089	9.925
Target Compounds							
10)	B gamma-Chl...	5.214	6.010f	51949155	-2054446	3.891	N.D. #
12)	B 4,4'-DDE	5.434	6.265	258.4E6	58198604	20.372	21.079
13)	MA Dieldrin	5.581f	0.000	16257677	0	1.249	N.D. #
16)	A 4,4'-DDD	5.944	6.756	21796872	6802507	2.239	3.031 #
17)	MA 4,4'-DDT	6.177	7.054	9269385	3743347	0.923	1.595 #
25)	Chlordane-3	5.214	6.010f	51949155	-2054446	32.993	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
Data File : PL048943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2019 19:57
Operator : SM\AJ
Sample : K3026-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-5-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 22:22:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

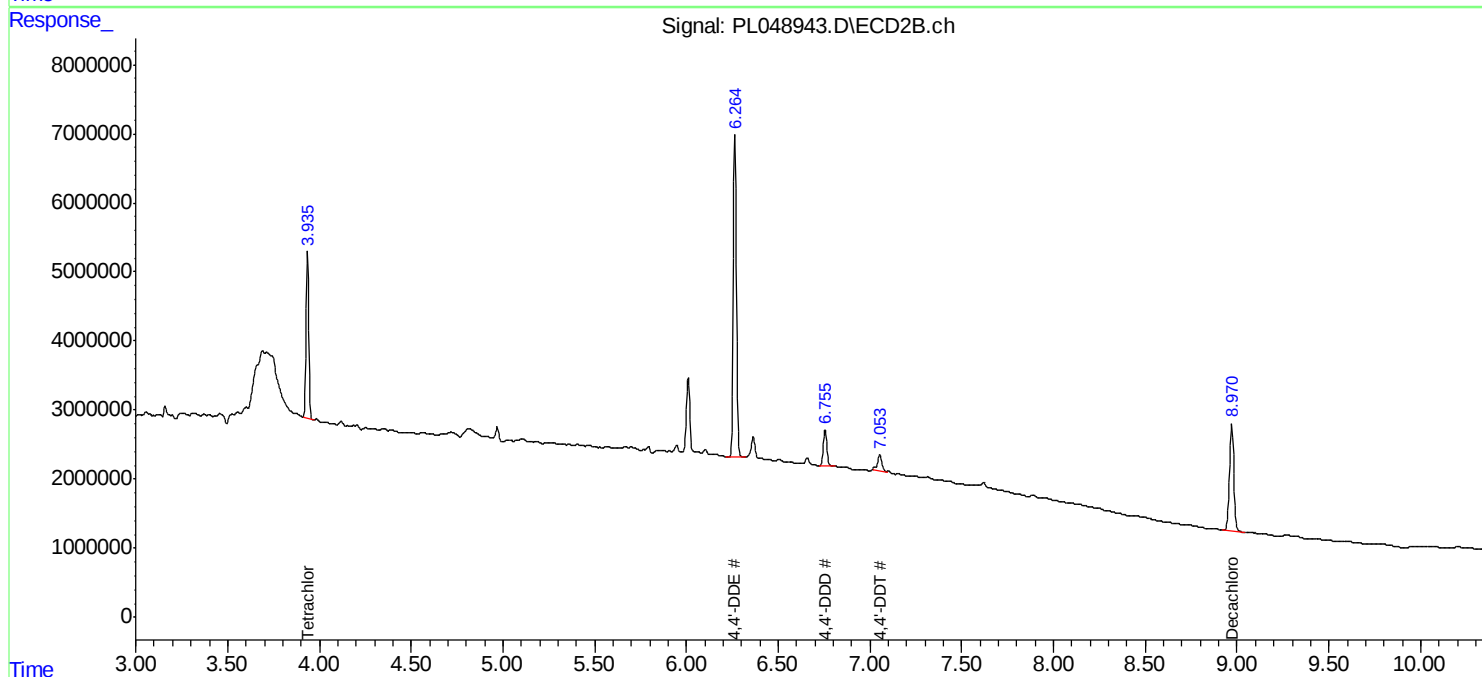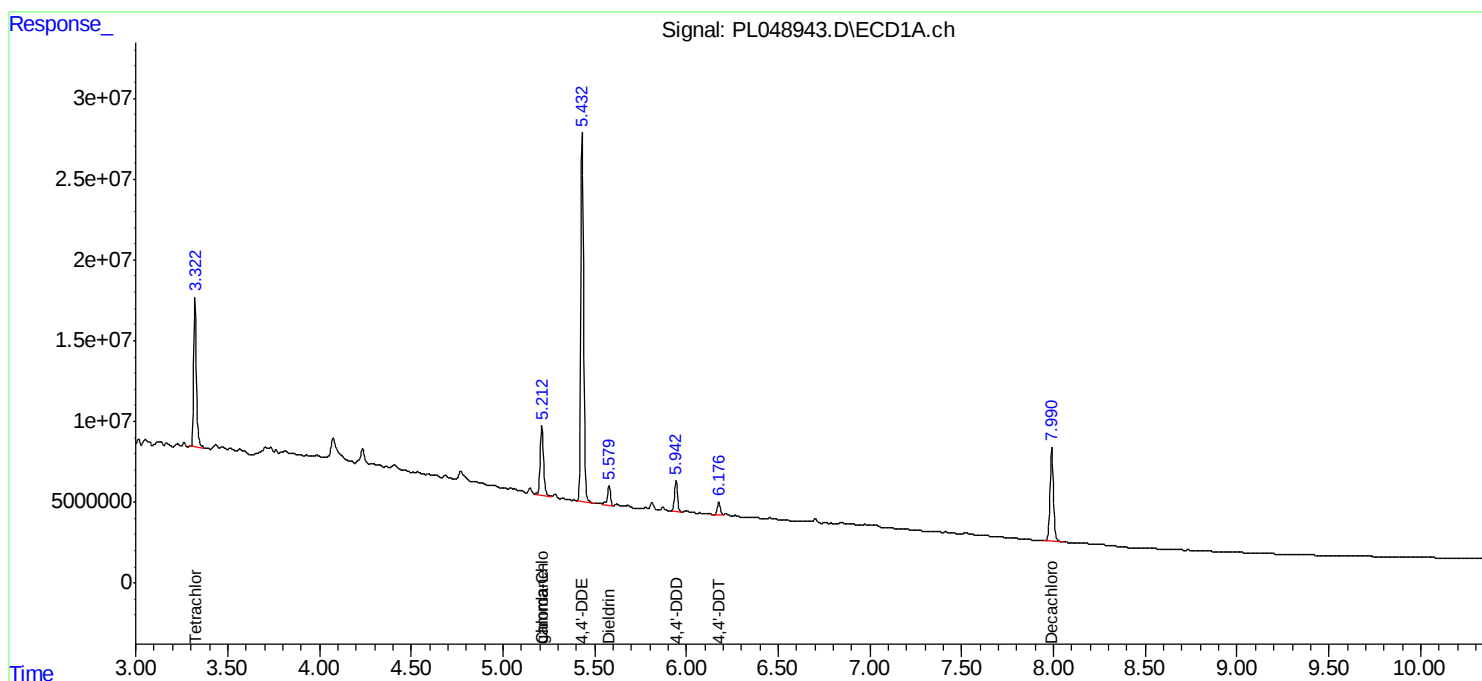


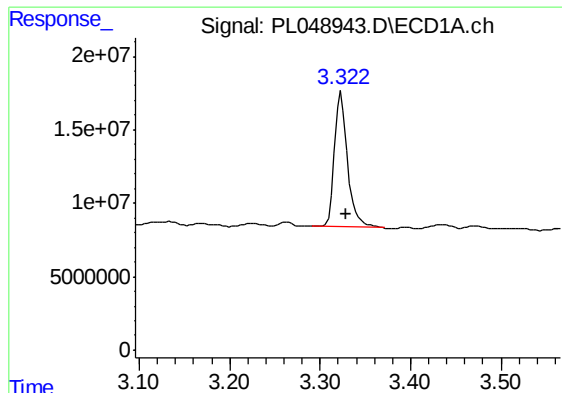

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.004 min
Response: 91623854
Conc: 9.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-S

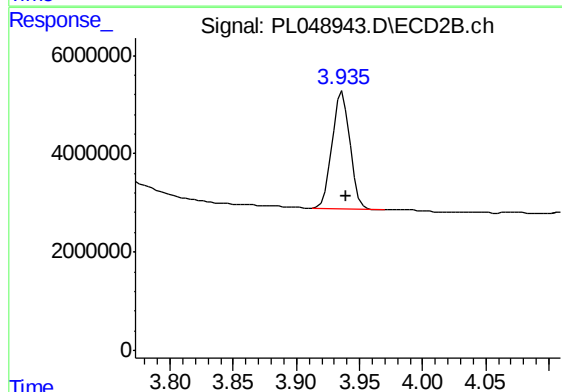


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.003 min
Response: 23612436
Conc: 9.48 ng/ml

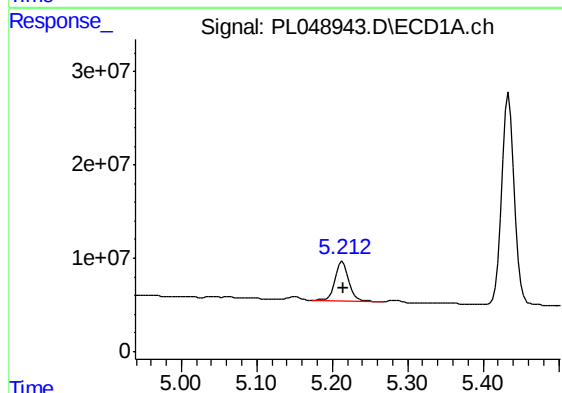


#10 gamma-Chlordane

R.T.: 5.214 min
Delta R.T.: -0.001 min
Response: 51949155
Conc: 3.89 ng/ml

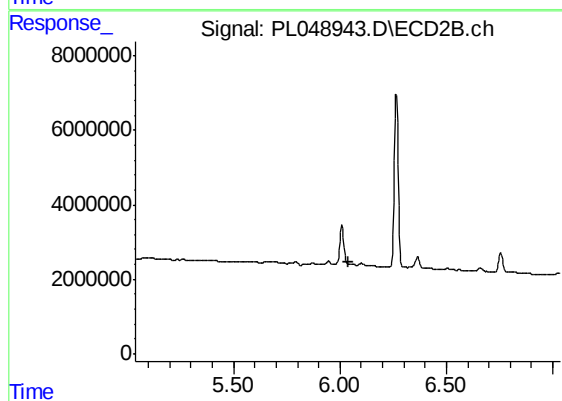

#10 gamma-Chlordane


R.T.: 6.010 min
Delta R.T.: -0.029 min
Response: -2054446
Conc: N.D.

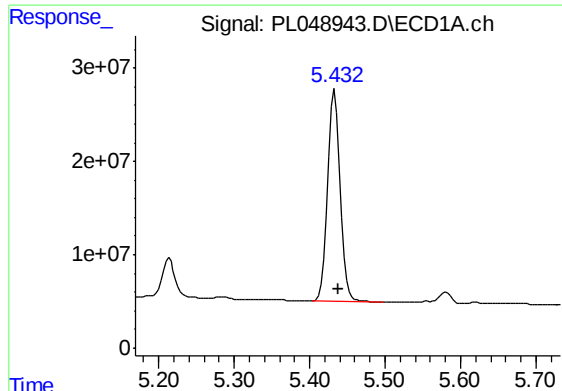

#12 4,4'-DDE


R.T.: 5.434 min
Delta R.T.: -0.005 min
Response: 258430165
Conc: 20.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-S

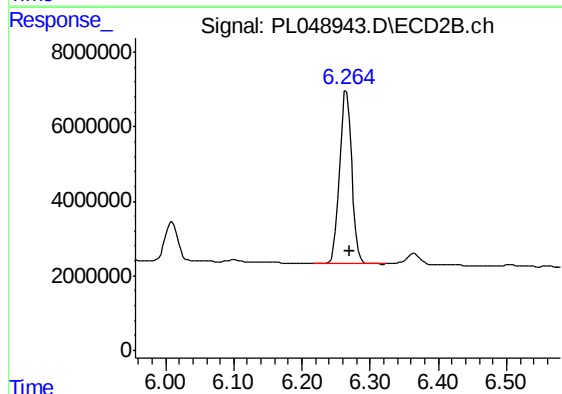


#12 4,4'-DDE

R.T.: 6.265 min
Delta R.T.: -0.004 min
Response: 58198604
Conc: 21.08 ng/ml

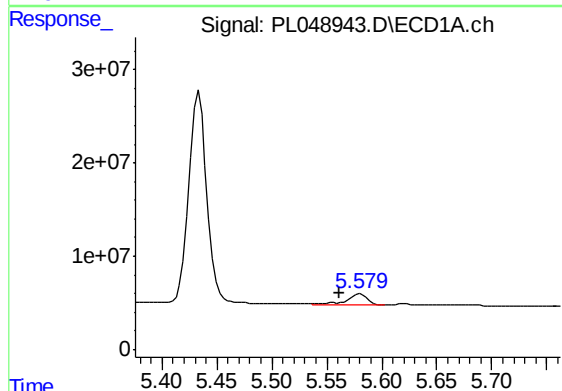


#13 Dieldrin

R.T.: 5.581 min
Delta R.T.: 0.019 min
Response: 16257677
Conc: 1.25 ng/ml

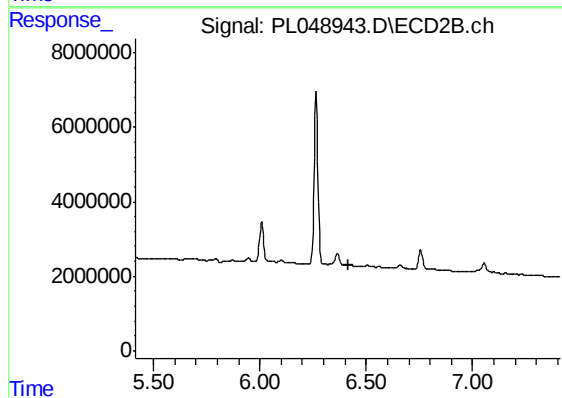

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

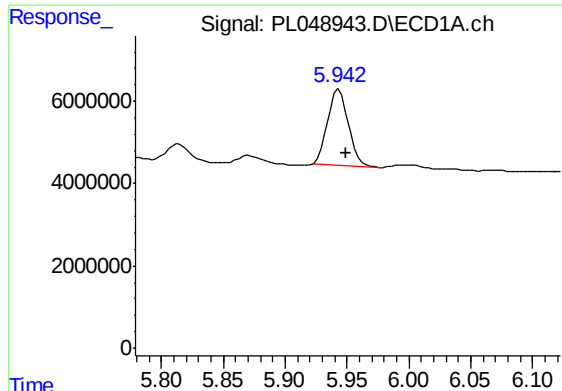

#16 4,4'-DDD


R.T.: 5.944 min
Delta R.T.: -0.005 min
Response: 21796872
Conc: 2.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-S

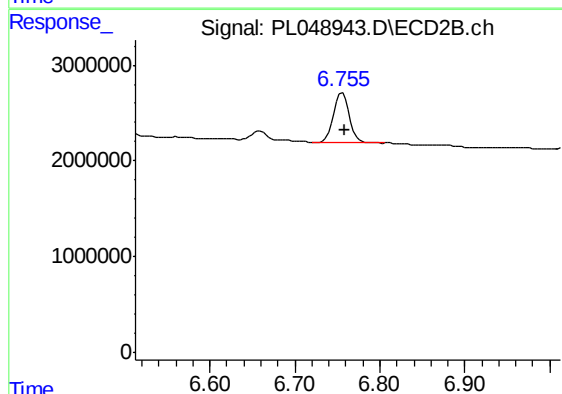


#16 4,4'-DDD

R.T.: 6.756 min
Delta R.T.: -0.003 min
Response: 6802507
Conc: 3.03 ng/ml

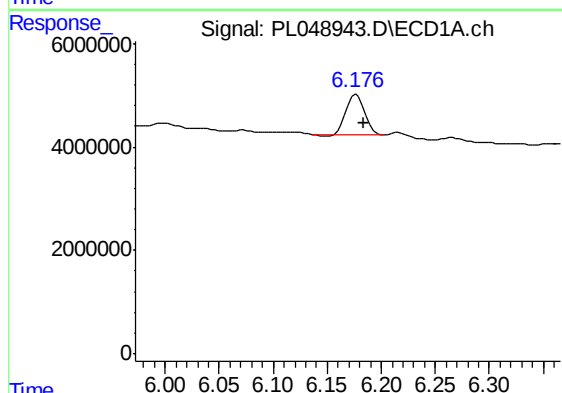


#17 4,4'-DDT

R.T.: 6.177 min
Delta R.T.: -0.007 min
Response: 9269385
Conc: 0.92 ng/ml

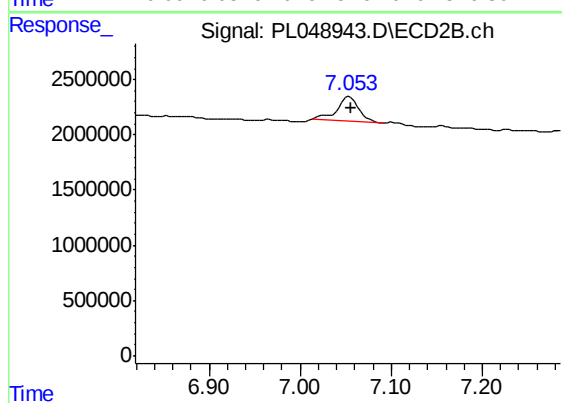

#17 4,4'-DDT


R.T.: 7.054 min
Delta R.T.: -0.002 min
Response: 3743347
Conc: 1.60 ng/ml

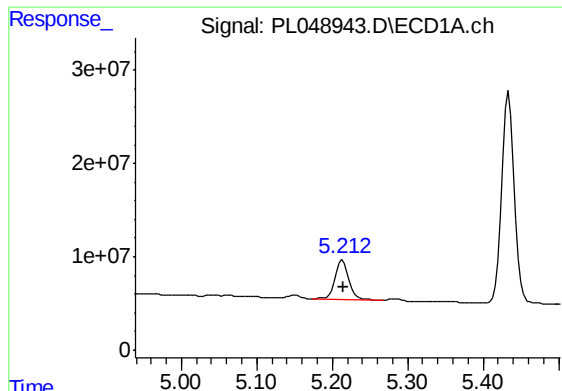

#25 Chlordane-3


R.T.: 5.214 min
Delta R.T.: -0.002 min
Response: 51949155
Conc: 32.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-S

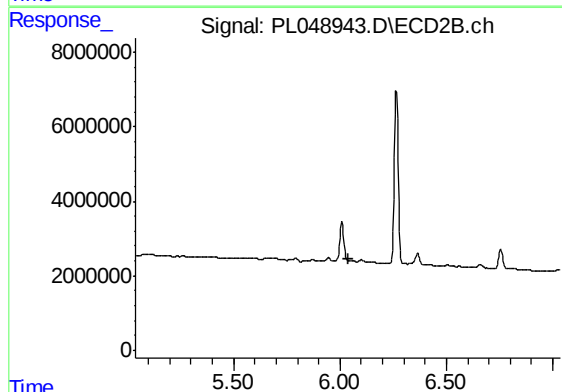


#25 Chlordane-3

R.T.: 6.010 min
Delta R.T.: -0.028 min
Response: -2054446
Conc: N.D.

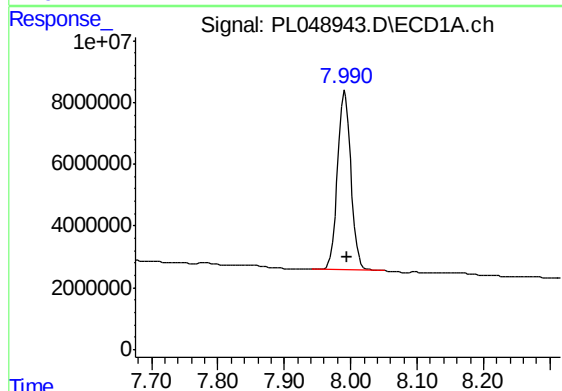

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.005 min
Response: 81324115
Conc: 8.09 ng/ml

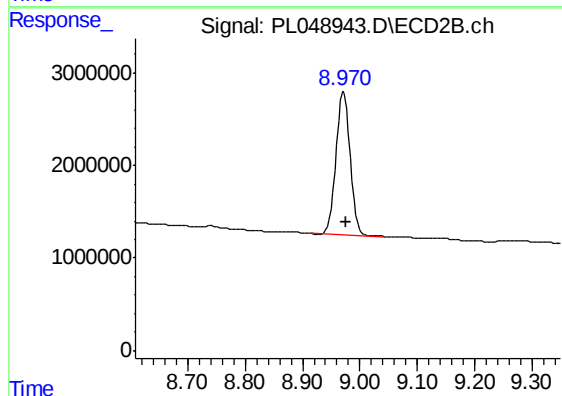

#28 Decachlorobiphenyl

R.T.: 8.971 min
Delta R.T.: -0.004 min
Response: 26343104
Conc: 9.92 ng/ml