

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
 Data File : PL048952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2019 22:10
 Operator : SM\AJ
 Sample : K3023-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-0523-S-TCLP-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 00:21:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.326	3.937	190.7E6	52134699	19.691	20.930
28) SA Decachlor...	7.991	8.972	199.0E6	58237505	19.798	21.941
Target Compounds						
7) B delta-BHC	0.000	4.972f	0	4665564	N.D.	1.650 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
Data File : PL048952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2019 22:10
Operator : SM\AJ
Sample : K3023-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SSSI-0523-S-TCLP-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 00:21:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

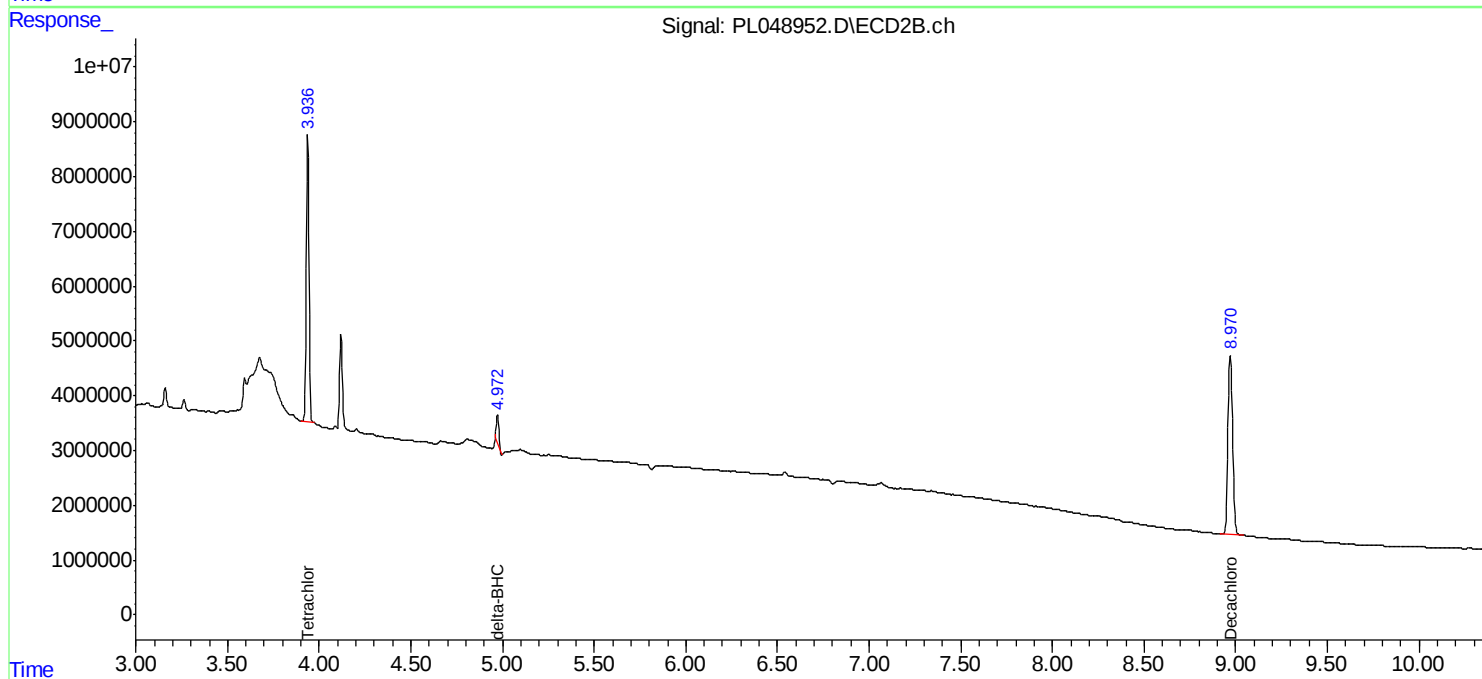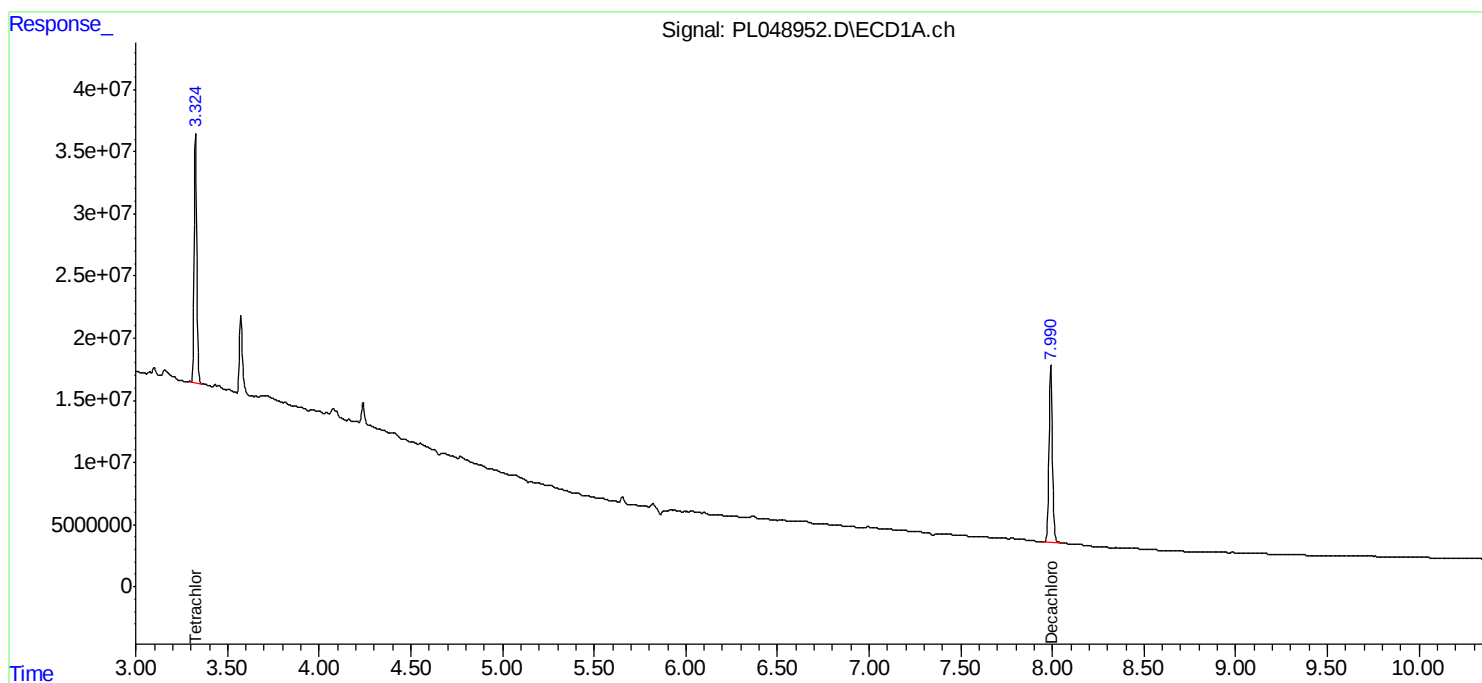


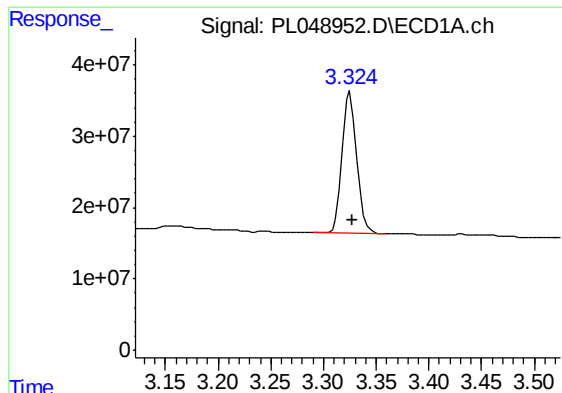

#1 Tetrachloro-m-xylene


R.T.: 3.326 min
Delta R.T.: -0.002 min
Response: 190743511
Conc: 19.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0523-S-TCLP-11

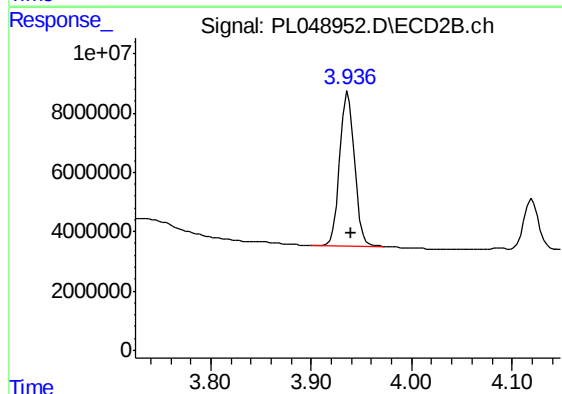


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.003 min
Response: 52134699
Conc: 20.93 ng/ml

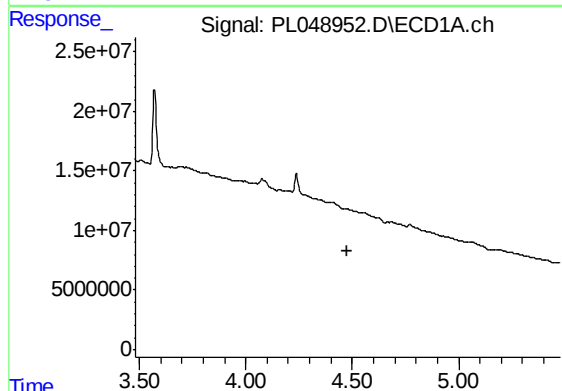


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

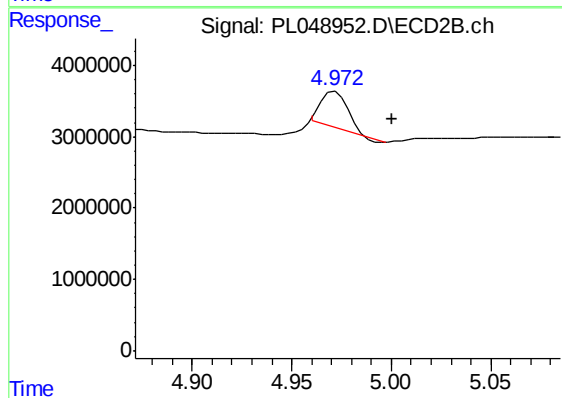

#7 delta-BHC


R.T.: 4.972 min
Delta R.T.: -0.028 min
Response: 4665564
Conc: 1.65 ng/ml

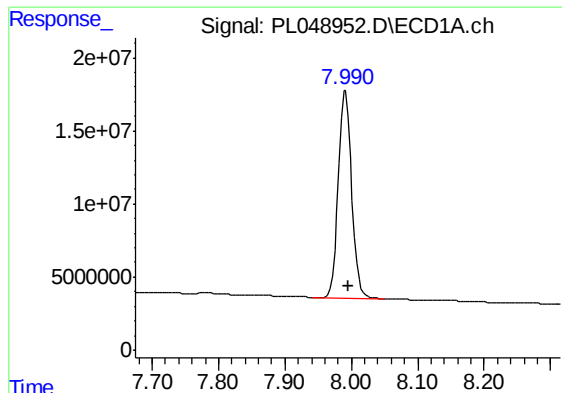

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.004 min
Response: 199049564
Conc: 19.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0523-S-TCLP-11

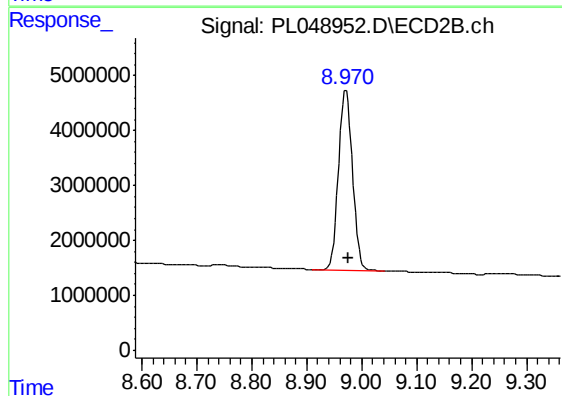

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: -0.003 min
Response: 58237505
Conc: 21.94 ng/ml