

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
 Data File : PL048955.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2019 22:56
 Operator : SM\AJ
 Sample : K3026-16
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 00:22:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.326	3.938	197.8E6	53220087	20.415	21.366
28) SA Decachlor...	7.993	8.972	136.4E6	40050042	13.565	15.089
Target Compounds						
4) MA Heptachlor	0.000	5.096f	0	10411433	N.D.	3.007 #
7) B delta-BHC	0.000	4.972f	0	4472922	N.D.	1.582 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
Data File : PL048955.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2019 22:56
Operator : SM\AJ
Sample : K3026-16
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-3-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 00:22:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

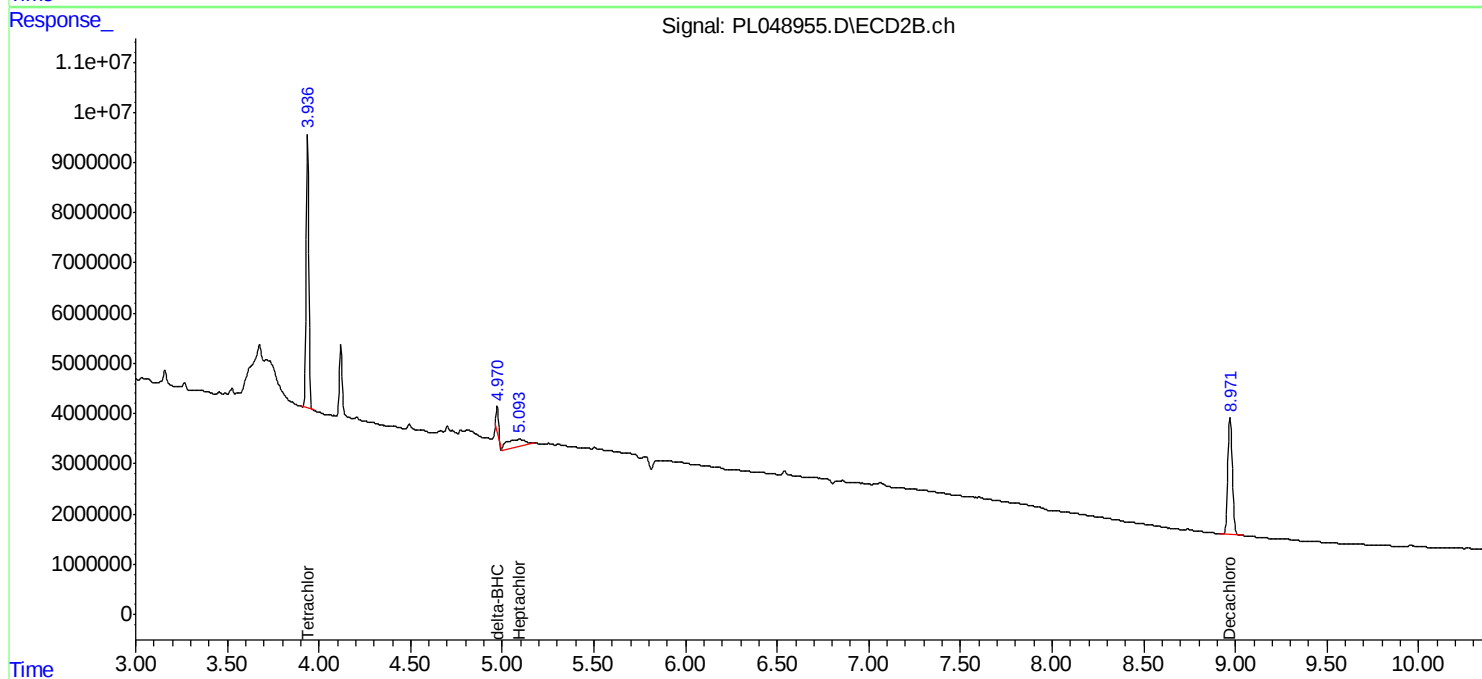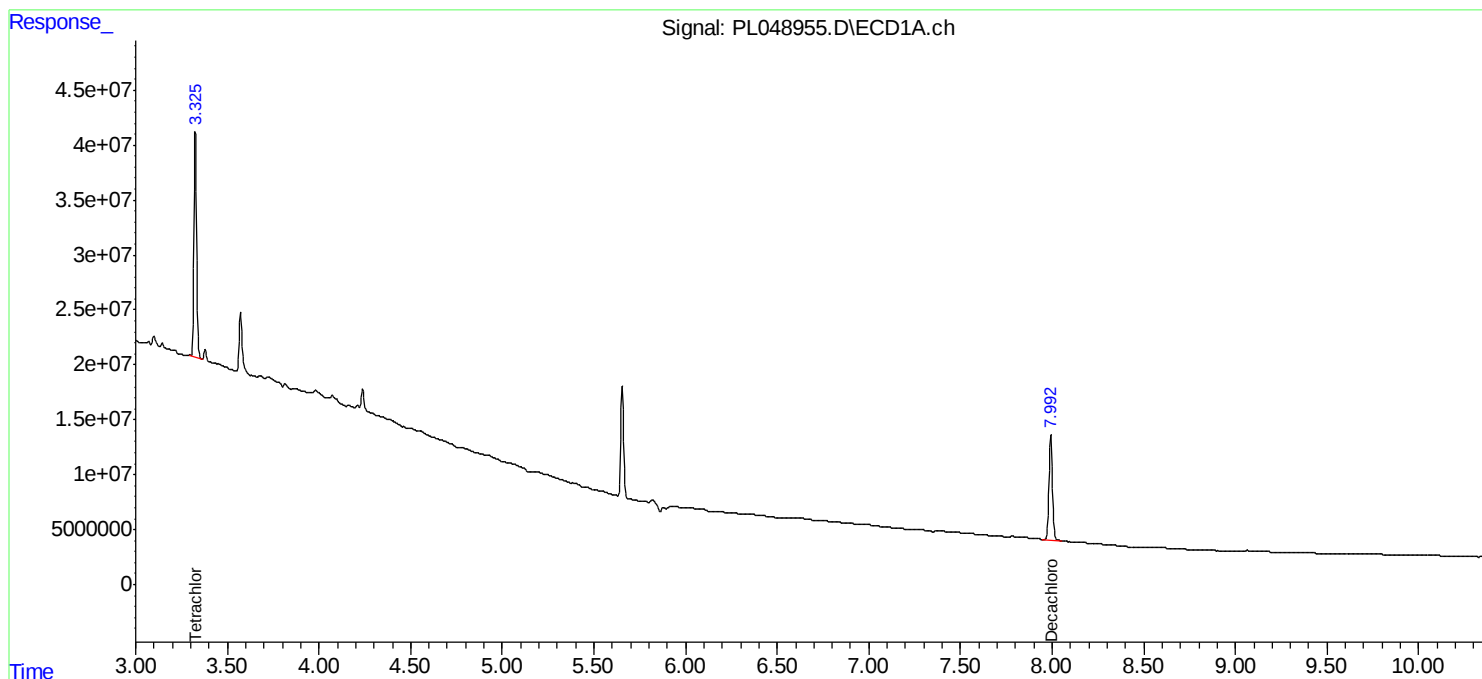


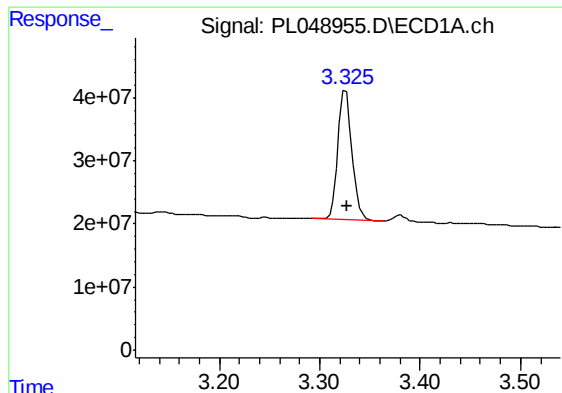

#1 Tetrachloro-m-xylene


R.T.: 3.326 min
Delta R.T.: -0.002 min
Response: 197759014
Conc: 20.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3-S

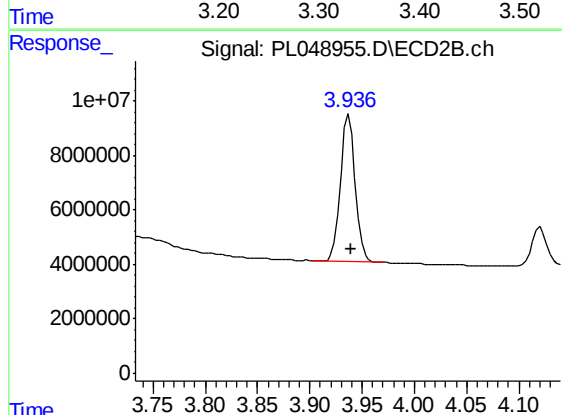


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: -0.002 min
Response: 53220087
Conc: 21.37 ng/ml

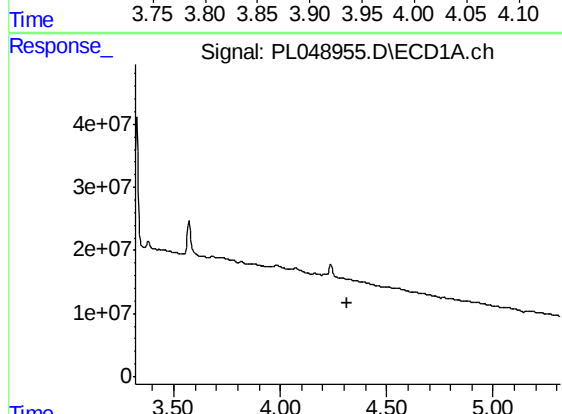


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

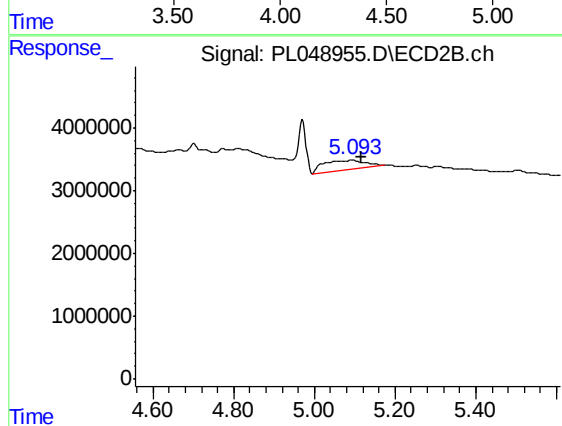

#4 Heptachlor


R.T.: 5.096 min
Delta R.T.: -0.019 min
Response: 10411433
Conc: 3.01 ng/ml

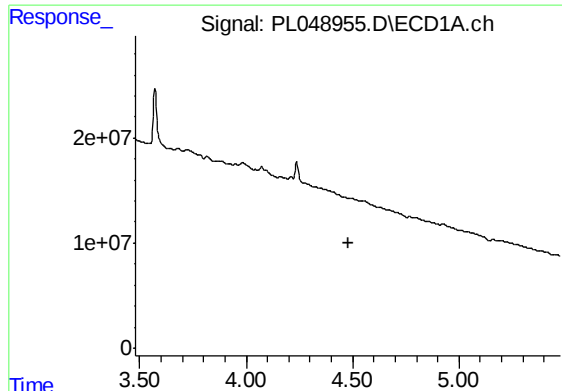

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3-S

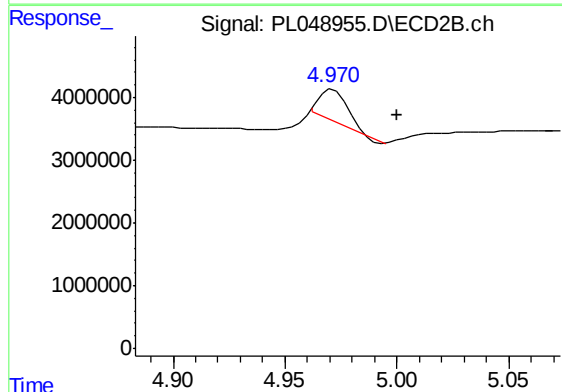


#7 delta-BHC

R.T.: 4.972 min
Delta R.T.: -0.028 min
Response: 4472922
Conc: 1.58 ng/ml

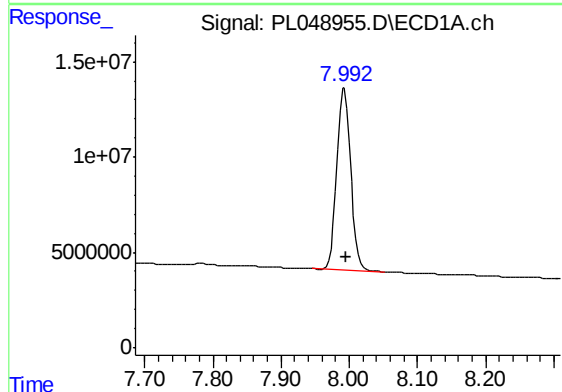

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.003 min
Response: 136385158
Conc: 13.57 ng/ml

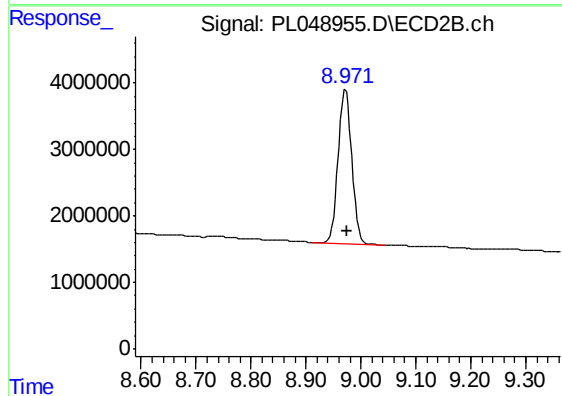

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: -0.003 min
Response: 40050042
Conc: 15.09 ng/ml