

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
 Data File : PL048922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2019 13:50
 Operator : SM\AJ
 Sample : K3004-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-26835

Manual Integrations
 APPROVED

Ankita
 5/28/2019 8:32:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 22:17:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.328	3.935	79942726	22941891	8.253m	9.210m
28) SA Decachlor...	7.993	8.974	103.6E6	35412602	10.309	13.342 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
Data File : PL048922.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2019 13:50
Operator : SM\AJ
Sample : K3004-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CHRT-26835


Manual Integrations
APPROVED

Ankita
5/28/2019 8:32:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 22:17:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm



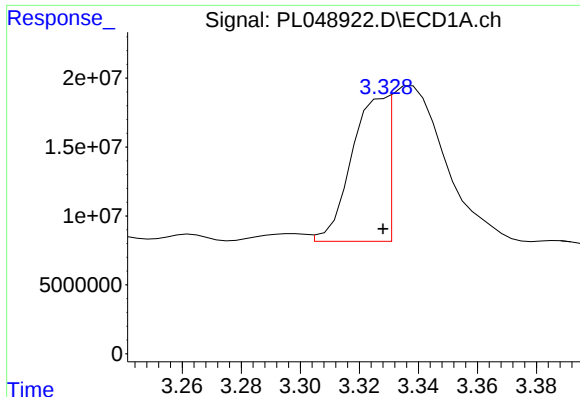


#1 Tetrachloro-m-xylene

R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 79942726
Conc: 8.25 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CHRT-26835


Manual Integrations
APPROVED

Ankita
5/28/2019 8:32:37 AM

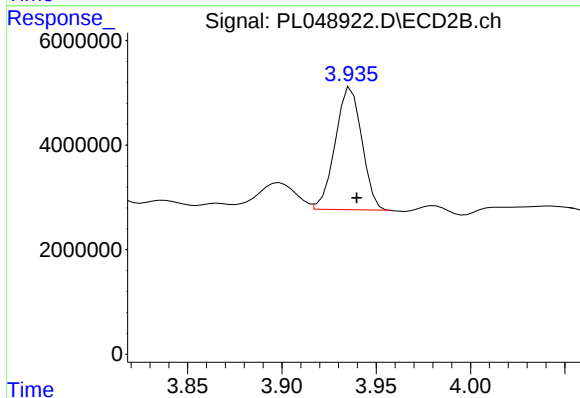


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.004 min
Response: 22941891
Conc: 9.21 ng/ml m

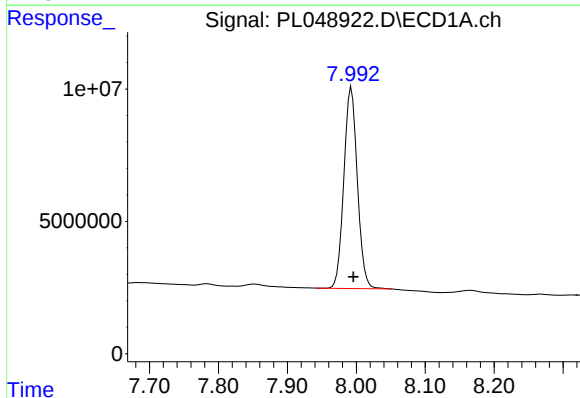

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.003 min
Response: 103649908
Conc: 10.31 ng/ml

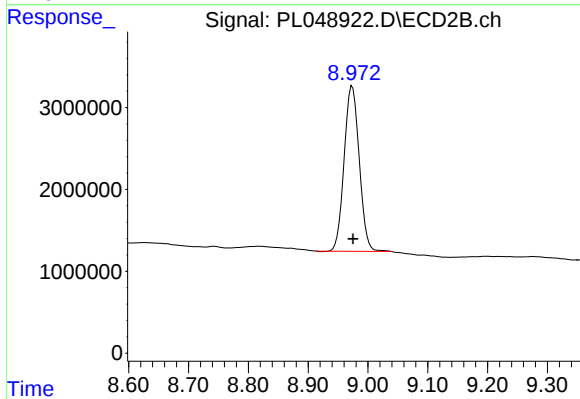

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: -0.001 min
Response: 35412602
Conc: 13.34 ng/ml