

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
 Data File : PL048924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2019 14:18
 Operator : SM\AJ
 Sample : K3008-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-20

Manual Integrations
 APPROVED

Ankita
 5/28/2019 8:32:41 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 22:17:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.324	3.937	89879193	21352672	9.278	8.572
28) SA Decachlor...	7.992	8.973	77680504	26385452	7.726	9.941 #
Target Compounds						
12) B 4,4'-DDE	5.434	6.264	28540012	7794343	2.250	2.823m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
Data File : PL048924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2019 14:18
Operator : SM\AJ
Sample : K3008-03
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
COMP-20


Manual Integrations
APPROVED

Ankita
5/28/2019 8:32:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 22:17:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

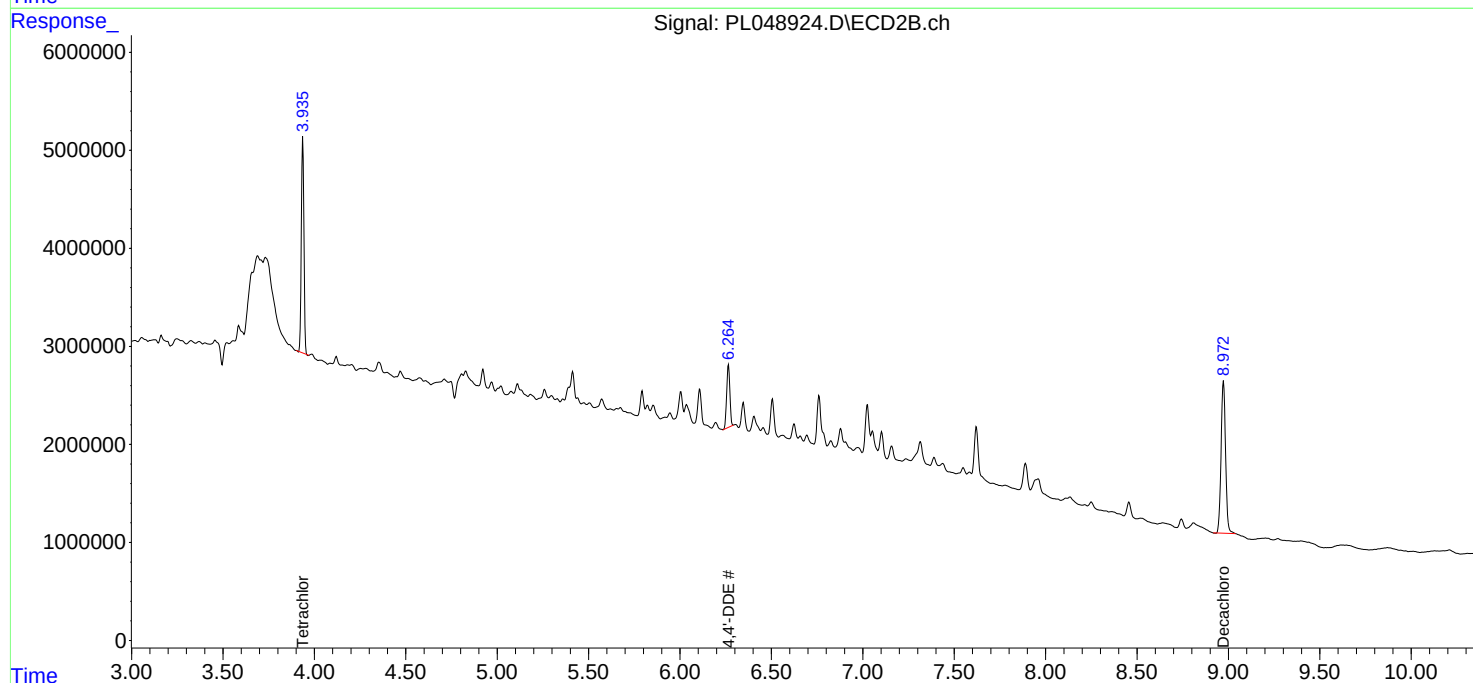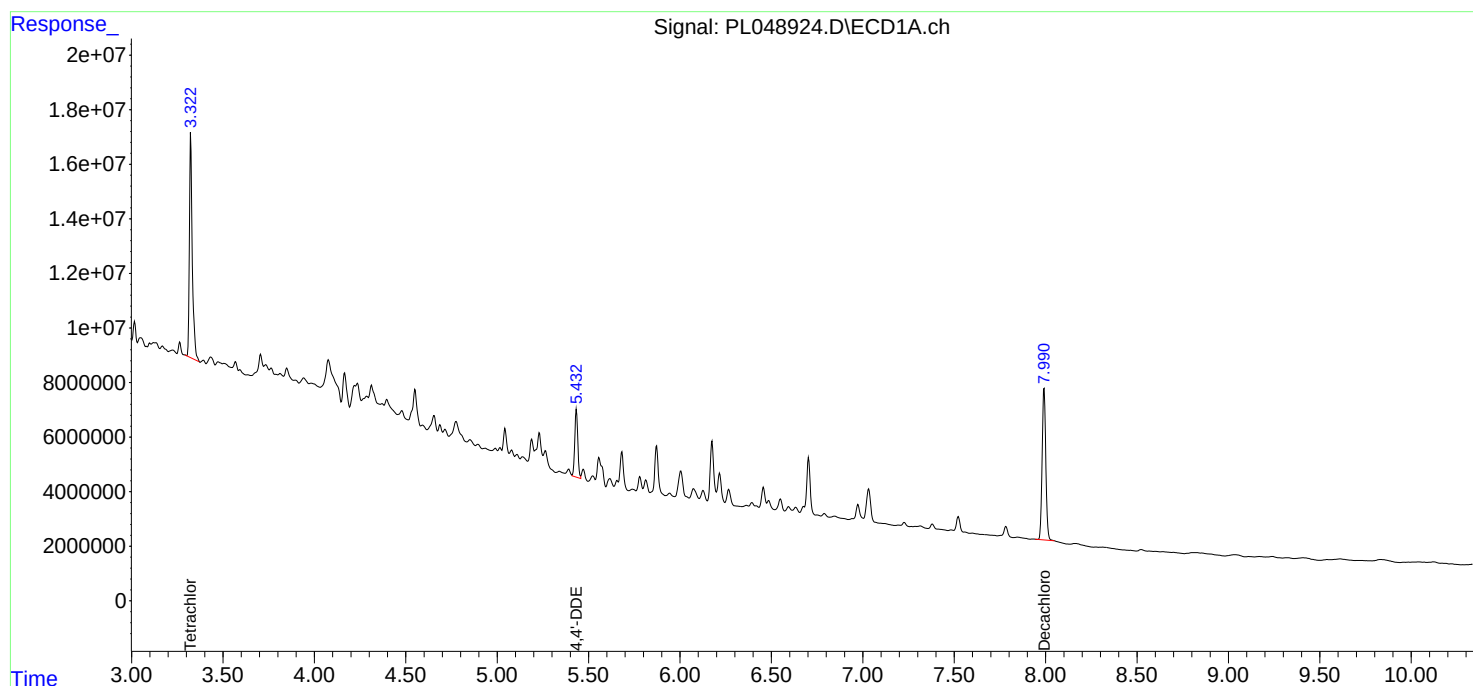

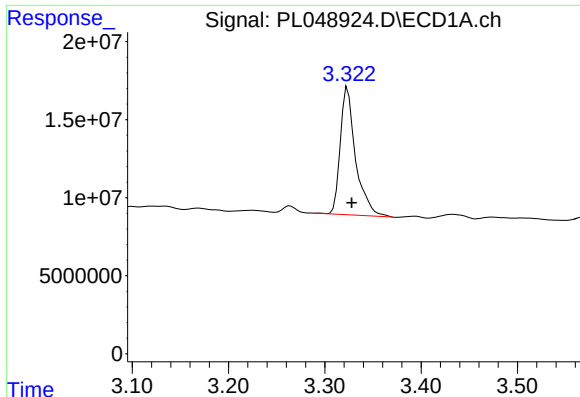


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: -0.004 min
Response: 89879193
Conc: 9.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-20


Manual Integrations
APPROVED

Ankita
5/28/2019 8:32:41 AM

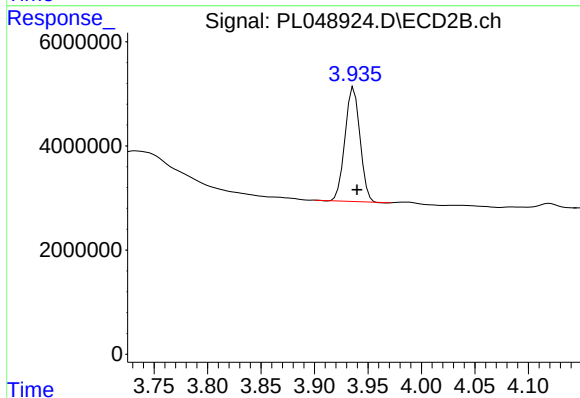


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.003 min
Response: 21352672
Conc: 8.57 ng/ml

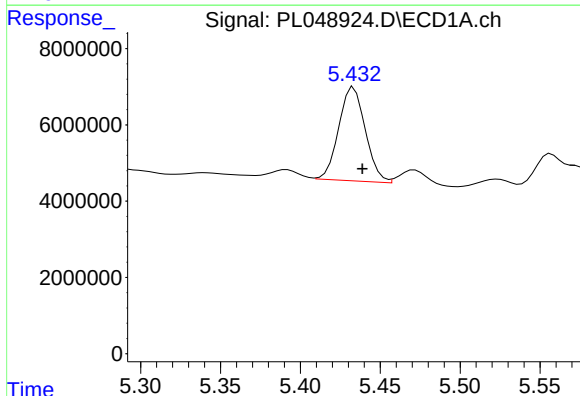


#12 4,4'-DDE

R.T.: 5.434 min
Delta R.T.: -0.005 min
Response: 28540012
Conc: 2.25 ng/ml

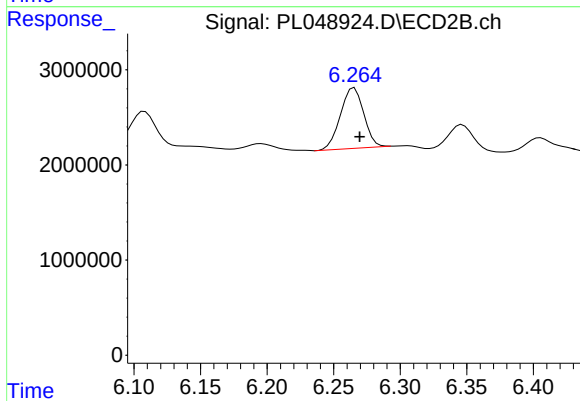

#12 4,4'-DDE

R.T.: 6.264 min
Delta R.T.: -0.005 min
Response: 7794343
Conc: 2.82 ng/ml m

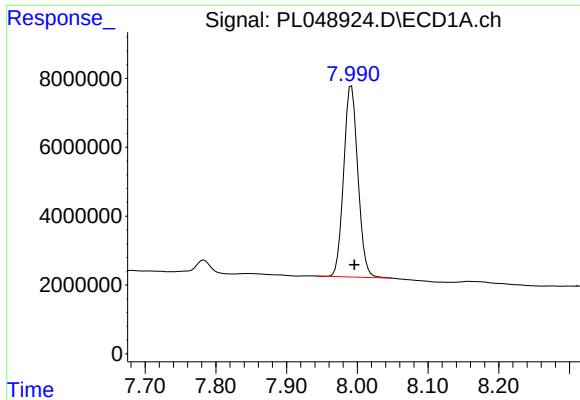


#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.004 min
Response: 77680504
Conc: 7.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-20

Manual Integrations
APPROVED

Ankita
5/28/2019 8:32:41 AM

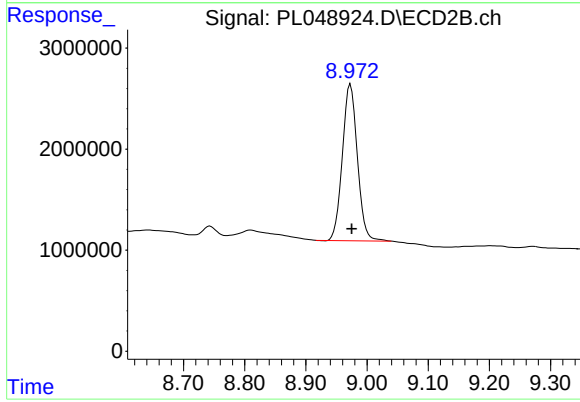

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: -0.002 min
Response: 26385452
Conc: 9.94 ng/ml