

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
 Data File : PL048925.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2019 14:32
 Operator : SM\AJ
 Sample : K3008-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-21

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 22:17:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.937	81222553	22161616	8.385	8.897
28)	SA Decachlor...	7.992	8.972	94665669	31828336	9.416	11.991 #
Target Compounds							
12)	B 4,4'-DDE	5.434	6.266	25353265	8156384	1.999	2.954 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
Data File : PL048925.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2019 14:32
Operator : SM\AJ
Sample : K3008-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-21

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 22:17:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

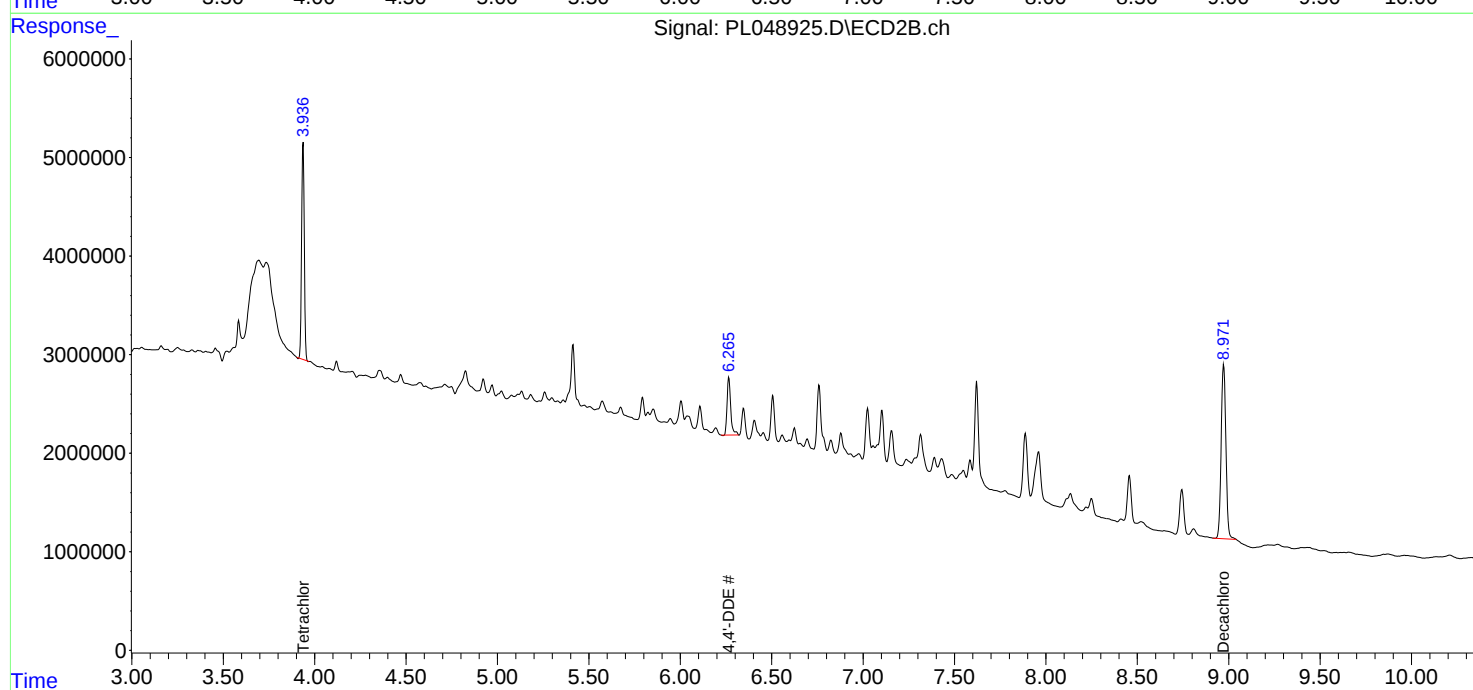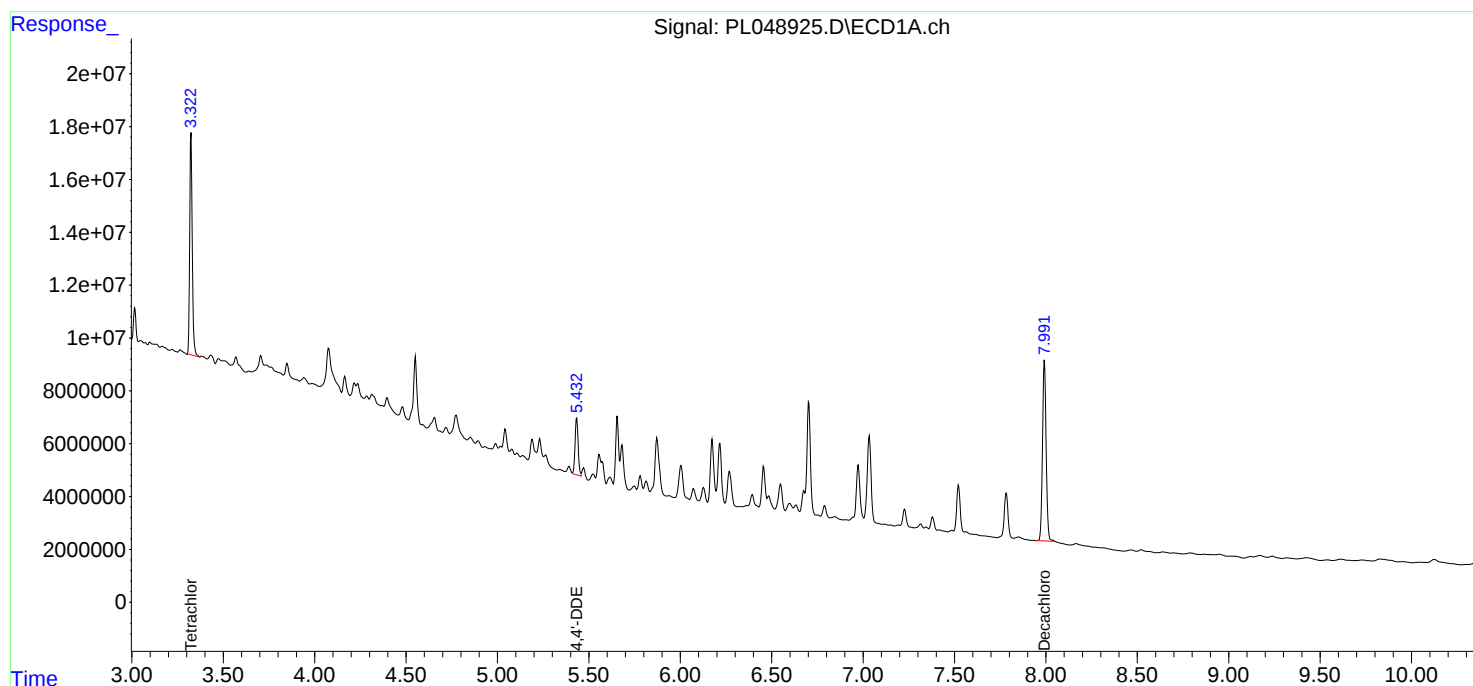


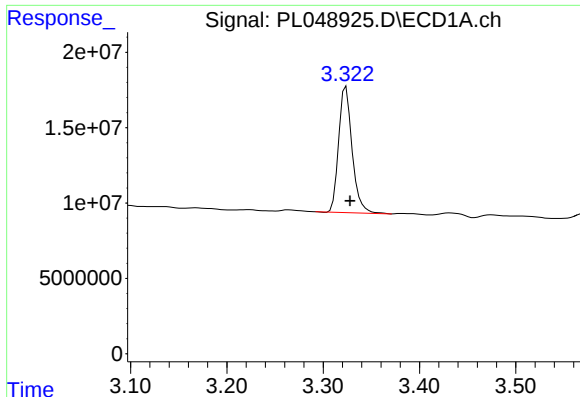

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.004 min
Response: 81222553
Conc: 8.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-21

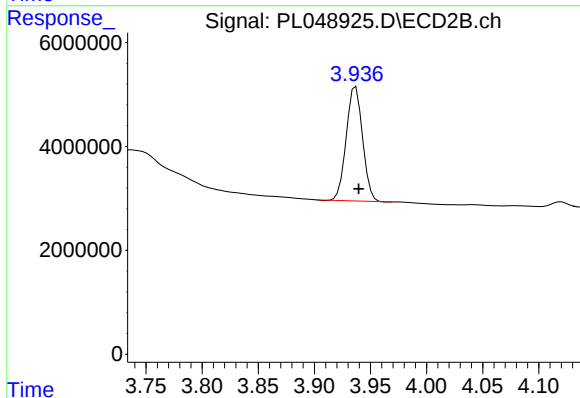


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.003 min
Response: 22161616
Conc: 8.90 ng/ml

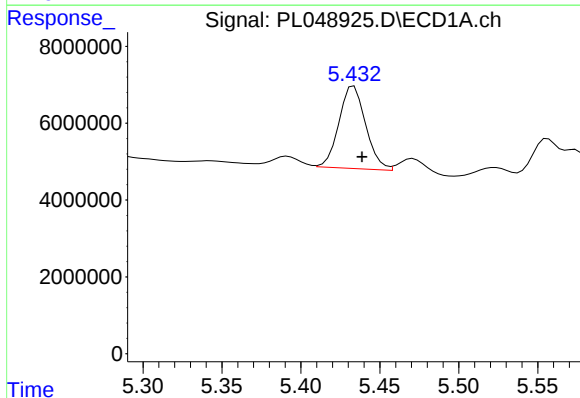


#12 4,4'-DDE

R.T.: 5.434 min
Delta R.T.: -0.005 min
Response: 25353265
Conc: 2.00 ng/ml

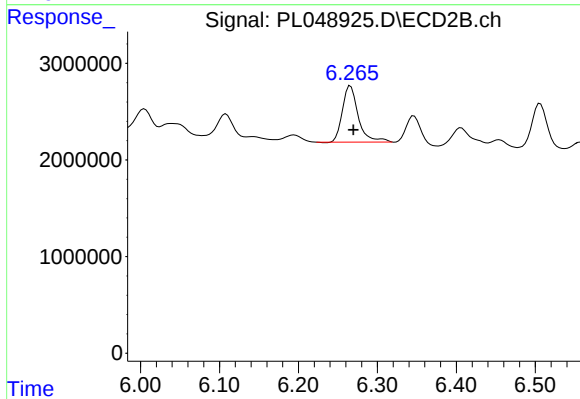

#12 4,4'-DDE


R.T.: 6.266 min
Delta R.T.: -0.004 min
Response: 8156384
Conc: 2.95 ng/ml

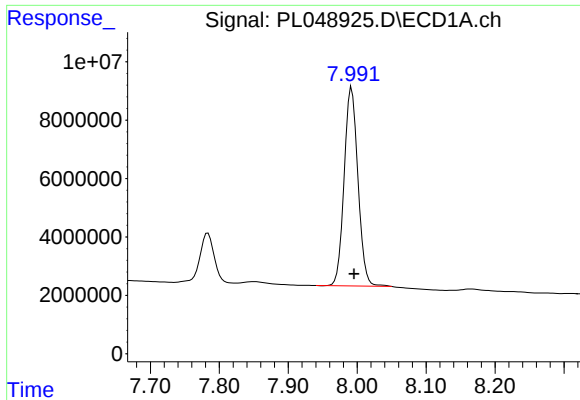

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.004 min
Response: 94665669
Conc: 9.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-21

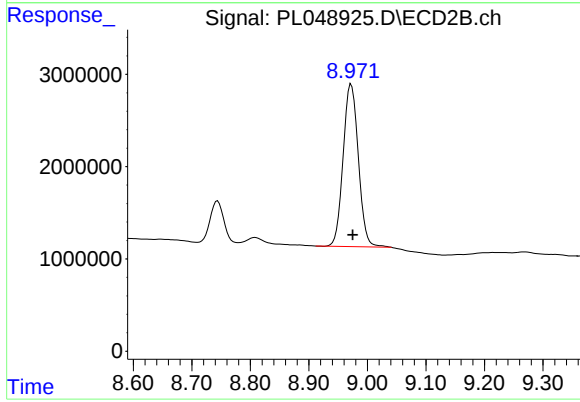

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: -0.003 min
Response: 31828336
Conc: 11.99 ng/ml