

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
 Data File : PL048984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2019 06:26
 Operator : SM\AJ
 Sample : K2993-15
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-15 1.5-2.0

Manual Integrations
 APPROVED

Ankita
 5/28/2019 8:33:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 08:54:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.937	198.6E6	52023890	20.505	20.886
28)	SA Decachlor...	7.989	8.971	177.5E6	49316553	17.658	18.580
Target Compounds							
10)	B gamma-Chl...	5.208	6.033	5935393	1824433	0.445m	0.593m#
11)	B alpha-Chl...	5.265	6.104	6790084	1862889	0.519m	0.607m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052419\
Data File : PL048984.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2019 06:26
Operator : SM\AJ
Sample : K2993-15
Misc :
ALS Vial : 68 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-15 1.5-2.0


Manual Integrations
APPROVED

Ankita
5/28/2019 8:33:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 08:54:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

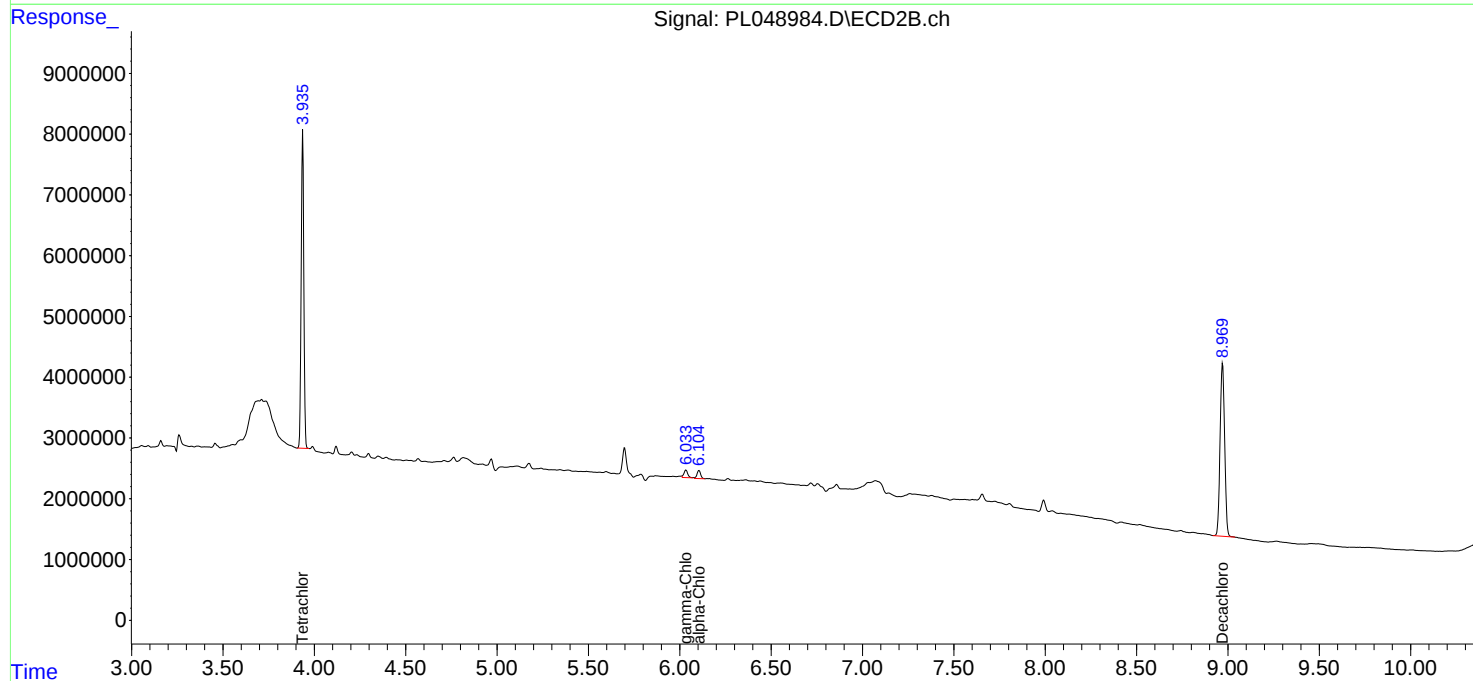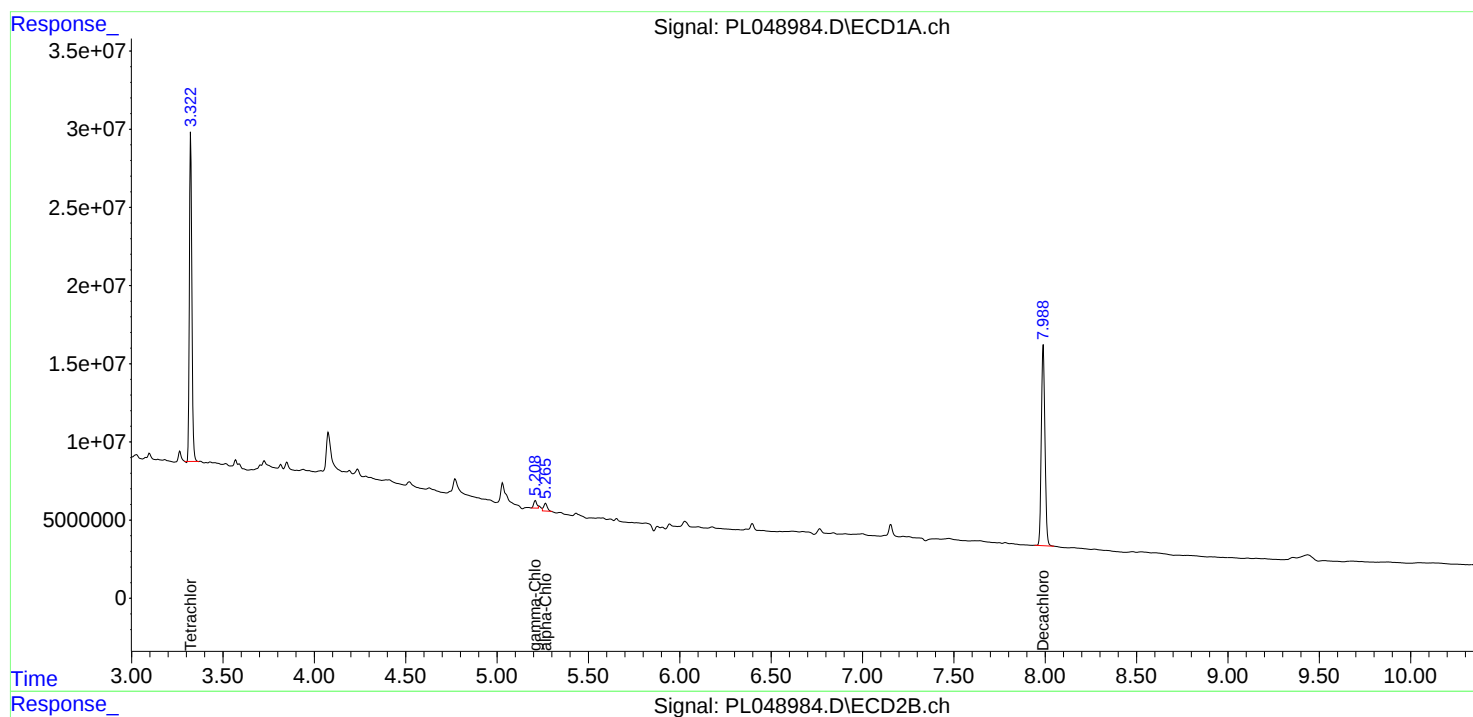

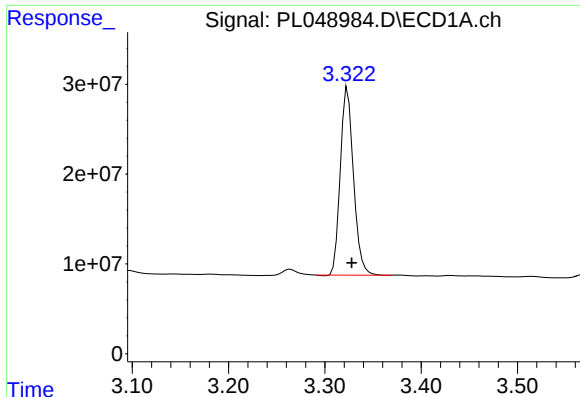


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: -0.004 min
Response: 198626887
Conc: 20.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-15 1.5-2.0


Manual Integrations
APPROVED

Ankita
5/28/2019 8:33:43 AM

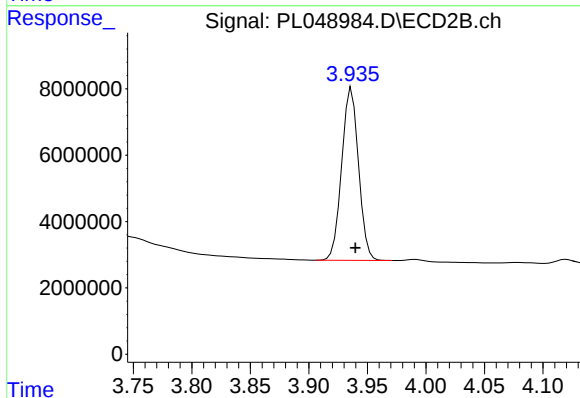


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: -0.003 min
Response: 52023890
Conc: 20.89 ng/ml

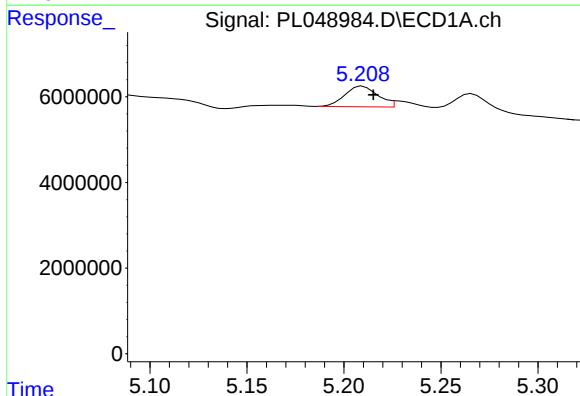


#10 gamma-Chlordane

R.T.: 5.208 min
Delta R.T.: -0.007 min
Response: 5935393
Conc: 0.44 ng/ml m

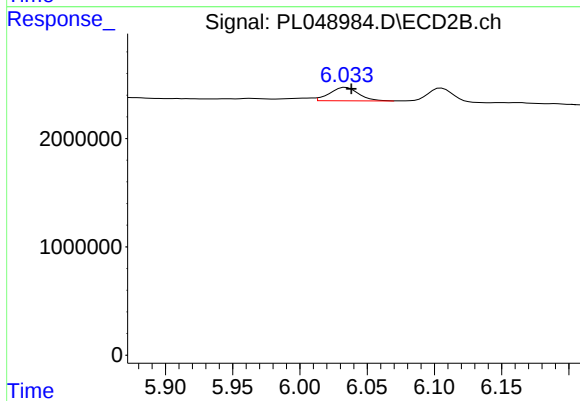

#10 gamma-Chlordane

R.T.: 6.033 min
Delta R.T.: -0.006 min
Response: 1824433
Conc: 0.59 ng/ml m

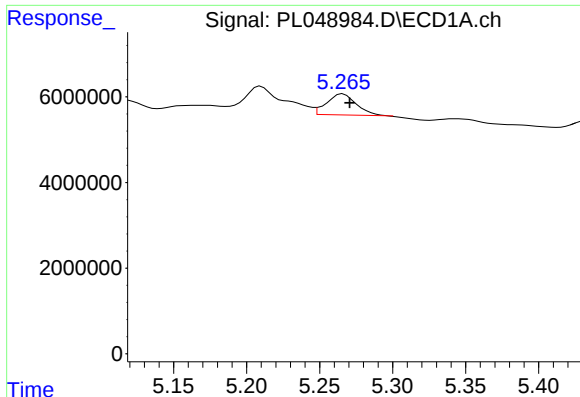


#11 alpha-Chlordane

R.T.: 5.265 min
Delta R.T.: -0.006 min
Response: 6790084
Conc: 0.52 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-15 1.5-2.0


Manual Integrations
APPROVED

Ankita
5/28/2019 8:33:43 AM

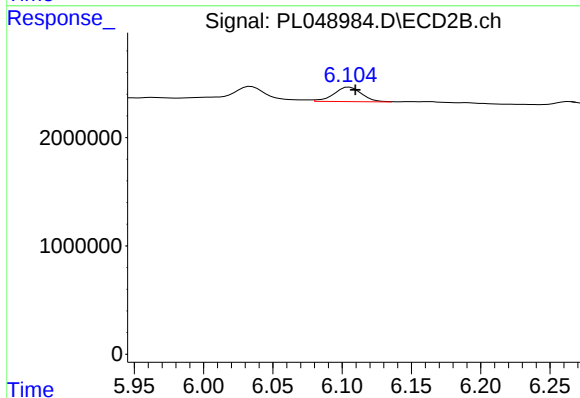


#11 alpha-Chlordane

R.T.: 6.104 min
Delta R.T.: -0.006 min
Response: 1862889
Conc: 0.61 ng/ml m

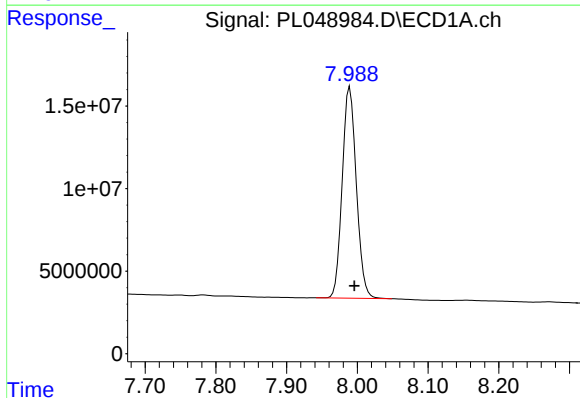

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.006 min
Response: 177537328
Conc: 17.66 ng/ml

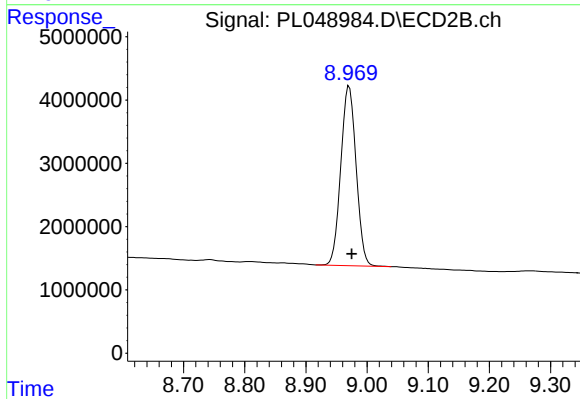

#28 Decachlorobiphenyl

R.T.: 8.971 min
Delta R.T.: -0.004 min
Response: 49316553
Conc: 18.58 ng/ml