

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052421\
 Data File : PL066844.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 20:26
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 05:57:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052421.M
 Quant Title : GC Extractables
 QLast Update : Tue May 25 05:57:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.532	59565369	86030065	102.161	102.740
28)	SA Decachlor...	10.225	11.432	68050553	78182358	94.407	94.506
Target Compounds							
23)	Chlordane-1	5.801	6.914	21561844	30757662	1039.750	1033.735
24)	Chlordane-2	6.487	7.505	27697535	35764983	983.073	967.451
25)	Chlordane-3	7.186	8.261	80755231	132.8E6	1017.376	1040.985
26)	Chlordane-4	7.252	8.344	86908722	157.5E6	1011.305	1023.266
27)	Chlordane-5	8.193	9.229	27694424	27773268	983.450	998.577



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052421\
Data File : PL066844.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 20:26
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 05:57:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052421.M
Quant Title : GC Extractables
QLast Update : Tue May 25 05:57:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

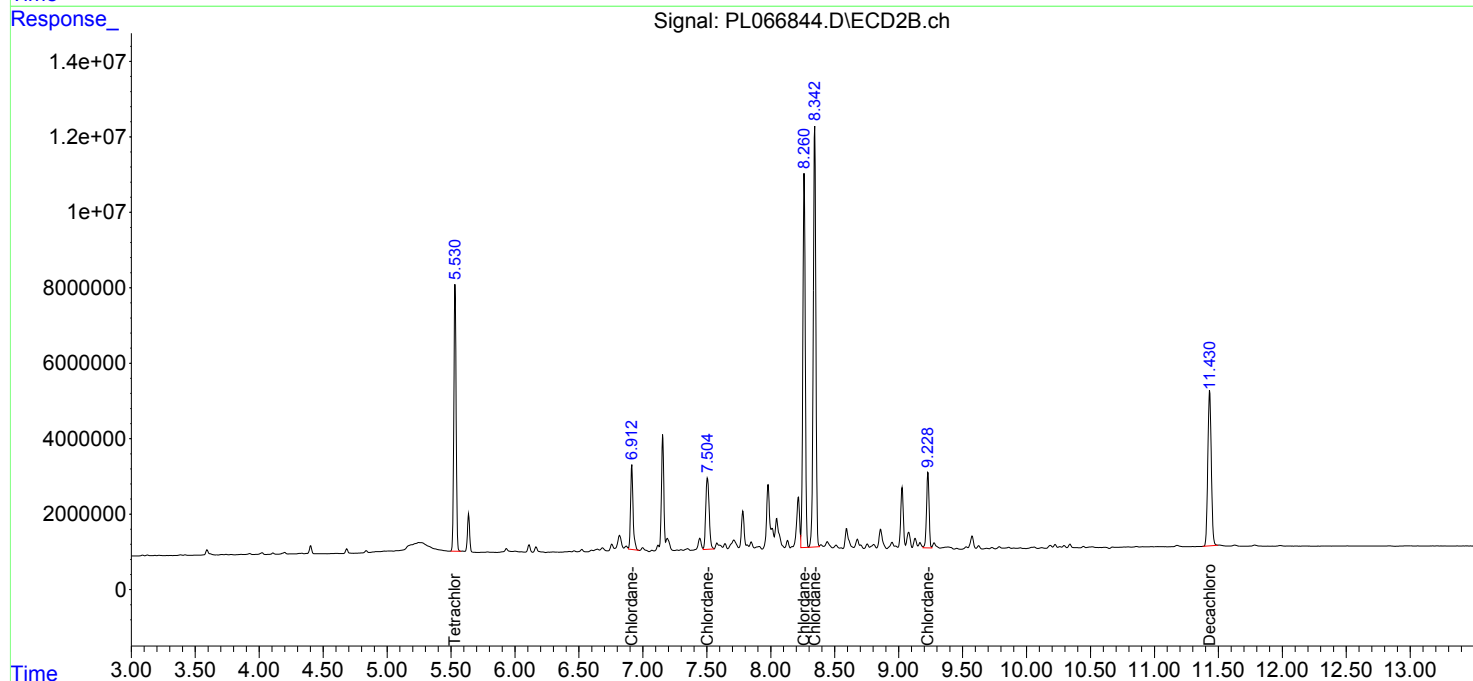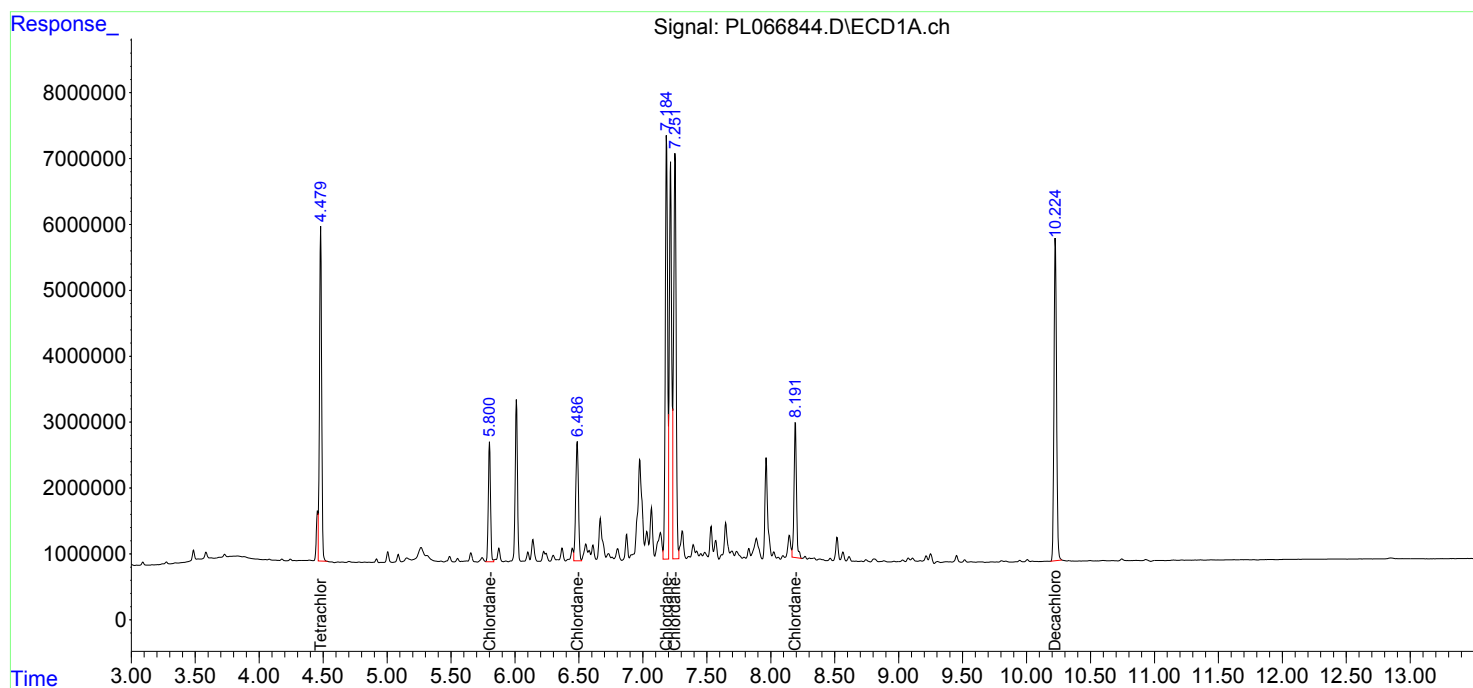


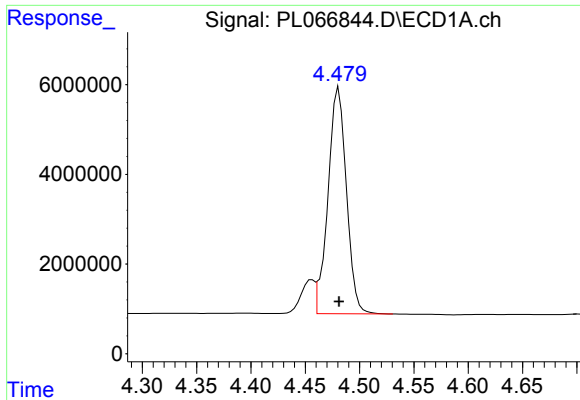

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 59565369
Conc: 102.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

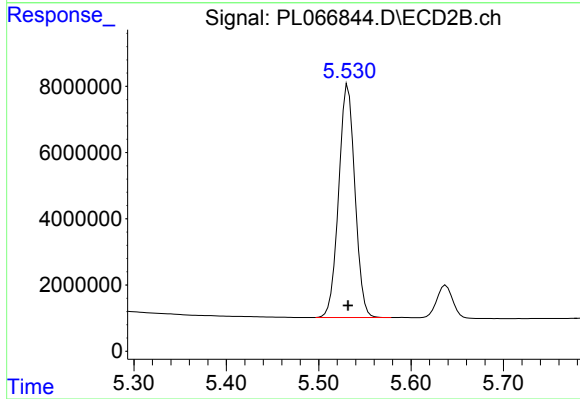


#1 Tetrachloro-m-xylene

R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 86030065
Conc: 102.74 ng/ml

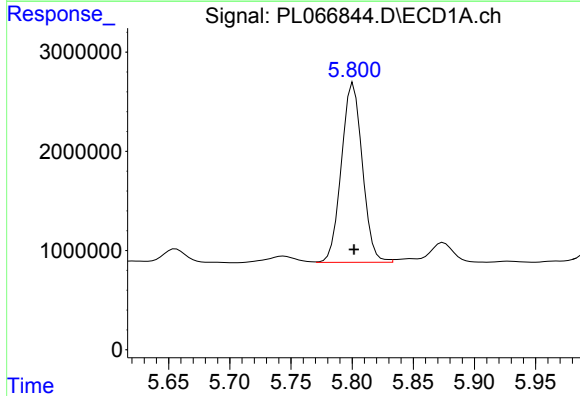


#23 Chlordane-1

R.T.: 5.801 min
Delta R.T.: 0.000 min
Response: 21561844
Conc: 1039.75 ng/ml

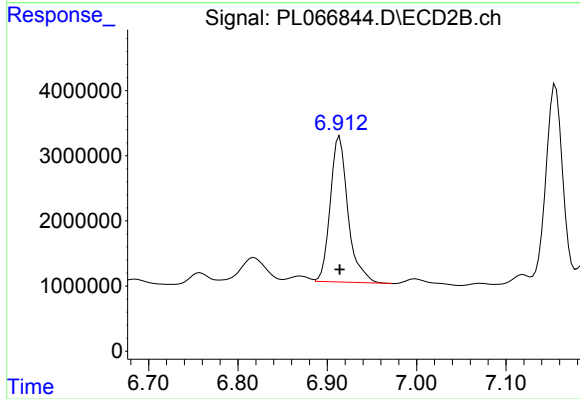

#23 Chlordane-1


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 30757662
Conc: 1033.74 ng/ml

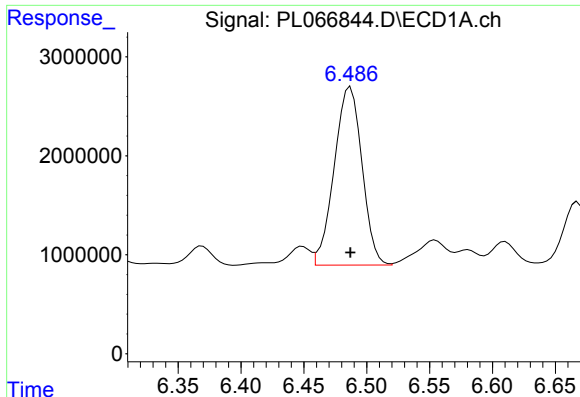

#24 Chlordane-2


R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 27697535
Conc: 983.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

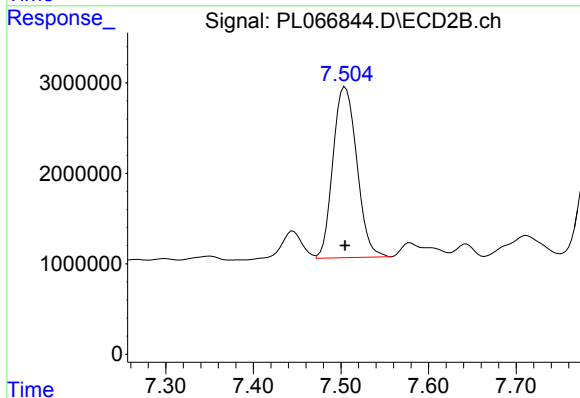


#24 Chlordane-2

R.T.: 7.505 min
Delta R.T.: 0.000 min
Response: 35764983
Conc: 967.45 ng/ml

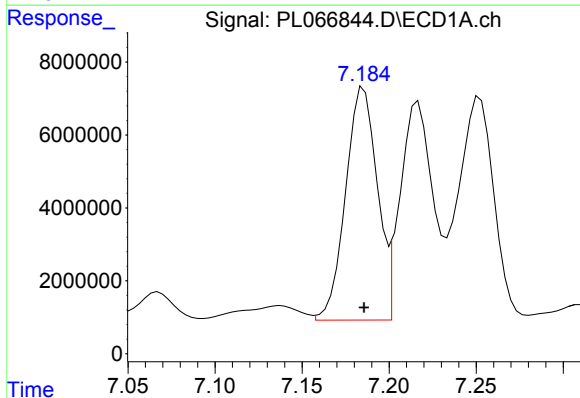


#25 Chlordane-3

R.T.: 7.186 min
Delta R.T.: 0.000 min
Response: 80755231
Conc: 1017.38 ng/ml

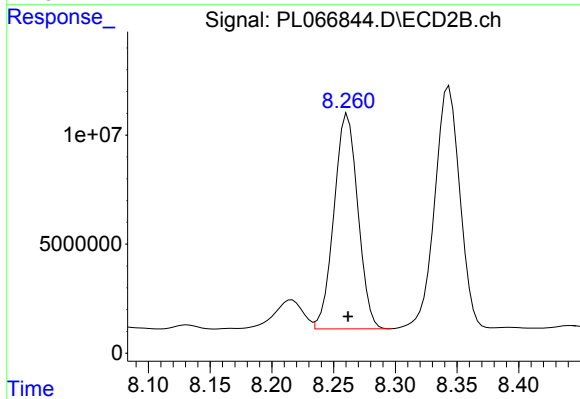

#25 Chlordane-3


R.T.: 8.261 min
Delta R.T.: 0.000 min
Response: 132763058
Conc: 1040.99 ng/ml

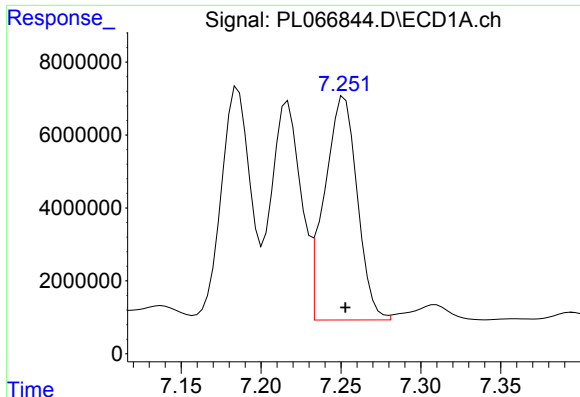

#26 Chlordane-4


R.T.: 7.252 min
Delta R.T.: 0.000 min
Response: 86908722
Conc: 1011.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

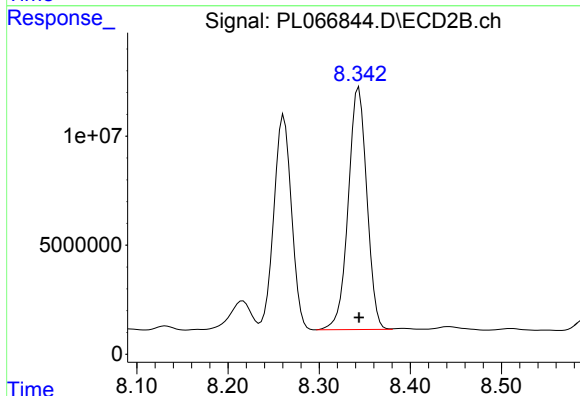


#26 Chlordane-4

R.T.: 8.344 min
Delta R.T.: 0.000 min
Response: 157474850
Conc: 1023.27 ng/ml

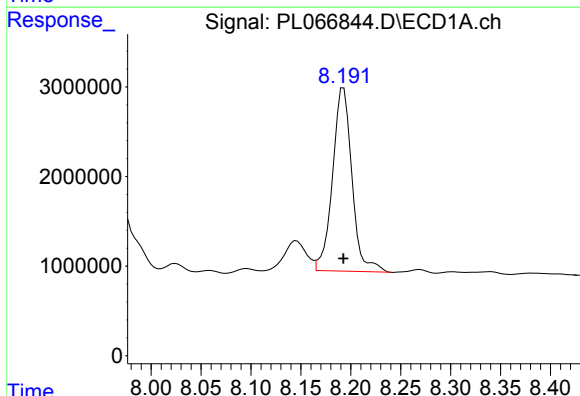


#27 Chlordane-5

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 27694424
Conc: 983.45 ng/ml

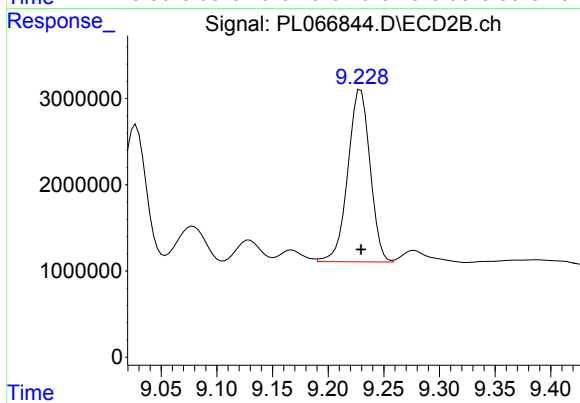

#27 Chlordane-5


R.T.: 9.229 min
Delta R.T.: 0.000 min
Response: 27773268
Conc: 998.58 ng/ml

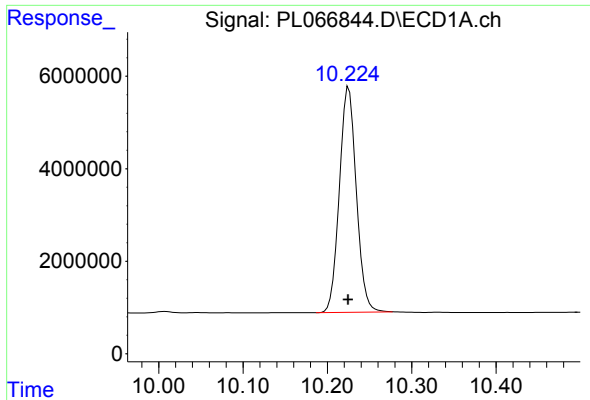

#28 Decachlorobiphenyl

R.T.: 10.225 min
Delta R.T.: 0.001 min
Response: 68050553
Conc: 94.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

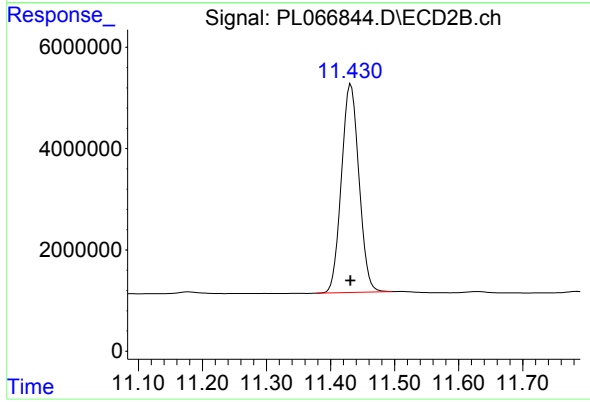

#28 Decachlorobiphenyl

R.T.: 11.432 min
Delta R.T.: 0.000 min
Response: 78182358
Conc: 94.51 ng/ml