

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052421\
 Data File : PL066845.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 20:46
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 05:57:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052421.M
 Quant Title : GC Extractables
 QLast Update : Tue May 25 05:57:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.532	43748044	63077102	75.032	75.329
28)	SA Decachlor...	10.225	11.431	52045531	59496423	72.203	71.919
Target Compounds							
23)	Chlordane-1	5.801	6.914	16036105	22542541	773.289	757.633
24)	Chlordane-2	6.487	7.505	21027685	27098480	746.339	733.020
25)	Chlordane-3	7.186	8.262	59715866	97027583	752.317	760.786
26)	Chlordane-4	7.252	8.344	64507345	116.1E6	750.633	754.617
27)	Chlordane-5	8.192	9.230	20890666	20740177	741.843	745.705



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052421\
Data File : PL066845.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 20:46
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 05:57:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052421.M
Quant Title : GC Extractables
QLast Update : Tue May 25 05:57:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

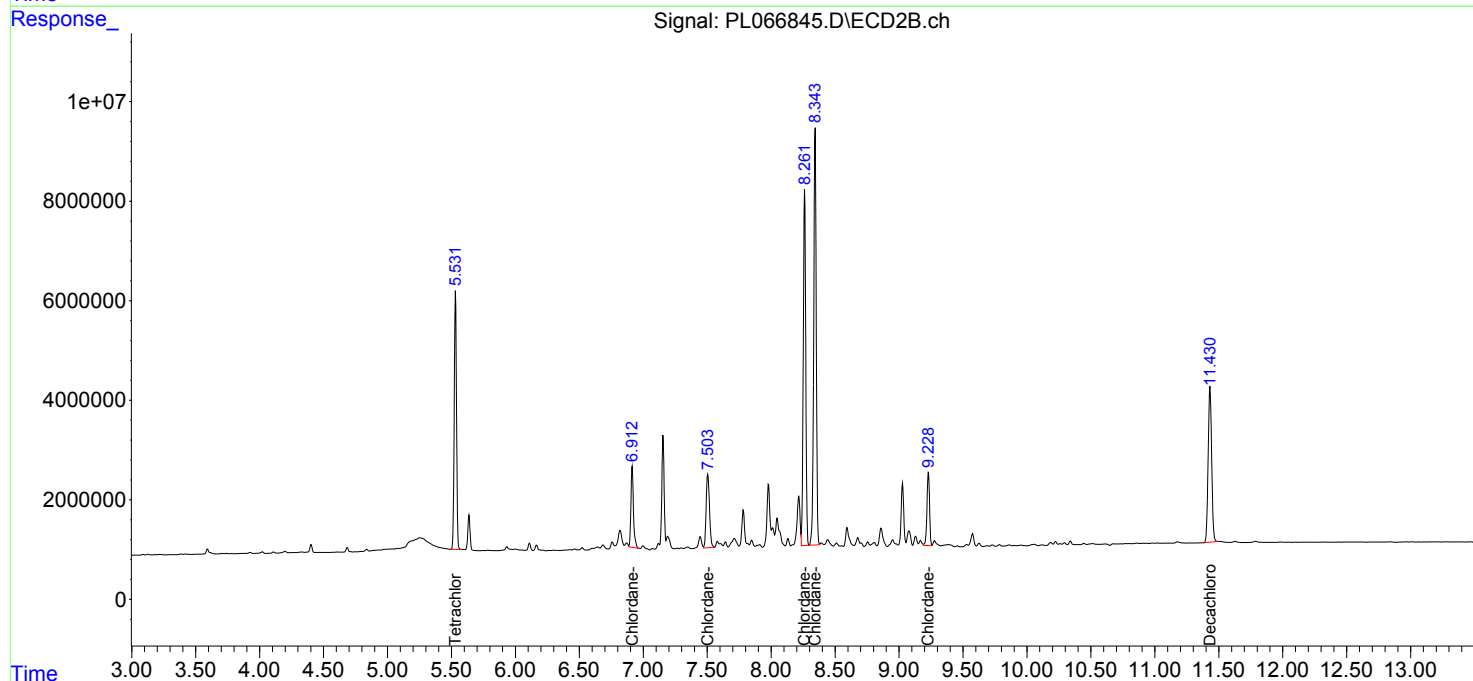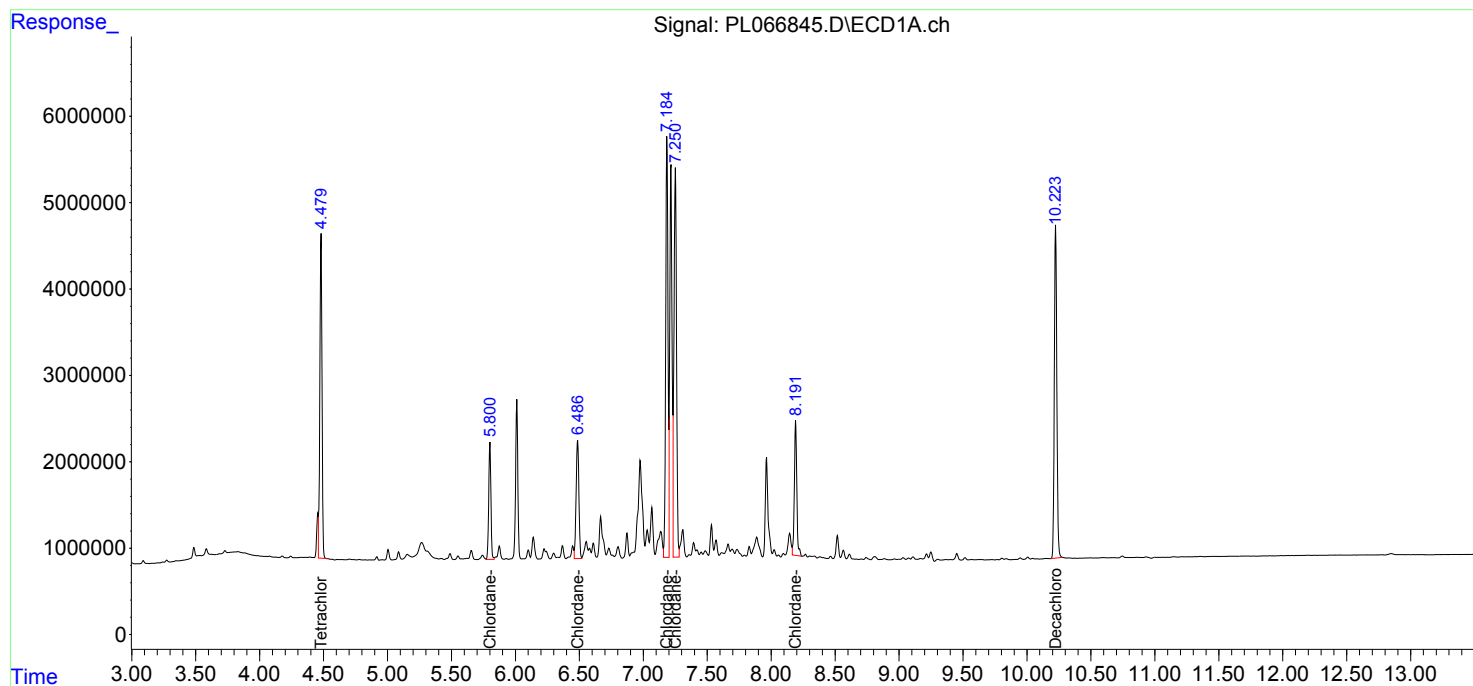


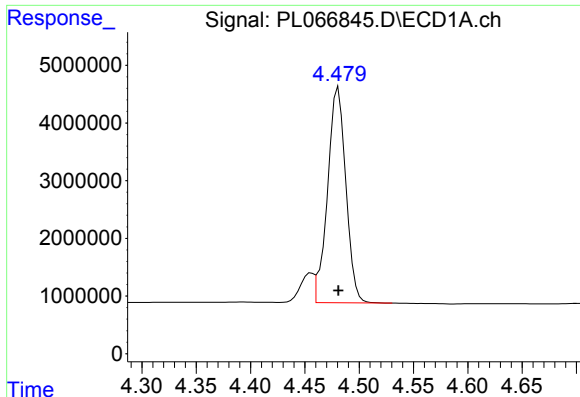

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 43748044
Conc: 75.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

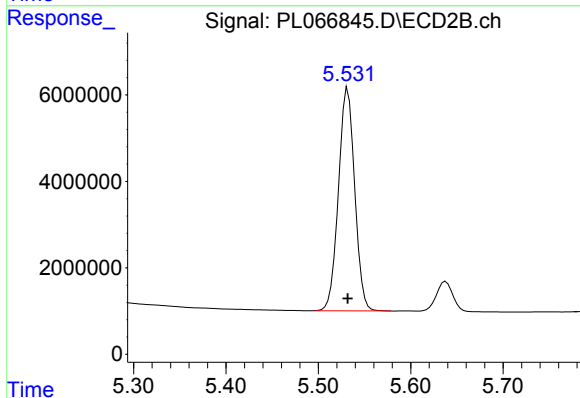


#1 Tetrachloro-m-xylene

R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 63077102
Conc: 75.33 ng/ml

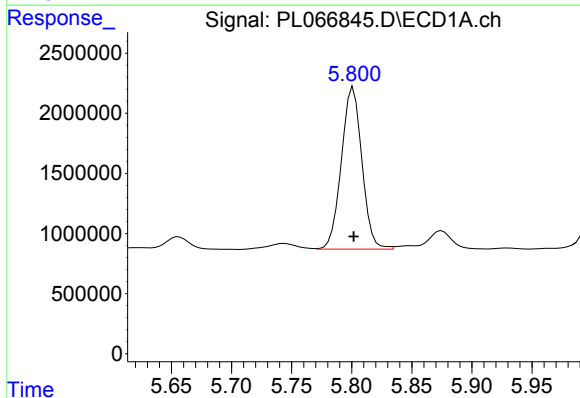


#23 Chlordane-1

R.T.: 5.801 min
Delta R.T.: 0.000 min
Response: 16036105
Conc: 773.29 ng/ml

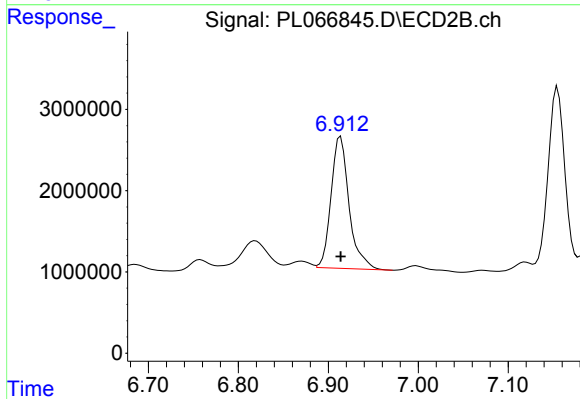

#23 Chlordane-1


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 22542541
Conc: 757.63 ng/ml

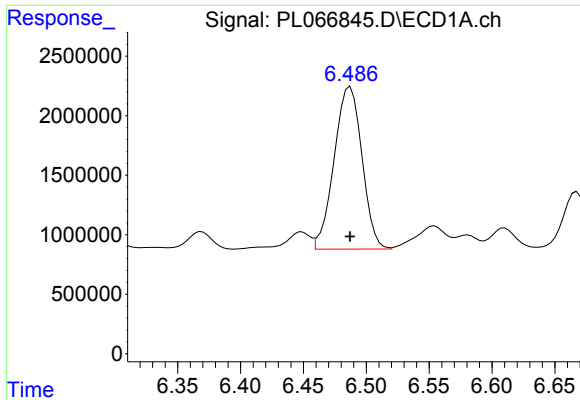

#24 Chlordane-2


R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 21027685
Conc: 746.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

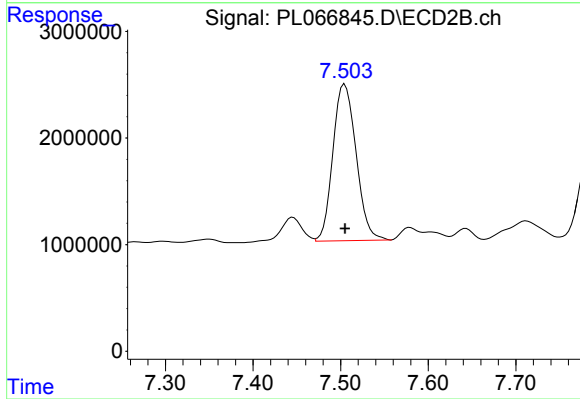


#24 Chlordane-2

R.T.: 7.505 min
Delta R.T.: 0.000 min
Response: 27098480
Conc: 733.02 ng/ml

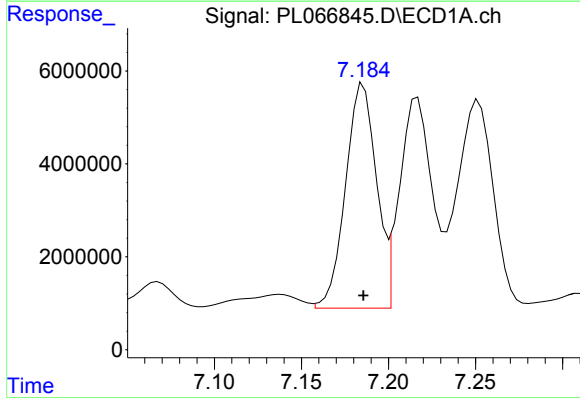


#25 Chlordane-3

R.T.: 7.186 min
Delta R.T.: 0.000 min
Response: 59715866
Conc: 752.32 ng/ml

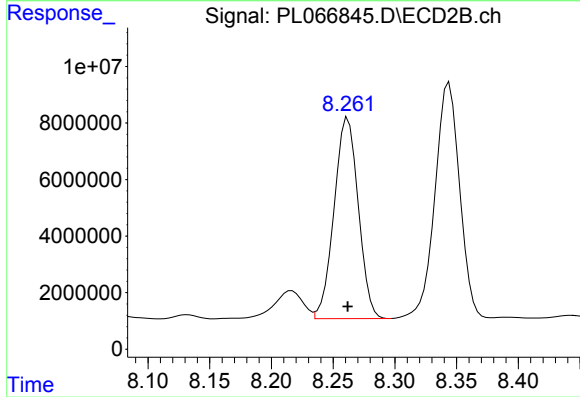

#25 Chlordane-3


R.T.: 8.262 min
Delta R.T.: 0.000 min
Response: 97027583
Conc: 760.79 ng/ml

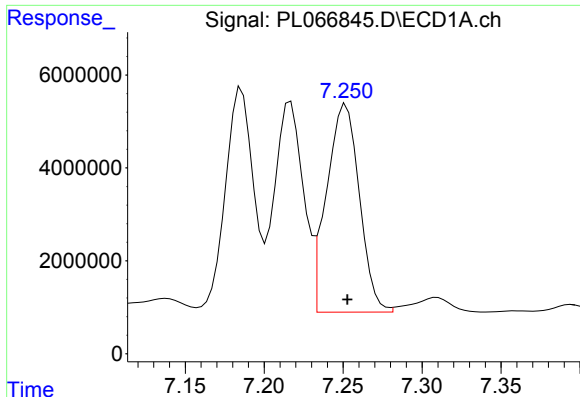

#26 Chlordane-4


R.T.: 7.252 min
Delta R.T.: 0.000 min
Response: 64507345
Conc: 750.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

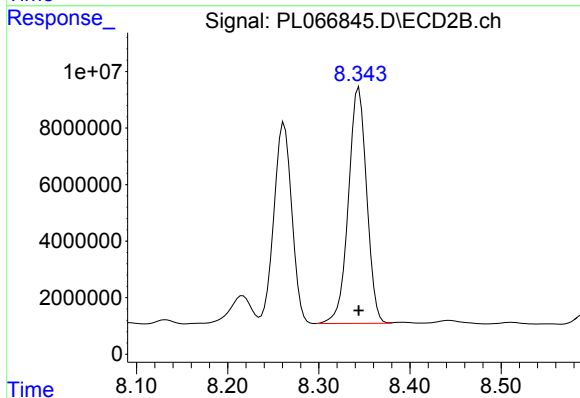


#26 Chlordane-4

R.T.: 8.344 min
Delta R.T.: 0.000 min
Response: 116131221
Conc: 754.62 ng/ml

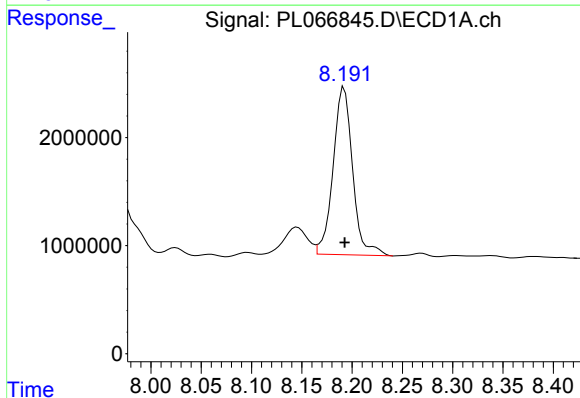


#27 Chlordane-5

R.T.: 8.192 min
Delta R.T.: 0.000 min
Response: 20890666
Conc: 741.84 ng/ml

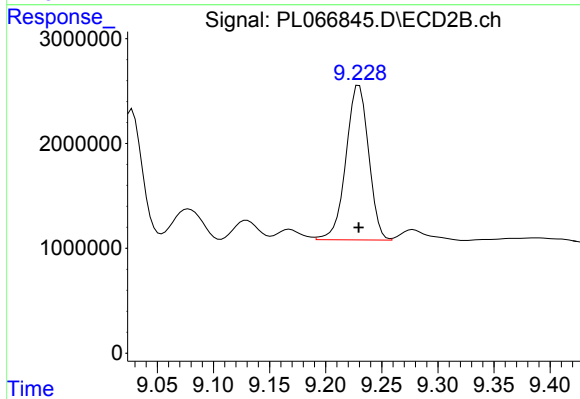

#27 Chlordane-5


R.T.: 9.230 min
Delta R.T.: 0.000 min
Response: 20740177
Conc: 745.71 ng/ml

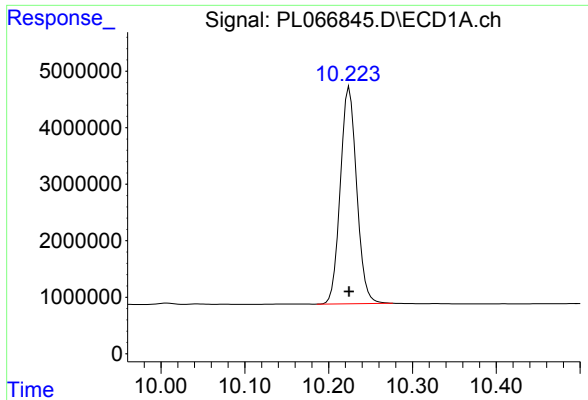

#28 Decachlorobiphenyl

R.T.: 10.225 min
Delta R.T.: 0.000 min
Response: 52045531
Conc: 72.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

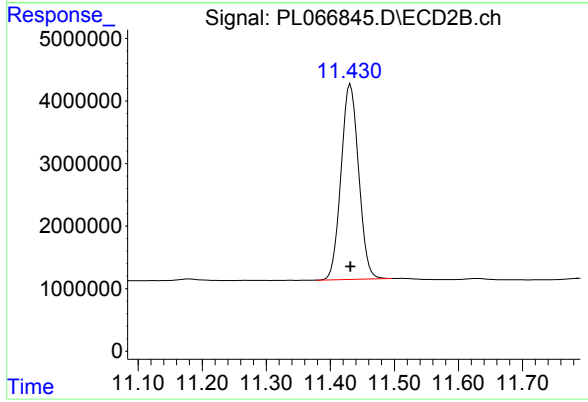

#28 Decachlorobiphenyl

R.T.: 11.431 min
Delta R.T.: 0.000 min
Response: 59496423
Conc: 71.92 ng/ml